

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059642.D
 Acq On : 5 Nov 2023 5:32
 Operator : MA/JU
 Sample : PB156686BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.081	113	118	124	rBV	92703	153291	12.12%	1.290%
2	4.164	130	132	135	rVB2	5507	4153	0.33%	0.035%
3	4.522	190	193	194	rBV2	4413	3996	0.32%	0.034%
4	5.315	326	328	331	rBV2	4791	5633	0.45%	0.047%
5	5.486	355	357	362	rBV2	5084	10036	0.79%	0.084%
6	5.650	383	385	389	rBV2	4182	5010	0.40%	0.042%
7	5.768	403	405	407	rBV	4506	3741	0.30%	0.031%
8	5.826	411	415	417	rBV	4094	6534	0.52%	0.055%
9	6.044	448	452	457	rBV	4912	7994	0.63%	0.067%
10	6.120	463	465	469	rVB	3568	4913	0.39%	0.041%
11	6.473	522	525	529	rVB	4317	5358	0.42%	0.045%
12	6.520	531	533	537	rBV	5368	6225	0.49%	0.052%
13	6.602	545	547	550	rBV	5625	5559	0.44%	0.047%
14	6.767	569	575	576	rBV	11615	12640	1.00%	0.106%
15	7.266	656	660	661	rBV	5128	5964	0.47%	0.050%
16	7.460	687	693	701	rBV	170190	305000	24.12%	2.566%
17	7.665	723	728	736	rVB2	104037	179263	14.18%	1.508%
18	7.865	752	762	770	rBV2	171594	313446	24.79%	2.637%
19	8.036	789	791	794	rVB	6339	3569	0.28%	0.030%
20	8.353	836	845	853	rBV2	128144	238823	18.89%	2.009%
21	8.670	896	899	906	rVB2	4597	9495	0.75%	0.080%
22	8.794	919	920	924	rBV2	3498	4684	0.37%	0.039%
23	9.034	953	961	971	rVB2	238308	414315	32.77%	3.485%
24	9.546	1042	1048	1055	rVB2	171341	308254	24.38%	2.593%
25	9.845	1096	1099	1104	rVB	4725	6898	0.55%	0.058%
26	10.268	1165	1171	1178	rVB2	168091	295058	23.33%	2.482%
27	10.791	1254	1260	1267	rBV3	240269	440715	34.85%	3.708%
28	11.103	1309	1313	1316	rBV3	4510	7178	0.57%	0.060%
29	11.197	1323	1329	1337	rVB	191943	366286	28.97%	3.081%
30	11.344	1347	1354	1364	rVV	239853	441449	34.91%	3.714%
31	11.414	1364	1366	1369	rVB	5668	5159	0.41%	0.043%
32	11.526	1383	1385	1389	rBV	3752	4381	0.35%	0.037%
33	11.584	1394	1395	1398	rVB	6760	5151	0.41%	0.043%
34	11.608	1398	1399	1401	rBV	5150	4442	0.35%	0.037%
35	11.626	1401	1402	1406	rVB	5270	4596	0.36%	0.039%
36	11.725	1415	1419	1422	rBV	5819	6599	0.52%	0.056%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059642.D
 Acq On : 5 Nov 2023 5:32
 Operator : MA/JU
 Sample : PB156686BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK686

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

37	11.814	1431	1434	1436	rBV	3450	4889	0.39%	0.041%
38	12.002	1465	1466	1471	rVB	4045	3877	0.31%	0.033%
39	12.354	1524	1526	1530	rVB	3995	4403	0.35%	0.037%
40	12.489	1546	1549	1551	rBV	4132	4944	0.39%	0.042%
41	12.654	1574	1577	1579	rBV	4663	4392	0.35%	0.037%
42	12.953	1626	1628	1630	rBV	4404	3716	0.29%	0.031%
43	13.735	1759	1761	1766	rBV	3638	4154	0.33%	0.035%
44	13.952	1796	1798	1801	rVB	4040	3841	0.30%	0.032%
45	14.322	1858	1861	1862	rBV	3916	3606	0.29%	0.030%
46	14.375	1864	1870	1875	rVB	539826	790492	62.52%	6.650%
47	14.534	1893	1897	1899	rBV	5480	6672	0.53%	0.056%
48	14.681	1916	1922	1930	rVB	563639	895818	70.85%	7.536%
49	14.798	1940	1942	1944	rVB	4812	3818	0.30%	0.032%
50	14.834	1947	1948	1952	rVB	5079	4478	0.35%	0.038%
51	14.980	1967	1973	1980	rVB	335832	533888	42.22%	4.491%
52	15.151	1995	2002	2009	rBV	296385	463346	36.64%	3.898%
53	15.233	2015	2016	2019	rBV	4993	3790	0.30%	0.032%
54	15.392	2041	2043	2046	rBV	8632	7744	0.61%	0.065%
55	15.897	2128	2129	2132	rBV	5577	3748	0.30%	0.032%
56	15.968	2135	2141	2147	rVB	697454	1064573	84.19%	8.956%
57	16.067	2152	2158	2164	rBV	243040	361353	28.58%	3.040%
58	16.203	2179	2181	2186	rVB	10432	10135	0.80%	0.085%
59	16.526	2235	2236	2238	rBV	5131	3808	0.30%	0.032%
60	16.731	2269	2271	2274	rBV	3915	4928	0.39%	0.041%
61	16.802	2281	2283	2286	rBV	4546	4104	0.32%	0.035%
62	16.855	2290	2292	2295	rBV	3874	3981	0.31%	0.033%
63	17.730	2435	2441	2450	rVB	494461	720369	56.97%	6.060%
64	17.830	2452	2458	2464	rVB2	811403	1230706	97.33%	10.353%
65	18.030	2489	2492	2496	rBV	7427	12051	0.95%	0.101%
66	18.617	2590	2592	2594	rBV	5345	5167	0.41%	0.043%
67	19.005	2656	2658	2662	rVB	6652	7945	0.63%	0.067%
68	19.411	2725	2727	2729	rBV2	6979	5115	0.40%	0.043%
69	20.104	2839	2845	2851	rVB	895308	1264458	100.00%	10.637%
70	22.066	3173	3179	3188	rVB2	450882	830836	65.71%	6.989%




Sum of corrected areas: 11886953

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059642.D
Acq On : 5 Nov 2023 5:32
Operator : MA/JU
Sample : PB156686BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

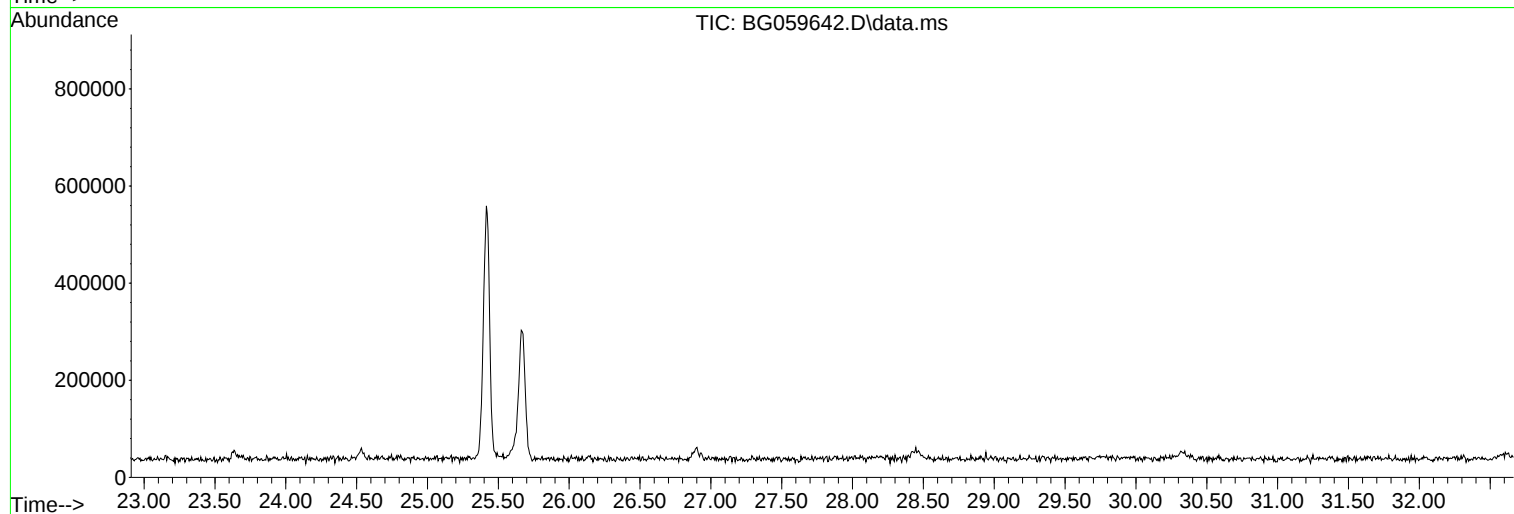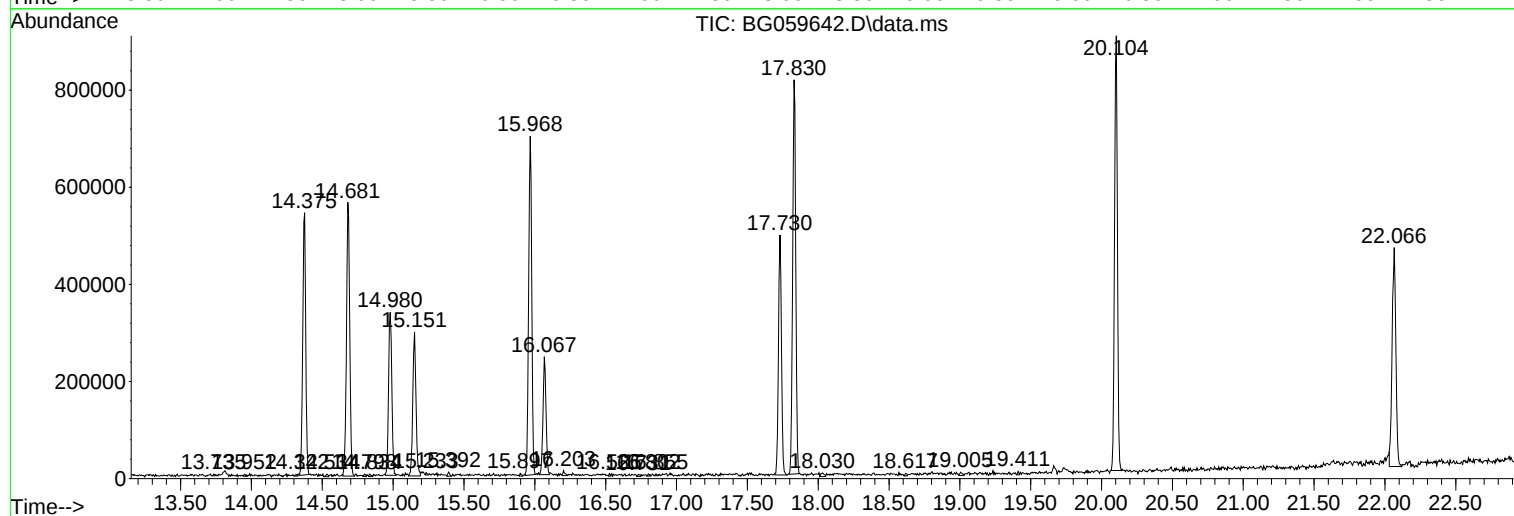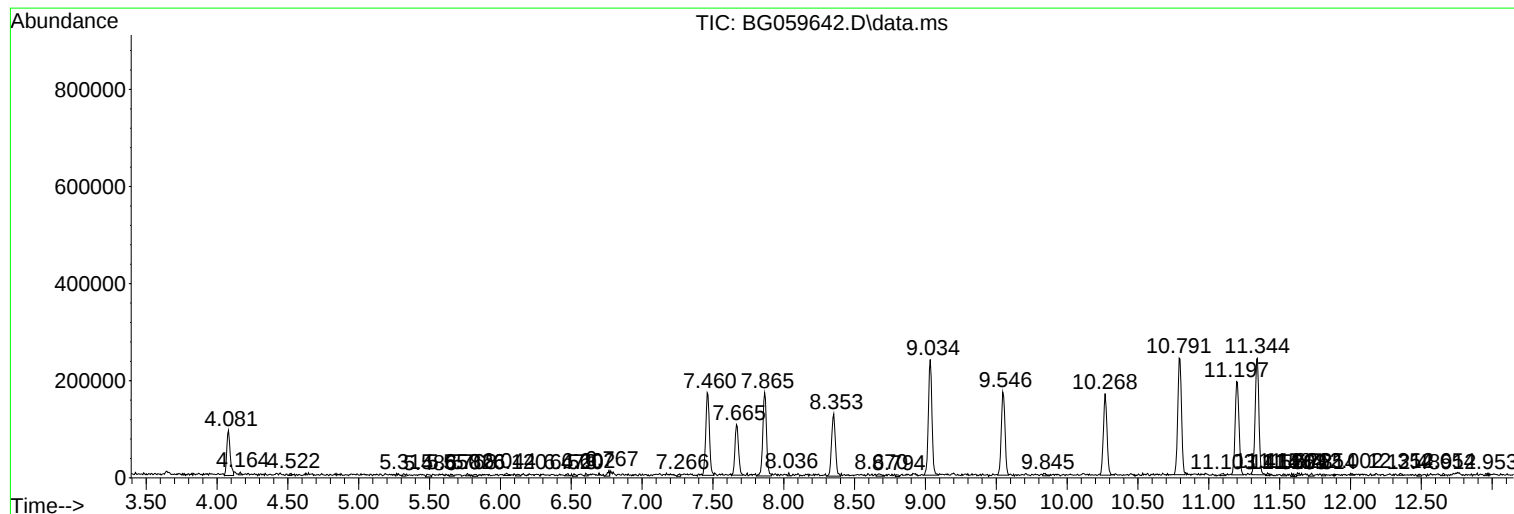

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059642.D
Acq On : 5 Nov 2023 5:32
Operator : MA/JU
Sample : PB156686BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059642.D
Acq On : 5 Nov 2023 5:32
Operator : MA/JU
Sample : PB156686BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK686

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc