

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059643.D
 Acq On : 5 Nov 2023 6:12
 Operator : MA/JU
 Sample : PB156685BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK685

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.749	58	61	62	rBV3	4137	4838	0.43%	0.049%
2	4.078	112	117	127	rBV	85171	140908	12.59%	1.426%
3	4.336	159	161	164	rBV	4359	3822	0.34%	0.039%
4	4.501	186	189	192	rBV2	4512	3889	0.35%	0.039%
5	4.566	197	200	201	rBV2	4149	4848	0.43%	0.049%
6	5.036	277	280	282	rBV2	3698	3623	0.32%	0.037%
7	5.059	282	284	287	rVV	3348	3803	0.34%	0.038%
8	5.153	299	300	304	rVB	6717	4519	0.40%	0.046%
9	5.470	352	354	358	rBV	5795	6433	0.57%	0.065%
10	5.611	374	378	379	rBV	7666	5446	0.49%	0.055%
11	5.964	435	438	440	rBV	5802	5783	0.52%	0.059%
12	6.005	443	445	447	rVB	5798	3553	0.32%	0.036%
13	6.275	488	491	494	rBV	3329	5243	0.47%	0.053%
14	6.504	528	530	532	rBV	4251	3404	0.30%	0.034%
15	6.575	540	542	545	rVB	4410	3514	0.31%	0.036%
16	6.687	558	561	564	rVB	5031	7100	0.63%	0.072%
17	6.722	564	567	568	rBV	3976	3820	0.34%	0.039%
18	6.828	584	585	590	rVB	5910	5101	0.46%	0.052%
19	7.027	618	619	625	rVB	5224	5189	0.46%	0.053%
20	7.104	630	632	635	rBV	2933	3407	0.30%	0.034%
21	7.139	637	638	642	rBV	4568	4889	0.44%	0.049%
22	7.227	650	653	654	rVB	6034	5399	0.48%	0.055%
23	7.251	654	657	658	rBV	4555	4671	0.42%	0.047%
24	7.462	686	693	700	rBV	148304	270487	24.17%	2.737%
25	7.668	723	728	734	rVB2	92743	160233	14.32%	1.622%
26	7.809	747	752	754	rBV2	2898	4692	0.42%	0.047%
27	7.868	754	762	769	rVB	148524	272451	24.35%	2.757%
28	8.197	816	818	822	rBV	3167	3833	0.34%	0.039%
29	8.349	839	844	851	rVB2	96291	163612	14.62%	1.656%
30	8.520	868	873	875	rBV2	4670	6473	0.58%	0.066%
31	8.814	921	923	927	rVB2	4029	4825	0.43%	0.049%
32	8.919	939	941	945	rBV2	3547	4282	0.38%	0.043%
33	9.031	948	960	966	rBV3	205058	359856	32.16%	3.642%
34	9.101	970	972	976	rVB3	4661	5509	0.49%	0.056%
35	9.237	993	995	1000	rVB3	3196	3679	0.33%	0.037%
36	9.313	1005	1008	1011	rBV3	3001	3455	0.31%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059643.D
 Acq On : 5 Nov 2023 6:12
 Operator : MA/JU
 Sample : PB156685BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK685

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

37	9.483	1034	1037	1041	rBV	3410	3773	0.34%	0.038%
38	9.548	1041	1048	1055	rBV2	151636	277469	24.80%	2.808%
39	9.906	1106	1109	1112	rBV2	2435	3489	0.31%	0.035%
40	10.206	1156	1160	1161	rBV2	3303	3813	0.34%	0.039%
41	10.271	1164	1171	1181	rVB3	142024	275101	24.59%	2.784%
42	10.394	1189	1192	1193	rBV3	4781	4770	0.43%	0.048%
43	10.794	1253	1260	1269	rBV2	225197	397608	35.54%	4.024%
44	10.899	1276	1278	1282	rVB2	6052	6395	0.57%	0.065%
45	10.935	1282	1284	1285	rBV2	6340	4292	0.38%	0.043%
46	11.052	1302	1304	1307	rBV	4849	6005	0.54%	0.061%
47	11.081	1307	1309	1312	rVB	4271	4013	0.36%	0.041%
48	11.199	1318	1329	1336	rBV	142900	256875	22.96%	2.600%
49	11.340	1346	1353	1361	rVB2	205415	377979	33.78%	3.825%
50	11.440	1368	1370	1372	rBV2	4439	3699	0.33%	0.037%
51	11.522	1379	1384	1385	rVV2	4308	4850	0.43%	0.049%
52	12.221	1501	1503	1504	rBV2	6267	3963	0.35%	0.040%
53	12.591	1563	1566	1567	rBV2	3562	4016	0.36%	0.041%
54	12.662	1575	1578	1581	rVB2	2693	3441	0.31%	0.035%
55	12.756	1592	1594	1600	rVB3	10827	13645	1.22%	0.138%
56	12.803	1600	1602	1604	rBV3	4600	4504	0.40%	0.046%
57	12.832	1604	1607	1609	rVB	4310	4331	0.39%	0.044%
58	12.862	1609	1612	1613	rBV	3568	3531	0.32%	0.036%
59	13.062	1644	1646	1650	rVB	3997	4776	0.43%	0.048%
60	13.120	1652	1656	1657	rBV	4372	4227	0.38%	0.043%
61	13.379	1697	1700	1703	rVB	4804	5215	0.47%	0.053%
62	13.802	1770	1772	1773	rBV	4894	4118	0.37%	0.042%
63	14.372	1863	1869	1877	rBV	477535	685250	61.24%	6.935%
64	14.619	1909	1911	1912	rBV	3421	3434	0.31%	0.035%
65	14.683	1915	1922	1930	rVV2	476917	763463	68.23%	7.726%
66	14.871	1952	1954	1957	rBV2	3667	4942	0.44%	0.050%
67	14.983	1967	1973	1980	rBV	227605	363360	32.48%	3.677%
68	15.042	1982	1983	1985	rVB	5831	3463	0.31%	0.035%
69	15.065	1985	1987	1988	rBV	4491	4207	0.38%	0.043%
70	15.147	1994	2001	2007	rBV	241254	400984	35.84%	4.058%
71	15.247	2016	2018	2021	rVB	5351	3388	0.30%	0.034%
72	15.418	2045	2047	2050	rVB	5858	4700	0.42%	0.048%
73	15.470	2053	2056	2058	rBV	3782	4231	0.38%	0.043%
74	15.535	2064	2067	2068	rVB	5281	4329	0.39%	0.044%
75	15.547	2068	2069	2071	rBV	3942	3567	0.32%	0.036%
76	15.764	2104	2106	2111	rBV	5123	6848	0.61%	0.069%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059643.D
 Acq On : 5 Nov 2023 6:12
 Operator : MA/JU
 Sample : PB156685BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK685

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

77	15.817	2111	2115	2118	rVV	7484	6986	0.62%	0.071%
78	15.846	2118	2120	2122	rVB	4223	3469	0.31%	0.035%
79	15.970	2133	2141	2148	rBV	595005	916713	81.93%	9.277%
80	16.023	2148	2150	2153	rBV	3333	4918	0.44%	0.050%
81	16.070	2153	2158	2166	rVB2	196056	295905	26.45%	2.994%
82	16.176	2175	2176	2178	rBV	3569	3752	0.34%	0.038%
83	16.275	2192	2193	2196	rBV	3766	3809	0.34%	0.039%
84	16.986	2312	2314	2317	rBV	5596	6587	0.59%	0.067%
85	17.368	2377	2379	2381	rBV	3738	3391	0.30%	0.034%
86	17.515	2402	2404	2407	rBV	5095	5365	0.48%	0.054%
87	17.556	2409	2411	2413	rBV	4495	3937	0.35%	0.040%
88	17.733	2435	2441	2447	rBV	300602	471099	42.10%	4.767%
89	17.832	2452	2458	2465	rVV	689184	1056445	94.42%	10.691%
90	17.903	2469	2470	2473	rBV	5052	4812	0.43%	0.049%
91	18.543	2575	2579	2580	rBV	5630	4706	0.42%	0.048%
92	18.573	2582	2584	2585	rBV	4847	4392	0.39%	0.044%
93	18.626	2592	2593	2595	rBV	6003	3984	0.36%	0.040%
94	18.761	2615	2616	2619	rBV	4637	3564	0.32%	0.036%
95	19.389	2721	2723	2726	rVB	6494	5370	0.48%	0.054%
96	19.542	2747	2749	2753	rBV	4116	4676	0.42%	0.047%
97	19.577	2753	2755	2758	rBV3	5100	4937	0.44%	0.050%
98	19.671	2767	2771	2774	rBV4	12733	17310	1.55%	0.175%
99	20.100	2839	2844	2852	rVB	782547	1118877	100.00%	11.323%
100	22.063	3172	3178	3183	rBV	269070	478027	42.72%	4.838%




Sum of corrected areas: 9881684

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059643.D
Acq On : 5 Nov 2023 6:12
Operator : MA/JU
Sample : PB156685BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK685

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

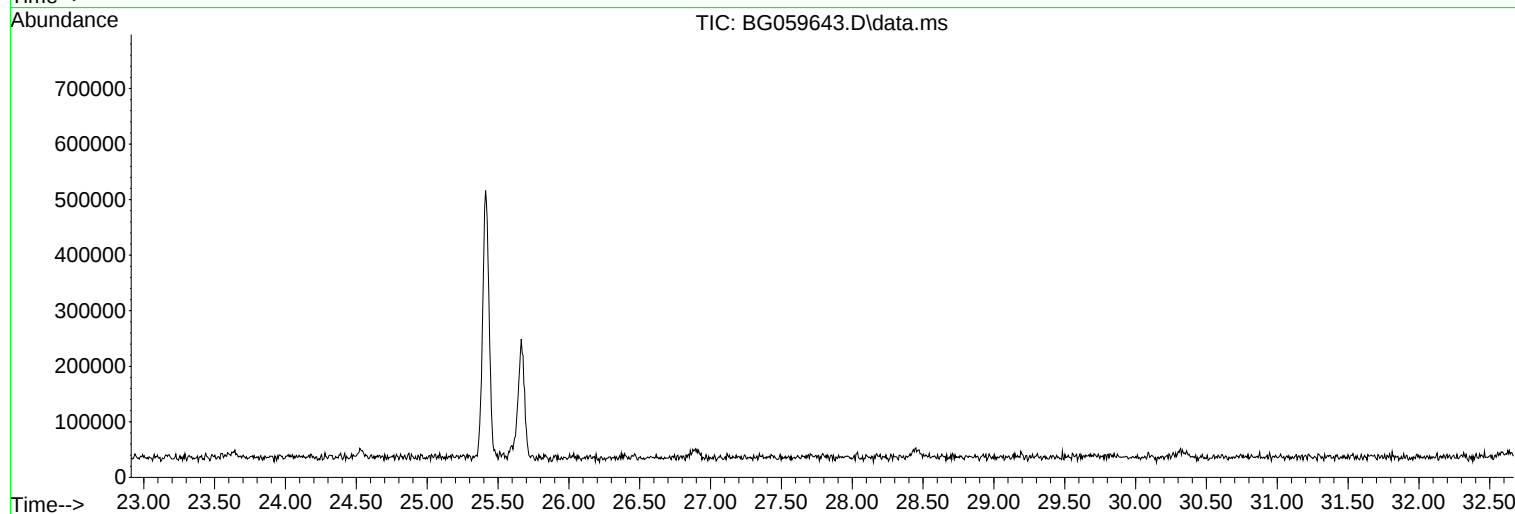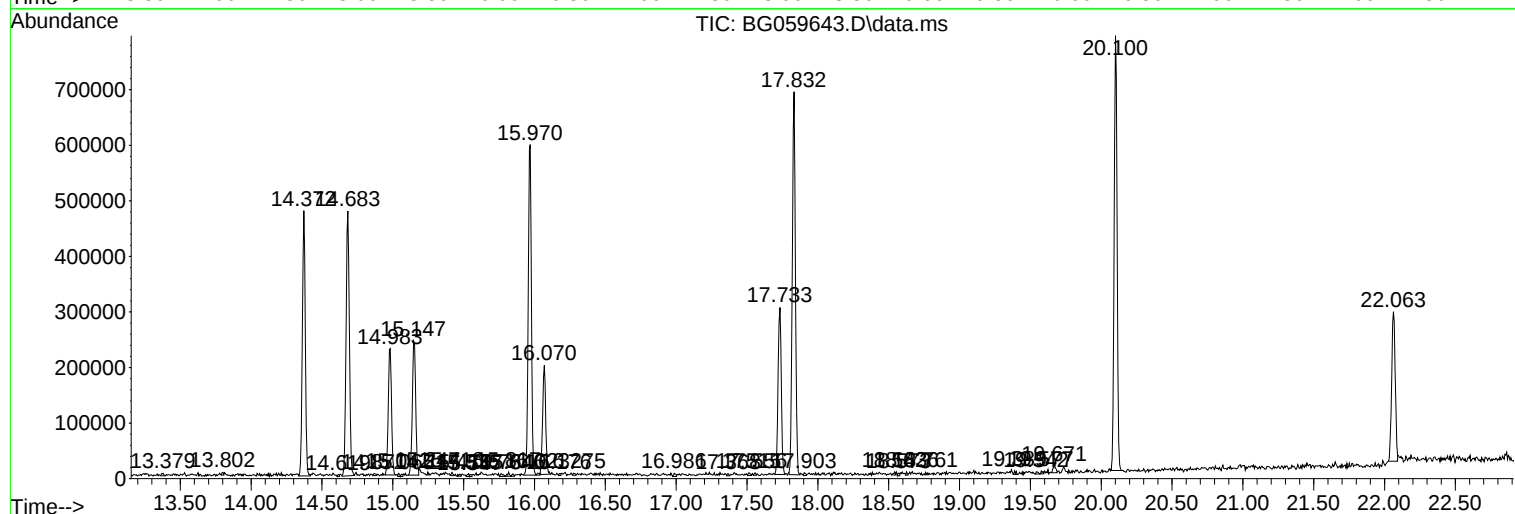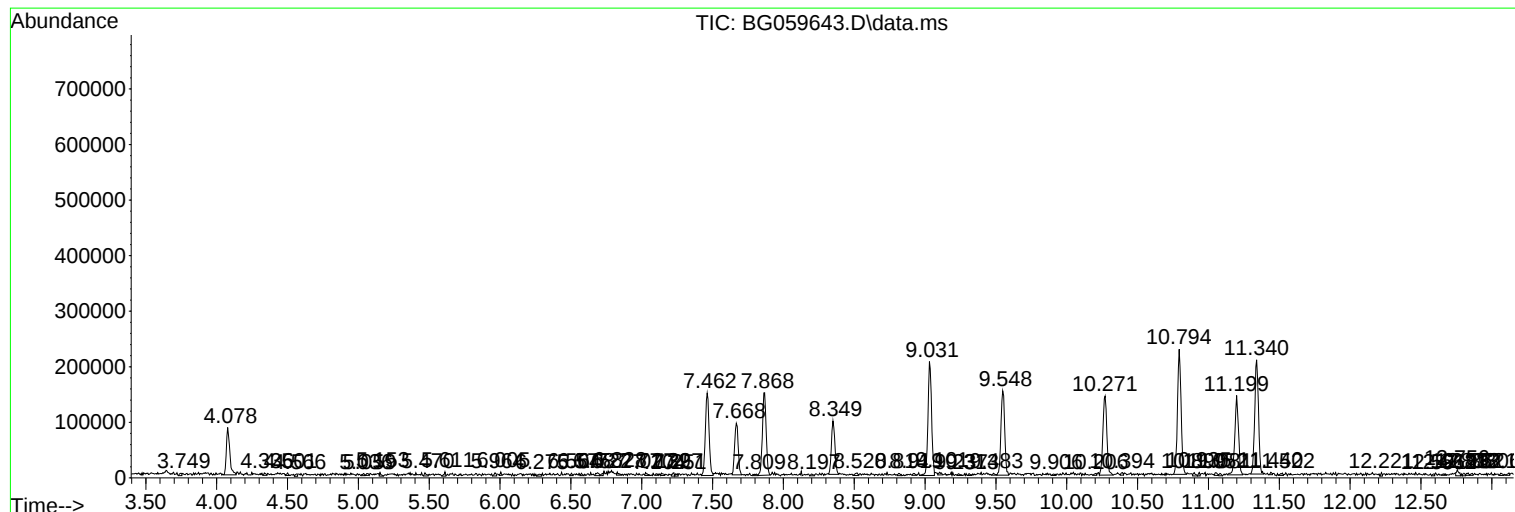

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059643.D
Acq On : 5 Nov 2023 6:12
Operator : MA/JU
Sample : PB156685BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK685

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059643.D
Acq On : 5 Nov 2023 6:12
Operator : MA/JU
Sample : PB156685BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK685

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------