

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059657.D
 Acq On : 5 Nov 2023 16:22
 Operator : MA/JU
 Sample : PB156653BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK653

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.647	42	44	49	rVB3	7597	8855	0.50%	0.059%
2	4.076	111	117	127	rBV	105746	184286	10.41%	1.235%
3	5.157	299	301	304	rBV	3724	4774	0.27%	0.032%
4	5.392	340	341	344	rBV	4799	5670	0.32%	0.038%
5	6.015	446	447	450	rBV	3878	4873	0.28%	0.033%
6	7.161	641	642	647	rVB	3754	4972	0.28%	0.033%
7	7.460	686	693	702	rBV	208245	365124	20.62%	2.447%
8	7.666	723	728	736	rVB2	122443	202105	11.42%	1.354%
9	7.778	741	747	749	rBV2	5698	7920	0.45%	0.053%
10	7.866	755	762	768	rBV	211345	361274	20.41%	2.421%
11	8.189	815	817	822	rBV	4490	6441	0.36%	0.043%
12	8.348	838	844	854	rVB2	126091	219923	12.42%	1.474%
13	8.753	911	913	917	rBV2	4995	5391	0.30%	0.036%
14	8.829	923	926	929	rBV	6018	7137	0.40%	0.048%
15	9.035	952	961	969	rBV	286184	494831	27.95%	3.316%
16	9.329	1008	1011	1013	rBV	4002	5071	0.29%	0.034%
17	9.546	1041	1048	1055	rBV	214239	372848	21.06%	2.499%
18	9.617	1058	1060	1063	rVB	7202	6363	0.36%	0.043%
19	10.216	1160	1162	1164	rBV	3829	5072	0.29%	0.034%
20	10.269	1164	1171	1178	rVV2	207674	371503	20.99%	2.490%
21	10.574	1220	1223	1229	rBV2	3787	8240	0.47%	0.055%
22	10.704	1242	1245	1248	rBV2	4499	5092	0.29%	0.034%
23	10.792	1253	1260	1267	rVB2	289707	528616	29.86%	3.543%
24	11.197	1321	1329	1335	rBV	187918	341764	19.31%	2.290%
25	11.338	1343	1353	1361	rBV2	267004	516840	29.19%	3.464%
26	11.450	1369	1372	1375	rBV2	5388	6361	0.36%	0.043%
27	11.491	1375	1379	1380	rBV2	3942	5481	0.31%	0.037%
28	11.697	1412	1414	1417	rVB2	6089	5295	0.30%	0.035%
29	11.732	1417	1420	1423	rBV2	5489	6756	0.38%	0.045%
30	11.990	1461	1464	1466	rBV	5263	5222	0.29%	0.035%
31	12.590	1561	1566	1568	rBV	4124	7489	0.42%	0.050%
32	12.737	1587	1591	1592	rBV	5128	5147	0.29%	0.034%
33	12.754	1592	1594	1600	rVB3	9784	14617	0.83%	0.098%
34	12.837	1606	1608	1612	rBV3	4371	8124	0.46%	0.054%
35	13.289	1683	1685	1688	rVB3	6228	6570	0.37%	0.044%
36	13.806	1769	1773	1778	rVB3	7753	12214	0.69%	0.082%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059657.D
 Acq On : 5 Nov 2023 16:22
 Operator : MA/JU
 Sample : PB156653BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK653

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

37	14.247	1847	1848	1851	rVB3	6088	5121	0.29%	0.034%
38	14.370	1863	1869	1878	rBV	588511	900286	50.85%	6.033%
39	14.681	1916	1922	1929	rBV	645100	979384	55.32%	6.563%
40	14.981	1967	1973	1982	rVB	305935	490035	27.68%	3.284%
41	15.151	1995	2002	2011	rBV2	333886	526504	29.74%	3.528%
42	15.257	2018	2020	2024	rVB2	5117	4831	0.27%	0.032%
43	15.968	2135	2141	2148	rVB	758911	1167420	65.94%	7.824%
44	16.068	2152	2158	2164	rBV2	294678	417871	23.60%	2.800%
45	16.462	2223	2225	2227	rBV	4832	4915	0.28%	0.033%
46	16.720	2267	2269	2273	rBV	3947	6618	0.37%	0.044%
47	16.808	2281	2284	2285	rBV	5171	5005	0.28%	0.034%
48	17.267	2360	2362	2367	rVB	3644	5439	0.31%	0.036%
49	17.331	2369	2373	2374	rBV	5855	5627	0.32%	0.038%
50	17.731	2435	2441	2450	rVB	398353	608177	34.35%	4.076%
51	17.831	2452	2458	2465	rBV2	879688	1333869	75.35%	8.939%
52	18.853	2631	2632	2636	rBV	3929	5852	0.33%	0.039%
53	19.112	2674	2676	2680	rVB2	8719	6743	0.38%	0.045%
54	20.104	2839	2845	2851	rBV	1213803	1770325	100.00%	11.864%
55	22.061	3173	3178	3186	rVB	444374	800325	45.21%	5.363%
56	25.422	3742	3750	3762	rVB2	576742	1749266	98.81%	11.723%




Sum of corrected areas: 14921874

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059657.D
Acq On : 5 Nov 2023 16:22
Operator : MA/JU
Sample : PB156653BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK653

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

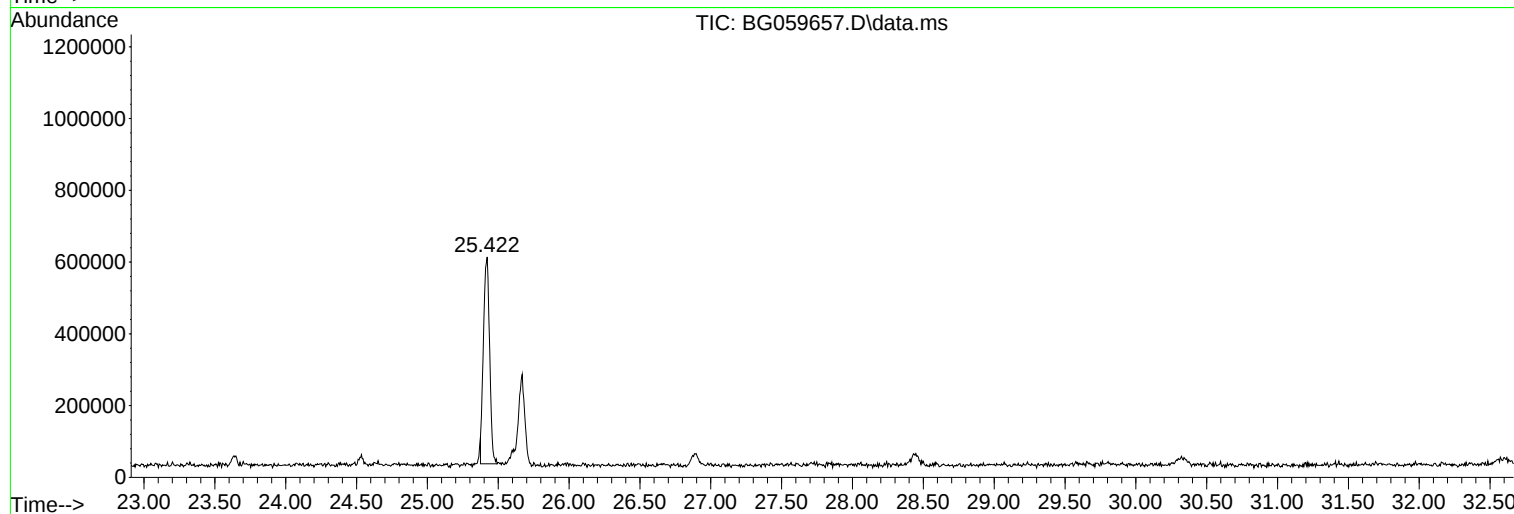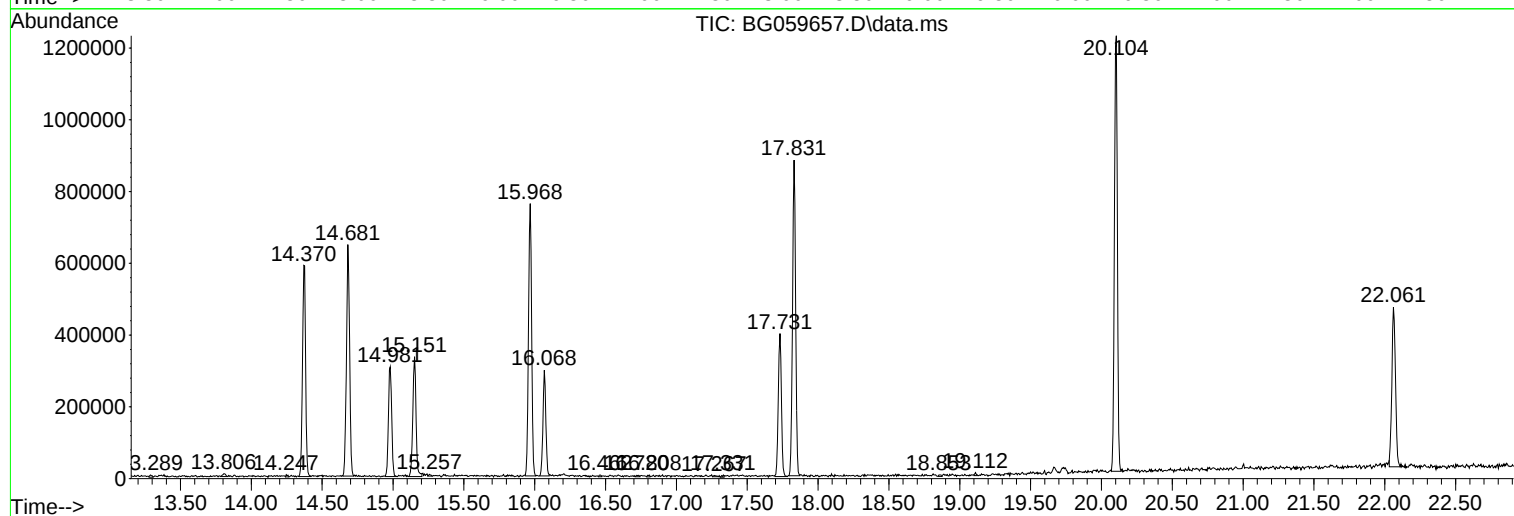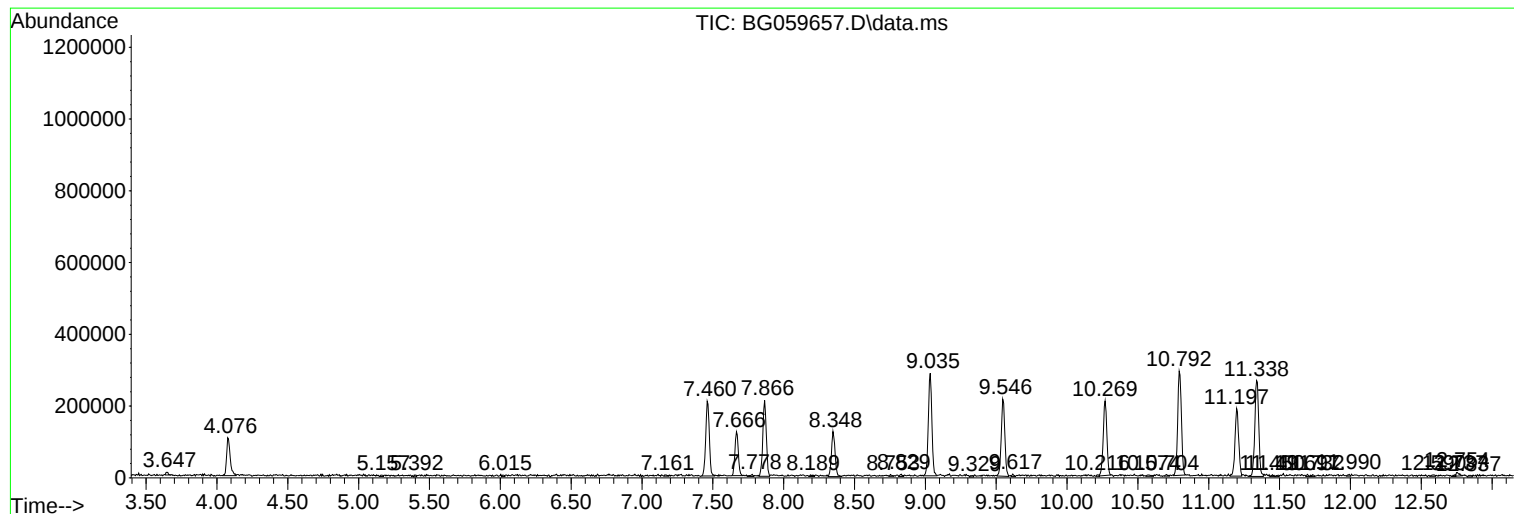

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059657.D
Acq On : 5 Nov 2023 16:22
Operator : MA/JU
Sample : PB156653BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK653

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059657.D
Acq On : 5 Nov 2023 16:22
Operator : MA/JU
Sample : PB156653BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK653

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc