

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059665.D
 Acq On : 5 Nov 2023 21:46
 Operator : MA/JU
 Sample : 05013-09
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.471	13	14	18	rBV2	5494	4748	0.51%	0.066%
2	3.735	57	59	61	rVB2	8613	5023	0.54%	0.070%
3	3.758	61	63	65	rBV	5956	3844	0.41%	0.054%
4	4.076	114	117	127	rBV3	33014	62944	6.79%	0.877%
5	4.346	161	163	168	rVB4	6177	4897	0.53%	0.068%
6	4.640	211	213	214	rBV4	5698	3762	0.41%	0.052%
7	4.693	220	222	225	rBV2	6059	5083	0.55%	0.071%
8	4.845	247	248	250	rBV	5858	3663	0.40%	0.051%
9	5.263	318	319	321	rBV	7366	4788	0.52%	0.067%
10	5.362	334	336	338	rBV	6094	7553	0.81%	0.105%
11	5.439	347	349	352	rBV2	8794	6746	0.73%	0.094%
12	5.850	417	419	423	rVB2	8650	8933	0.96%	0.124%
13	5.891	423	426	430	rBV2	7693	11790	1.27%	0.164%
14	6.020	445	448	450	rBV	7529	9006	0.97%	0.126%
15	6.179	474	475	477	rVB	9417	6029	0.65%	0.084%
16	6.308	495	497	498	rBV	8145	5538	0.60%	0.077%
17	6.426	515	517	520	rBV	6947	8571	0.92%	0.119%
18	6.455	520	522	523	rVB	8549	4150	0.45%	0.058%
19	6.925	601	602	605	rBV	7341	6852	0.74%	0.095%
20	7.102	630	632	633	rBV	4970	3799	0.41%	0.053%
21	7.319	667	669	670	rBV	8672	5905	0.64%	0.082%
22	7.460	690	693	696	rBV2	22099	26981	2.91%	0.376%
23	7.666	723	728	736	rVB	78167	127591	13.76%	1.778%
24	7.865	756	762	768	rBV	95927	166519	17.96%	2.321%
25	7.965	777	779	780	rBV	8776	5926	0.64%	0.083%
26	8.347	837	844	852	rVB2	136398	237523	25.61%	3.310%
27	8.547	876	878	879	rBV2	6090	4907	0.53%	0.068%
28	8.588	884	885	886	rVV2	8741	4024	0.43%	0.056%
29	8.606	886	888	892	rVB2	8140	7273	0.78%	0.101%
30	8.817	922	924	926	rBV	5052	3663	0.40%	0.051%
31	9.035	956	961	968	rVB2	76891	140092	15.11%	1.952%
32	9.187	983	987	988	rVB	5151	4415	0.48%	0.062%
33	9.416	1025	1026	1027	rBV	6816	3639	0.39%	0.051%
34	9.487	1037	1038	1039	rBV	7046	4475	0.48%	0.062%
35	9.546	1042	1048	1055	rVB2	130462	245617	26.49%	3.423%
36	9.910	1108	1110	1111	rBV2	6432	3958	0.43%	0.055%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059665.D
 Acq On : 5 Nov 2023 21:46
 Operator : MA/JU
 Sample : 05013-09
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

37	9.928	1111	1113	1116	rVB	6796	5728	0.62%	0.080%
38	9.951	1116	1117	1120	rVB	6504	4690	0.51%	0.065%
39	9.986	1120	1123	1124	rBV	4924	5569	0.60%	0.078%
40	10.133	1146	1148	1150	rBV	5835	5082	0.55%	0.071%
41	10.157	1150	1152	1155	rVV	5269	6489	0.70%	0.090%
42	10.186	1155	1157	1158	rVB	6614	3853	0.42%	0.054%
43	10.216	1160	1162	1163	rVV	6232	3743	0.40%	0.052%
44	10.268	1165	1171	1180	rVB2	102312	198549	21.41%	2.767%
45	10.550	1217	1219	1221	rVB2	7079	4996	0.54%	0.070%
46	10.727	1247	1249	1252	rBV	5135	5304	0.57%	0.074%
47	10.797	1254	1261	1268	rVB4	160863	314755	33.94%	4.386%
48	11.197	1323	1329	1337	rBV	135588	239130	25.79%	3.332%
49	11.338	1347	1353	1361	rVB3	162629	306836	33.09%	4.276%
50	11.538	1385	1387	1390	rVB	3937	4149	0.45%	0.058%
51	11.673	1405	1410	1412	rBV	4589	5865	0.63%	0.082%
52	11.872	1442	1444	1448	rVB	4331	4598	0.50%	0.064%
53	12.013	1466	1468	1472	rBV	4245	3862	0.42%	0.054%
54	12.154	1489	1492	1496	rBV	4676	6862	0.74%	0.096%
55	12.266	1508	1511	1513	rBV	6161	5912	0.64%	0.082%
56	12.360	1524	1527	1531	rBV	2949	3752	0.40%	0.052%
57	12.577	1562	1564	1567	rVB	5155	4637	0.50%	0.065%
58	12.601	1567	1568	1570	rBV	4513	3655	0.39%	0.051%
59	12.660	1576	1578	1581	rBV	3736	4526	0.49%	0.063%
60	12.801	1599	1602	1604	rVB	3853	3824	0.41%	0.053%
61	12.860	1606	1612	1613	rBV	3092	5872	0.63%	0.082%
62	12.983	1631	1633	1634	rBV	3988	3926	0.42%	0.055%
63	13.065	1645	1647	1651	rBV	4034	5786	0.62%	0.081%
64	13.142	1659	1660	1663	rBV	4681	3649	0.39%	0.051%
65	13.218	1671	1673	1675	rVB	5763	4312	0.47%	0.060%
66	13.277	1680	1683	1685	rVV	4378	3889	0.42%	0.054%
67	13.459	1713	1714	1717	rBV	4014	4183	0.45%	0.058%
68	13.570	1729	1733	1736	rVB	5447	6496	0.70%	0.091%
69	13.606	1736	1739	1740	rBV	3861	4140	0.45%	0.058%
70	13.805	1768	1773	1778	rVV4	19789	29566	3.19%	0.412%
71	13.888	1785	1787	1790	rBV	5809	5299	0.57%	0.074%
72	14.246	1846	1848	1851	rVB	3680	3771	0.41%	0.053%
73	14.311	1854	1859	1860	rBV	4012	6015	0.65%	0.084%
74	14.370	1863	1869	1878	rVB	320439	457289	49.31%	6.372%
75	14.552	1897	1900	1901	rBV	6275	6187	0.67%	0.086%
76	14.628	1910	1913	1915	rVB	3592	4154	0.45%	0.058%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059665.D
 Acq On : 5 Nov 2023 21:46
 Operator : MA/JU
 Sample : 05013-09
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A49A5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

77	14.681	1915	1922	1929	rBV	303795	466847	50.35%	6.506%
78	14.975	1966	1972	1979	rBV2	229690	364767	39.34%	5.083%
79	15.151	1996	2002	2009	rVB5	19504	45022	4.86%	0.627%
80	15.198	2009	2010	2012	rBV	4708	4251	0.46%	0.059%
81	15.216	2012	2013	2018	rVB	6988	6543	0.71%	0.091%
82	15.404	2042	2045	2046	rBV	5561	5704	0.62%	0.079%
83	15.456	2050	2054	2056	rVV	3857	3606	0.39%	0.050%
84	15.968	2135	2141	2147	rVB	379631	575493	62.06%	8.020%
85	16.062	2153	2157	2164	rVB3	67561	102090	11.01%	1.423%
86	16.203	2179	2181	2182	rVB	7926	3822	0.41%	0.053%
87	16.320	2198	2201	2204	rBV	2614	3663	0.40%	0.051%
88	16.344	2204	2205	2209	rVB	4655	5165	0.56%	0.072%
89	16.461	2222	2225	2228	rBV	4834	6530	0.70%	0.091%
90	16.620	2250	2252	2254	rVB	6567	4244	0.46%	0.059%
91	16.825	2284	2287	2290	rBV	3324	4698	0.51%	0.065%
92	16.884	2294	2297	2300	rBV	3884	5864	0.63%	0.082%
93	17.178	2345	2347	2349	rBV	5182	5404	0.58%	0.075%
94	17.395	2380	2384	2387	rBV2	5213	8681	0.94%	0.121%
95	17.730	2435	2441	2448	rBV	299464	455301	49.10%	6.345%
96	17.830	2451	2458	2464	rBV2	407780	662264	71.42%	9.229%
97	18.018	2488	2490	2494	rBV	3544	3954	0.43%	0.055%
98	19.487	2737	2740	2744	rVB4	28109	36946	3.98%	0.515%
99	20.098	2839	2844	2851	rVB2	648337	927290	100.00%	12.922%
100	22.060	3173	3178	3185	rVB2	340087	586715	63.27%	8.176%




Sum of corrected areas: 7175991

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059665.D
Acq On : 5 Nov 2023 21:46
Operator : MA/JU
Sample : 05013-09
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A49A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

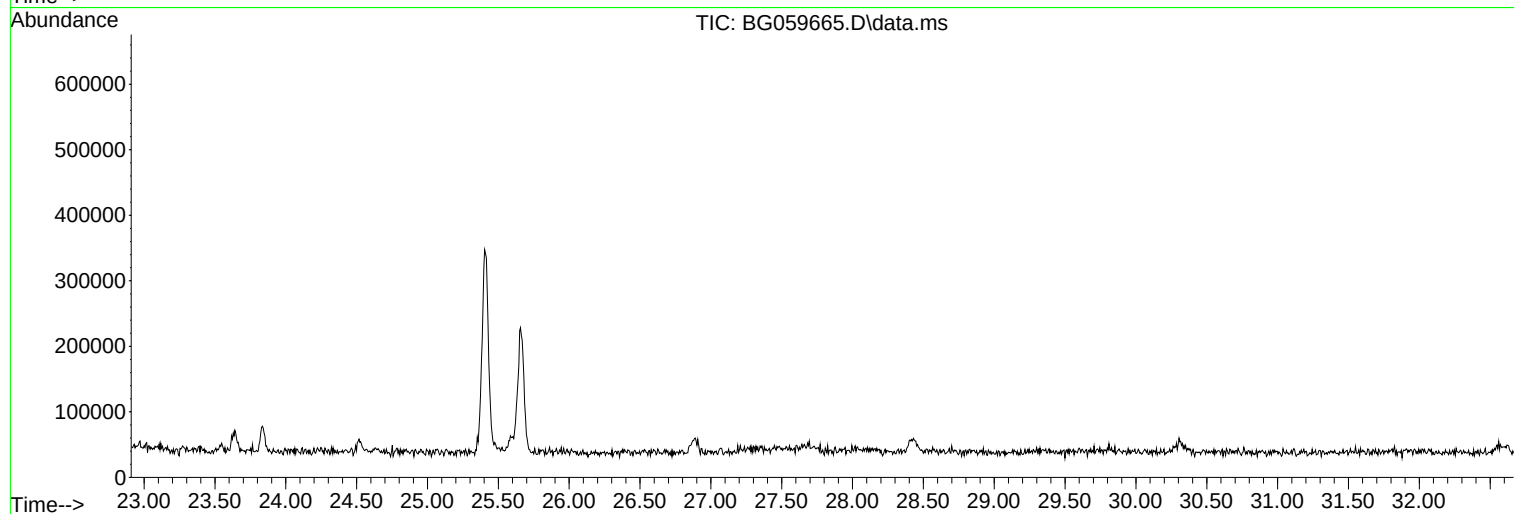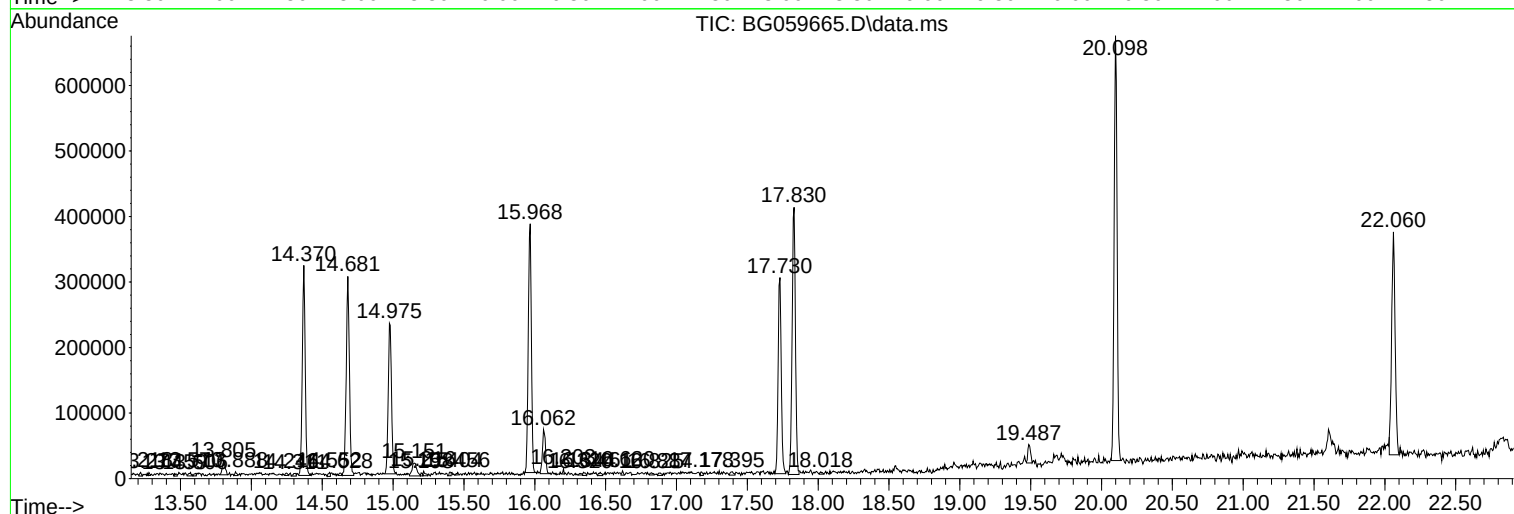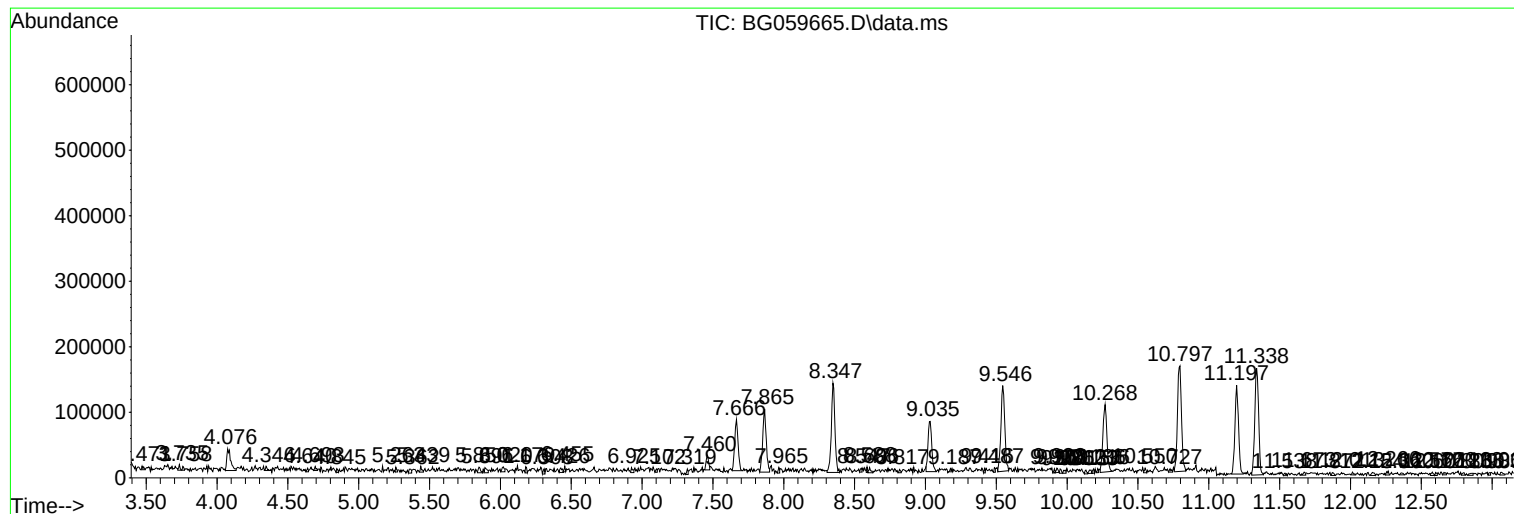

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059665.D
Acq On : 5 Nov 2023 21:46
Operator : MA/JU
Sample : 05013-09
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A49A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059665.D
Acq On : 5 Nov 2023 21:46
Operator : MA/JU
Sample : 05013-09
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A49A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc