

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059670.D
 Acq On : 6 Nov 2023 1:50
 Operator : MA/JU
 Sample : PB156606BL
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK606

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.646	40	44	49	rBV5	11605	14108	0.98%	0.109%
2	3.875	82	83	86	rBV2	6588	4073	0.28%	0.031%
3	4.080	113	118	125	rBV	87845	146741	10.17%	1.133%
4	4.362	163	166	167	rBV2	4742	4106	0.28%	0.032%
5	4.791	237	239	241	rBV2	4228	3821	0.26%	0.029%
6	4.956	265	267	269	rBV	7429	4042	0.28%	0.031%
7	4.997	272	274	277	rVB	4526	5804	0.40%	0.045%
8	5.044	277	282	283	rBV	4955	7567	0.52%	0.058%
9	5.103	289	292	293	rVB	4663	4070	0.28%	0.031%
10	5.120	293	295	296	rBV	4972	4345	0.30%	0.034%
11	5.238	311	315	317	rBV	4515	6489	0.45%	0.050%
12	5.849	417	419	420	rBV	5289	4017	0.28%	0.031%
13	6.348	501	504	506	rBV	4422	5151	0.36%	0.040%
14	6.513	530	532	535	rBV	4545	4525	0.31%	0.035%
15	6.624	550	551	554	rVB	5537	4367	0.30%	0.034%
16	6.701	560	564	567	rBV2	4463	7263	0.50%	0.056%
17	6.765	572	575	577	rBV2	3737	3858	0.27%	0.030%
18	6.795	577	580	582	rVB	4561	4458	0.31%	0.034%
19	6.812	582	583	586	rBV	4180	3605	0.25%	0.028%
20	7.153	637	641	644	rBV2	3424	6291	0.44%	0.049%
21	7.218	650	652	654	rVB2	4679	4313	0.30%	0.033%
22	7.459	687	693	701	rVB	172045	303791	21.06%	2.345%
23	7.564	707	711	712	rVB	4684	4892	0.34%	0.038%
24	7.664	722	728	737	rBV	102439	180563	12.52%	1.394%
25	7.864	755	762	770	rVB2	168650	306714	21.26%	2.367%
26	8.346	839	844	851	rBV2	115670	206496	14.31%	1.594%
27	8.440	857	860	861	rBV2	5873	5666	0.39%	0.044%
28	8.957	946	948	951	rBV2	3075	4192	0.29%	0.032%
29	9.033	954	961	969	rVV3	242715	424240	29.41%	3.274%
30	9.327	1008	1011	1013	rBV3	4208	5252	0.36%	0.041%
31	9.415	1024	1026	1029	rVB	3646	3834	0.27%	0.030%
32	9.544	1041	1048	1057	rBV	167176	313084	21.70%	2.416%
33	9.650	1065	1066	1069	rBV	3712	3600	0.25%	0.028%
34	9.844	1095	1099	1100	rBV	5717	4371	0.30%	0.034%
35	9.938	1113	1115	1118	rBV	3763	4115	0.29%	0.032%
36	10.267	1163	1171	1179	rBV2	182589	320654	22.23%	2.475%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059670.D
 Acq On : 6 Nov 2023 1:50
 Operator : MA/JU
 Sample : PB156606BL
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK606

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

37	10.396	1191	1193	1195	rBV2	3791	3863	0.27%	0.030%
38	10.555	1216	1220	1221	rBV2	6396	6429	0.45%	0.050%
39	10.790	1253	1260	1268	rBV2	244030	450590	31.23%	3.478%
40	11.096	1310	1312	1315	rBV	4196	3860	0.27%	0.030%
41	11.196	1323	1329	1338	rBV	174286	313471	21.73%	2.419%
42	11.290	1342	1345	1346	rBV	3245	3613	0.25%	0.028%
43	11.337	1346	1353	1361	rBV2	221609	417792	28.96%	3.224%
44	11.554	1386	1390	1391	rBV2	2978	3609	0.25%	0.028%
45	11.671	1407	1410	1411	rBV2	4511	3661	0.25%	0.028%
46	11.889	1446	1447	1449	rBV2	6221	3893	0.27%	0.030%
47	12.059	1471	1476	1477	rBV	4729	5790	0.40%	0.045%
48	12.570	1562	1563	1567	rBV	3621	3909	0.27%	0.030%
49	12.741	1590	1592	1594	rBV	5285	5960	0.41%	0.046%
50	13.087	1648	1651	1653	rBV	4548	6352	0.44%	0.049%
51	13.270	1679	1682	1684	rBV	3920	3605	0.25%	0.028%
52	13.563	1730	1732	1735	rBV	3009	3614	0.25%	0.028%
53	13.657	1745	1748	1752	rVB	3028	4855	0.34%	0.037%
54	14.022	1808	1810	1811	rBV	5353	4266	0.30%	0.033%
55	14.333	1859	1863	1864	rBV	3612	3810	0.26%	0.029%
56	14.368	1864	1869	1876	rVB	544465	764551	52.99%	5.901%
57	14.456	1882	1884	1885	rBV	4856	3606	0.25%	0.028%
58	14.574	1903	1904	1909	rBV	4068	3905	0.27%	0.030%
59	14.680	1915	1922	1931	rBV	540557	845273	58.59%	6.524%
60	14.903	1957	1960	1963	rBV	4260	4691	0.33%	0.036%
61	14.973	1967	1972	1981	rVB	298498	481071	33.35%	3.713%
62	15.150	1995	2002	2011	rBV2	271788	443978	30.77%	3.427%
63	15.473	2055	2057	2059	rVB2	5229	4424	0.31%	0.034%
64	15.508	2059	2063	2066	rVB	5195	7775	0.54%	0.060%
65	15.555	2066	2071	2073	rBV	3950	5352	0.37%	0.041%
66	15.608	2078	2080	2085	rBV2	4518	8357	0.58%	0.064%
67	15.702	2094	2096	2098	rVB	4830	3669	0.25%	0.028%
68	15.966	2133	2141	2147	rBV	681903	1022295	70.86%	7.890%
69	16.066	2152	2158	2166	rVB	232884	356559	24.71%	2.752%
70	16.119	2166	2167	2170	rBV2	4821	4190	0.29%	0.032%
71	16.871	2293	2295	2298	rVB2	5835	5891	0.41%	0.045%
72	16.965	2308	2311	2312	rBV2	4312	4253	0.29%	0.033%
73	17.188	2346	2349	2352	rVB	5831	7407	0.51%	0.057%
74	17.224	2352	2355	2357	rBV	6280	6394	0.44%	0.049%
75	17.271	2361	2363	2366	rBV	3135	3695	0.26%	0.029%
76	17.365	2377	2379	2381	rBV	2852	3722	0.26%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
 Data File : BG059670.D
 Acq On : 6 Nov 2023 1:50
 Operator : MA/JU
 Sample : PB156606BL
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK606

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
 Title : SVOA CALIBRATION

77	17.688	2431	2434	2435	rBV	5062	5288	0.37%	0.041%
78	17.729	2435	2441	2448	rVV	394613	608696	42.19%	4.698%
79	17.829	2451	2458	2465	rVB2	731881	1127185	78.13%	8.699%
80	17.970	2479	2482	2484	rBV2	6187	5208	0.36%	0.040%
81	18.040	2492	2494	2495	rBV	5368	3686	0.26%	0.028%
82	18.228	2524	2526	2530	rVB	4233	4748	0.33%	0.037%
83	18.275	2532	2534	2537	rVB	5247	4075	0.28%	0.031%
84	18.305	2537	2539	2541	rBV2	5815	4853	0.34%	0.037%
85	18.651	2596	2598	2601	rVB2	5949	4449	0.31%	0.034%
86	18.675	2601	2602	2604	rBV2	5465	4449	0.31%	0.034%
87	19.098	2672	2674	2676	rBV	6647	5308	0.37%	0.041%
88	19.157	2683	2684	2686	rBV	4591	3699	0.26%	0.029%
89	19.339	2713	2715	2718	rBV2	6517	6620	0.46%	0.051%
90	19.721	2779	2780	2781	rBV	10520	5555	0.39%	0.043%
91	20.097	2838	2844	2853	rVB	918202	1363942	94.54%	10.527%
92	20.255	2869	2871	2872	rBV	13695	8423	0.58%	0.065%
93	22.059	3172	3178	3185	rVB2	434445	759762	52.66%	5.864%
94	25.408	3740	3748	3760	rVB2	482645	1442708	100.00%	11.134%




Sum of corrected areas: 12957132

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059670.D
Acq On : 6 Nov 2023 1:50
Operator : MA/JU
Sample : PB156606BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK606

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

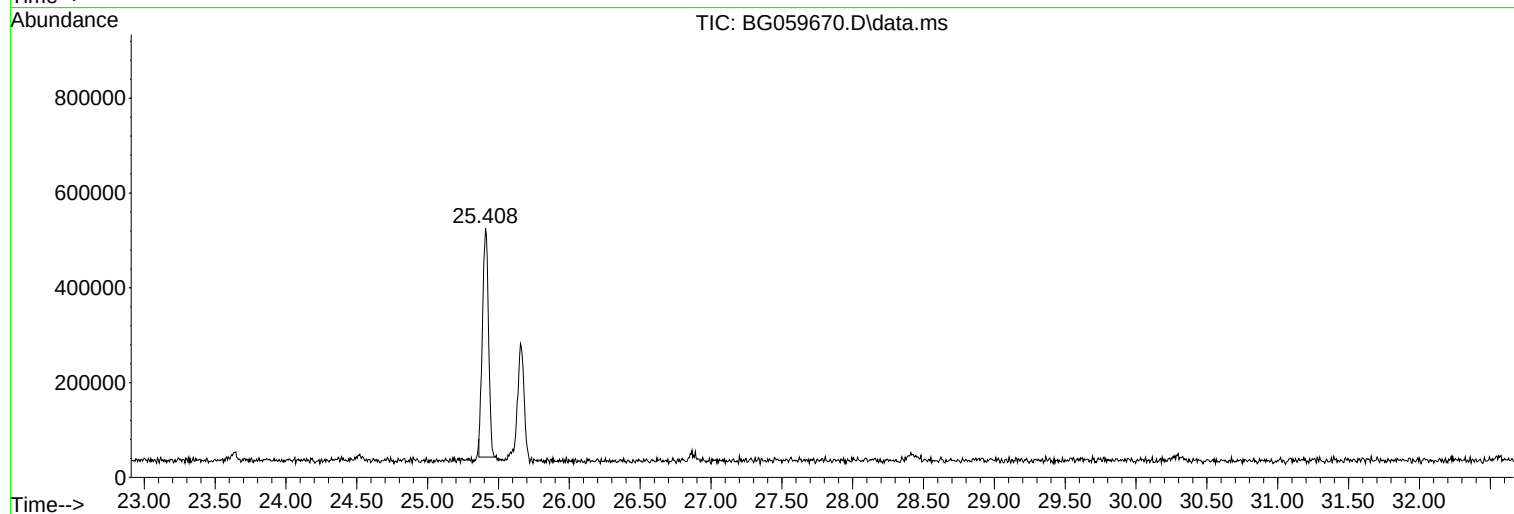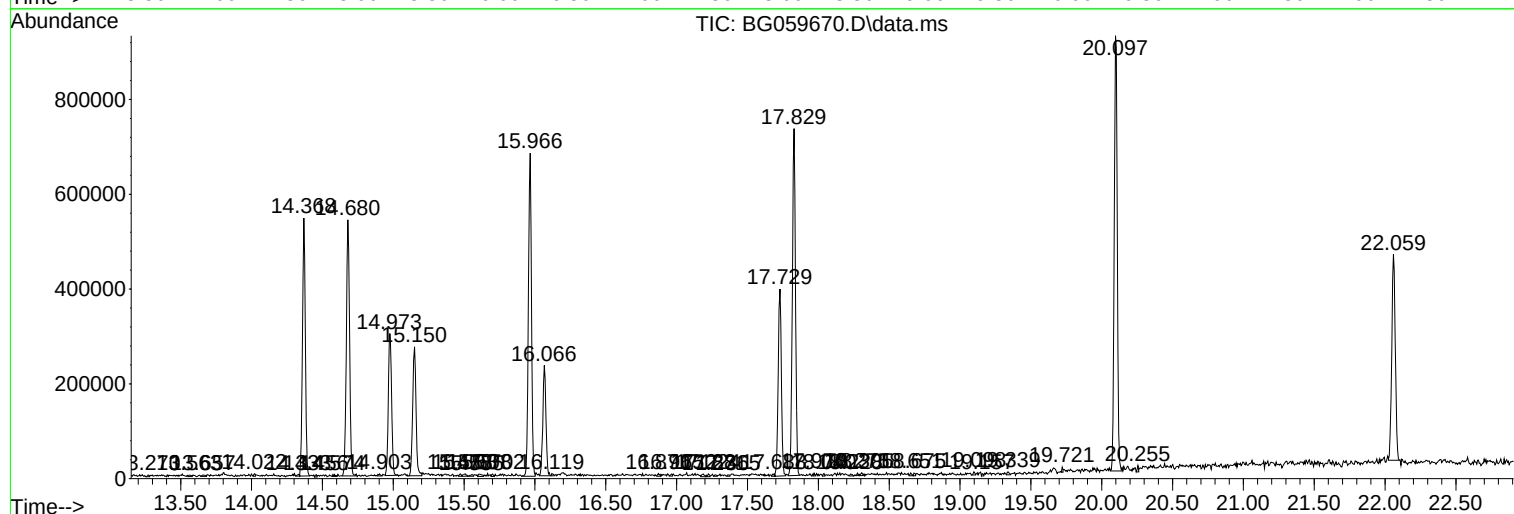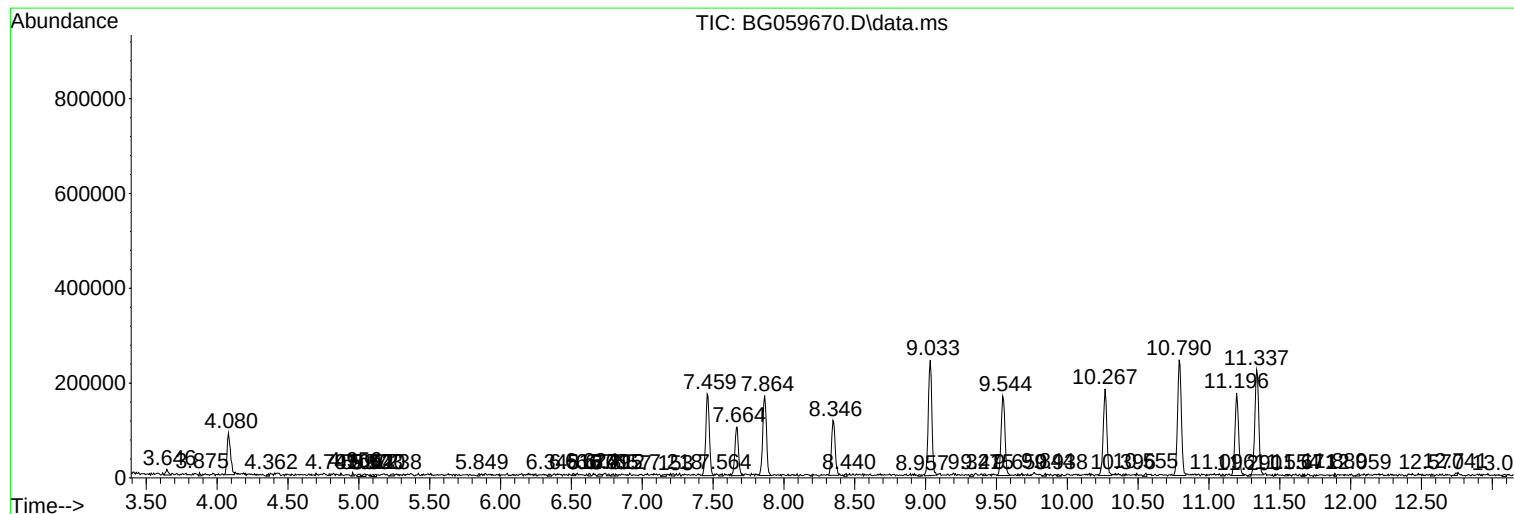

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059670.D
Acq On : 6 Nov 2023 1:50
Operator : MA/JU
Sample : PB156606BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK606

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110423\
Data File : BG059670.D
Acq On : 6 Nov 2023 1:50
Operator : MA/JU
Sample : PB156606BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK606

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc