
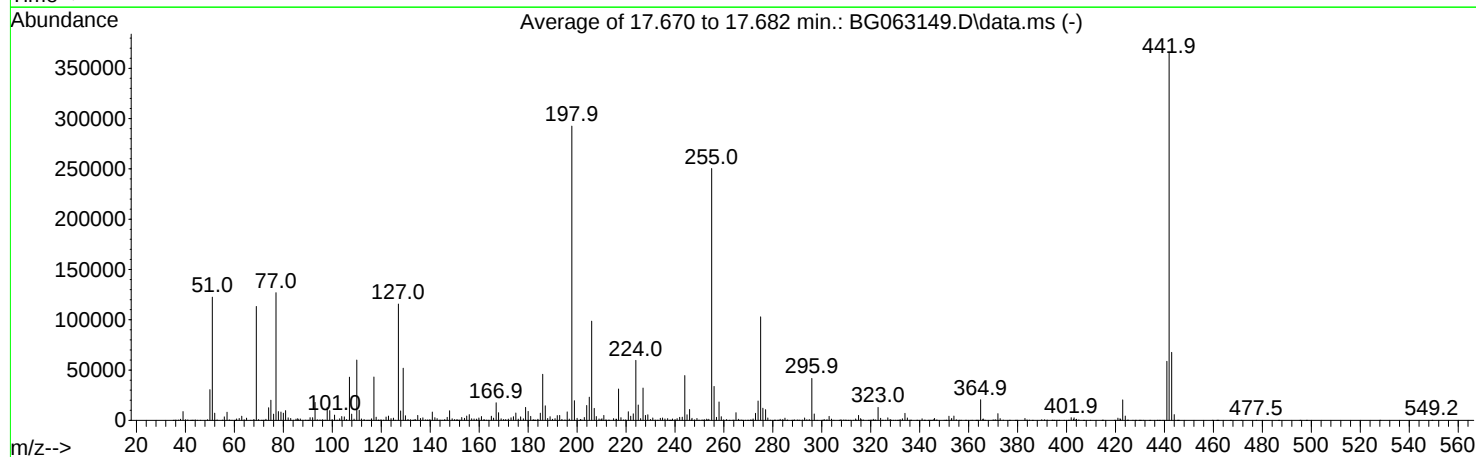


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110424\
Data File : BG063149.D
Acq On : 4 Nov 2024 10:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG103124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 01 05:13:40 2024

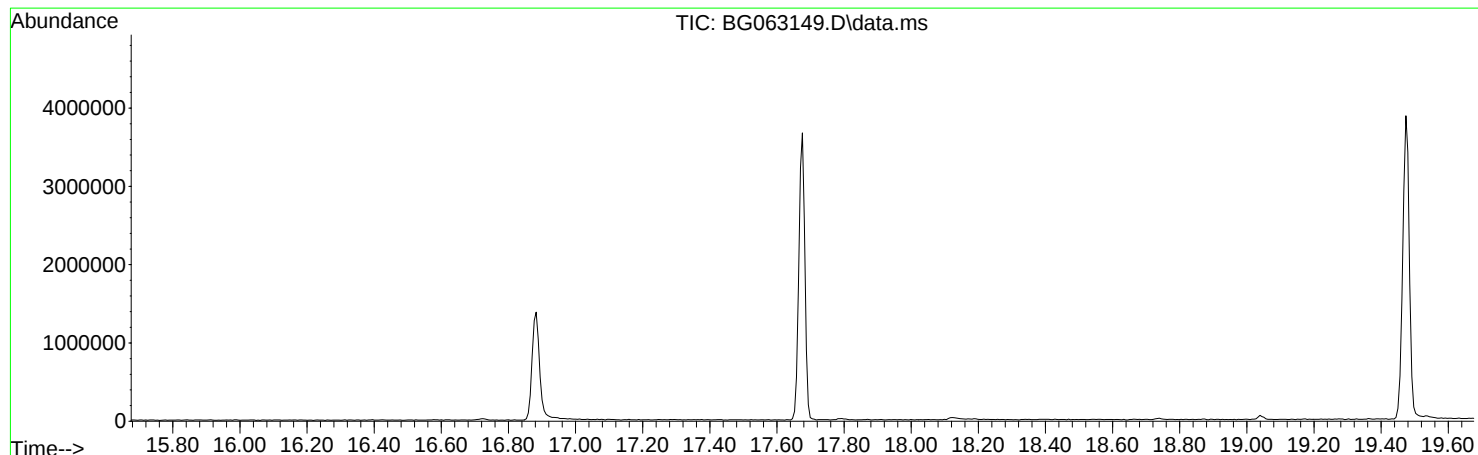




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	122520	PASS
68	69	0.00	2	0.8	955	PASS
69	198	0.00	100	38.7	113288	PASS
70	69	0.00	2	0.7	748	PASS
127	198	10	80	39.5	115653	PASS
197	198	0.00	2	0.5	1328	PASS
198	198	100	100	100.0	292523	PASS
199	198	5	9	6.7	19539	PASS
275	198	10	60	35.2	102880	PASS
365	198	1	100	7.0	20571	PASS
441	198	0.01	100	20.1	58739	PASS
442	442	50	100	100.0	365696	PASS
443	442	15	24	18.5	67683	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110424\
Data File : BG063149.D
Acq On : 4 Nov 2024 10:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 04 11:13:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 01 05:13:40 2024
Response via : Initial Calibration

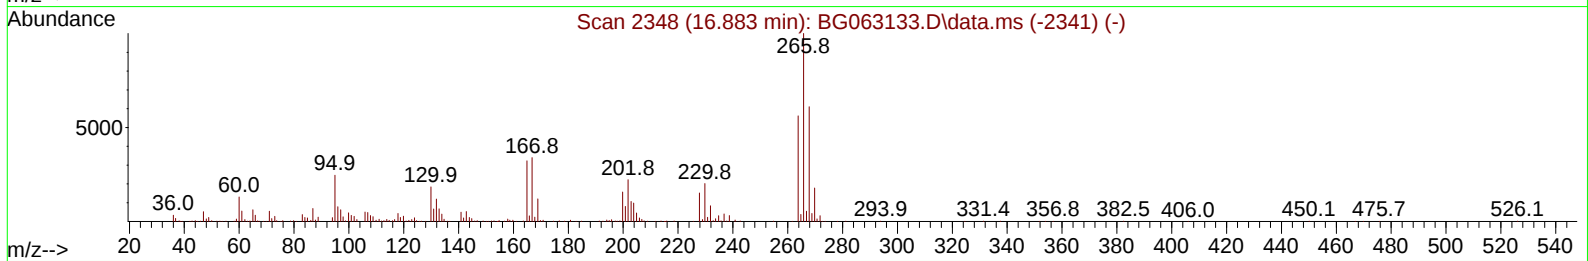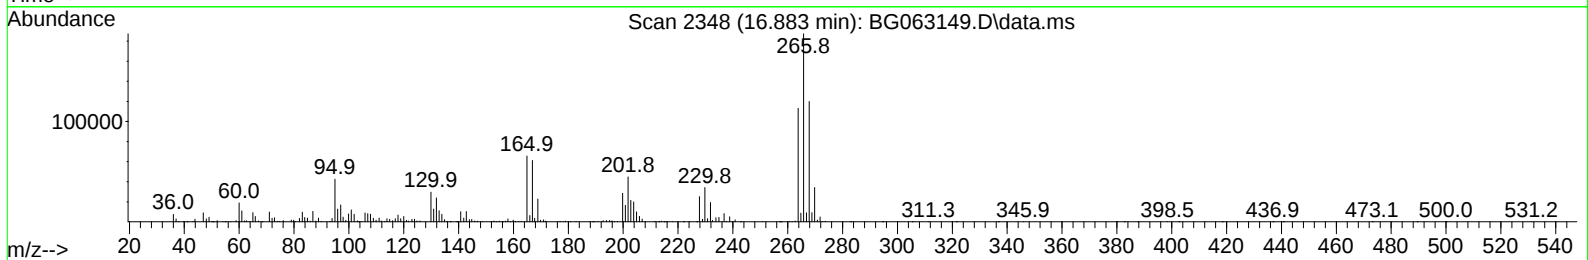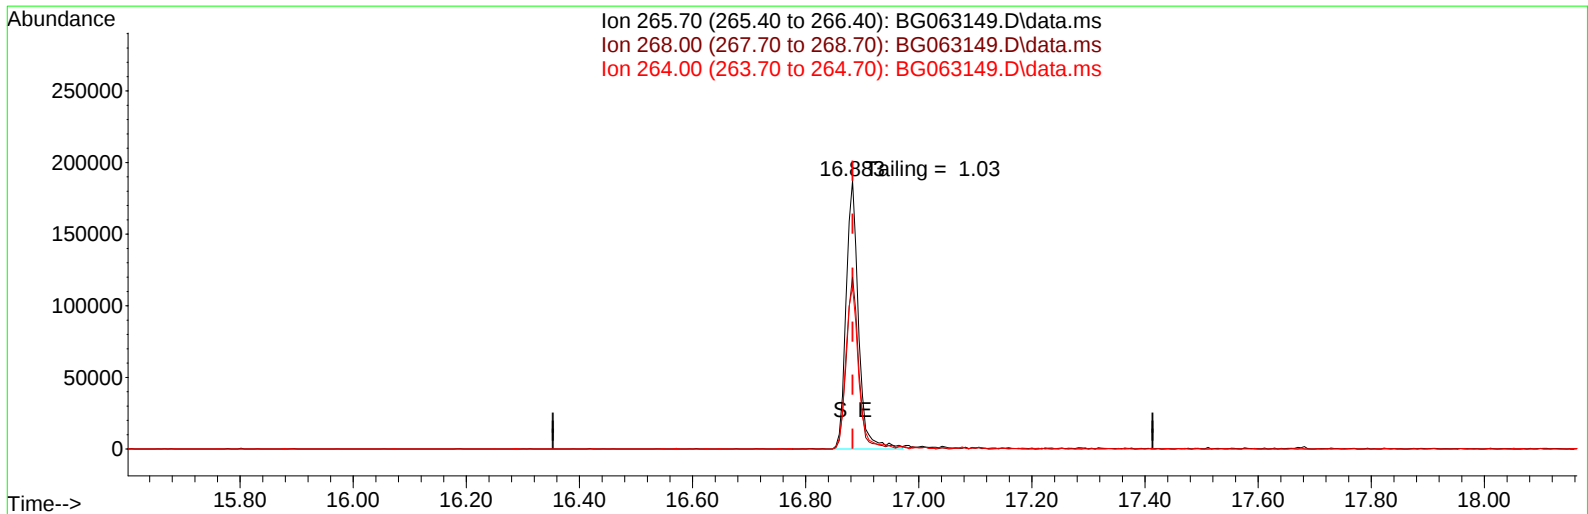

TIC: BG063149.D\data.ms

(70) Pentachlorophenol (C)

16.883min (-0.001) 275557.26 ng




response 286127

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.04
264.00	56.20	60.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110424\
Data File : BG063149.D
Acq On : 4 Nov 2024 10:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 04 11:13:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 01 05:13:40 2024
Response via : Initial Calibration

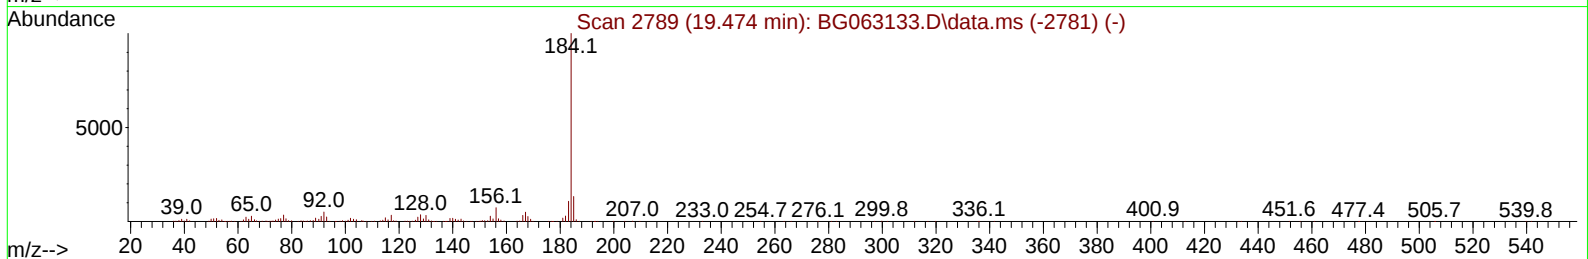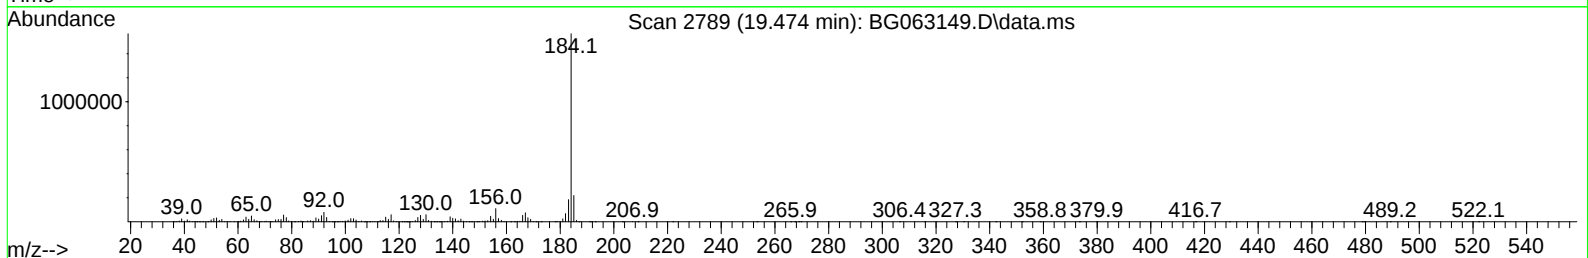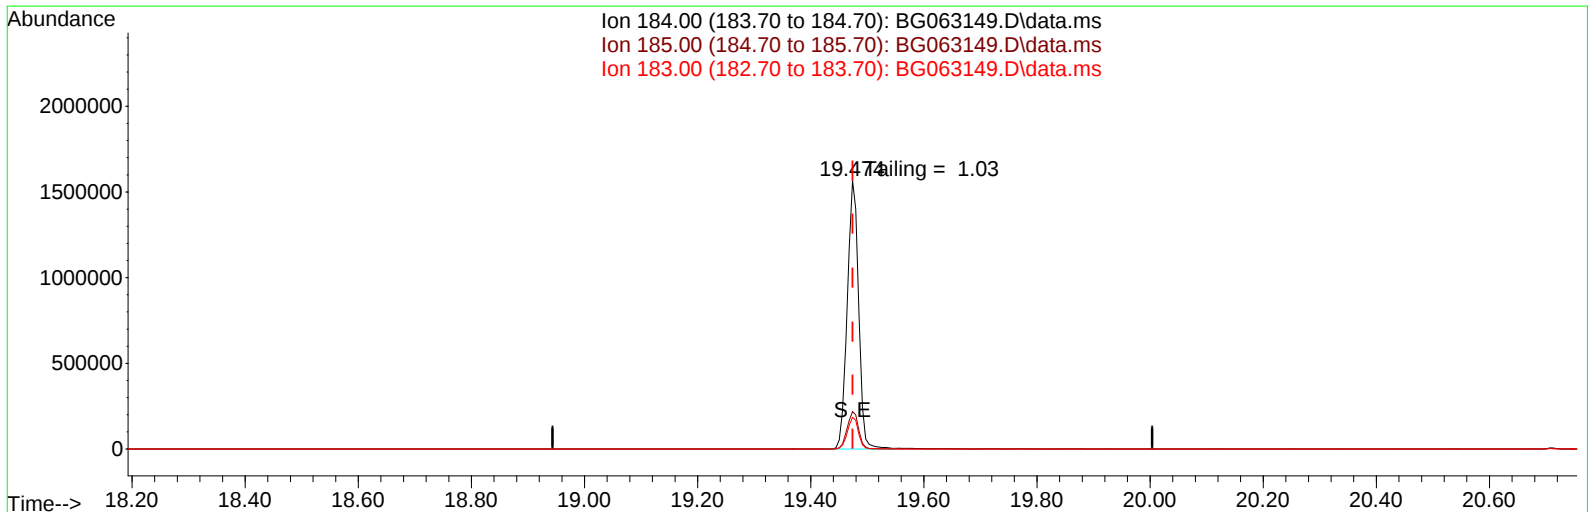

TIC: BG063149.D\data.ms

(77) Benzidine

19.474min (-0.000) 941478.64 ng

response 2190382

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	13.98
183.00	10.70	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/4/2024	BNA_G	<u>BG063149.D</u>
Compound Name	Response	Retention Time
DDT	1165080	20.713
DDD	23900	20.273
DDE	1178	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25078	1190158	2.11

Instrument :
BNA_G
ClientSampleId :
DFTPP