

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110515\
 Data File : BG019486.D
 Acq On : 5 Nov 2015 10:59
 Operator : UM/NP
 Sample : PB86442BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK42

Quant Time: Nov 06 02:13:28 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 06 02:11:58 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	29054	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	125159	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	105191	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	298545	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	390807	20.00	ng/ul	0.00
86) Perylene-d12	25.18	264	372245	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	4223	6.96	ng/uL	0.00
5) Phenol-d5	7.33	99	90125	33.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	66090	39.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	59592	35.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	74027	34.85	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	30747	33.43	ng/ul	0.00
22) 2-Nitrophenol-d4	10.08	143	36537	33.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	77316	32.64	ng/ul	0.00
29) 4-Chloroaniline-d4	11.13	131	91046	37.99	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	298571	34.43	ng/ul	0.00
47) Acenaphthylene-d8	14.51	160	322792	33.61	ng/ul	0.00
52) 4-Nitrophenol-d4	14.99	143	46223	33.55	ng/ul	0.00
58) Fluorene-d10	15.79	176	266200	33.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.91	200	58690	30.37	ng/ul	0.00
71) Anthracene-d10	17.64	188	474719	34.88	ng/ul	0.00
79) Pyrene-d10	19.92	212	572269	33.46	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.94	264	648929	34.74	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.88	70	2389	1.02 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110515\
Data File : BG019486.D
Acq On : 5 Nov 2015 10:59
Operator : UM/NP
Sample : PB86442BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK42

Quant Time: Nov 06 02:13:28 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 06 02:11:58 2015
Response via : Initial Calibration

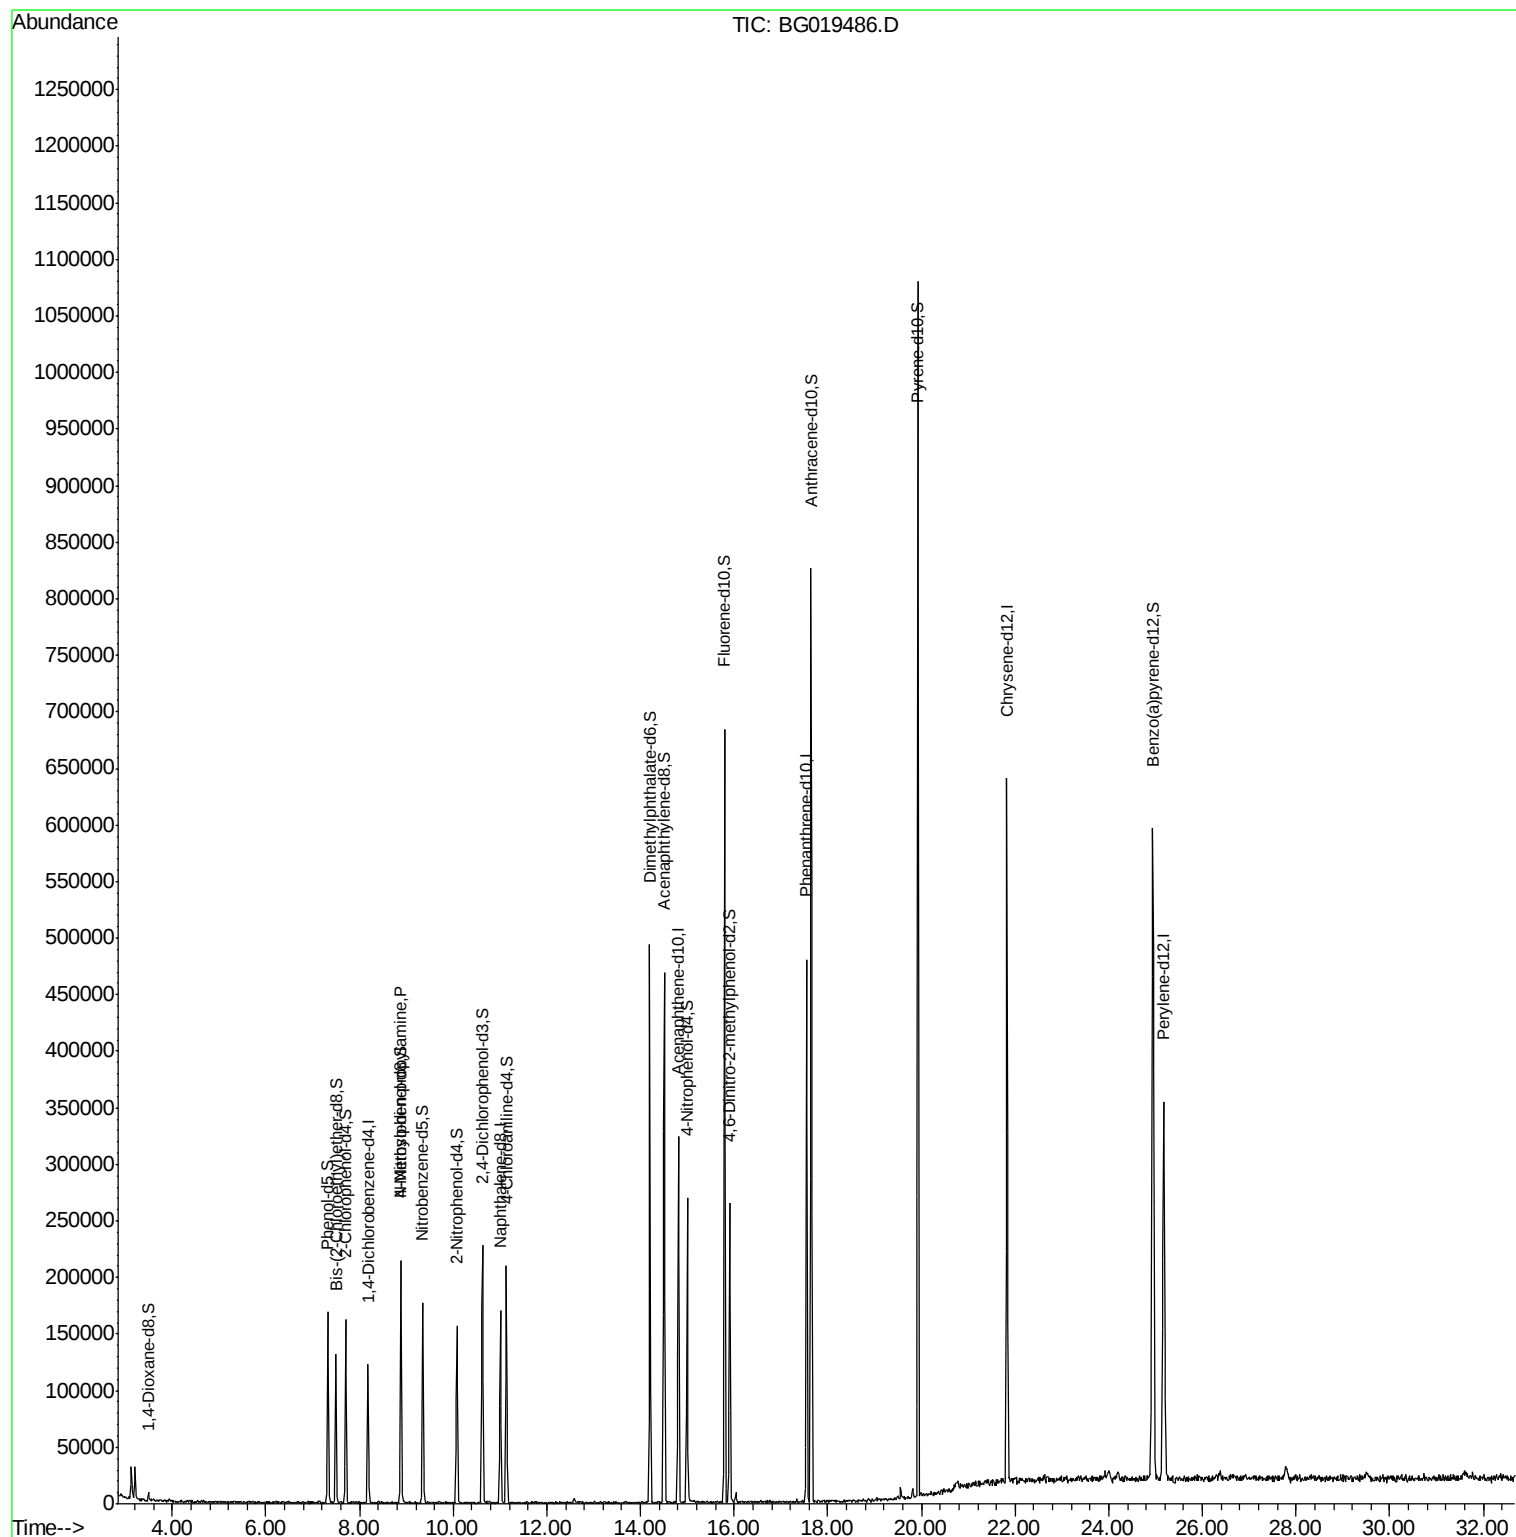

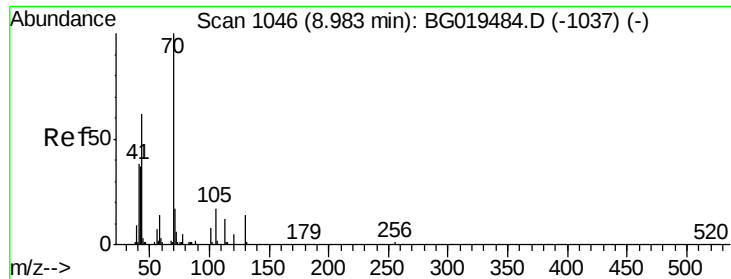

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.02 ng/ul
 RT: 8.88 min Scan# 1029
 Delta R.T. -0.10 min
 Lab File: BG019486.D
 Acq: 5 Nov 2015 10:59

Instrument :
 BNA_G
 ClientSampleId :
 SBLK42

Tgt Ion: 70 Resp: 2389
 Ion Ratio Lower Upper
 70 100
 42 247.1 36.6 55.0#
 101 0.0 5.8 8.8#
 130 0.0 14.6 22.0#

