

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110515\
 Data File : BG019490.D
 Acq On : 5 Nov 2015 13:32
 Operator : UM/NP
 Sample : G4273-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AN9

Manual Integrations
 APPROVED

Mmdadoda
 11/6/2015 3:43:16 PM

Quant Time: Nov 06 05:47:47 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 06 02:11:58 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	36549	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	155470	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	124468	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	353761	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	475007	20.00	ng/ul	0.00
86) Perylene-d12	25.17	264	452543	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	3489	4.57	ng/uL	0.00
5) Phenol-d5	7.32	99	83299	24.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	62100	29.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	52352	25.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	72069	26.97	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	30371	26.58	ng/ul	0.00
22) 2-Nitrophenol-d4	10.08	143	33550	24.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	72516	24.64	ng/ul	0.00
29) 4-Chloroaniline-d4	11.14	131	83444	28.03	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	284467	27.72	ng/ul	0.00
47) Acenaphthylene-d8	14.50	160	312964	27.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.99	143	46963	28.81	ng/ul	0.00
58) Fluorene-d10	15.80	176	256790	27.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.91	200	55193	24.10	ng/ul	0.00
71) Anthracene-d10	17.65	188	457170	28.35	ng/ul	0.00
79) Pyrene-d10	19.92	212	572446	27.54	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.94	264	656769	28.92	ng/ul	0.00

Target Compounds

						Ovalue
45) Dimethylphthalate	14.25	163	143875	13.71	ng/ul	96
50) Acenaphthene	14.87	153	27285	3.47	ng/ul	89
54) Dibenzofuran	15.20	168	13710	1.18	ng/ul	88
59) Fluorene	15.85	166	32241	3.19	ng/ul	98
70) Phenanthrene	17.59	178	81803	4.58	ng/ul	97
72) Anthracene	17.68	178	65124	3.58	ng/ul	96
77) Fluoranthene	19.59	202	202231	8.75	ng/ul	98
80) Pyrene	19.95	202	140185	5.26	ng/ul#	88
83) Benzo(a)anthracene	21.81	228	79158	2.86	ng/ul	98
84) Bis(2-ethylhexyl)phthalate	21.69	149	22859	1.86	ng/ul	93
85) Chrysene	21.88	228	82075	3.16	ng/ul	94
88) Benzo(b)fluoranthene	24.10	252	59328	2.22	ng/ul#	99
91) Benzo(a)pyrene	25.02	252	47590m	1.86	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG110515\
Data File : BG019490.D
Acq On : 5 Nov 2015 13:32
Operator : UM/NP
Sample : G4273-04
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C0AN9

Manual Integrations
APPROVED

Mmdadoda
11/6/2015 3:43:16 PM

Quant Time: Nov 06 05:47:47 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 06 02:11:58 2015
Response via : Initial Calibration

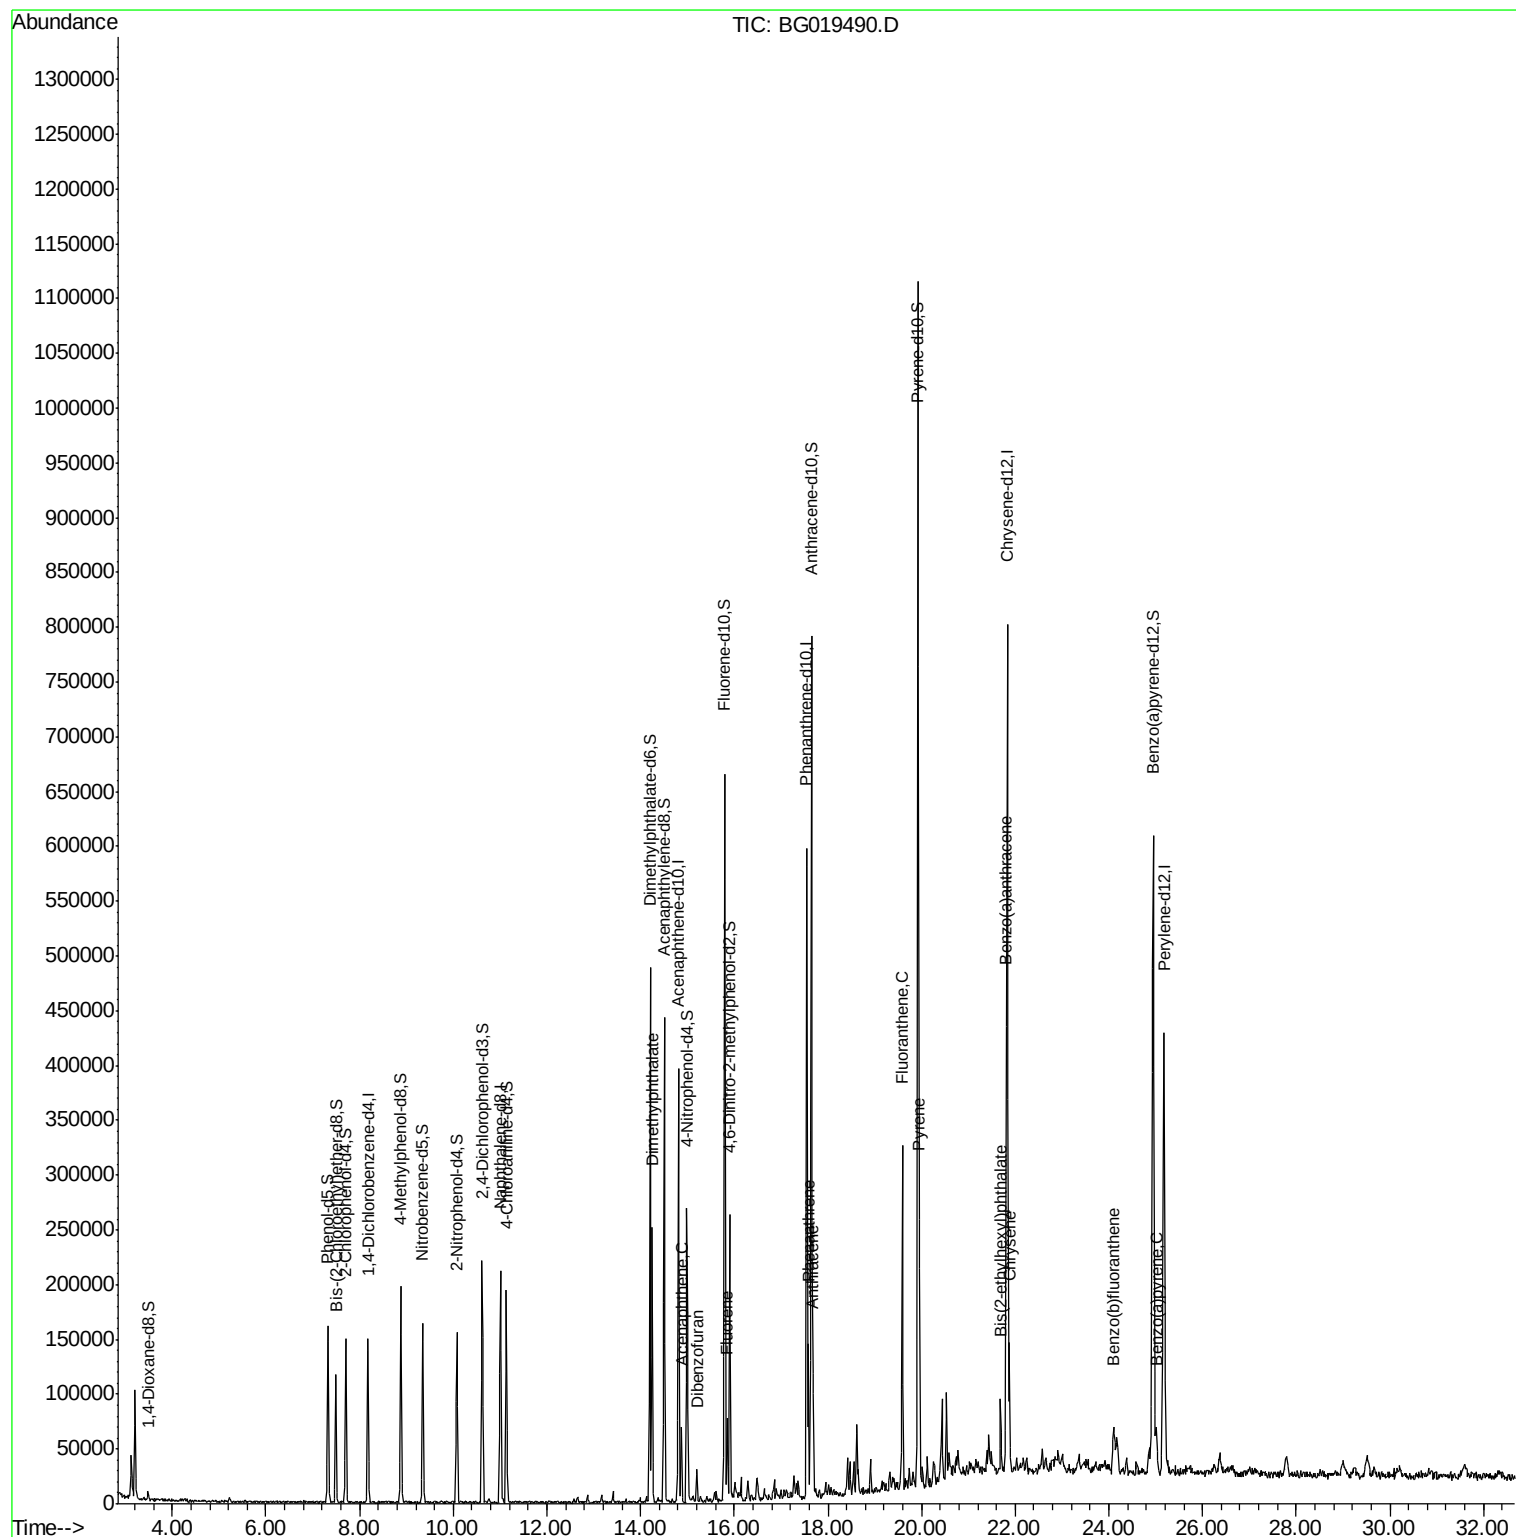

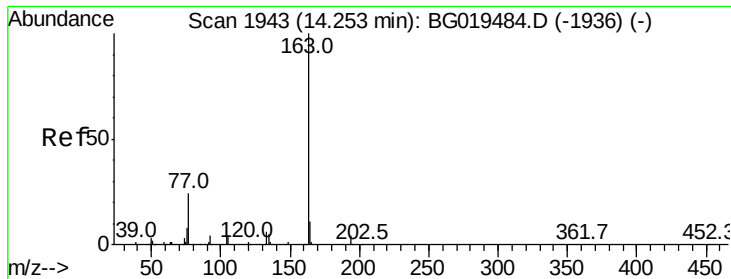


#45
Dimethylphthalate
Concen: 13.71 ng/ul
RT: 14.25 min Scan# 1942
Delta R.T. -0.00 min
Lab File: BG019490.D
Acq: 5 Nov 2015 13:32

Instrument :
BNA_G
ClientSampleId :
C0AN9




Tot Ion	Ratio	Resp	Lower	Upper
163	100	143875		
194	4.7		4.3	6.5
164	11.1		7.5	11.3

Manual Integrations
APPROVED

Mmdadoda
11/6/2015 3:43:16 PM

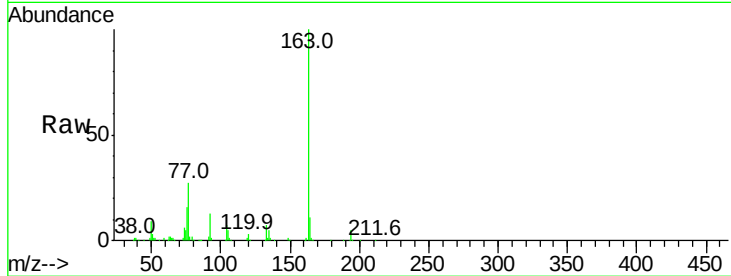


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

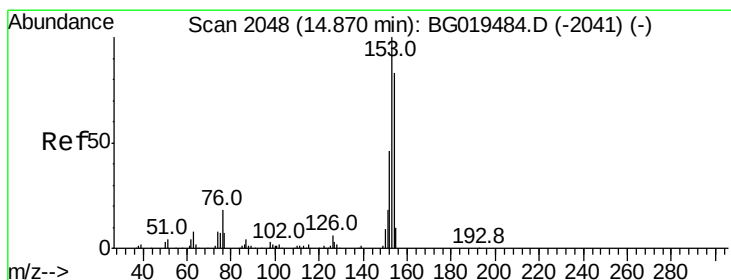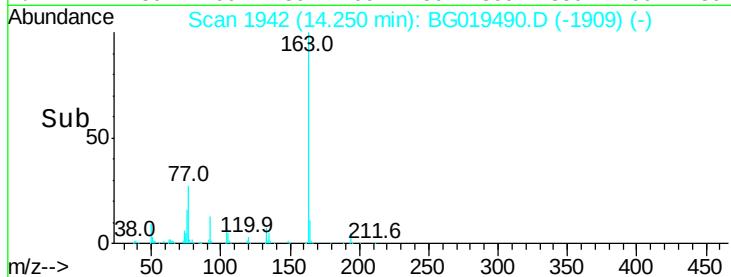
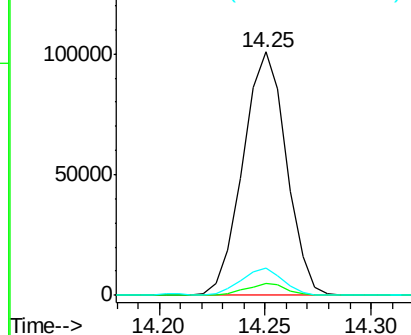



#50
Acenaphthene
Concen: 3.47 ng/ul
RT: 14.87 min Scan# 2047
Delta R.T. -0.00 min
Lab File: BG019490.D
Acq: 5 Nov 2015 13:32

Tgt Ion	Ratio	Resp	Lower	Upper
153	100	27285		
152	42.3		38.8	58.2
154	78.5		71.5	107.3

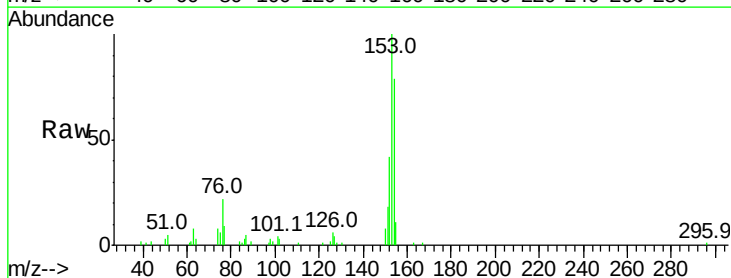

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

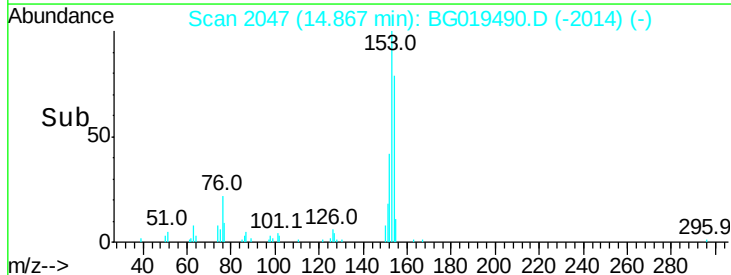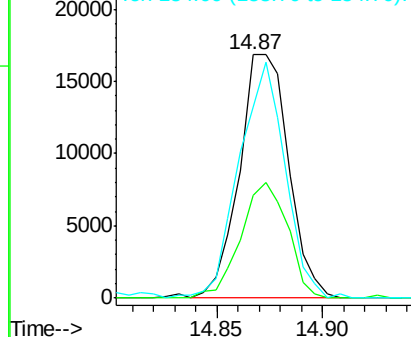

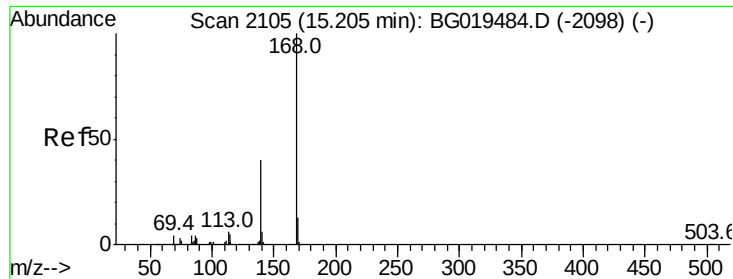

#54

Dibenzenofuran

Concen: 1.18 ng/ul

RT: 15.20 min Scan# 2104

Delta R.T. -0.00 min

Lab File: BG019490.D

Acq: 5 Nov 2015 13:32

Instrument :

BNA_G

ClientSampleId :

C0AN9

Tot Ion:168 Resp: 13710


Ion Ratio Lower Upper

168 100

139 48.0 32.4 48.6

Manual Integrations
APPROVED

Mmdadoda
11/6/2015 3:43:16 PM

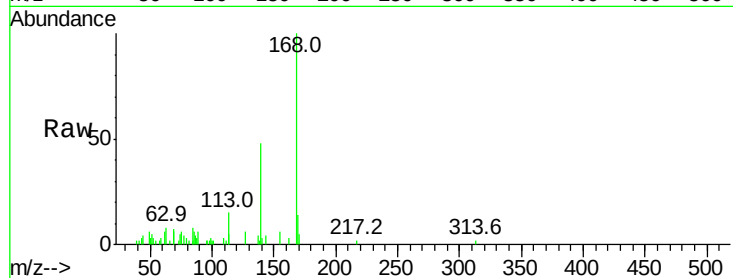

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

15.20

10000

8000



6000

4000

2000

0

Time--> 15.15 15.20 15.25

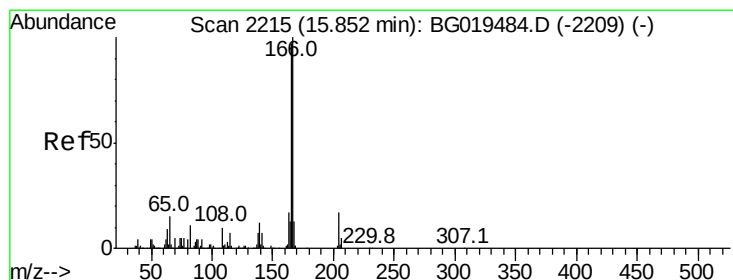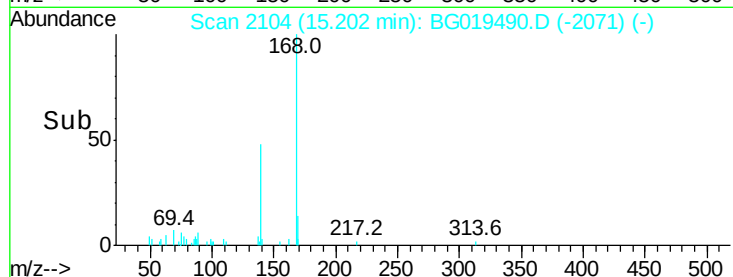

#59

Fluorene

Concen: 3.19 ng/ul

RT: 15.85 min Scan# 2215

Delta R.T. 0.00 min

Lab File: BG019490.D

Acq: 5 Nov 2015 13:32


Tgt Ion:166 Resp: 32241

Ion Ratio Lower Upper

166 100

165 95.2 77.6 116.4

167 12.0 9.6 14.4

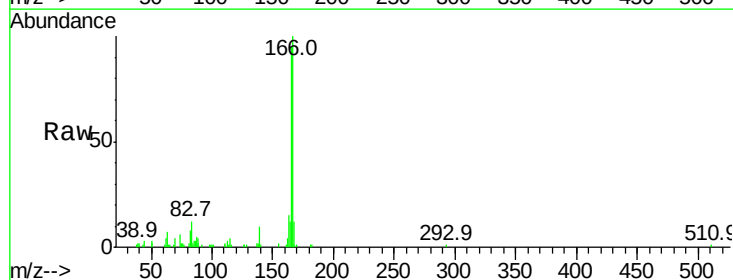

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

15.85

25000

20000


15000


10000

5000

0

Time--> 15.80 15.85 15.90

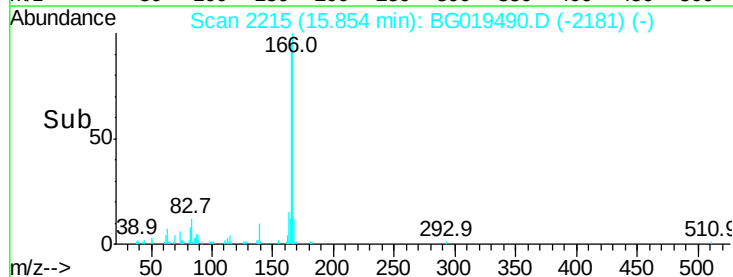

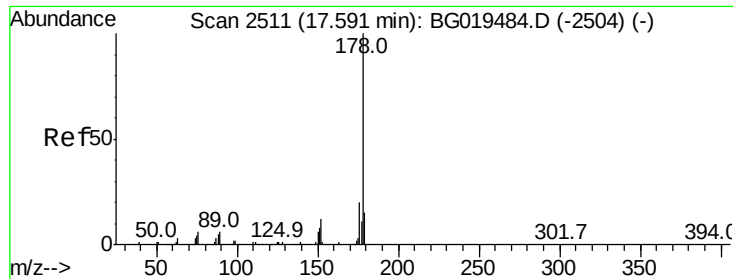





#70
 Phenanthrene
 Concen: 4.58 ng/ul
 RT: 17.59 min Scan# 2510
 Delta R.T. -0.00 min
 Lab File: BG019490.D
 Acq: 5 Nov 2015 13:32

Instrument :
 BNA_G
 ClientSampleId :
 C0AN9

Tot Ion	Ratio	Lower	Upper
178	100		
179	14.8	12.6	18.8
176	19.3	14.3	21.5




Manual Integrations
 APPROVED


Mmdadoda
 11/6/2015 3:43:16 PM

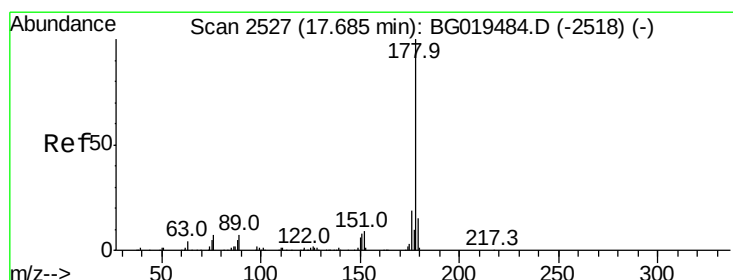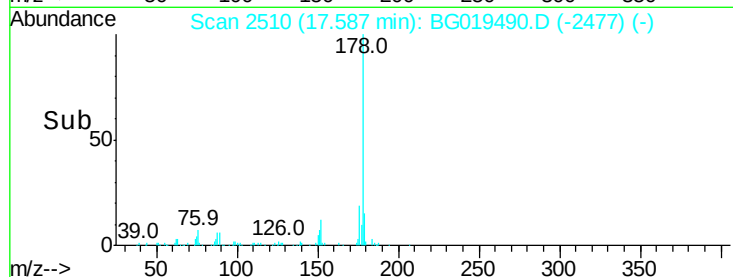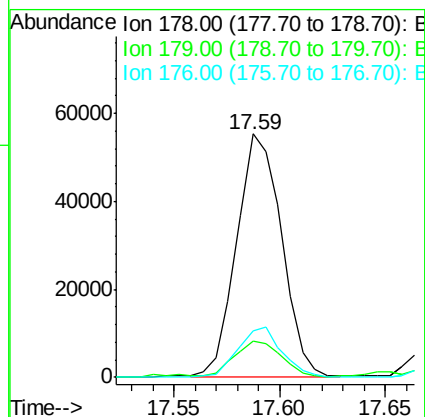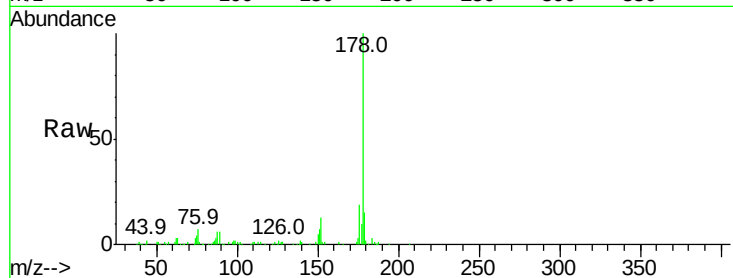

#72
 Anthracene
 Concen: 3.58 ng/ul
 RT: 17.68 min Scan# 2526
 Delta R.T. -0.00 min
 Lab File: BG019490.D
 Acq: 5 Nov 2015 13:32

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.0	11.6	17.4
176	20.6	14.2	21.4

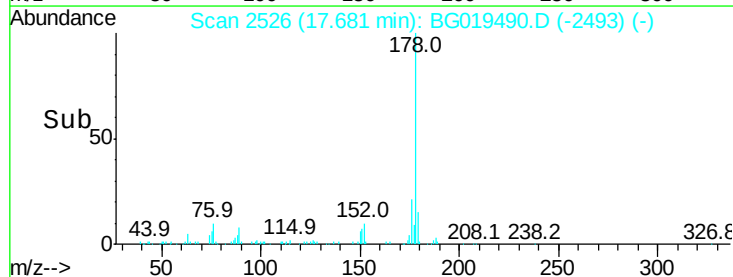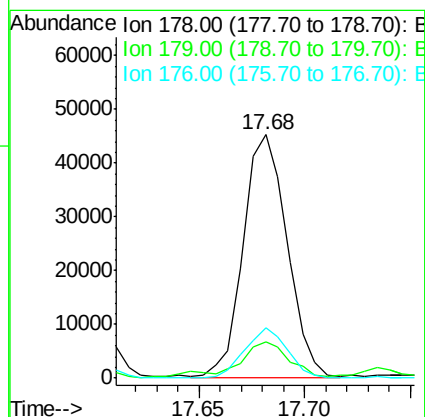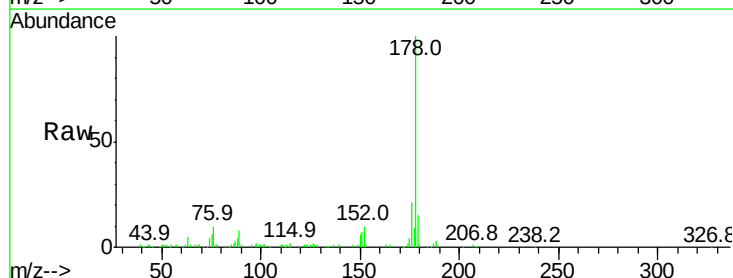

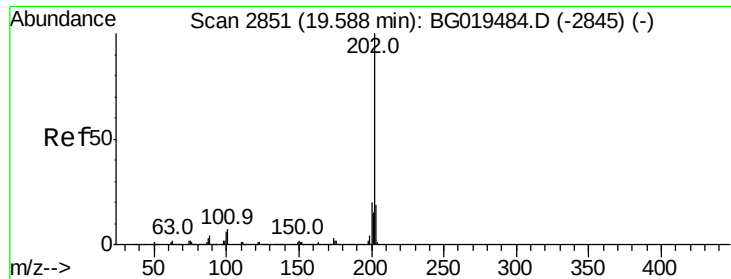





#77
 Fluoranthene
 Concen: 8.75 ng/ul
 RT: 19.59 min Scan# 2851
 Delta R.T. 0.00 min
 Lab File: BG019490.D
 Acq: 5 Nov 2015 13:32

Instrument :
 BNA_G
 ClientSampleId :
 C0AN9

Tot Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	6.0	4.0	6.0
100	4.8	3.6	5.4




Manual Integrations
 APPROVED


Mmdadoda
 11/6/2015 3:43:16 PM

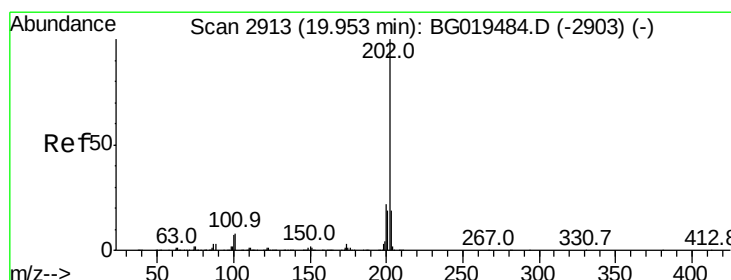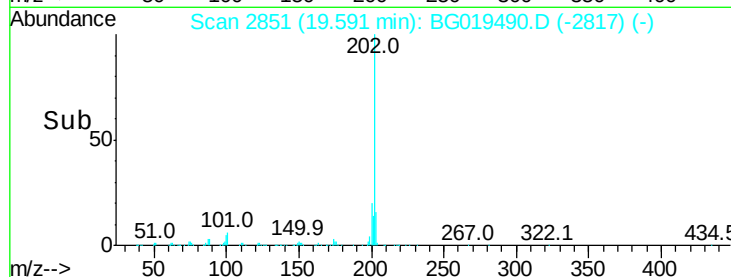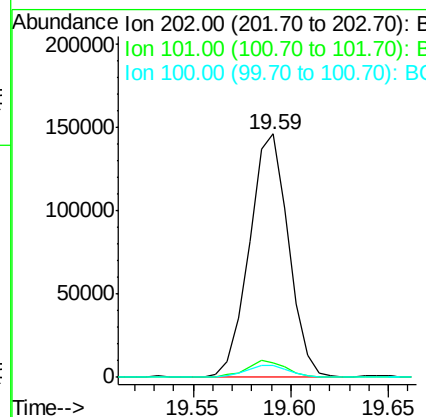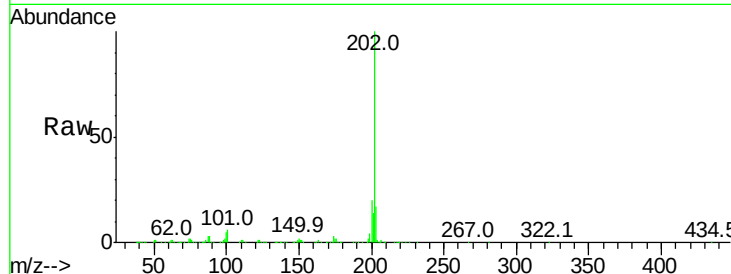

#80
 Pyrene
 Concen: 5.26 ng/ul
 RT: 19.95 min Scan# 2912
 Delta R.T. -0.00 min
 Lab File: BG019490.D
 Acq: 5 Nov 2015 13:32

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	9.3	4.3	6.5#
100	8.2	3.6	5.4#

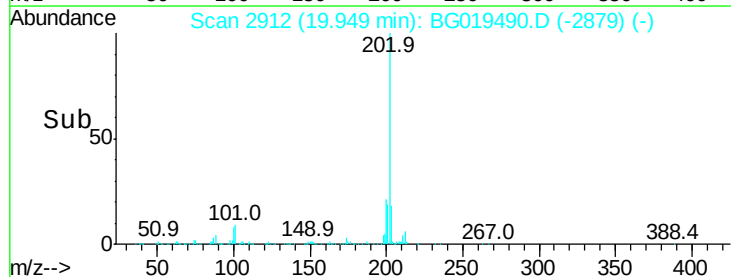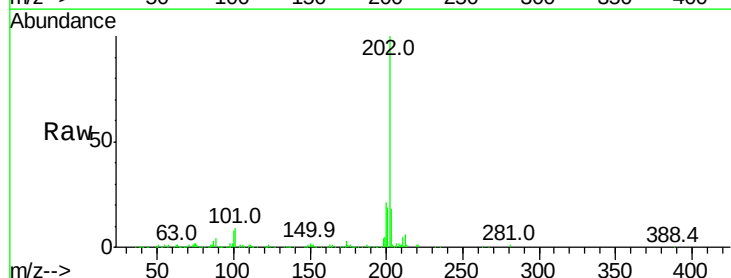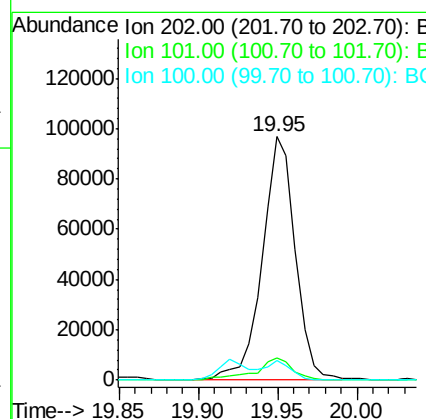

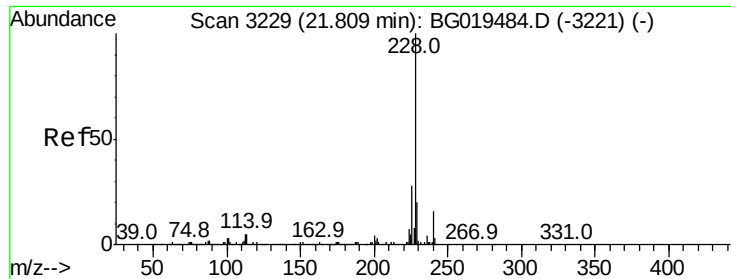





#83
 Benzo(a)anthracene
 Concen: 2.86 ng/ul
 RT: 21.81 min Scan# 3228
 Delta R.T. -0.00 min
 Lab File: BG019490.D
 Acq: 5 Nov 2015 13:32

Instrument :
 BNA_G
 ClientSampleId :
 C0AN9

Tot Ion	Ratio	Lower	Upper
228	100		
229	20.1	15.8	23.8
226	28.6	21.8	32.6




Manual Integrations
 APPROVED


Mmdadoda
 11/6/2015 3:43:16 PM

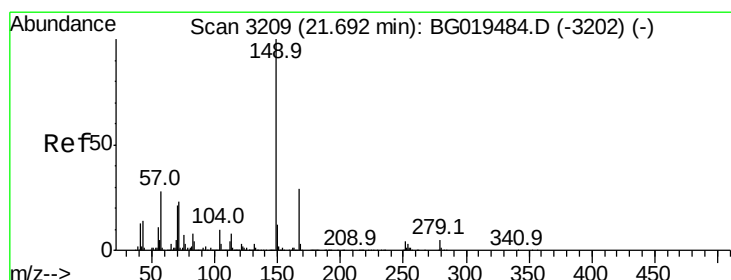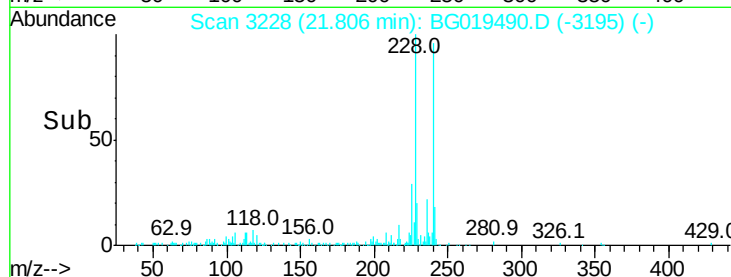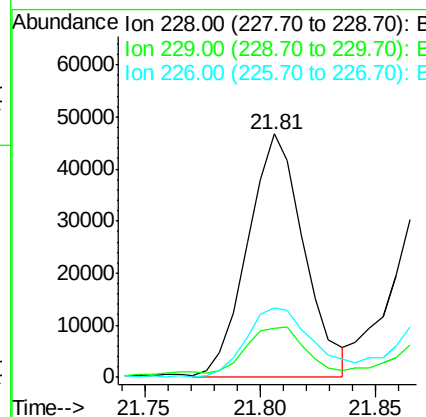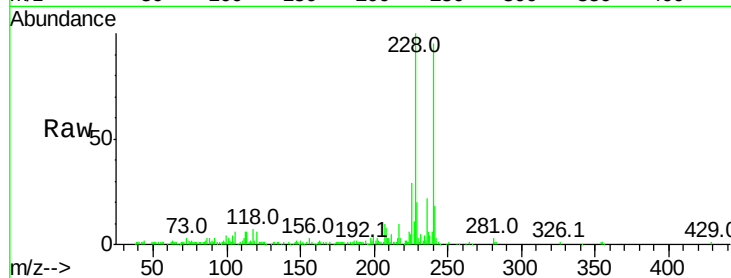

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 1.86 ng/ul
 RT: 21.69 min Scan# 3208
 Delta R.T. -0.00 min
 Lab File: BG019490.D
 Acq: 5 Nov 2015 13:32

Tgt Ion	Ratio	Lower	Upper
149	100		
167	25.0	23.2	34.8
279	5.5	5.0	7.4

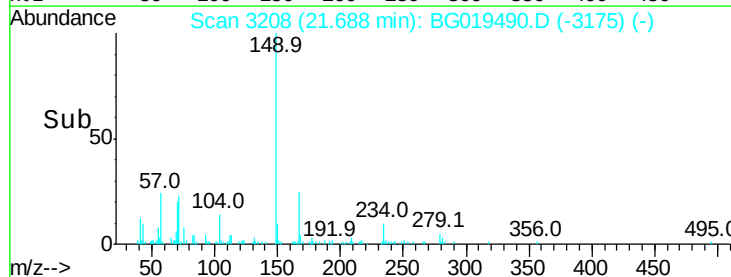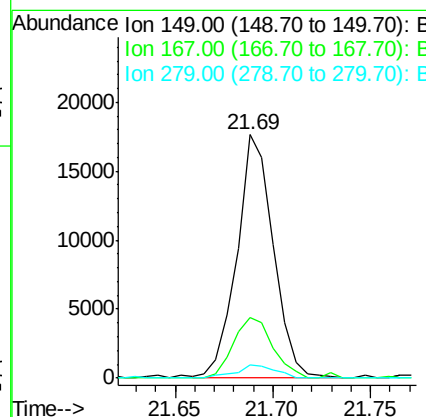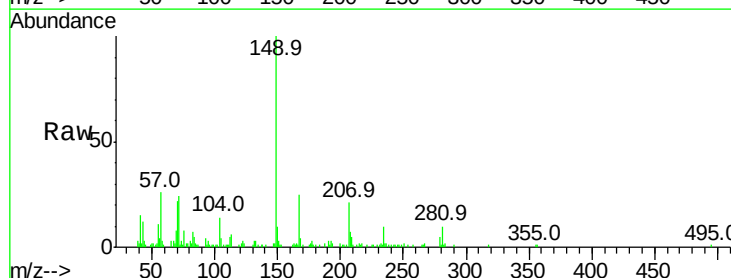

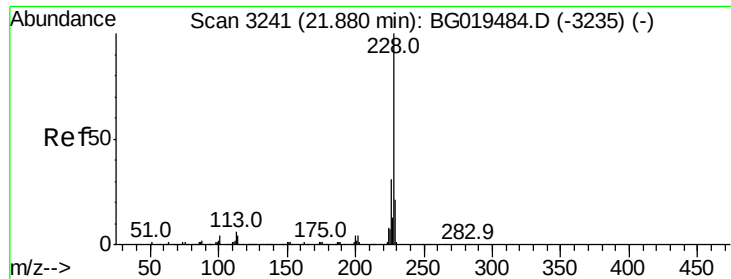





#85
Chrysene
Concen: 3.16 ng/ul
RT: 21.88 min Scan# 3240
Delta R.T. -0.00 min
Lab File: BG019490.D
Acq: 5 Nov 2015 13:32

Instrument :
BNA_G
ClientSampleId :
C0AN9

Tot Ion:228	Resp:	82075
Ion Ratio	Lower	Upper
228 100		
226 27.3	24.6	36.8
229 19.2	17.3	25.9




Manual Integrations
APPROVED


Mmdadoda
11/6/2015 3:43:16 PM

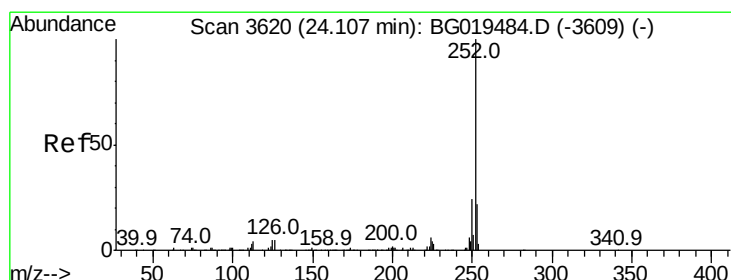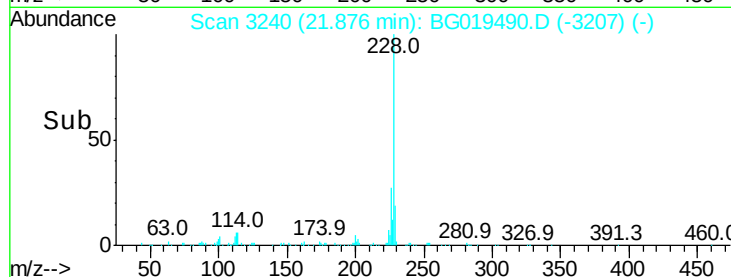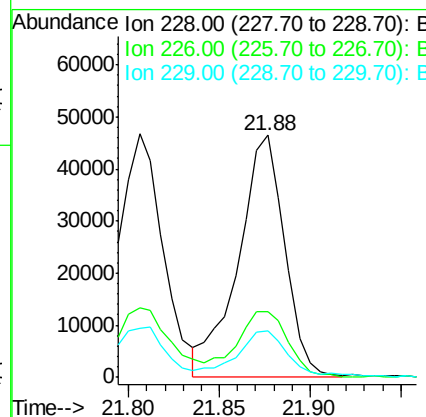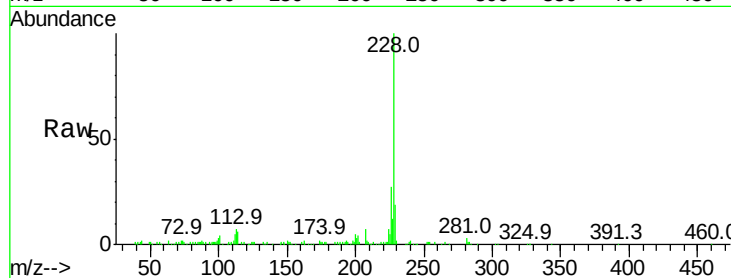

#88
Benzo(b)fluoranthene
Concen: 2.22 ng/ul
RT: 24.10 min Scan# 3619
Delta R.T. -0.00 min
Lab File: BG019490.D
Acq: 5 Nov 2015 13:32

Tgt Ion:252	Resp:	59328
Ion Ratio	Lower	Upper
252 100		
253 21.5	17.1	25.7
125 4.6	2.5	3.7#

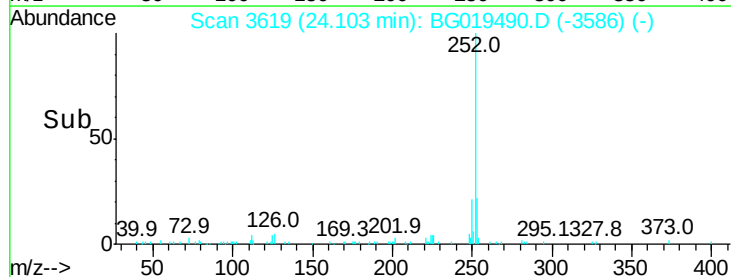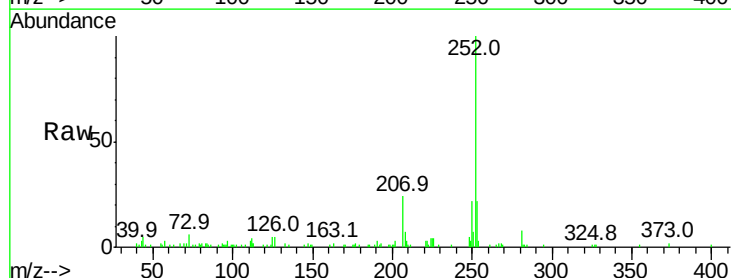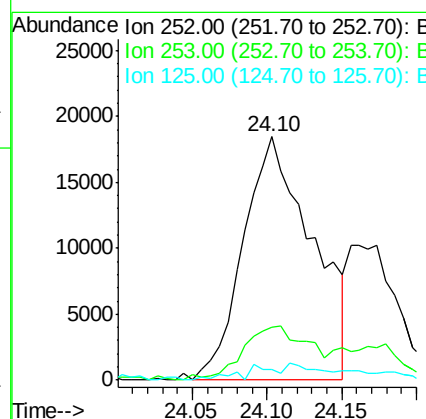

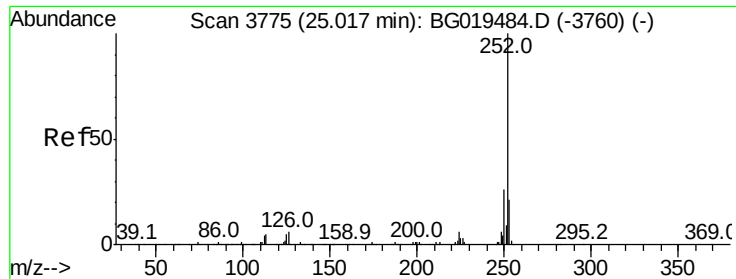

#91
 Benzo(a)pyrene
 Concen: 1.86 ng/ul m
 RT: 25.02 min Scan# 3775
 Delta R.T. 0.00 min
 Lab File: BG019490.D
 Acq: 5 Nov 2015 13:32

Instrument :
 BNA_G
 ClientSampleId :
 C0AN9

Tot Ion:	252	Resp:	47590
Ion Ratio	Lower	Upper	
252	100		
253	21.9	16.0	24.0
125	6.2	3.3	4.9#

Manual Integrations
 APPROVED

Mmdadoda
 11/6/2015 3:43:16 PM

