

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110517\
 Data File : BG030737.D
 Acq On : 5 Nov 2017 14:21
 Operator : SJ/JU
 Sample : I6107-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B0E79

Quant Time: Nov 06 00:53:27 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 06 00:53:03 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	65009	20.00	ng/ul	0.00
18) Naphthalene-d8	10.97	136	281772	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.77	164	182990	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	453259	20.00	ng/ul	0.00
75) Chrysene-d12	21.78	240	586761	20.00	ng/ul	-0.01
83) Perylene-d12	25.09	264	612390	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	7172	4.48	ng/uL	0.00
5) Phenol-d5	7.31	99	120984	19.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.46	67	74674	19.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	99858	22.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	101652	20.17	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	47164	23.32	ng/ul	0.00
22) 2-Nitrophenol-d4	10.04	143	52915	25.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	101332	21.46	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	80891	14.74	ng/ul	0.00
43) Dimethylphthalate-d6	14.16	166	364941	23.33	ng/ul	0.00
46) Acenaphthylene-d8	14.46	160	435560	22.89	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	56502	19.56	ng/ul	0.00
57) Fluorene-d10	15.76	176	329081	25.68	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.87	200	56243	25.42	ng/ul	0.00
70) Anthracene-d10	17.61	188	529096	24.68	ng/ul	0.00
76) Pyrene-d10	19.88	212	676480	22.27	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.86	264	739041	25.48	ng/ul	-0.02

Target Compounds


					Ovalue
6) Phenol	7.34	94	9880	1.530	ng/ul 94
44) Dimethylphthalate	14.21	163	229059	15.011	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG110517\
Data File : BG030737.D
Acq On : 5 Nov 2017 14:21
Operator : SJ/JU
Sample : I6107-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B0E79

Quant Time: Nov 06 00:53:27 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 06 00:53:03 2017
Response via : Initial Calibration

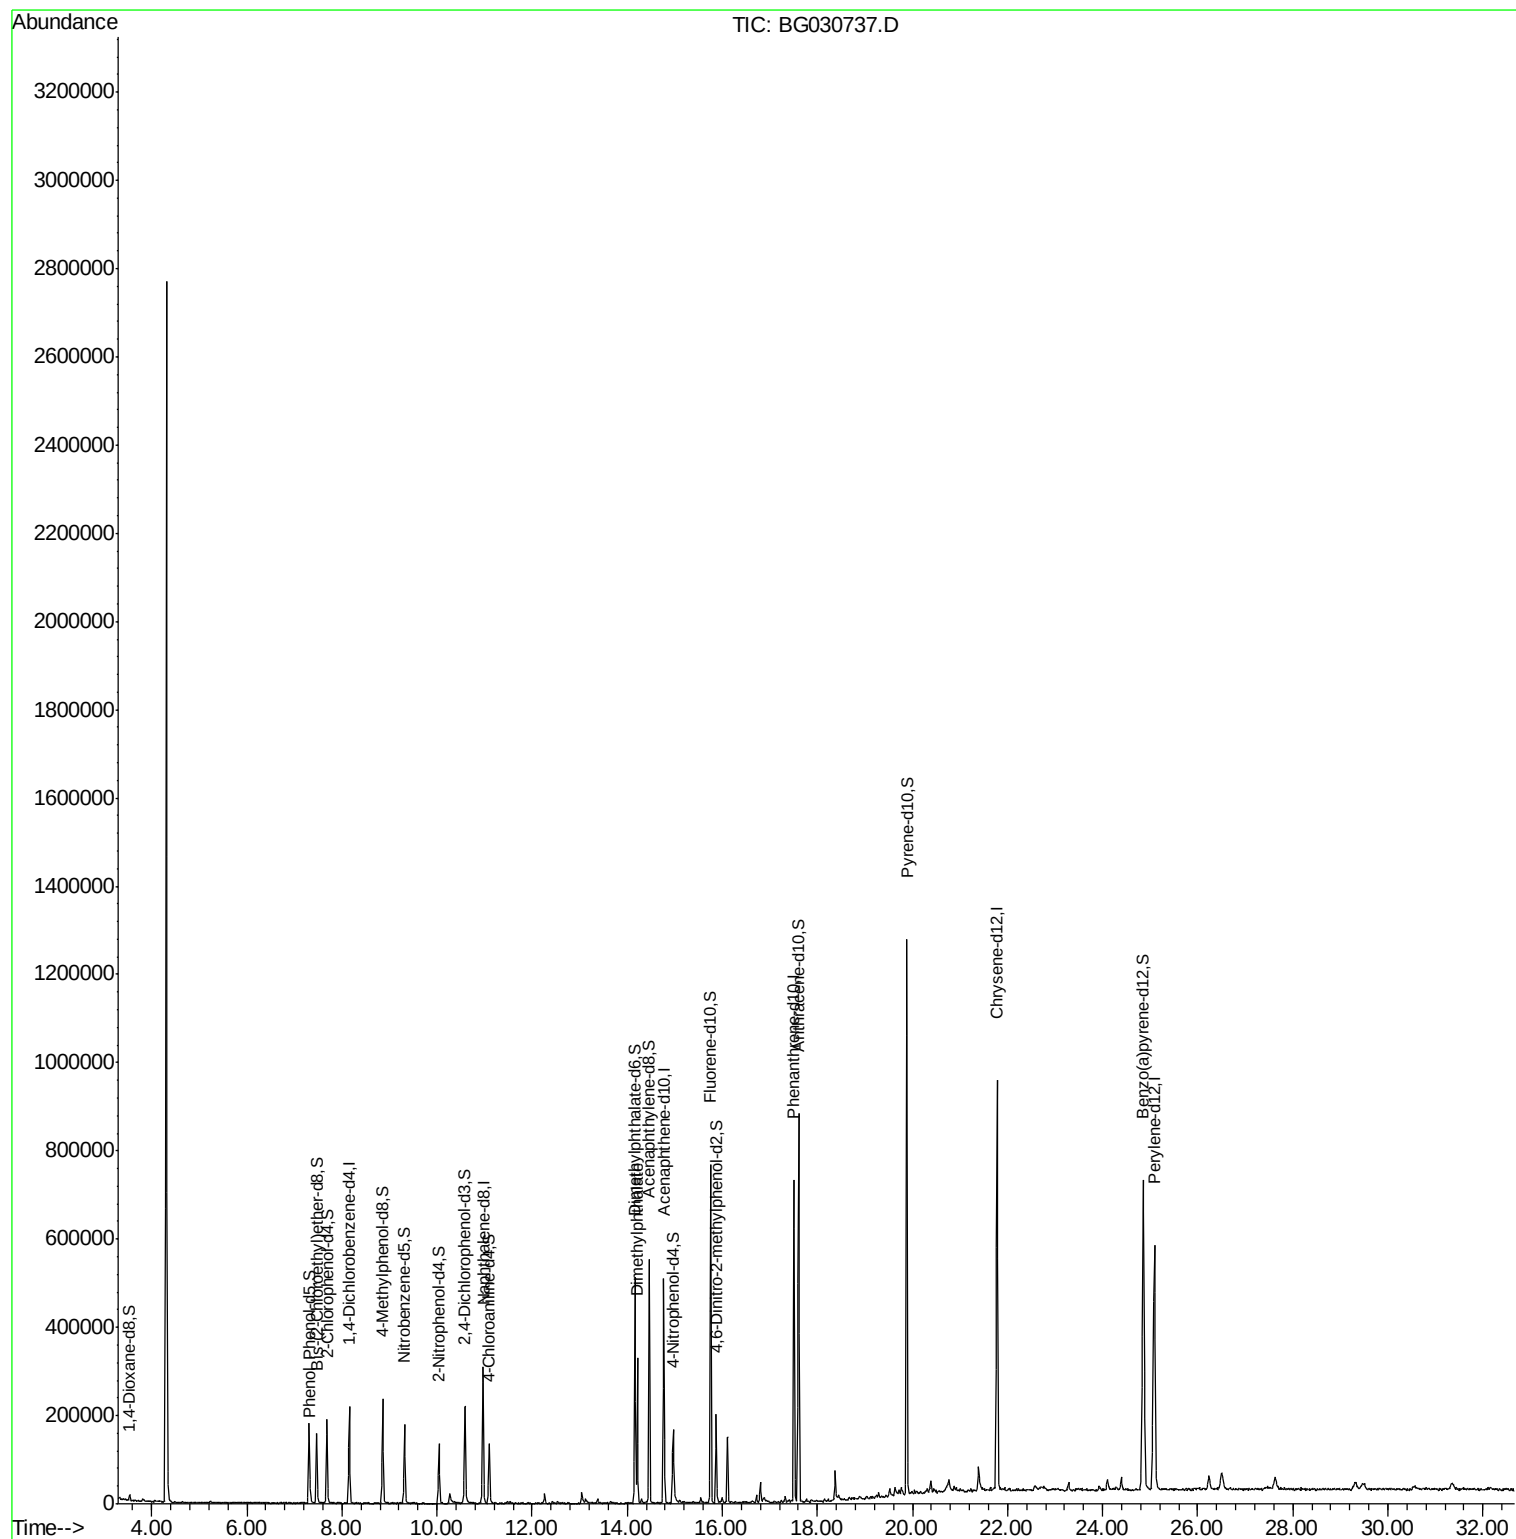

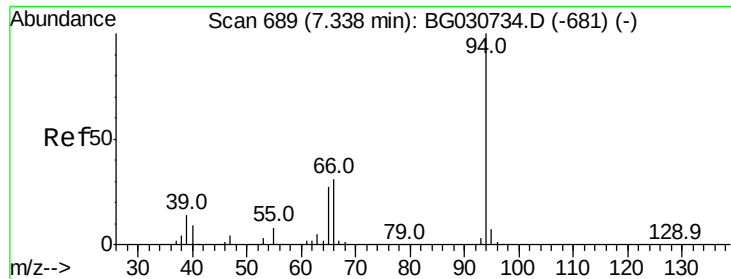





#6

Phenol

Concen: 1.530 ng/ul
 RT: 7.34 min Scan# 689
 Delta R.T. -0.00 min
 Lab File: BG030737.D
 Acq: 5 Nov 2017 14:21

Instrument :
 BNA_G
 ClientSampleId :
 B0E79

Tot Ion	94	Resp	9880
Ion Ratio	Lower	Upper	
94	100		
65	27.9	27.1	40.7
66	45.5	34.6	52.0

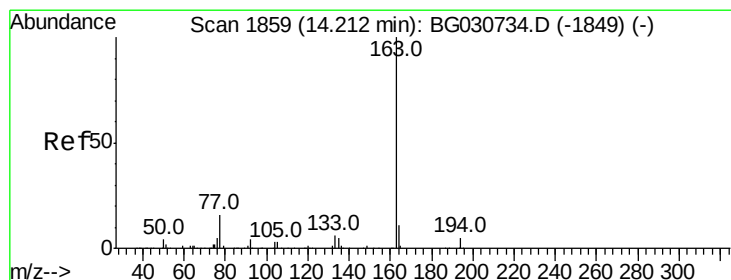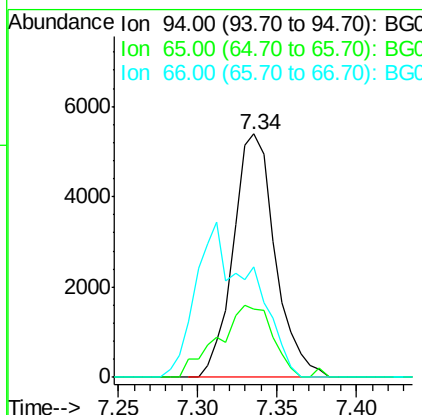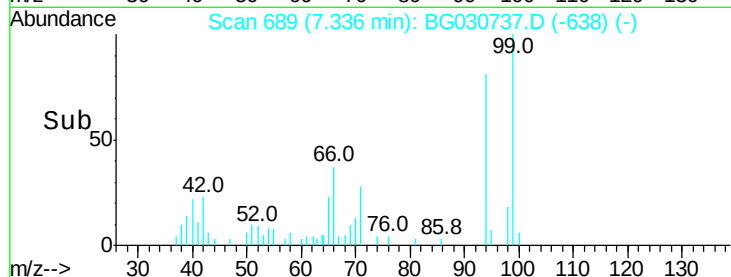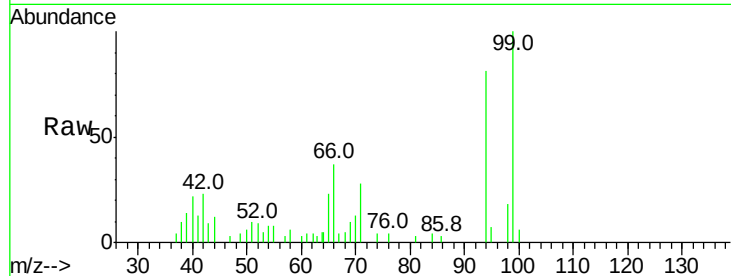

#44

Dimethylphthalate

Concen: 15.011 ng/ul
 RT: 14.21 min Scan# 1859
 Delta R.T. -0.00 min
 Lab File: BG030737.D
 Acq: 5 Nov 2017 14:21

Tgt Ion	163	Resp	229059
Ion Ratio	Lower	Upper	
163	100		
194	4.5	3.5	5.3
164	10.1	7.6	11.4

