
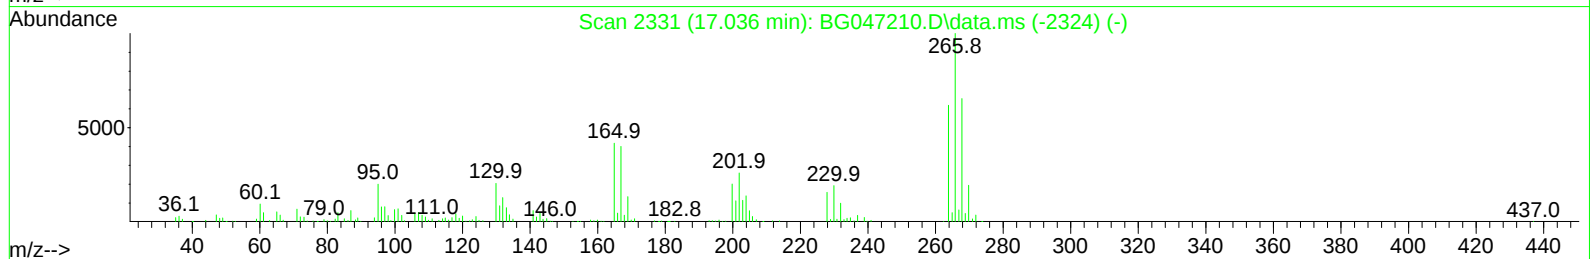
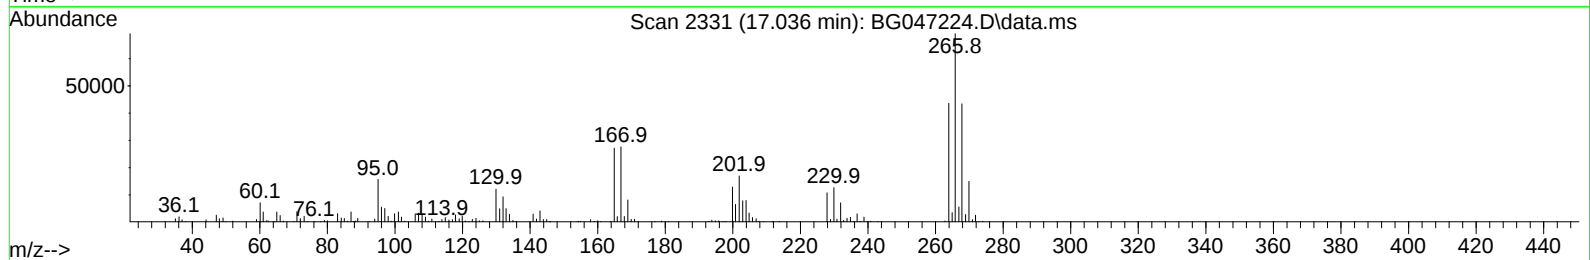


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110520\
Data File : BG047224.D
Acq On : 5 Nov 2020 17:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 03:50:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 04 16:19:40 2020
Response via : Initial Calibration

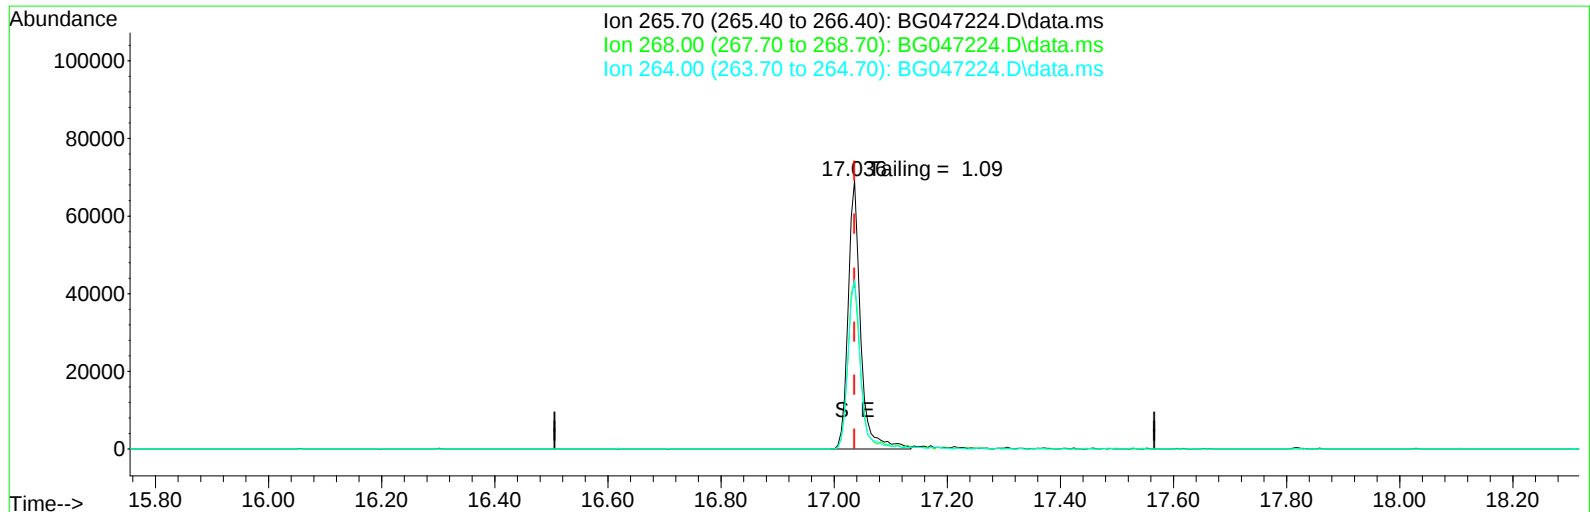

TIC: BG047224.D\data.ms

(70) Pentachlorophenol (C)




17.036min (+ 0.000) 28542.80 ng

response 106213

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.79
264.00	61.60	63.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110520\
Data File : BG047224.D
Acq On : 5 Nov 2020 17:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 03:50:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 04 16:19:40 2020
Response via : Initial Calibration

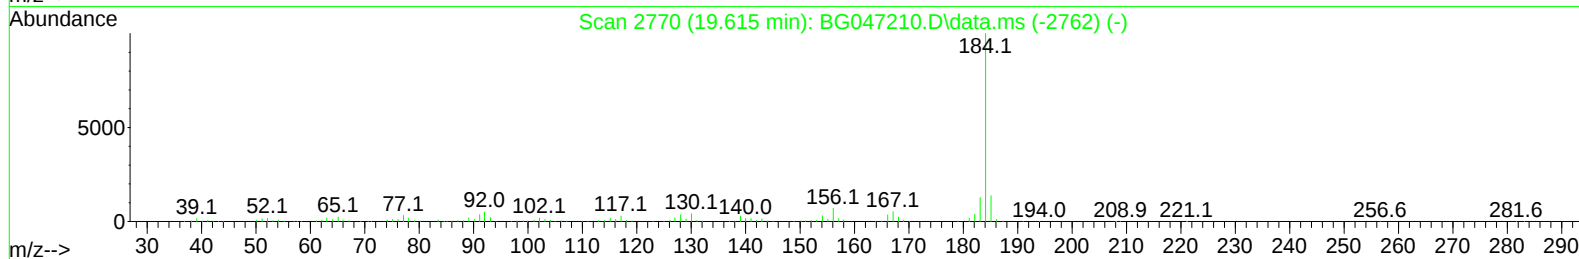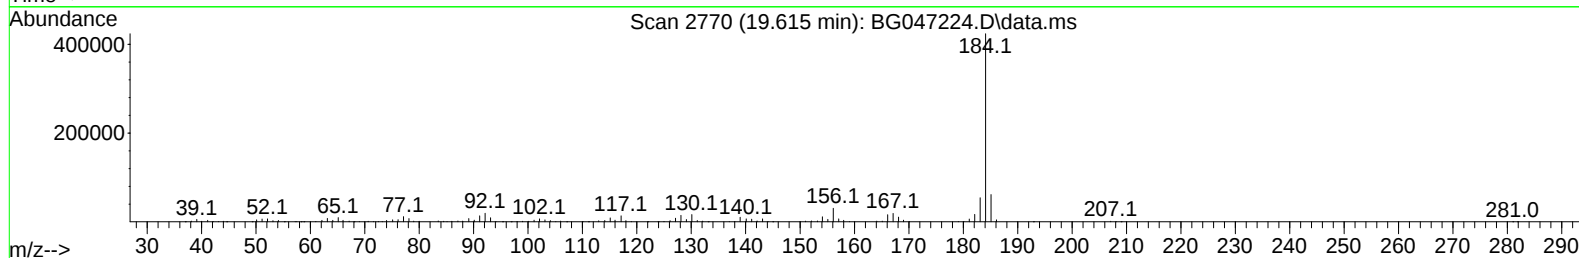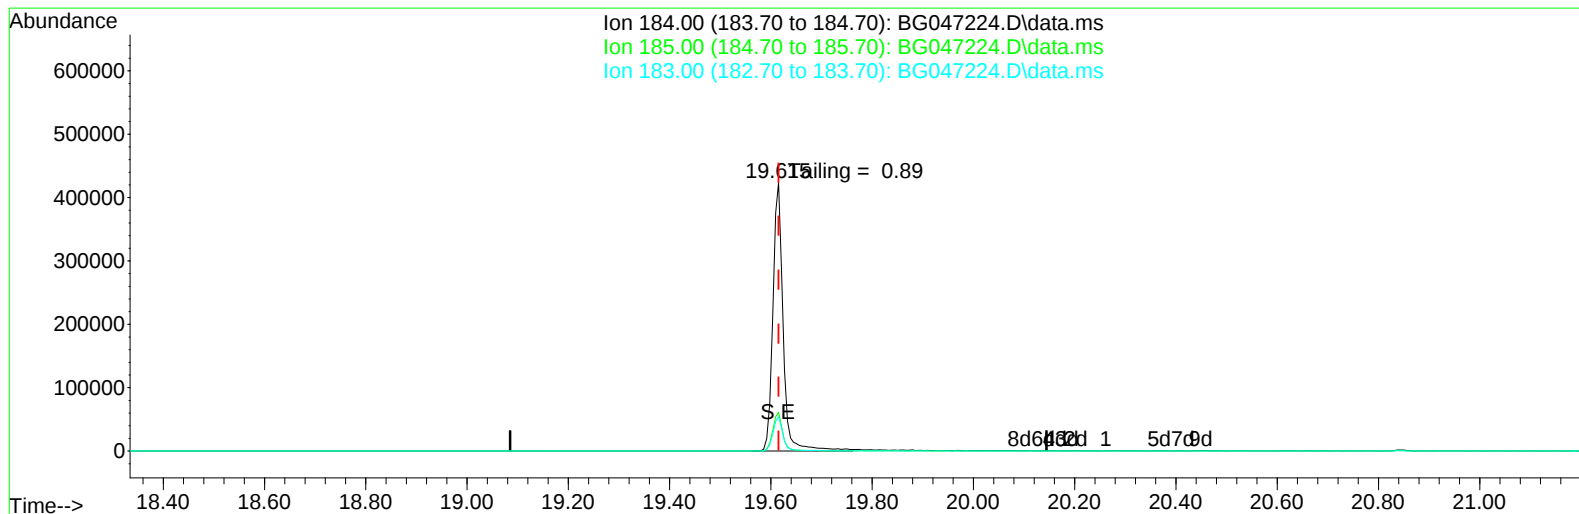

TIC: BG047224.D\data.ms

(77) Benzidine

19.615min (+ 0.000) 330798.10 ng m

response 621292

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.47
183.00	13.20	12.80
0.00	0.00	0.00