


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110520\
 Data File : BG047216.D
 Acq On : 5 Nov 2020 8:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG110420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 04 16:19:40 2020

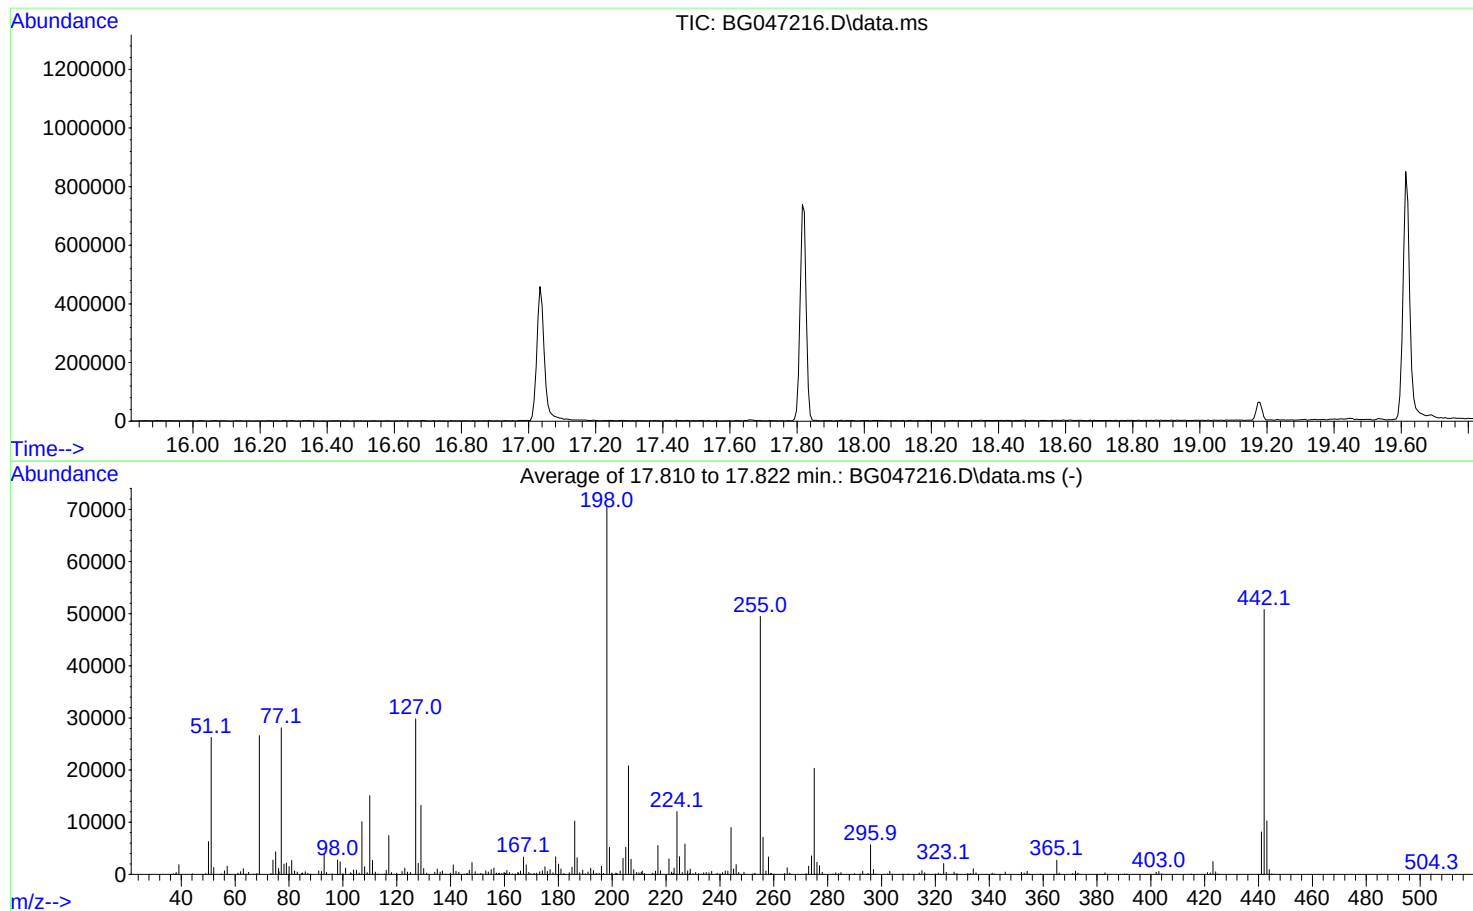

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	26267	PASS
68	69	0.00	2	0.7	198	PASS
69	198	0.00	100	37.7	26624	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.3	29843	PASS
197	198	0.00	2	0.3	178	PASS
198	198	100	100	100.0	70560	PASS
199	198	5	9	7.3	5178	PASS
275	198	10	60	28.8	20336	PASS
365	198	1	100	3.9	2719	PASS
441	198	0.01	100	11.5	8141	PASS
442	198	50	100	72.0	50800	PASS
443	442	15	24	20.2	10251	PASS