

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110615\
 Data File : BG019503.D
 Acq On : 6 Nov 2015 9:14
 Operator : UM/NP
 Sample : PB86447BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK47

Quant Time: Nov 06 22:27:33 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 06 22:26:17 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	35014	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	152181	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	127649	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	348131	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	455976	20.00	ng/ul	0.00
86) Perylene-d12	25.18	264	421391	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	4828	6.60	ng/uL	0.00
5) Phenol-d5	7.32	99	108390	33.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	77790	38.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.71	132	68301	34.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	90606	35.39	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	38020	34.00	ng/ul	0.00
22) 2-Nitrophenol-d4	10.08	143	43910	33.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	91433	31.74	ng/ul	0.00
29) 4-Chloroaniline-d4	11.14	131	106727	36.63	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	346568	32.93	ng/ul	0.00
47) Acenaphthylene-d8	14.51	160	384643	33.00	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	56028	33.51	ng/ul	0.00
58) Fluorene-d10	15.80	176	309583	31.80	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.91	200	65889	29.24	ng/ul	0.00
71) Anthracene-d10	17.65	188	544376	34.30	ng/ul	0.00
79) Pyrene-d10	19.93	212	656734	32.91	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.95	264	731578	34.60	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.89	70	3256	1.16 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110615\
Data File : BG019503.D
Acq On : 6 Nov 2015 9:14
Operator : UM/NP
Sample : PB86447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK47

Quant Time: Nov 06 22:27:33 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 06 22:26:17 2015
Response via : Initial Calibration

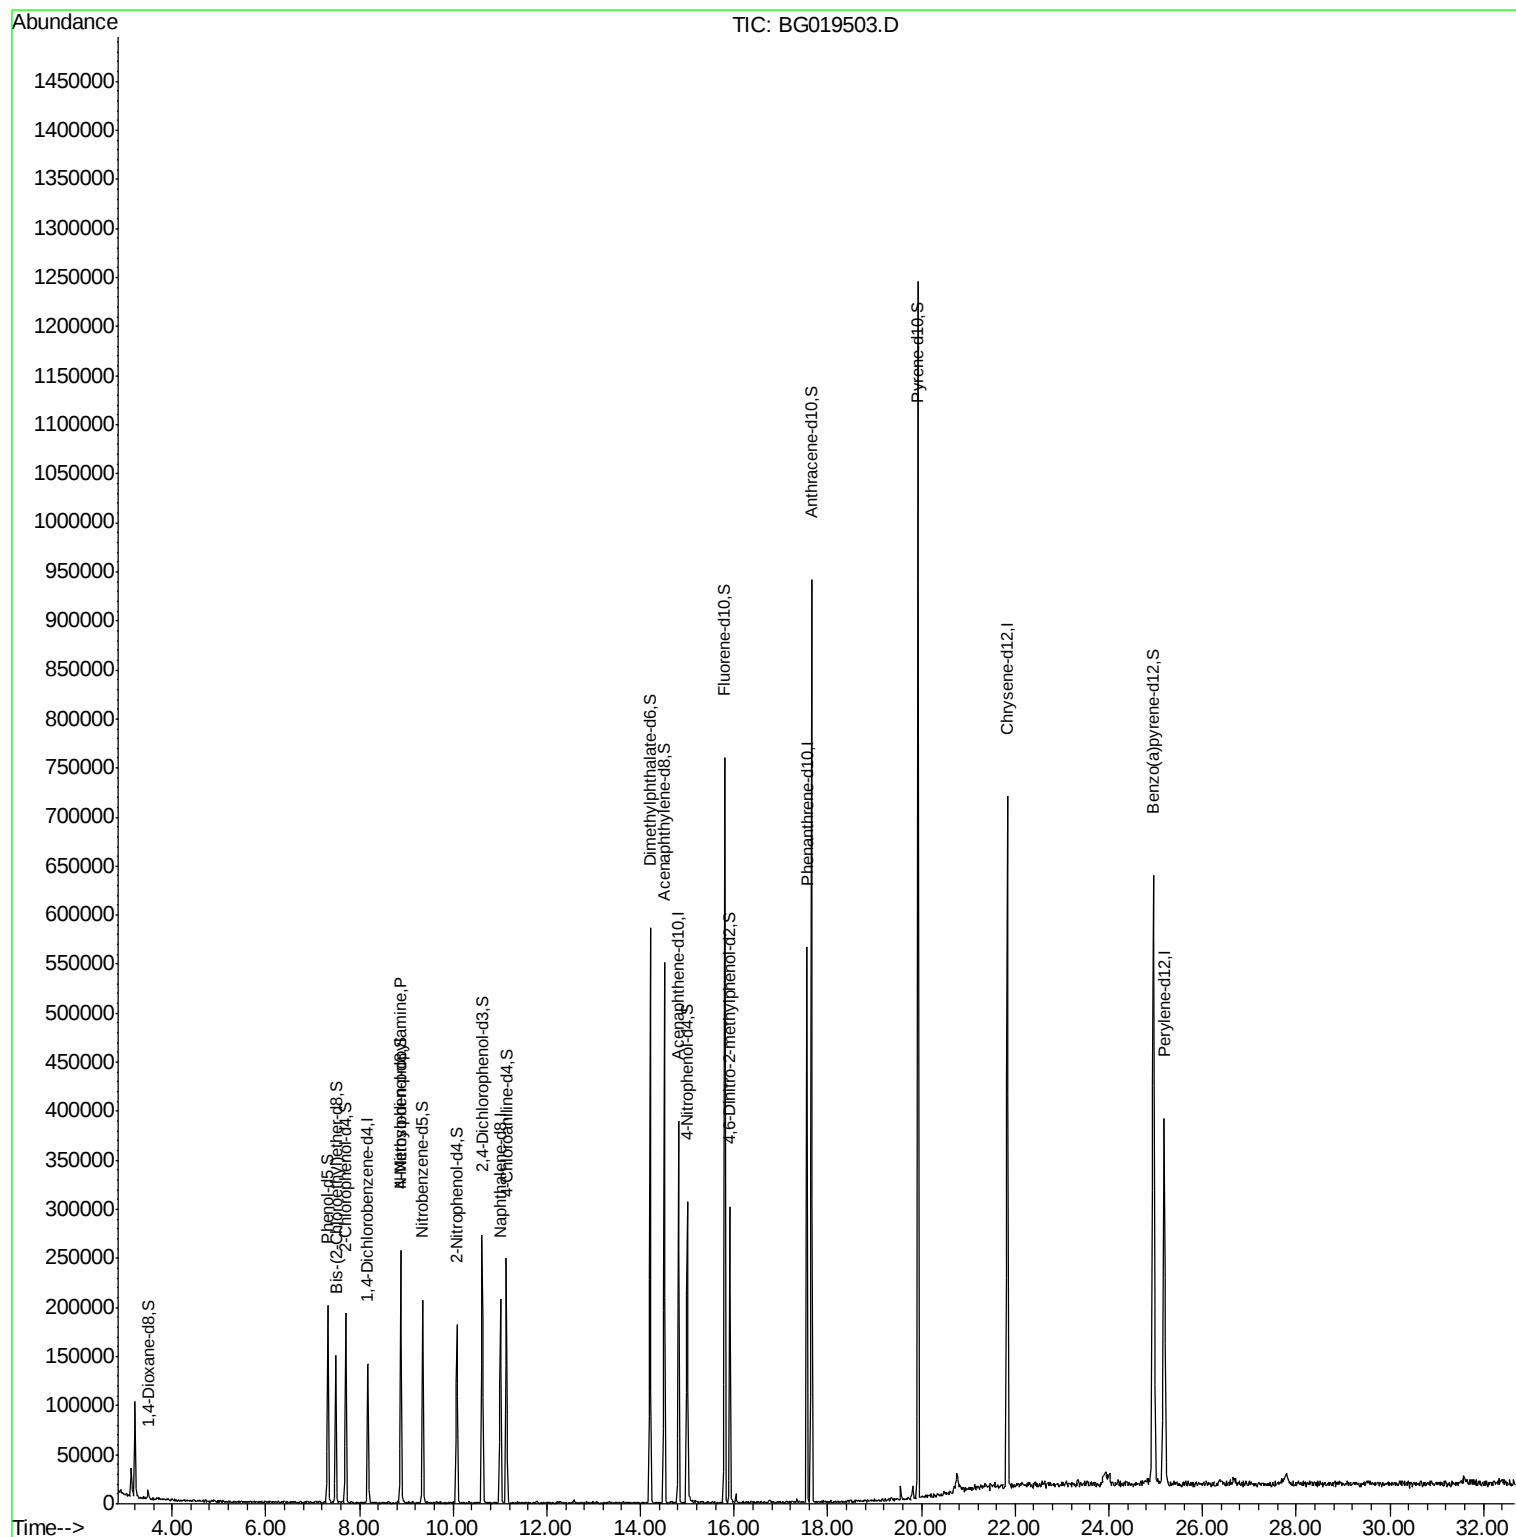

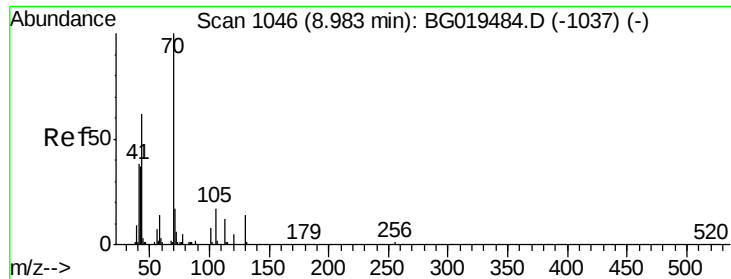

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.16 ng/ul
 RT: 8.89 min Scan# 1029
 Delta R.T. -0.10 min
 Lab File: BG019503.D
 Acq: 6 Nov 2015 9:14

Instrument :
 BNA_G
 ClientSampleId :
 SBLK47

Tgt Ion: 70 Resp: 3256
 Ion Ratio Lower Upper
 70 100
 42 213.2 36.6 55.0#
 101 0.0 5.8 8.8#
 130 0.0 14.6 22.0#

