

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110615\
 Data File : BG019512.D
 Acq On : 6 Nov 2015 15:01
 Operator : UM/NP
 Sample : PB86479BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK79

Quant Time: Nov 07 00:09:36 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 06 23:58:14 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	33145	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	135772	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	113328	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	327658	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	421783	20.00	ng/ul	0.00
86) Perylene-d12	25.18	264	393181	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	4605	6.65	ng/uL	0.00
5) Phenol-d5	7.32	99	109480	35.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	73180	37.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	67997	35.80	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	89286	36.84	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	37620	37.70	ng/ul	0.00
22) 2-Nitrophenol-d4	10.08	143	45235	38.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	90453	35.20	ng/ul	0.00
29) 4-Chloroaniline-d4	11.13	131	108175	41.61	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	354756	37.97	ng/ul	0.00
47) Acenaphthylene-d8	14.51	160	387982	37.49	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	58340	39.30	ng/ul	0.00
58) Fluorene-d10	15.80	176	322324	37.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.91	200	68060	32.09	ng/ul	0.00
71) Anthracene-d10	17.65	188	562634	37.67	ng/ul	0.00
79) Pyrene-d10	19.92	212	660562	35.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.95	264	737343	37.37	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.88	70	3074	1.15 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110615\
Data File : BG019512.D
Acq On : 6 Nov 2015 15:01
Operator : UM/NP
Sample : PB86479BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK79

Quant Time: Nov 07 00:09:36 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 06 23:58:14 2015
Response via : Initial Calibration

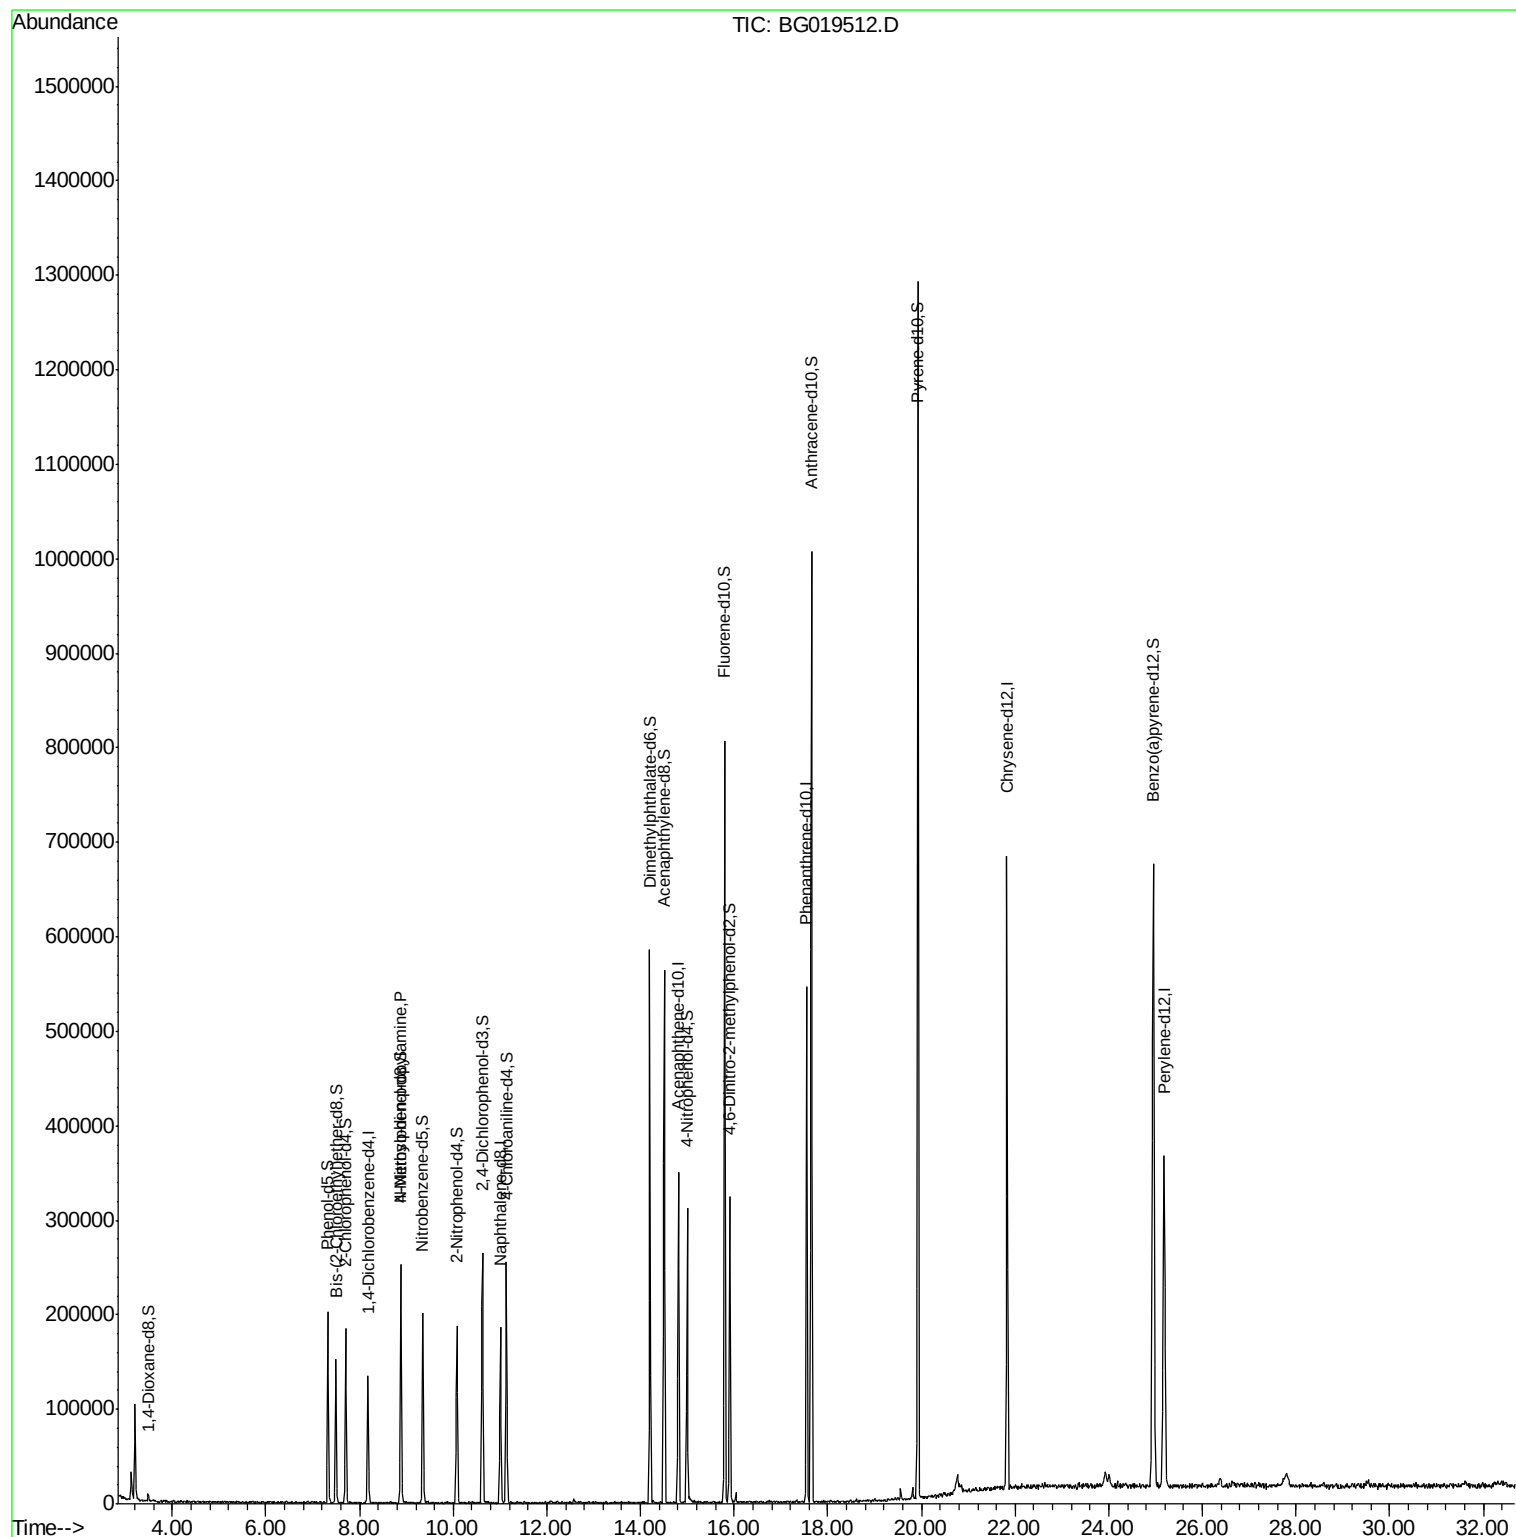

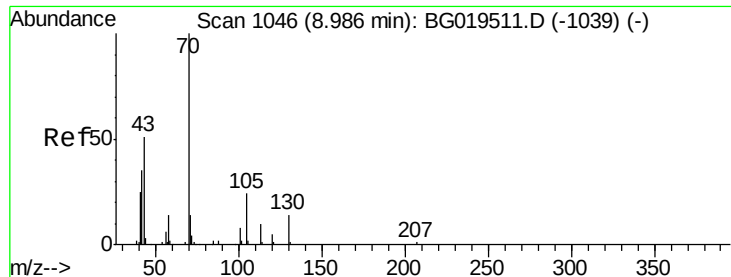

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.15 ng/ul
 RT: 8.88 min Scan# 1028
 Delta R.T. -0.11 min
 Lab File: BG019512.D
 Acq: 6 Nov 2015 15:01

Instrument :
 BNA_G
 ClientSampleId :
 SBLK79

Tgt Ion: 70 Resp: 3074
 Ion Ratio Lower Upper
 70 100
 42 271.1 36.6 55.0#
 101 0.0 5.8 8.8#
 130 0.0 14.6 22.0#

