

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110615\
 Data File : BG019508.D
 Acq On : 6 Nov 2015 12:26
 Operator : UM/NP
 Sample : G4297-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 H2TR1MSD

Quant Time: Nov 06 22:28:43 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 06 22:26:17 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.18	152	33793	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	144852	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	121279	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	354002	20.00	ng/ul	0.00
78) Chrysene-d12	21.83	240	449166	20.00	ng/ul	0.00
86) Perylene-d12	25.18	264	427109	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	2111	2.99	ng/uL	0.00
5) Phenol-d5	7.32	99	58247	18.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	37220	18.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	37262	19.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	47070	19.05	ng/ul	0.00
19) Nitrobenzene-d5	9.35	128	18600	17.47	ng/ul	0.00
22) 2-Nitrophenol-d4	10.08	143	23027	18.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	46882	17.10	ng/ul	0.00
29) 4-Chloroaniline-d4	11.14	131	49538	17.86	ng/ul	0.00
44) Dimethylphthalate-d6	14.20	166	179703	17.97	ng/ul	0.00
47) Acenaphthylene-d8	14.50	160	201093	18.16	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	28759	18.10	ng/ul	0.00
58) Fluorene-d10	15.79	176	163234	17.65	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.91	200	34722	15.15	ng/ul	0.00
71) Anthracene-d10	17.65	188	284411	17.62	ng/ul	0.00
79) Pyrene-d10	19.92	212	347356	17.67	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.94	264	381843	17.82	ng/ul	0.00

Target Compounds


						Ovalue
6) Phenol	7.35	94	60604	18.34	ng/ul	99
10) 2-Chlorophenol	7.74	128	32828	16.47	ng/ul	97
15) N-Nitroso-di-n-propylamine	8.98	70	46321	17.04	ng/ul#	87
33) 4-Chloro-3-methylphenol	12.27	107	63359	18.01	ng/ul#	93
45) Dimethylphthalate	14.25	163	66184	6.47	ng/ul#	95
50) Acenaphthene	14.87	153	121486	15.86	ng/ul	99
53) 4-Nitrophenol	15.01	109	39759	16.05	ng/ul#	74
55) 2,4-Dinitrotoluene	15.16	165	52747	16.14	ng/ul#	89
69) Pentachlorophenol	17.20	266	37725	14.32	ng/ul	94
80) Pyrene	19.95	202	402091	15.95	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110615\
Data File : BG019508.D
Acq On : 6 Nov 2015 12:26
Operator : UM/NP
Sample : G4297-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H2TR1MSD

Quant Time: Nov 06 22:28:43 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 06 22:26:17 2015
Response via : Initial Calibration

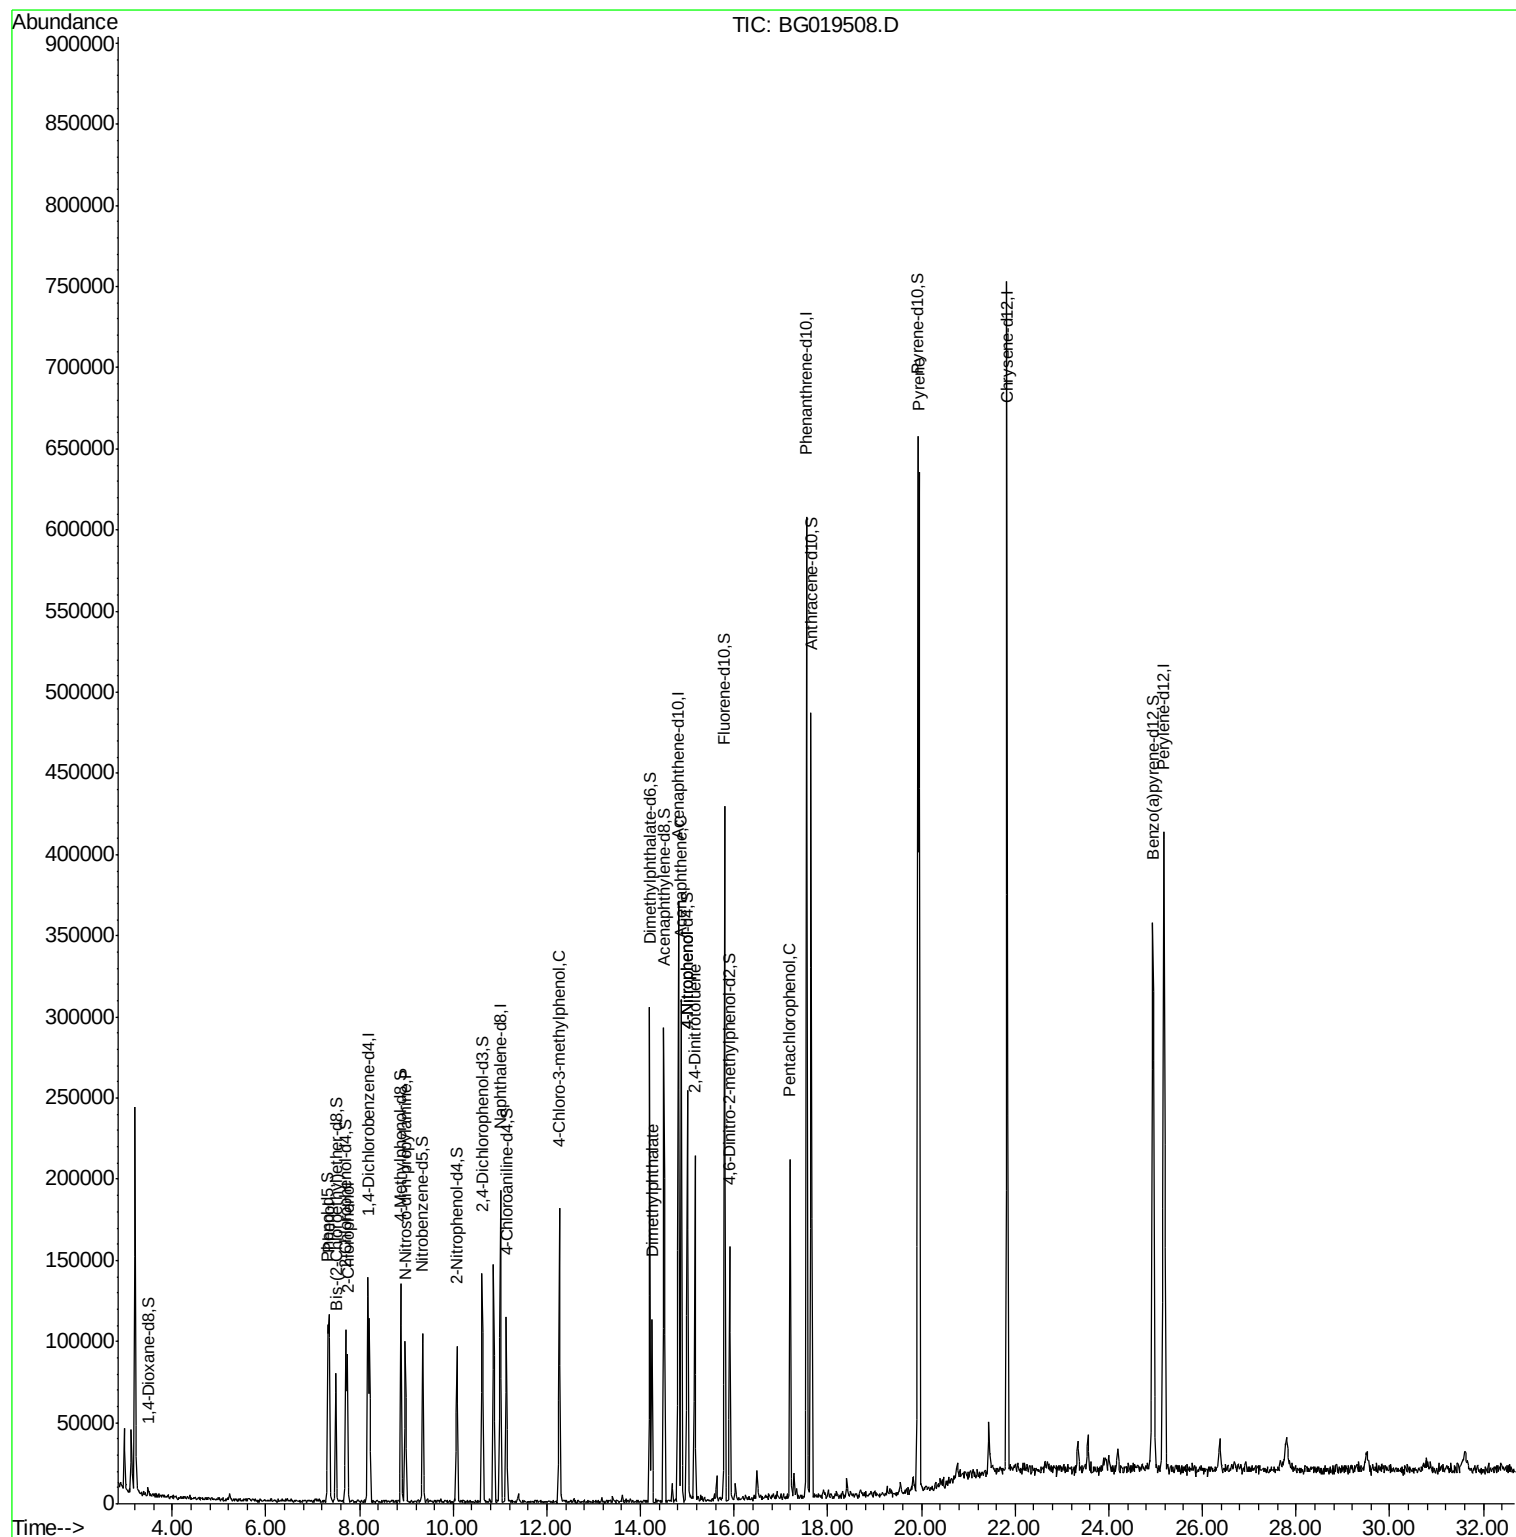

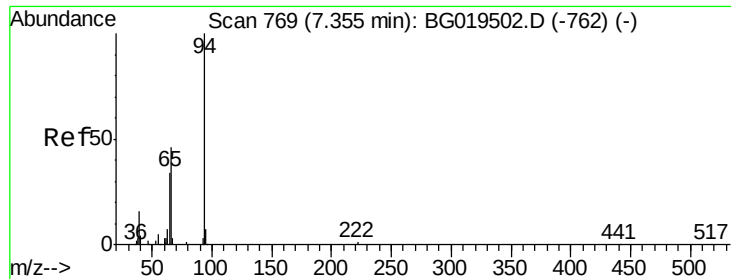

#6

Phenol

Concen: 18.34 ng/ul

RT: 7.35 min Scan# 768

Delta R.T. -0.00 min

Lab File: BG019508.D

Acq: 6 Nov 2015 12:26

Instrument :

BNA_G

ClientSampleId :

H2TR1MSD





Tot Ion: 94 Resp: 60604

Ion Ratio Lower Upper

94 100

65 37.0 29.3 43.9

66 57.1 45.0 67.6

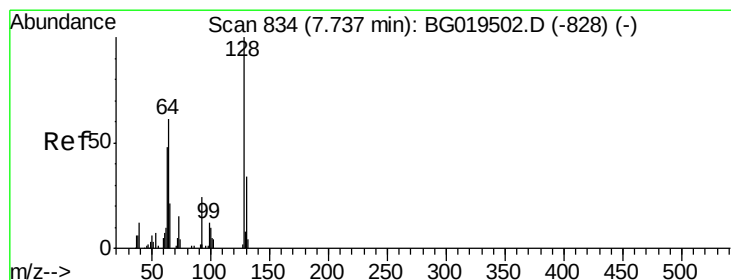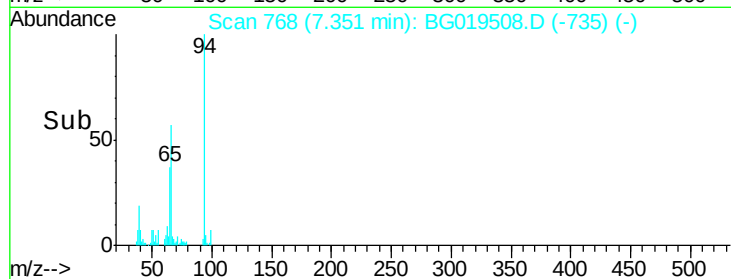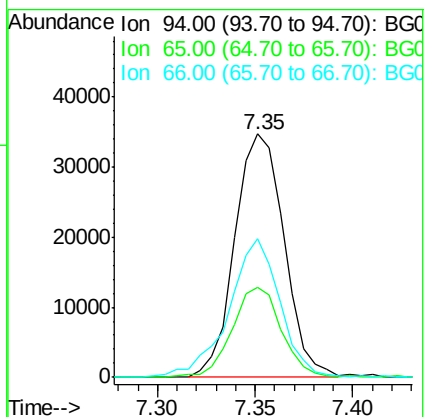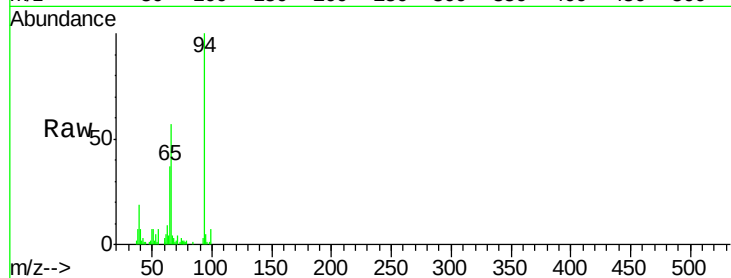

#10

2-Chlorophenol

Concen: 16.47 ng/ul

RT: 7.74 min Scan# 834

Delta R.T. 0.00 min

Lab File: BG019508.D

Acq: 6 Nov 2015 12:26




Tgt Ion:128 Resp: 32828


Ion Ratio Lower Upper

128 100

64 69.1 53.2 79.8

130 33.0 25.9 38.9

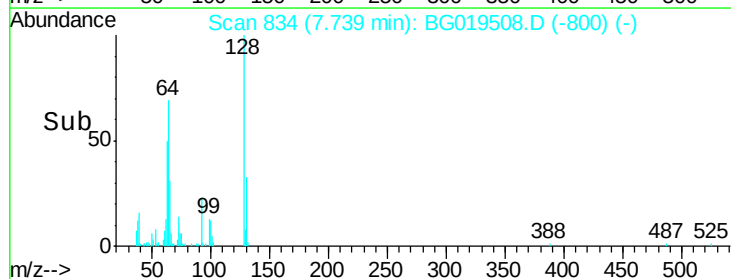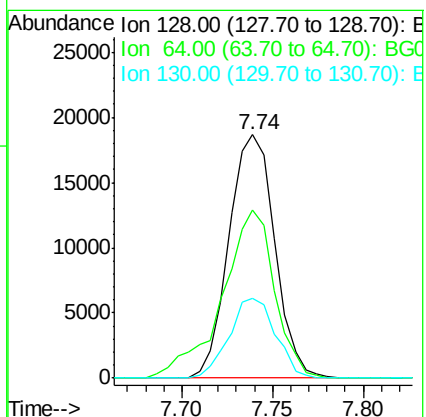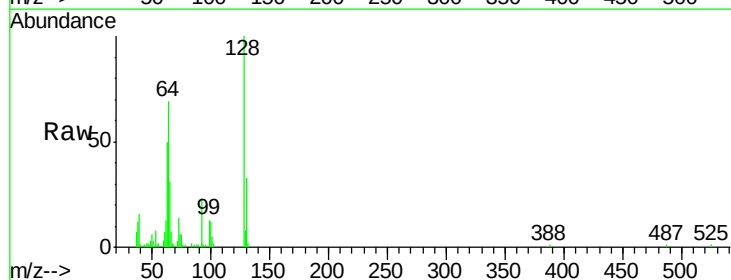

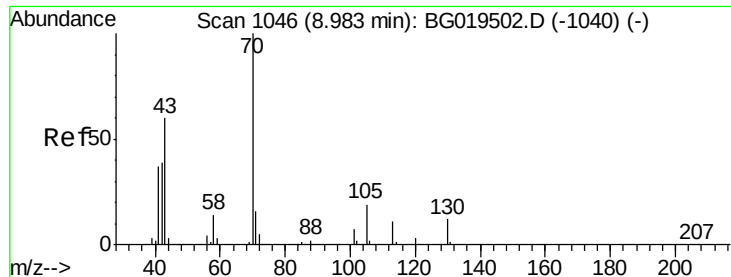

#15

N-Nitroso-di-n-propylamine

Concen: 17.04 ng/ul

RT: 8.98 min Scan# 1046

Delta R.T. 0.00 min

Lab File: BG019508.D

Acq: 6 Nov 2015 12:26

Instrument :

BNA_G

ClientSampleId :

H2TR1MSD

Tot Ion: 70 Resp: 46321


Ion Ratio Lower Upper

70 100

42 34.8 36.6 55.0#

101 8.7 5.8 8.8

130 14.8 14.6 22.0



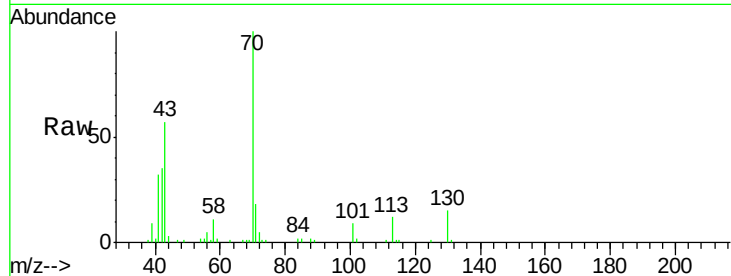


Abundance Ion 70.00 (69.70 to 70.70): BG019508.D (-1012) (-)

Ion 42.00 (41.70 to 42.70): BG019508.D (-1012) (-)

Ion 101.00 (100.70 to 101.70): BG019508.D (-1012) (-)

Ion 130.00 (129.70 to 130.70): BG019508.D (-1012) (-)

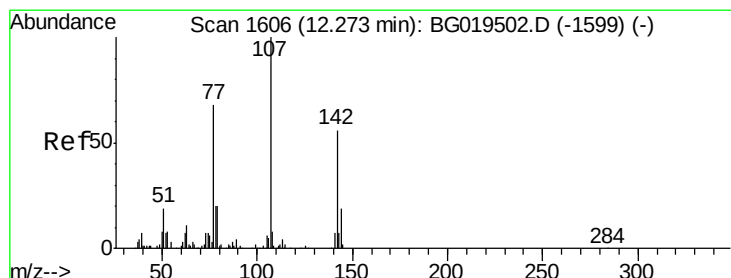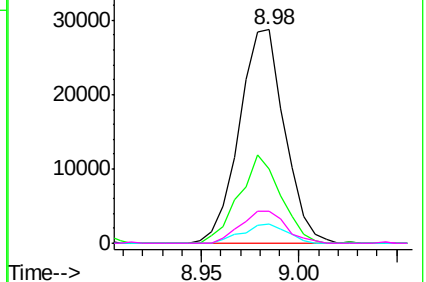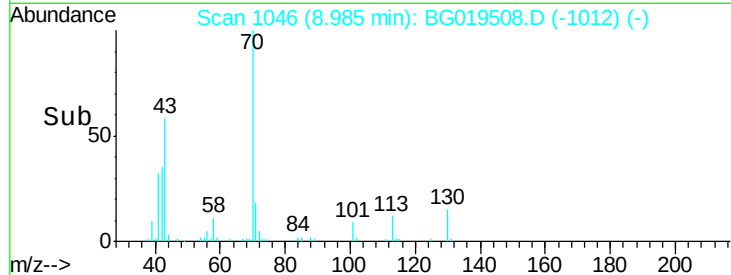

#33

4-Chloro-3-methylphenol

Concen: 18.01 ng/ul

RT: 12.27 min Scan# 1605

Delta R.T. -0.00 min

Lab File: BG019508.D

Acq: 6 Nov 2015 12:26


Tgt Ion: 107 Resp: 63359

Ion Ratio Lower Upper

107 100

144 19.6 13.0 19.6#



142 63.9 47.0 70.6

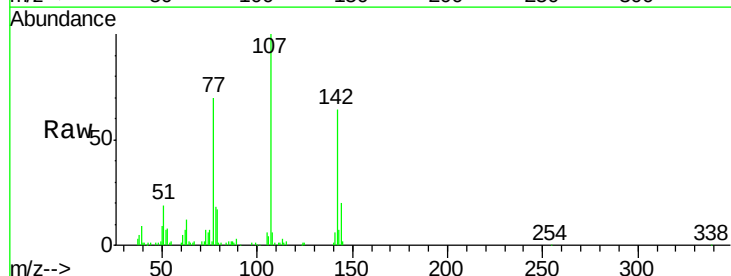


Abundance Ion 107.00 (106.70 to 107.70): BG019508.D (-1572) (-)

Ion 144.00 (143.70 to 144.70): BG019508.D (-1572) (-)

Ion 142.00 (141.70 to 142.70): BG019508.D (-1572) (-)



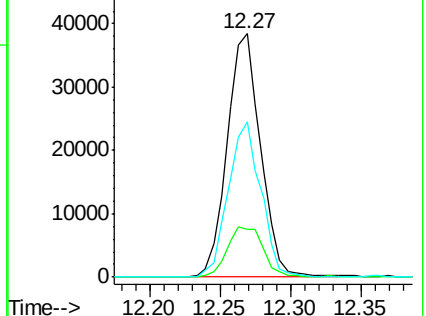
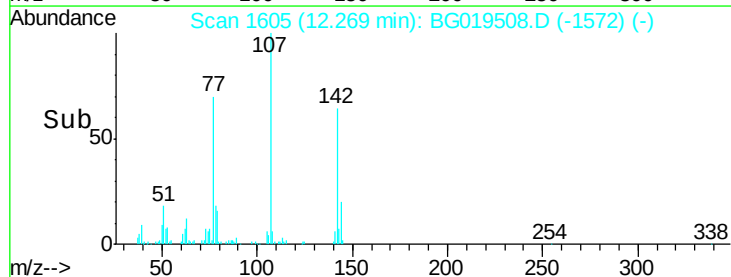


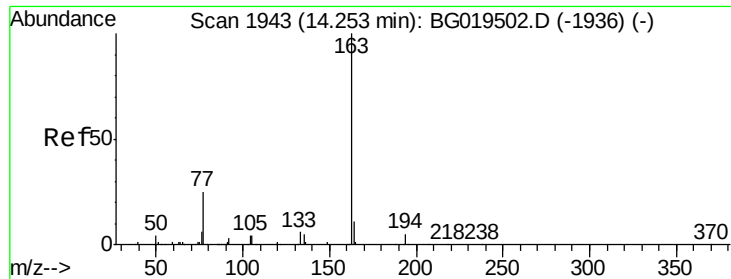

#45
Dimethylphthalate
Concen: 6.47 ng/ul
RT: 14.25 min Scan# 1942
Delta R.T. -0.00 min
Lab File: BG019508.D
Acq: 6 Nov 2015 12:26




Instrument :
BNA_G
ClientSampleId :
H2TR1MSD


Tot Ion	163	Resp	66184
Ion Ratio	100	Lower	Upper
194	4.2	4.3	6.5#
164	11.2	7.5	11.3

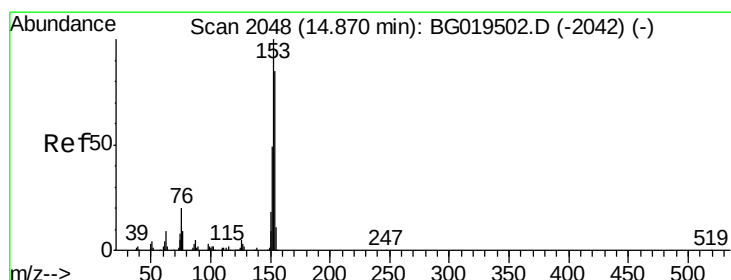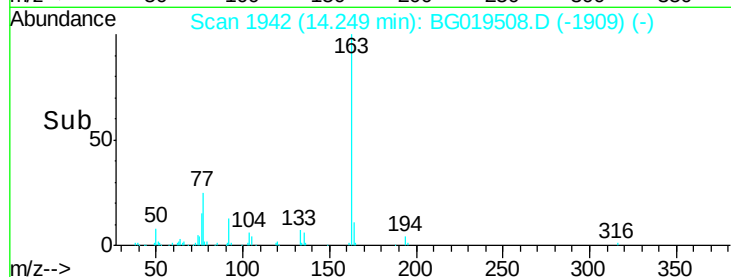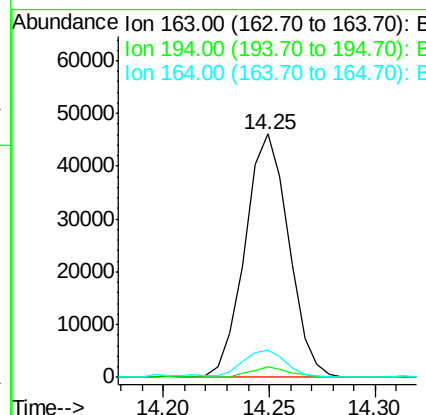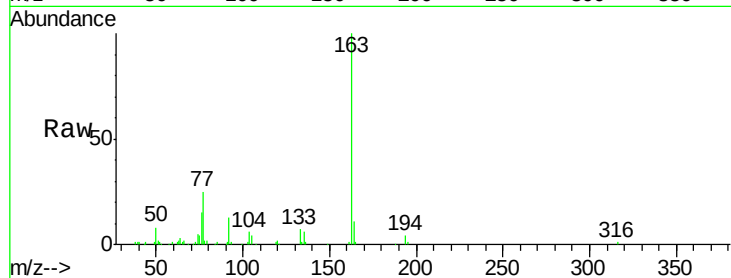

#50
Acenaphthene
Concen: 15.86 ng/ul
RT: 14.87 min Scan# 2048
Delta R.T. 0.00 min
Lab File: BG019508.D
Acq: 6 Nov 2015 12:26

Tgt Ion	153	Resp	121486
Ion Ratio	100	Lower	Upper
152	49.4	38.8	58.2
154	90.3	71.5	107.3


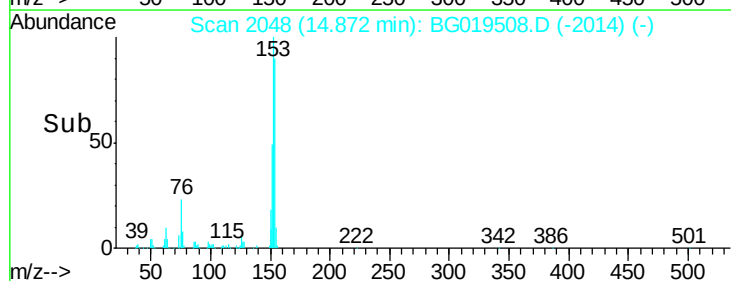
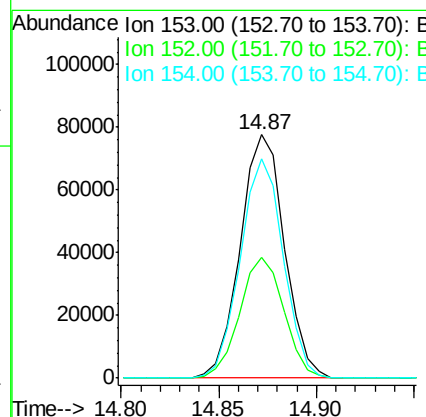
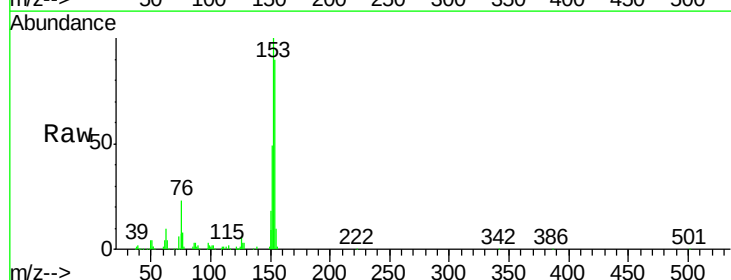


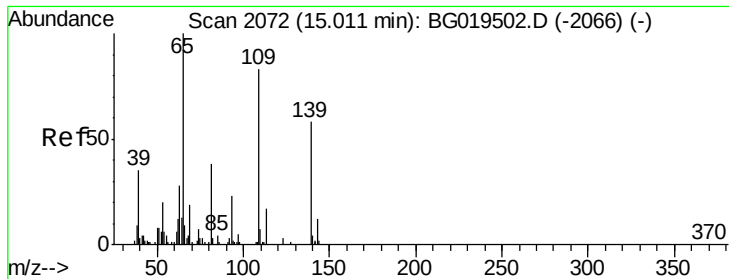

#53
4-Nitrophenol
Concen: 16.05 ng/ul
RT: 15.01 min Scan# 2071
Delta R.T. -0.00 min
Lab File: BG019508.D
Acq: 6 Nov 2015 12:26




Instrument :
BNA_G
ClientSampleId :
H2TR1MSD


Tot Ion	Ratio	Lower	Upper
109	100		
139	72.5	41.5	62.3#
65	114.6	73.7	110.5#

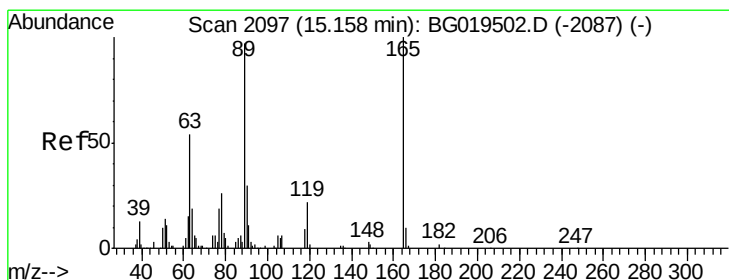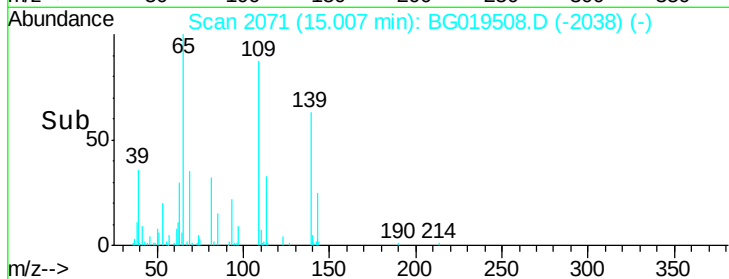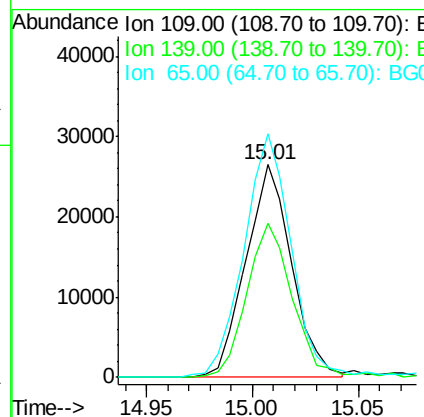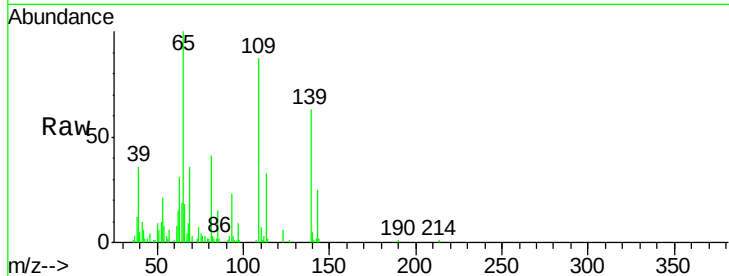

#55
2,4-Dinitrotoluene
Concen: 16.14 ng/ul
RT: 15.16 min Scan# 2097
Delta R.T. 0.00 min
Lab File: BG019508.D
Acq: 6 Nov 2015 12:26

Tgt Ion	Ratio	Lower	Upper
165	100		
63	55.0	51.1	76.7
182	3.1	3.3	4.9#


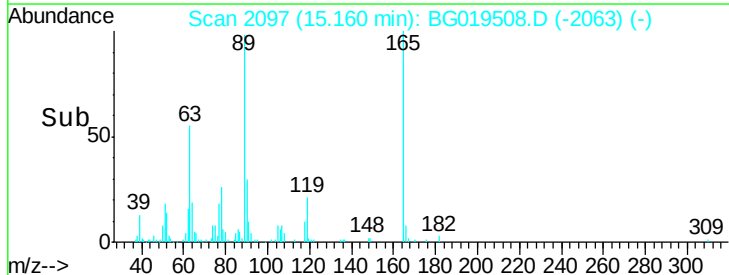
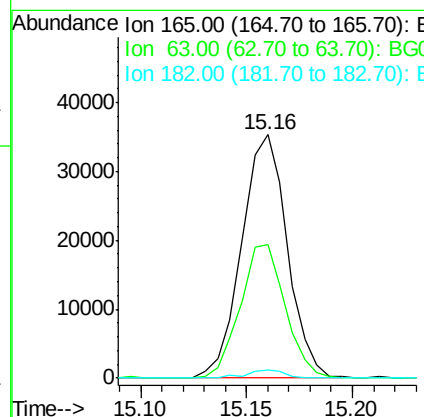
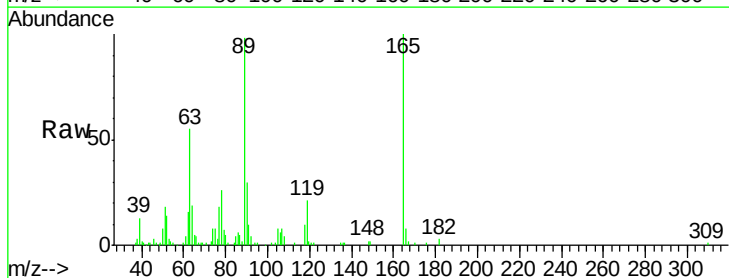


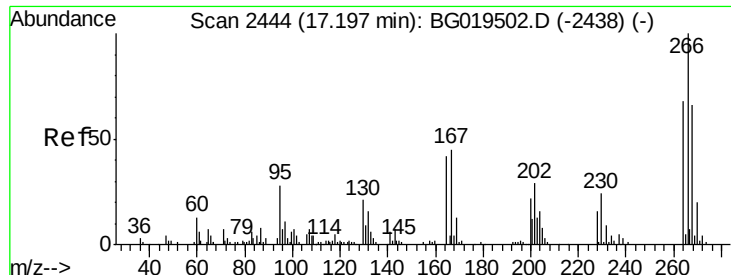

#69
Pentachlorophenol
 Concen: 14.32 ng/ul
 RT: 17.20 min Scan# 2444
 Delta R.T. 0.00 min
 Lab File: BG019508.D
 Acq: 6 Nov 2015 12:26

Instrument :
 BNA_G
 ClientSampleId :
 H2TR1MSD

Tot Ion	Ratio	Lower	Upper
266	100		
264	54.5	49.5	74.3
268	59.4	48.7	73.1

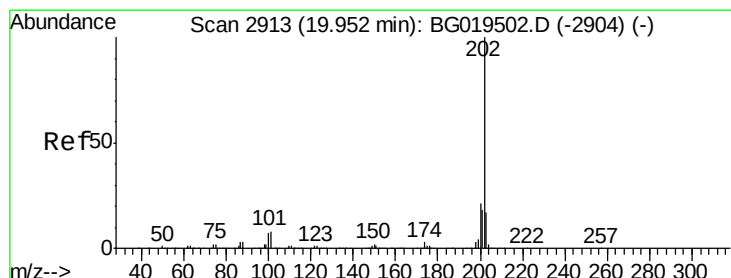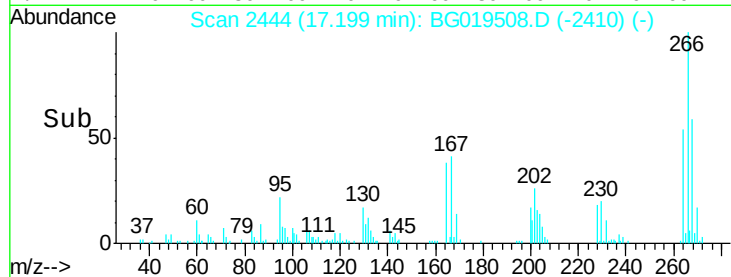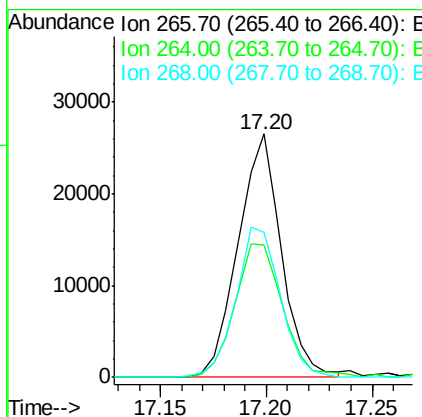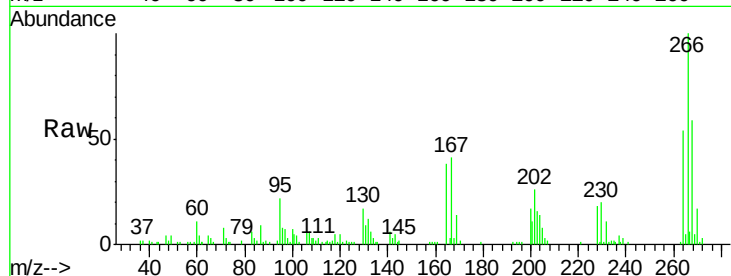

#80
Pyrene
 Concen: 15.95 ng/ul
 RT: 19.95 min Scan# 2913
 Delta R.T. 0.00 min
 Lab File: BG019508.D
 Acq: 6 Nov 2015 12:26

Tgt Ion	Ratio	Lower	Upper
202	100		
101	7.9	4.3	6.5#
100	7.0	3.6	5.4#

