

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110617\
 Data File : BG030782.D
 Acq On : 6 Nov 2017 19:34
 Operator : SJ/JU
 Sample : PB103846BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 07 06:57:18 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 07 06:56:14 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	52543	20.00	ng/ul	0.00
18) Naphthalene-d8	10.97	136	245975	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.77	164	165903	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	407997	20.00	ng/ul	0.00
75) Chrysene-d12	21.78	240	428733	20.00	ng/ul	0.00
83) Perylene-d12	25.09	264	430028	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	10666	8.25	ng/uL	0.00
5) Phenol-d5	7.32	99	186153	36.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	111391	35.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	154406	43.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	161152	39.57	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	78374	44.38	ng/ul	0.00
22) 2-Nitrophenol-d4	10.04	143	95758	52.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	166446	40.37	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	232753	48.59	ng/ul	0.00
43) Dimethylphthalate-d6	14.17	166	552155	38.93	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	694241	40.25	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	90105	34.41	ng/ul	0.00
57) Fluorene-d10	15.76	176	513752	44.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.88	200	48499	24.35	ng/ul	0.00
70) Anthracene-d10	17.61	188	815576	42.27	ng/ul	0.00
76) Pyrene-d10	19.88	212	915434	41.25	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.87	264	901466	44.26	ng/ul	0.00

Target Compounds


					Ovalue	
15) N-Nitroso-di-n-propylamine	8.86	70	3649	1.06	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110617\
Data File : BG030782.D
Acq On : 6 Nov 2017 19:34
Operator : SJ/JU
Sample : PB103846BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 07 06:57:18 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 07 06:56:14 2017
Response via : Initial Calibration

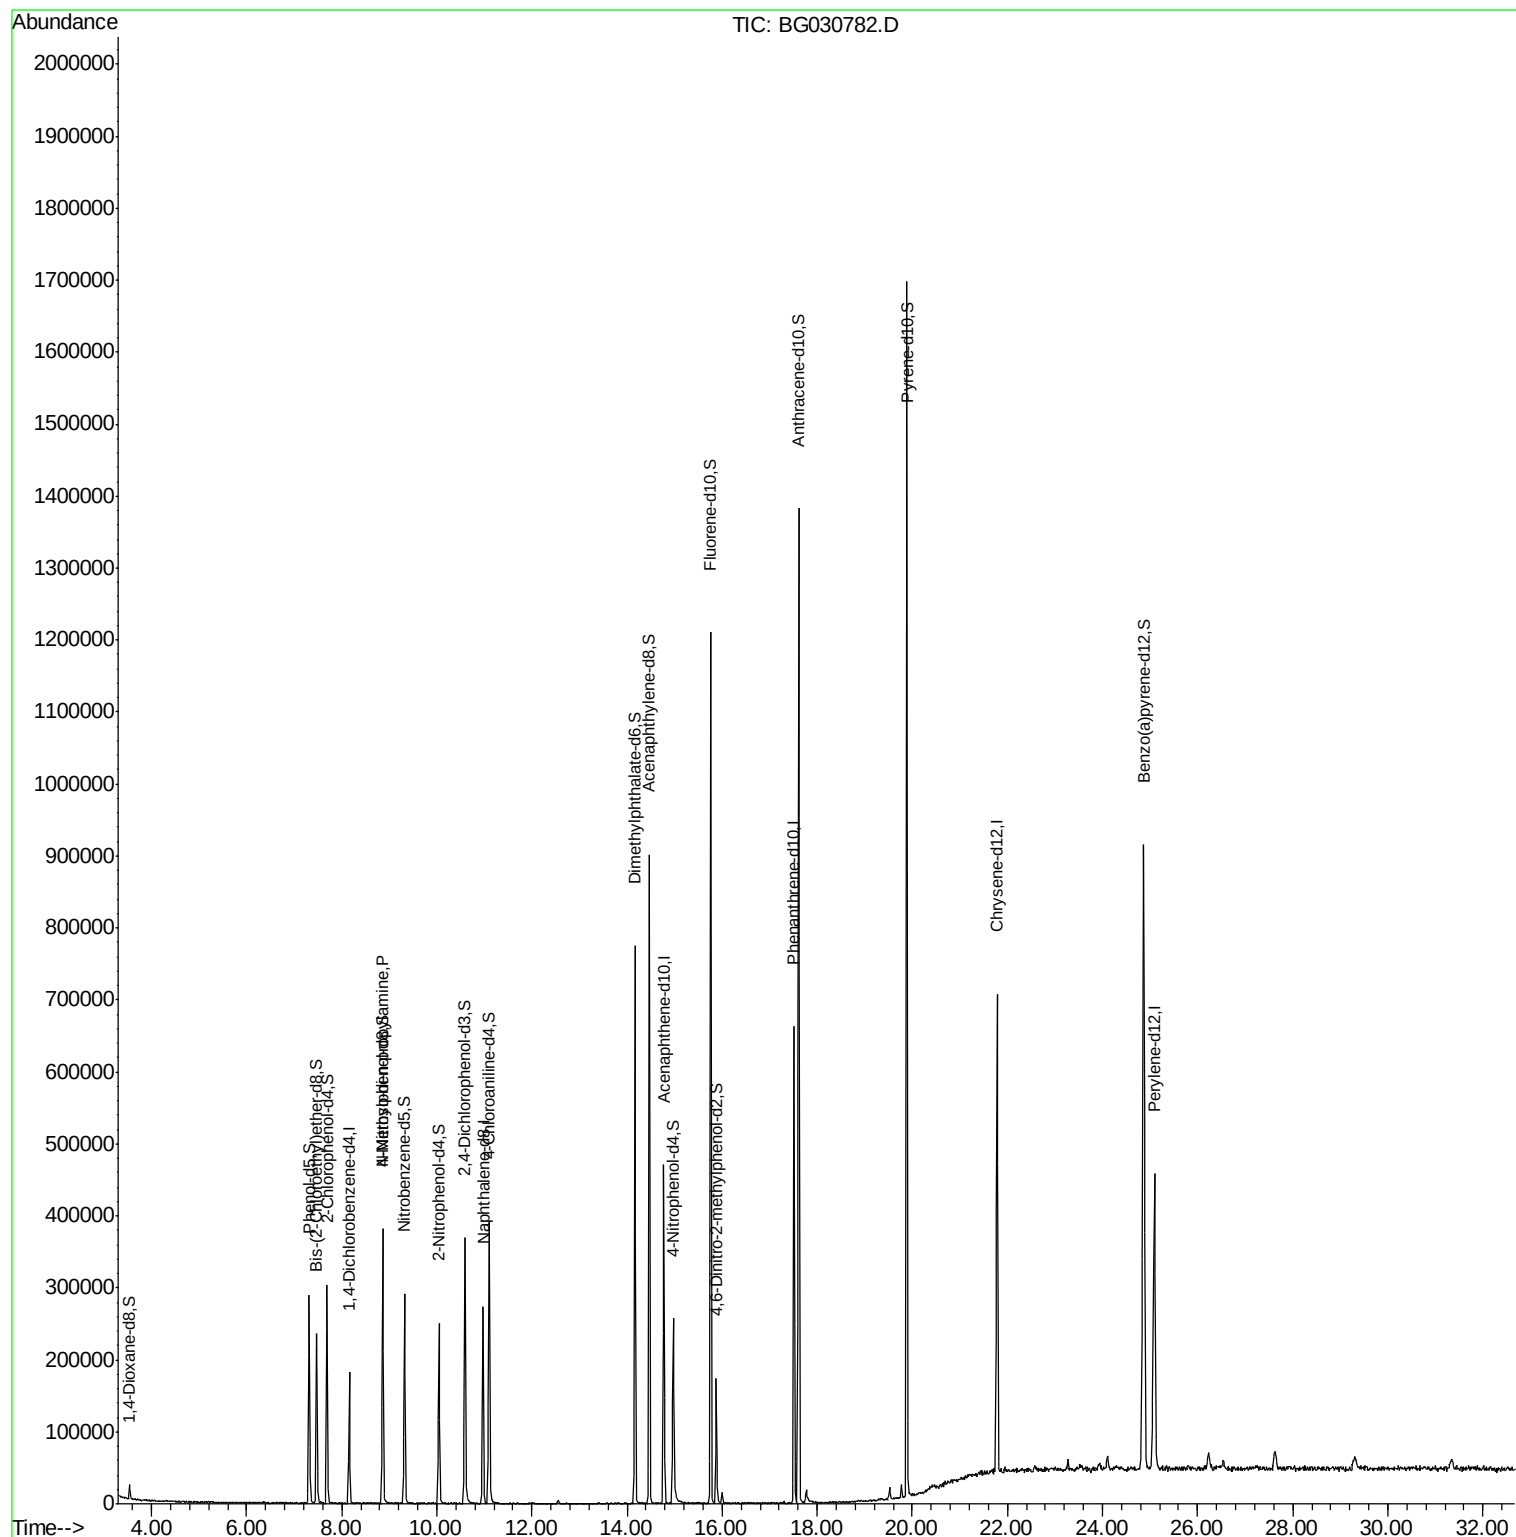

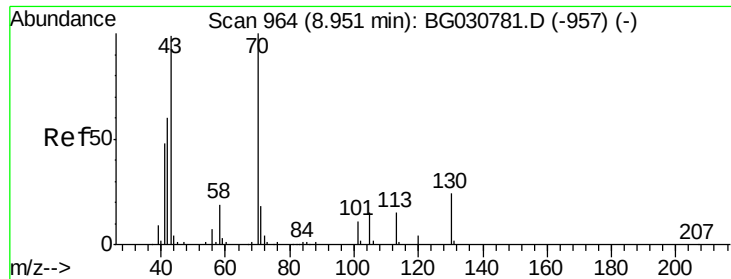

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.06 ng/ul
 RT: 8.86 min Scan# 948
 Delta R.T. -0.09 min
 Lab File: BG030782.D
 Acq: 6 Nov 2017 19:34

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion: 70 Resp: 3649
 Ion Ratio Lower Upper
 70 100
 42 322.8 51.7 77.5#
 101 0.0 7.6 11.4#
 130 0.0 14.6 22.0#

