

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110617\
 Data File : BG030786.D
 Acq On : 6 Nov 2017 22:04
 Operator : SJ/JU
 Sample : I6188-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B0EJ8

Quant Time: Nov 07 06:58:10 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 07 06:56:14 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	78037	20.00	ng/ul	0.00
18) Naphthalene-d8	10.97	136	368577	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.77	164	244215	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	608019	20.00	ng/ul	0.00
75) Chrysene-d12	21.78	240	651931	20.00	ng/ul	0.00
83) Perylene-d12	25.09	264	663755	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.54	96	9099	4.74	ng/uL	0.00
5) Phenol-d5	7.31	99	181495	24.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	108515	23.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	147299	27.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	149359	24.69	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	76319	28.84	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	89892	33.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	160329	25.95	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	207576	28.92	ng/ul	0.00
43) Dimethylphthalate-d6	14.17	166	542359	25.98	ng/ul	0.00
46) Acenaphthylene-d8	14.46	160	686958	27.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	94388	24.49	ng/ul	0.00
57) Fluorene-d10	15.76	176	510935	29.88	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.88	200	49480	16.67	ng/ul	0.00
70) Anthracene-d10	17.61	188	829198	28.84	ng/ul	0.00
76) Pyrene-d10	19.88	212	948797	28.12	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.86	264	961268	30.58	ng/ul	0.00
Target Compounds						
6) Phenol	7.34	94	16003	2.065	ng/ul#	89
44) Dimethylphthalate	14.21	163	30621	1.504	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110617\
Data File : BG030786.D
Acq On : 6 Nov 2017 22:04
Operator : SJ/JU
Sample : I6188-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B0EJ8

Quant Time: Nov 07 06:58:10 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 07 06:56:14 2017
Response via : Initial Calibration

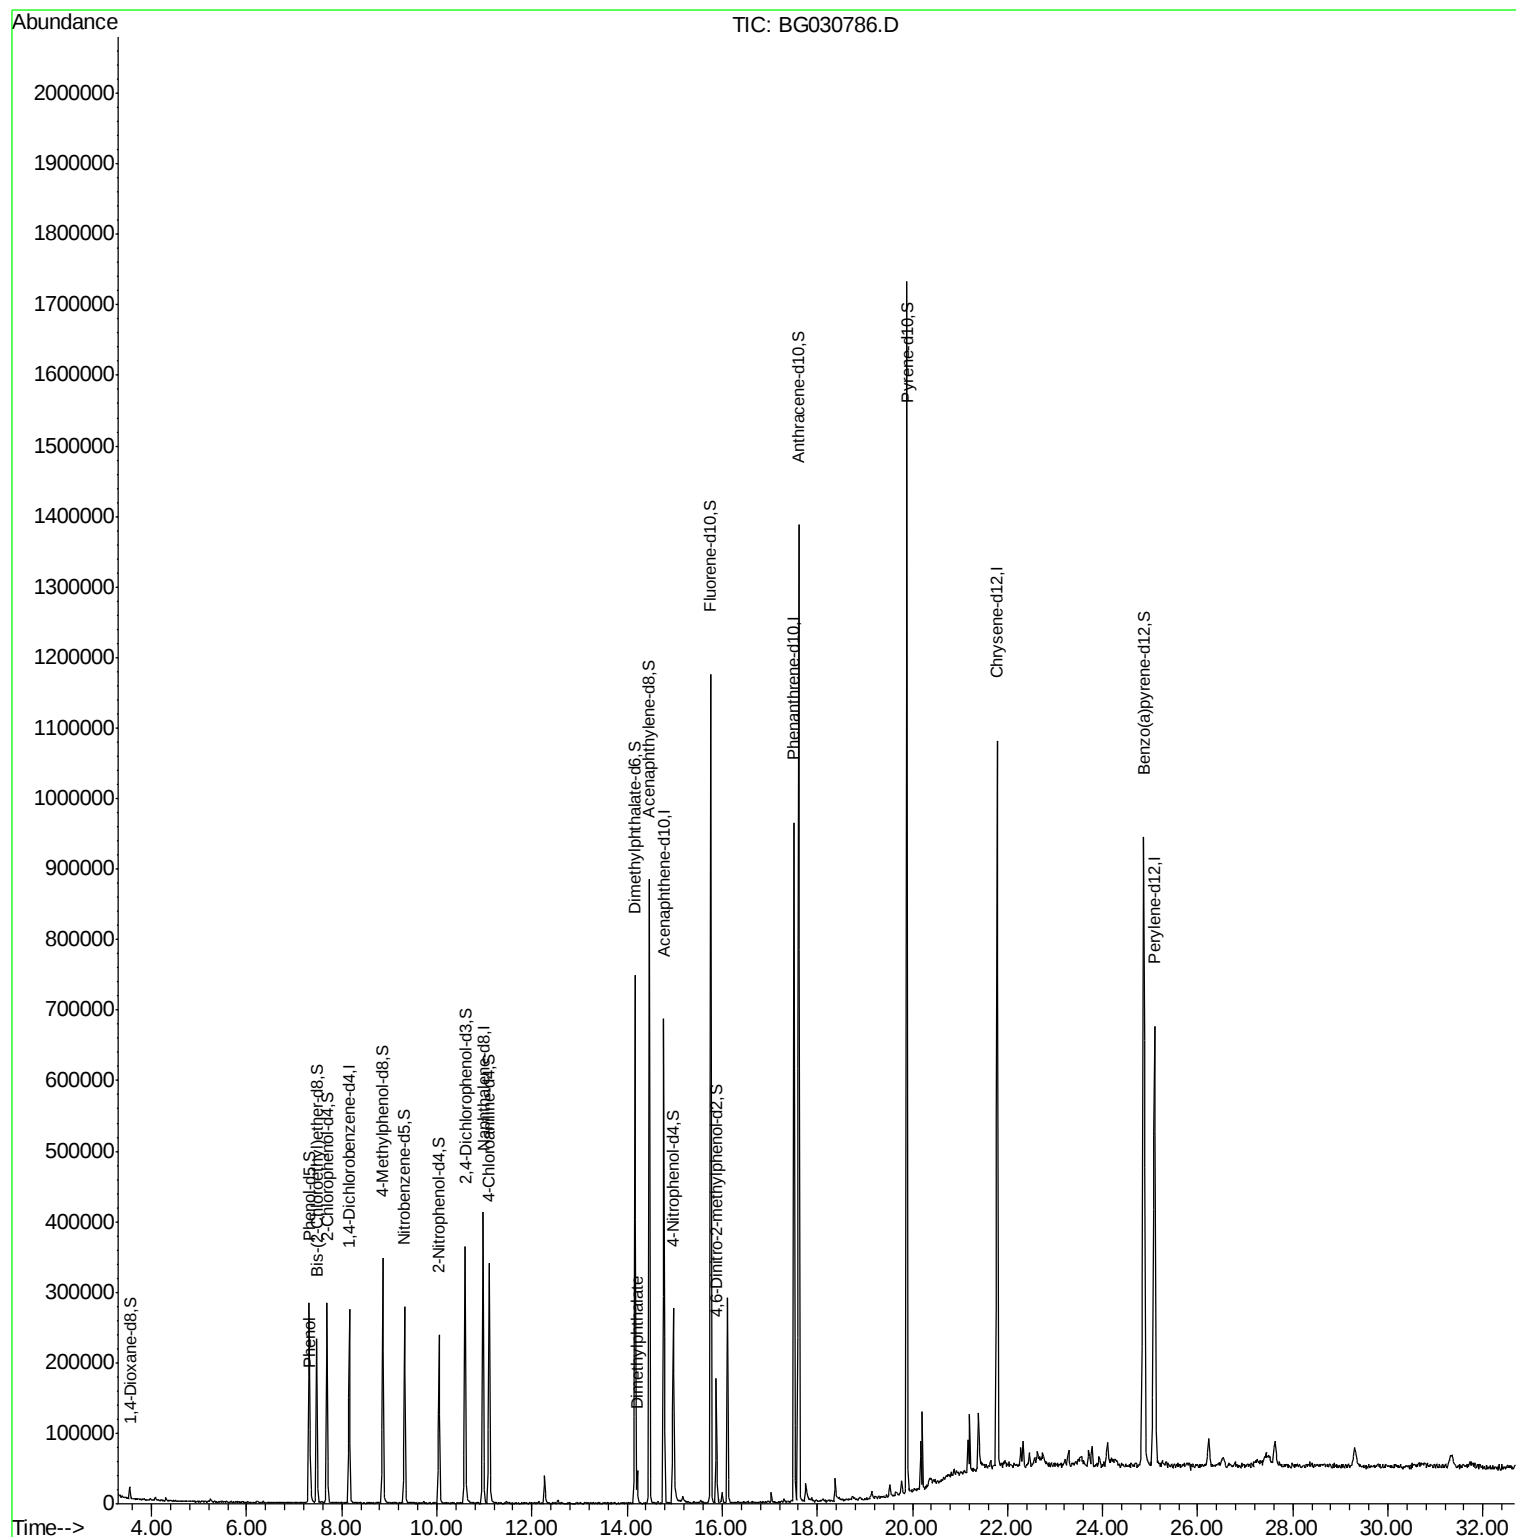

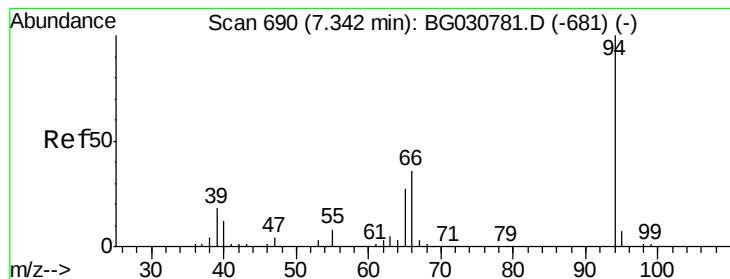





#6

Phenol

Concen: 2.065 ng/ul
 RT: 7.34 min Scan# 689
 Delta R.T. -0.00 min
 Lab File: BG030786.D
 Acq: 6 Nov 2017 22:04

Instrument :
 BNA_G
 ClientSampleId :
 B0EJ8

Tgt Ion: 94 Resp: 16003
 Ion Ratio Lower Upper
 94 100
 65 23.7 27.1 40.7#
 66 40.0 34.6 52.0

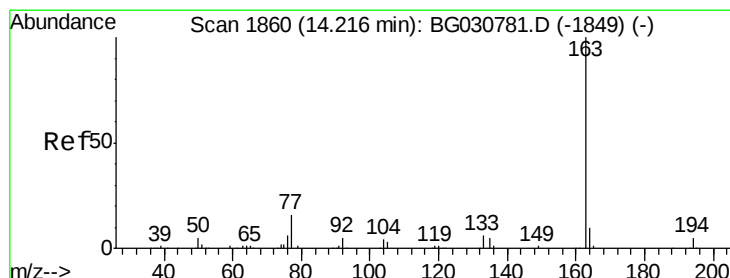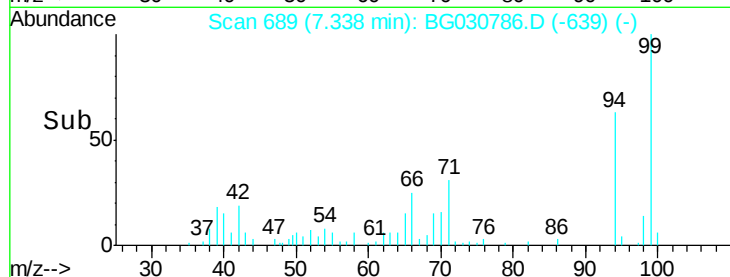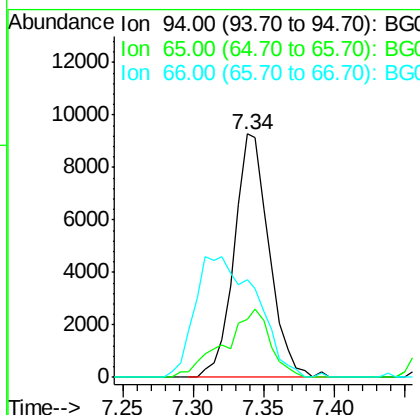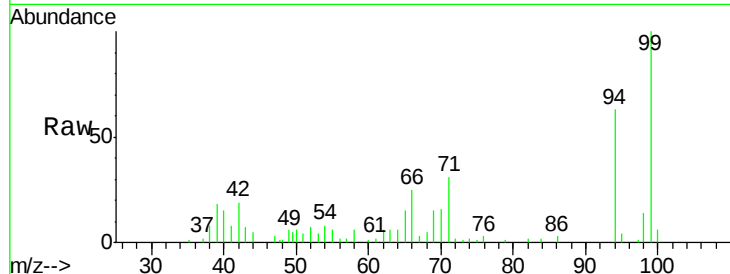

#44

Dimethylphthalate

Concen: 1.504 ng/ul
 RT: 14.21 min Scan# 1859
 Delta R.T. -0.00 min
 Lab File: BG030786.D
 Acq: 6 Nov 2017 22:04

Tgt Ion: 163 Resp: 30621
 Ion Ratio Lower Upper
 163 100
 194 5.3 3.5 5.3
 164 11.2 7.6 11.4

