

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110617\
 Data File : BG030791.D
 Acq On : 7 Nov 2017 1:12
 Operator : SJ/JU
 Sample : I6188-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B0ELO

Quant Time: Nov 07 06:59:09 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 07 06:56:14 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	95090	20.00	ng/ul	0.00
18) Naphthalene-d8	10.97	136	455333	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.77	164	302942	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	730357	20.00	ng/ul	0.00
75) Chrysene-d12	21.78	240	761220	20.00	ng/ul	0.00
83) Perylene-d12	25.09	264	790099	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	10371	4.43	ng/uL	0.00
5) Phenol-d5	7.31	99	214360	23.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	126744	22.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	174179	27.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	185961	25.23	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	90233	27.60	ng/ul	0.00
22) 2-Nitrophenol-d4	10.04	143	111030	33.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	197418	25.87	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	254303	28.68	ng/ul	0.00
43) Dimethylphthalate-d6	14.17	166	680300	26.27	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	834304	26.49	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	114142	23.87	ng/ul	0.00
57) Fluorene-d10	15.76	176	622213	29.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.88	200	69080	19.38	ng/ul	0.00
70) Anthracene-d10	17.61	188	989507	28.65	ng/ul	0.00
76) Pyrene-d10	19.89	212	1113924	28.27	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.87	264	1126412	30.10	ng/ul	0.00

Target Compounds


					Qvalue	
6) Phenol	7.34	94	24018	2.543	ng/ul	91
44) Dimethylphthalate	14.22	163	32556	1.289	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110617\
Data File : BG030791.D
Acq On : 7 Nov 2017 1:12
Operator : SJ/JU
Sample : I6188-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B0EL0

Quant Time: Nov 07 06:59:09 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 07 06:56:14 2017
Response via : Initial Calibration

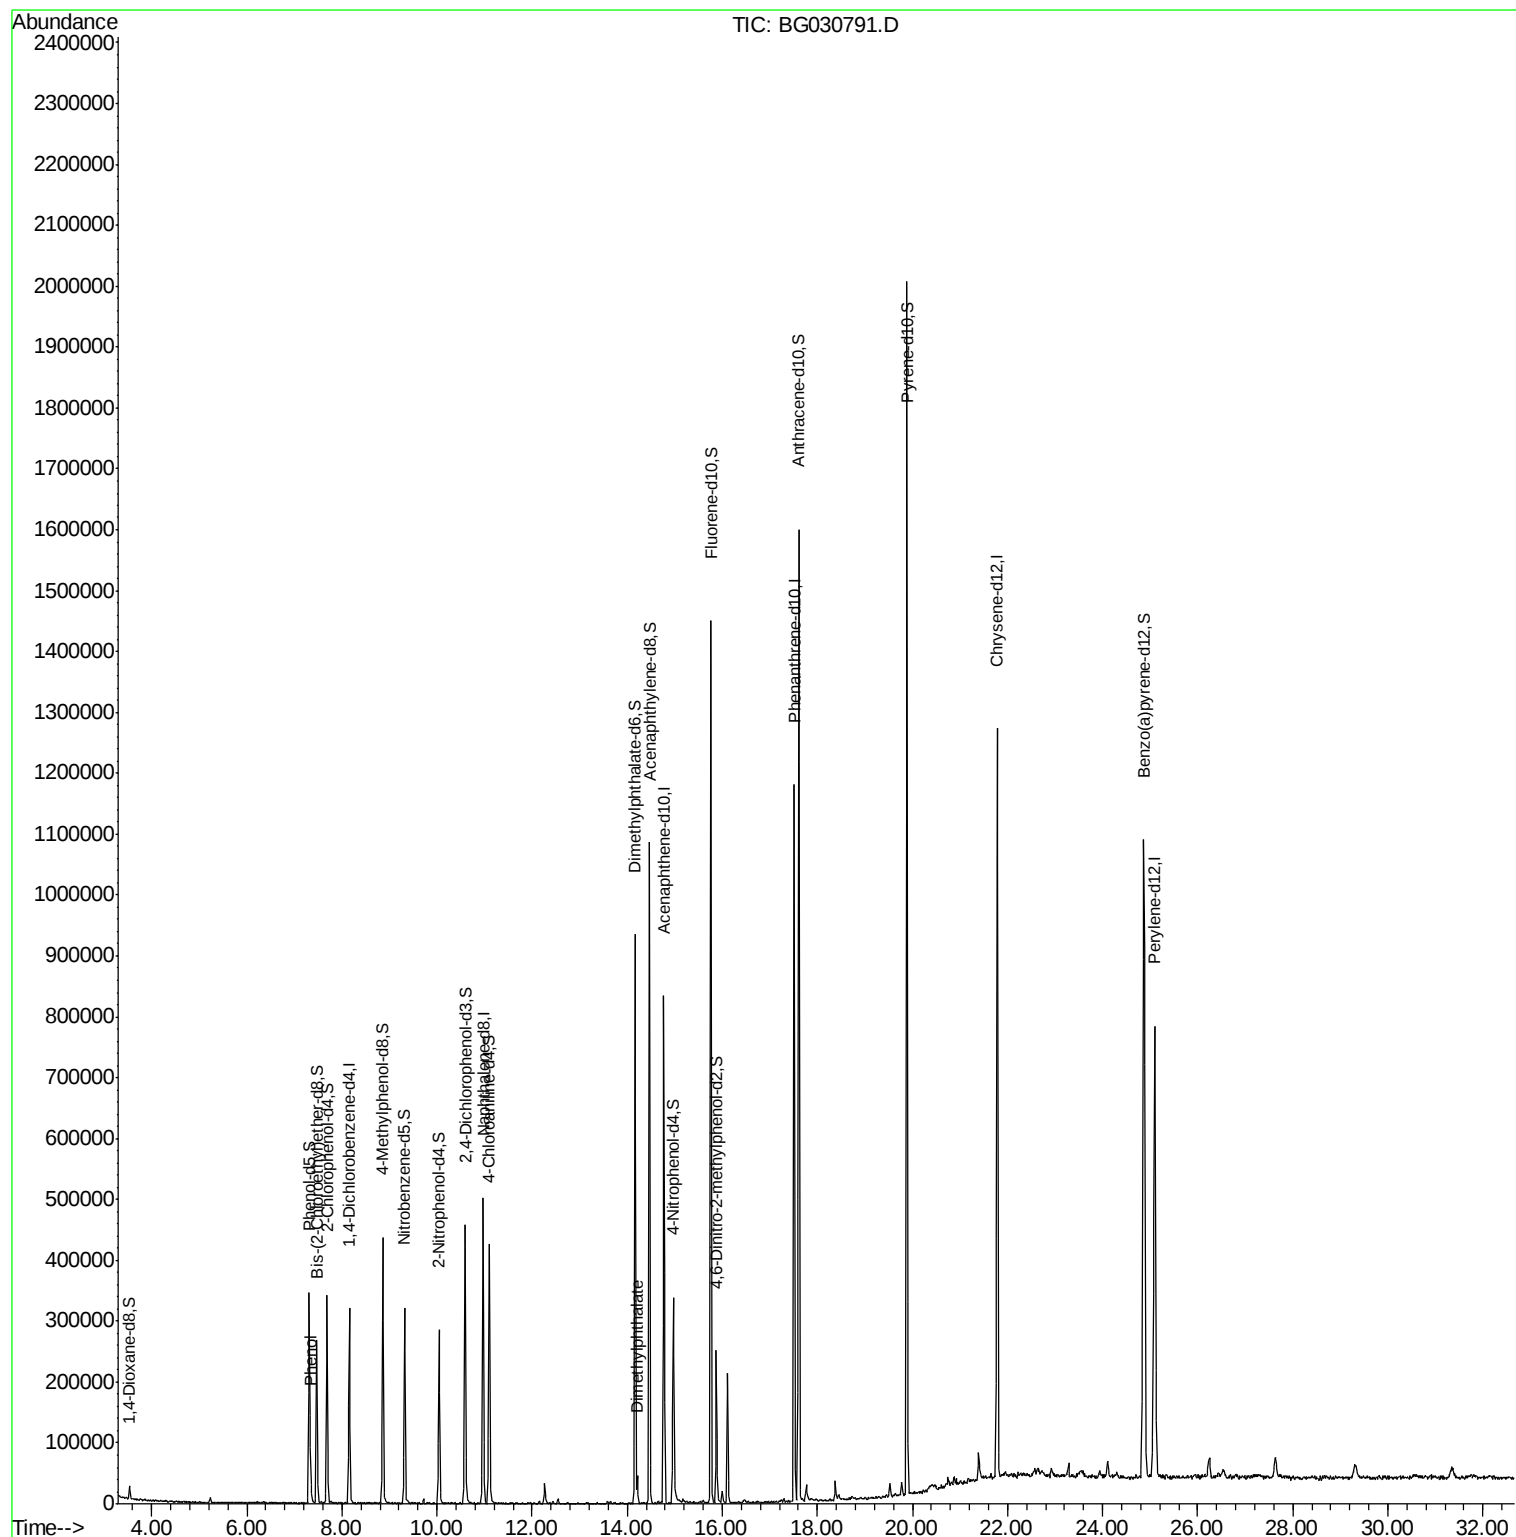

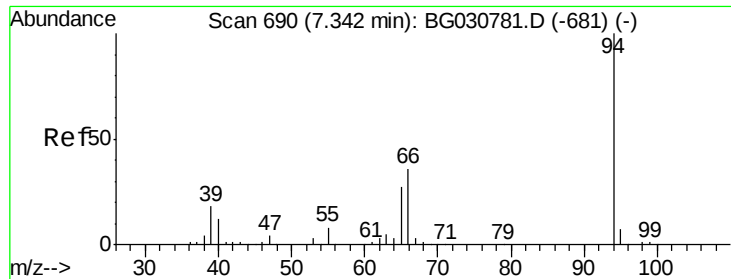

#6

Phenol

Concen: 2.543 ng/ul

RT: 7.34 min Scan# 690

Delta R.T. 0.00 min

Lab File: BG030791.D

Acq: 7 Nov 2017 1:12

Instrument :

BNA_G

ClientSampleId :

B0ELO


Tgt Ion: 94 Resp: 24018

Ion Ratio Lower Upper




94 100

65 27.2 27.1 40.7

66 38.6 34.6 52.0

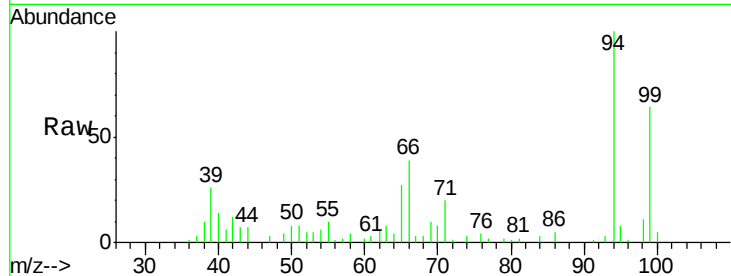

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

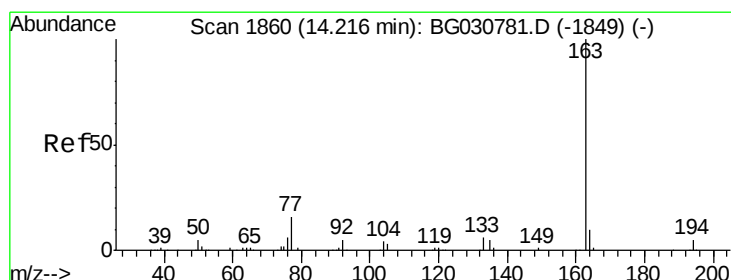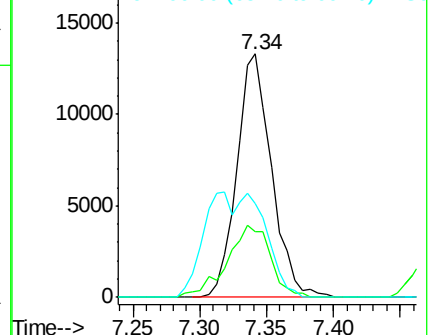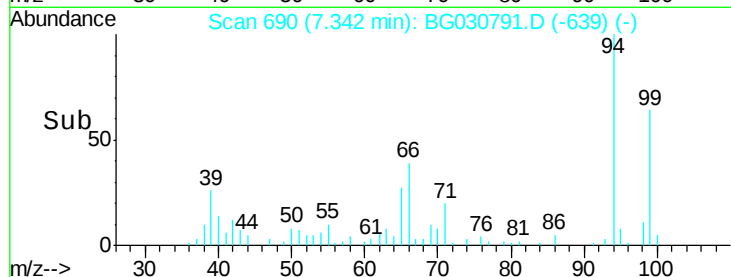

#44

Dimethylphthalate

Concen: 1.289 ng/ul

RT: 14.22 min Scan# 1860

Delta R.T. 0.00 min

Lab File: BG030791.D

Acq: 7 Nov 2017 1:12


Tgt Ion: 163 Resp: 32556

Ion Ratio Lower Upper

163 100

194 3.3 3.5 5.3#

164 8.2 7.6 11.4

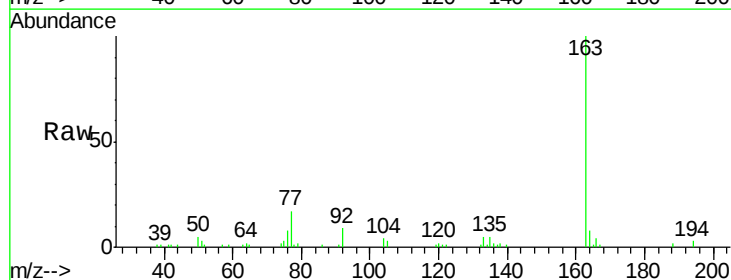

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

