




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063193.D
Acq On : 7 Nov 2024 8:11
Operator : RC/JU
Sample : PB164608BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK608

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/08/2024
Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 07 07:46:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

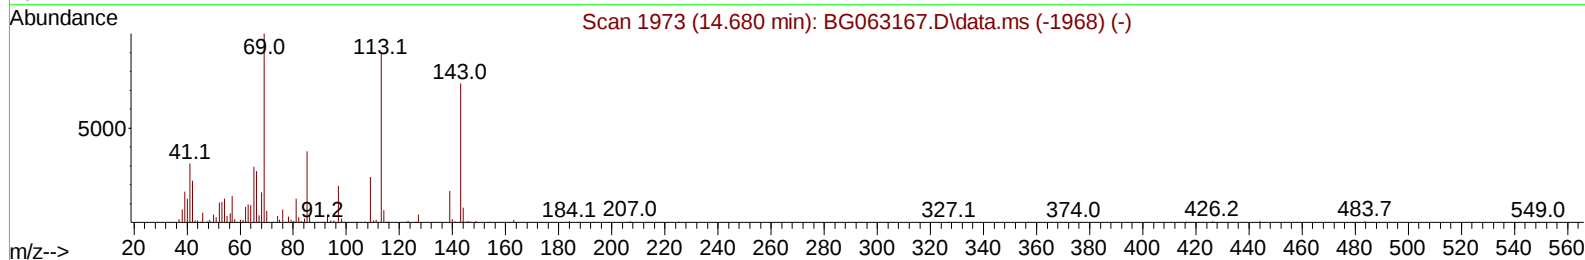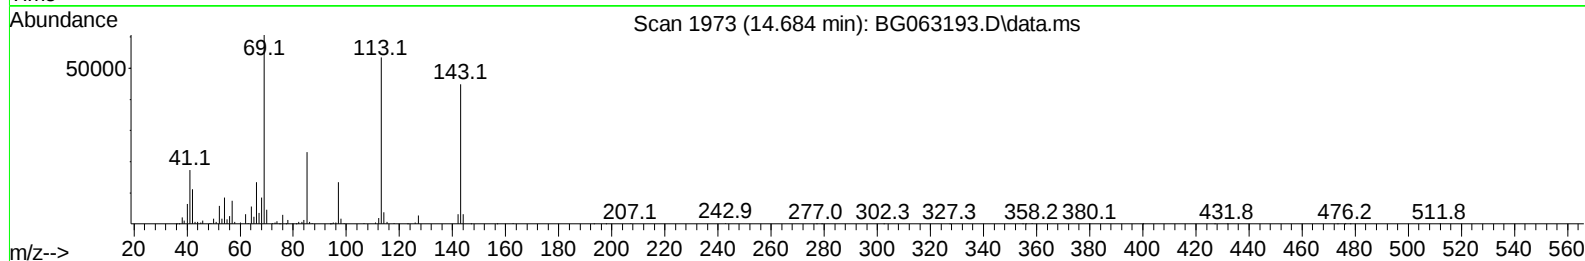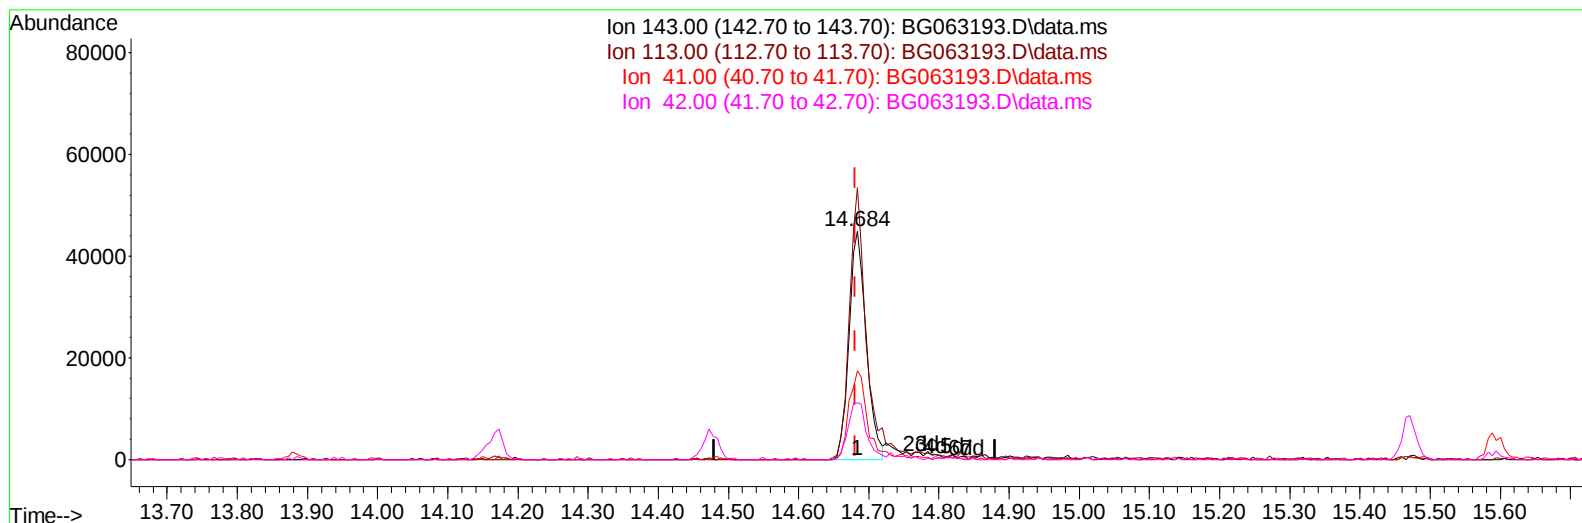

TIC: BG063193.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.684min (+ 0.004) 22.17 ng/u1

response 76849

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	123.00	118.96
41.00	42.60	38.86
42.00	30.90	24.83




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063193.D
Acq On : 7 Nov 2024 8:11
Operator : RC/JU
Sample : PB164608BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK608

Manual IntegrationsAPPROVED

Quant Time: Nov 07 07:46:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/08/2024
Supervised By :mohammad ahmed 11/11/2024

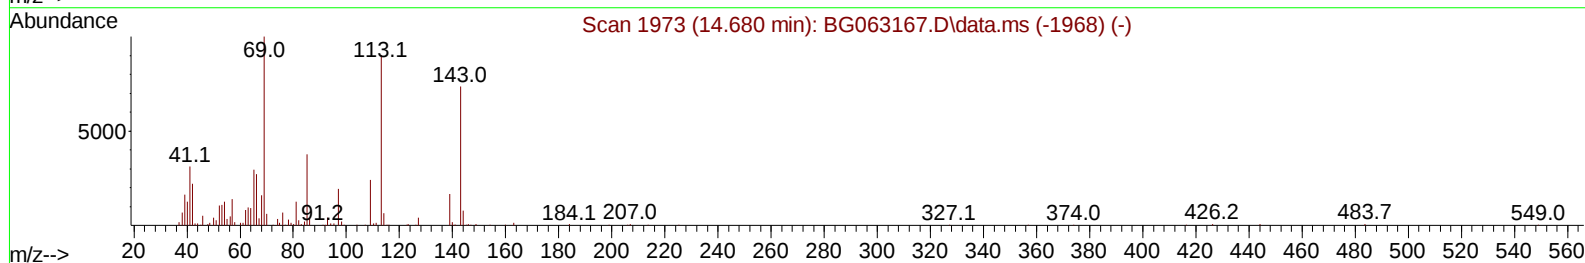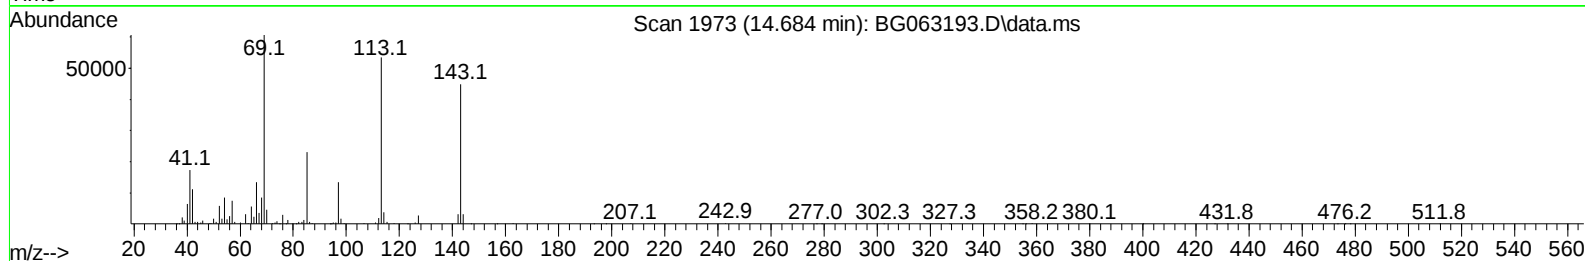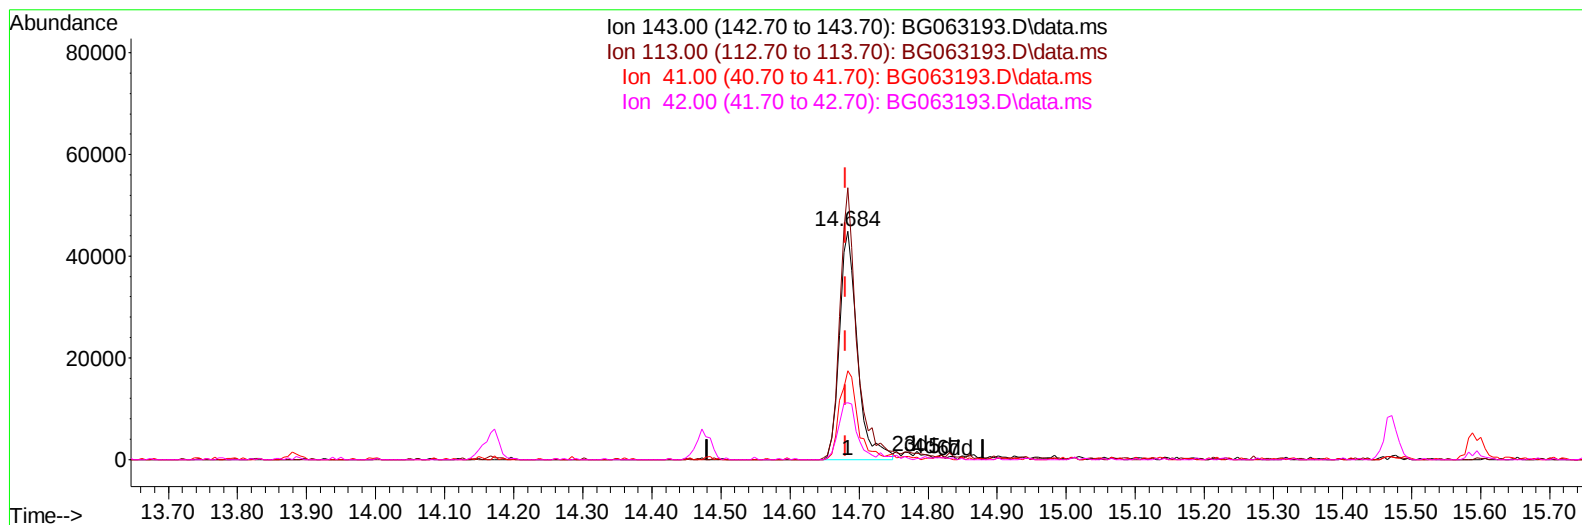

TIC: BG063193.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.684min (+ 0.004) 23.26 ng/ul m

response 80620

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	123.00	118.96
41.00	42.60	38.86
42.00	30.90	24.83

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063193.D
 Acq On : 7 Nov 2024 8:11
 Operator : RC/JU
 Sample : PB164608BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK608

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/08/2024
 Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 07 07:51:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.839	152	64544	20.000	ng/ul	0.00
20) Naphthalene-d8	10.630	136	321039	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.478	164	323181	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.228	188	818064	20.000	ng/ul	0.00
79) Chrysene-d12	21.476	240	877524	20.000	ng/ul	# 0.00
88) Perylene-d12	24.513	264	952142	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.303	96	6428	4.503	ng/uL	0.00
4) Pyridine-d5	3.708	84	111760	23.689	ng/ul	0.00
7) Phenol-d5	7.010	99	164393	28.226	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	92159	26.977	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	109596	28.992	ng/ul	0.00
15) 4-Methylphenol-d8	8.544	113	140984	28.560	ng/ul	0.00
21) Nitrobenzene-d5	8.990	128	58937	26.113	ng/ul	0.00
24) 2-Nitrophenol-d4	9.713	143	77630	26.612	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.254	165	160313	28.004	ng/ul	0.00
31) 4-Chloroaniline-d4	10.765	131	194404	26.072	ng/ul	0.00
46) Dimethylphthalate-d6	13.879	166	619761	24.482	ng/ul	0.00
49) Acenaphthylene-d8	14.167	160	670932	27.078	ng/ul	0.00
54) 4-Nitrophenol-d4	14.684	143	80620m	23.260	ng/ul	0.00
60) Fluorene-d10	15.471	176	569313	26.647	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.594	200	114754	22.320	ng/ul	0.00
73) Anthracene-d10	17.322	188	1008389	28.681	ng/ul	0.00
81) Pyrene-d10	19.625	212	1291284	29.350	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.302	264	1288511	28.029	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063193.D
Acq On : 7 Nov 2024 8:11
Operator : RC/JU
Sample : PB164608BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK608

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/08/2024
Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 07 07:51:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

