




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063197.D
Acq On : 7 Nov 2024 10:43
Operator : RC/JU
Sample : P4634-15DL 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CC0R4DL

Manual IntegrationsAPPROVED

Quant Time: Nov 07 11:11:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/08/2024
Supervised By :mohammad ahmed 11/11/2024

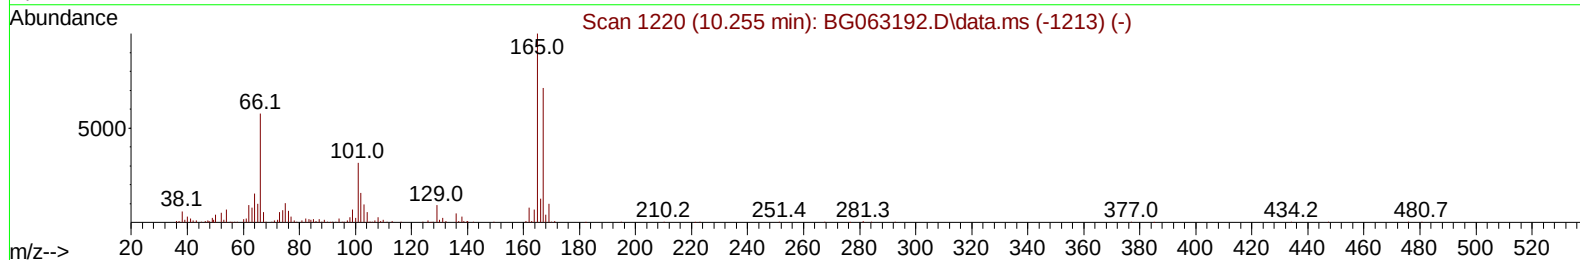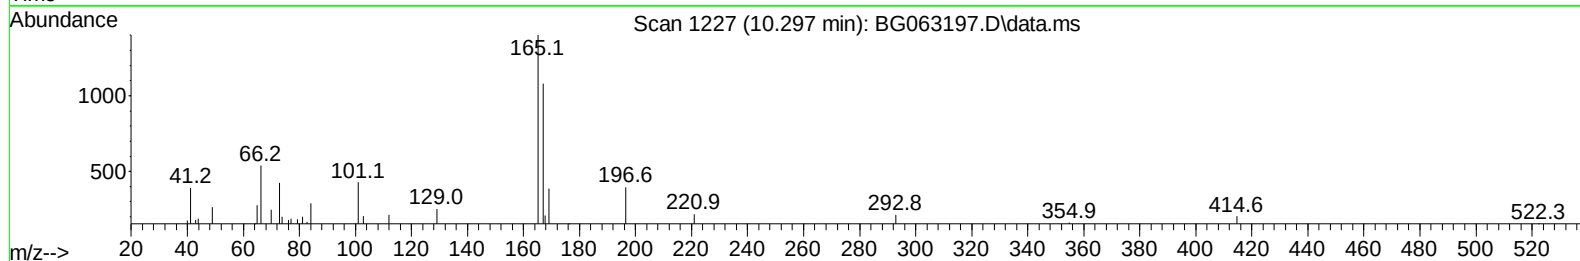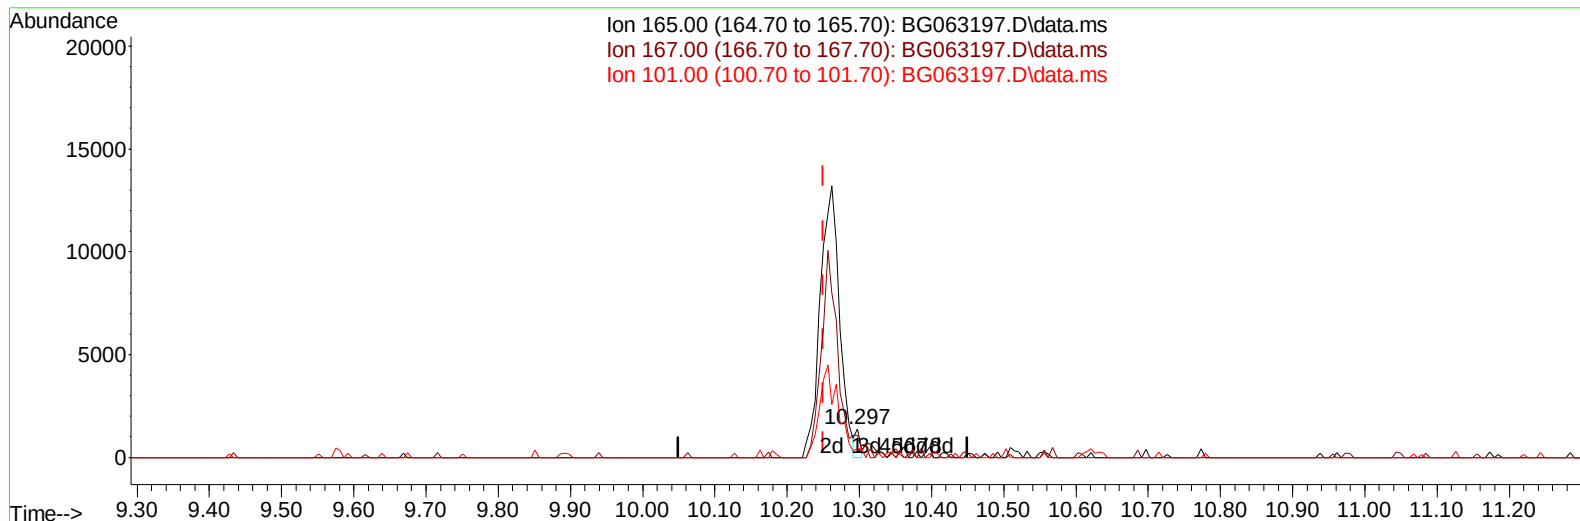

TIC: BG063197.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.297min (+ 0.047) 0.10 ng/ul

response 609

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.30	76.95
101.00	32.10	30.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063197.D
Acq On : 7 Nov 2024 10:43
Operator : RC/JU
Sample : P4634-15DL 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :

BNA_G




ClientSampleId :

CC0R4DL

Manual IntegrationsAPPROVED

Quant Time: Nov 07 11:11:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/08/2024
Supervised By :mohammad ahmed 11/11/2024

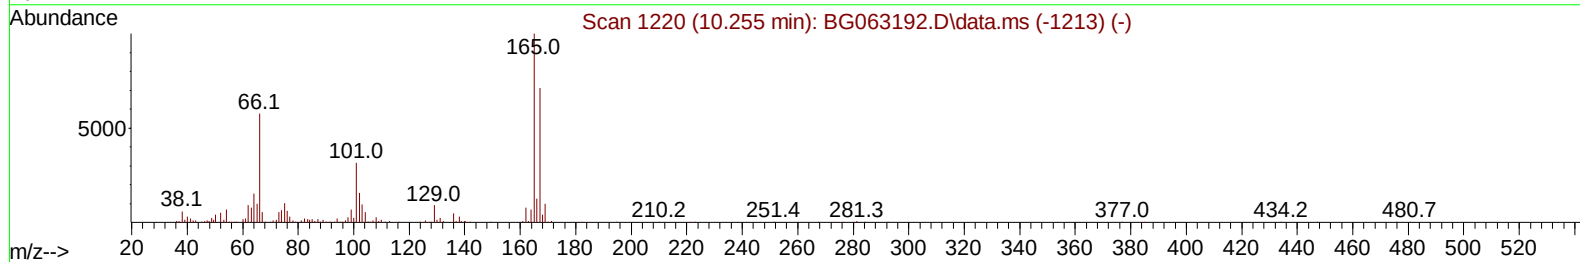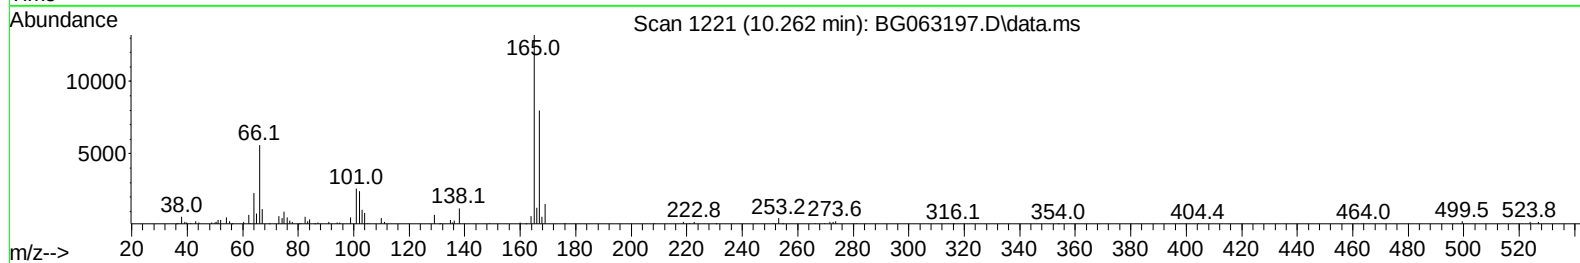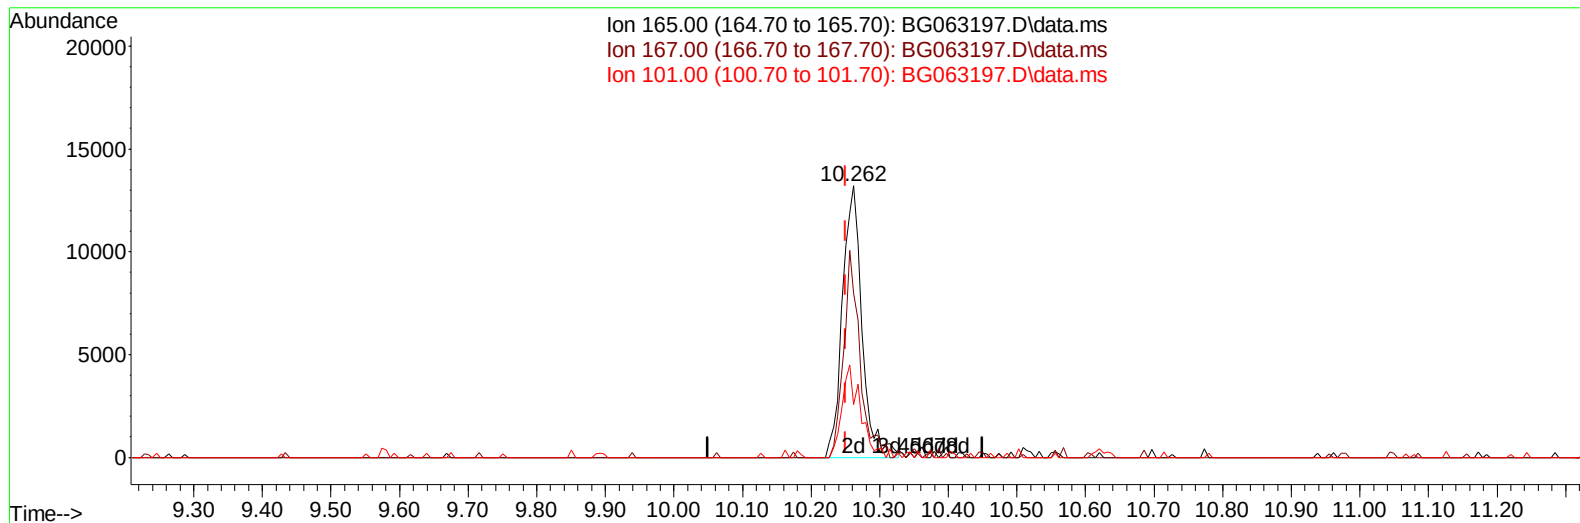

TIC: BG063197.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.262min (+ 0.012) 4.44 ng/ul m

response 26002

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.30	60.43
101.00	32.10	19.51#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063197.D
Acq On : 7 Nov 2024 10:43
Operator : RC/JU
Sample : P4634-15DL 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CC0R4DL

Manual IntegrationsAPPROVED

Quant Time: Nov 07 11:11:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/08/2024
Supervised By :mohammad ahmed 11/11/2024

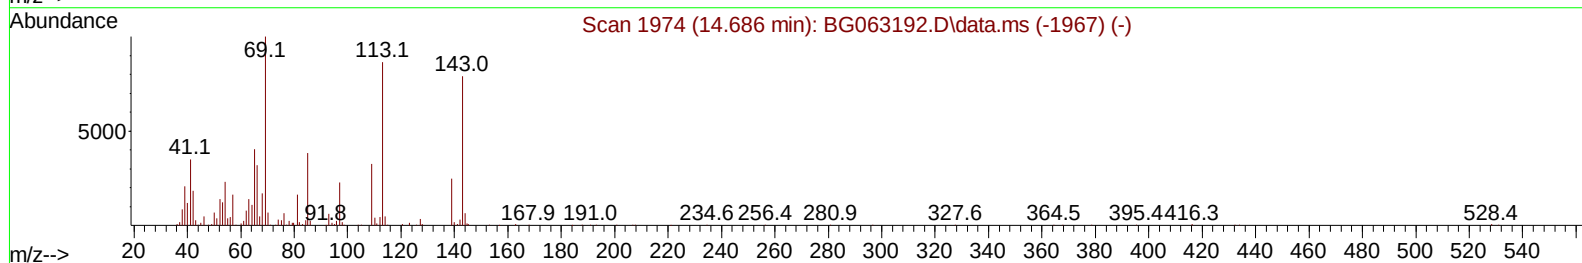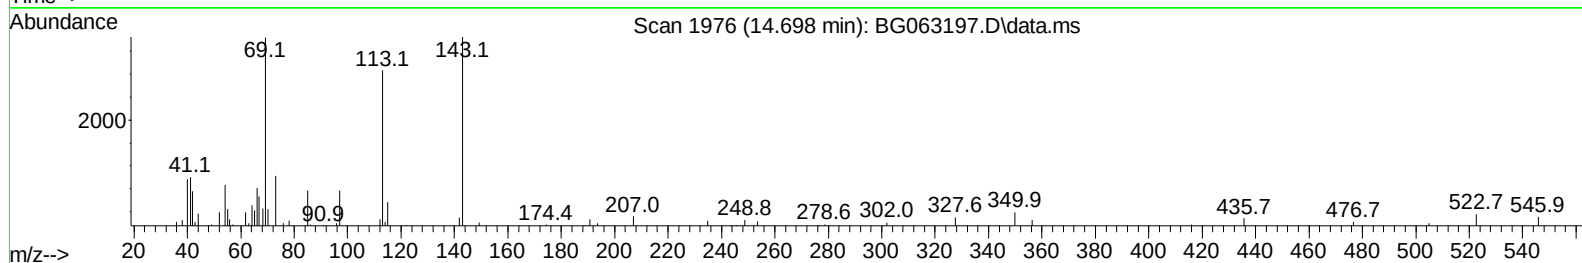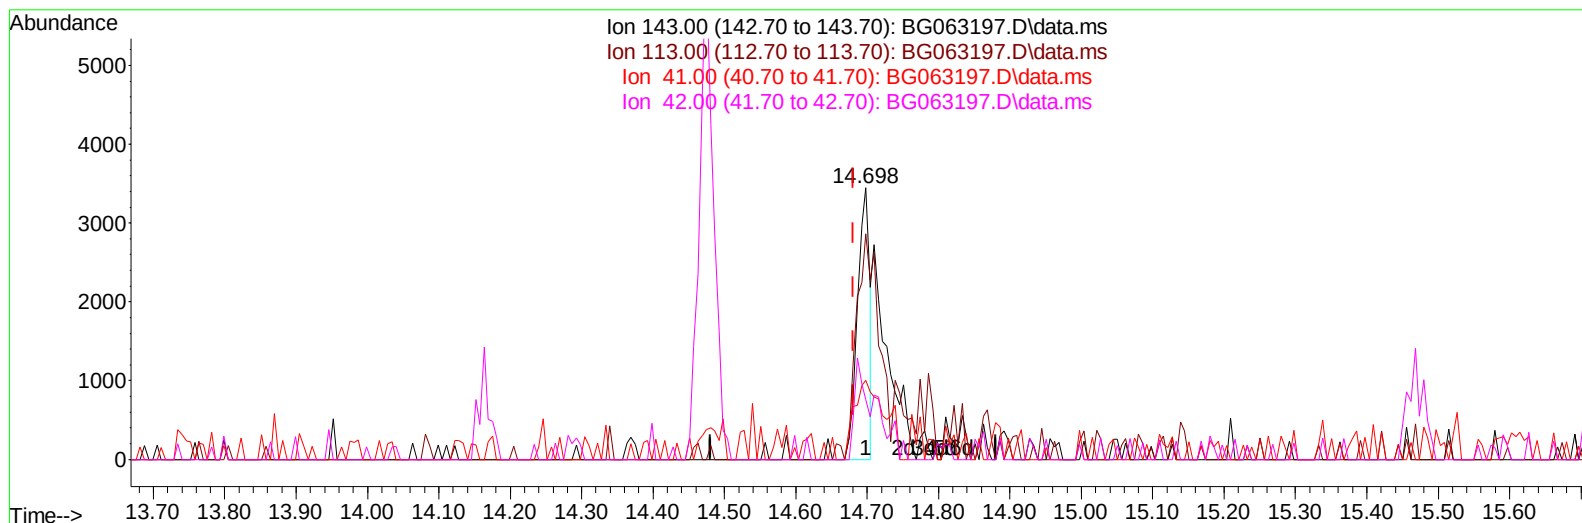

TIC: BG063197.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.698min (+ 0.018) 1.15 ng/ul

response 4081

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	123.00	83.11#
41.00	42.60	29.23#
42.00	30.90	22.06#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063197.D
 Acq On : 7 Nov 2024 10:43
 Operator : RC/JU
 Sample : P4634-15DL 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CC0R4DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/08/2024
 Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 07 11:12:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.841	152		69280	20.000	ng/ul	0.00
20) Naphthalene-d8	10.632	136		328761	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.475	164		330613	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.225	188		829951	20.000	ng/ul	0.00
79) Chrysene-d12	21.478	240		838353	20.000	ng/ul	0.00
88) Perylene-d12	24.510	264		923916	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.306	96		1114	0.727	ng/uL	0.00
4) Pyridine-d5	3.717	84		14210	2.806	ng/ul	0.00
7) Phenol-d5	7.013	99		25377	4.059	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.172	67		12455	3.397	ng/ul	0.00
11) 2-Chlorophenol-d4	7.371	132		17642	4.348	ng/ul	0.00
15) 4-Methylphenol-d8	8.552	113		21261	4.012	ng/ul	0.00
21) Nitrobenzene-d5	8.987	128		8673	3.752	ng/ul	0.00
24) 2-Nitrophenol-d4	9.716	143		11726	3.925	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.262	165		26002m	4.435	ng/ul	0.01
31) 4-Chloroaniline-d4	10.767	131		26266	3.440	ng/ul	0.00
46) Dimethylphthalate-d6	13.881	166		96598	3.730	ng/ul	0.00
49) Acenaphthylene-d8	14.169	160		109817	4.332	ng/ul	0.00
54) 4-Nitrophenol-d4	14.698	143		8261m	2.330	ng/ul	0.02
60) Fluorene-d10	15.474	176		94268	4.313	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.603	200		8034	1.540	ng/ul	0.00
73) Anthracene-d10	17.324	188		153623	4.307	ng/ul	0.00
81) Pyrene-d10	19.622	212		201761	4.800	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.304	264		191417	4.291	ng/ul	0.00
Target Compounds							
86) Bis(2-ethylhexyl)phtha...	21.378	149		1385197	67.569	ng/ul	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063197.D
Acq On : 7 Nov 2024 10:43
Operator : RC/JU
Sample : P4634-15DL 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CC0R4DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/08/2024
Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 07 11:12:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

