

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063178.D
 Acq On : 6 Nov 2024 22:03
 Operator : RC/JU
 Sample : P4634-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CC0Q1

Quant Time: Nov 06 22:16:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.837	152	67399	20.000	ng/u1	0.00
20) Naphthalene-d8	10.628	136	309734	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.477	164	292004	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.226	188	778510	20.000	ng/u1	0.00
79) Chrysene-d12	21.474	240	844310	20.000	ng/u1	0.00
88) Perylene-d12	24.512	264	924970	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.307	96	5893	3.954	ng/uL	0.00
4) Pyridine-d5	3.719	84	15961	3.240	ng/u1	0.00
7) Phenol-d5	7.009	99	141197	23.217	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.168	67	83067	23.286	ng/u1	0.00
11) 2-Chlorophenol-d4	7.373	132	99713	25.260	ng/u1	0.00
15) 4-Methylphenol-d8	8.542	113	123043	23.869	ng/u1	0.00
21) Nitrobenzene-d5	8.995	128	53719	24.670	ng/u1	0.00
24) 2-Nitrophenol-d4	9.712	143	67347	23.930	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	135246	24.488	ng/u1	0.00
31) 4-Chloroaniline-d4	10.763	131	111037	15.435	ng/u1	0.00
46) Dimethylphthalate-d6	13.883	166	533415	23.321	ng/u1	0.00
49) Acenaphthylene-d8	14.165	160	559885	25.009	ng/u1	0.00
54) 4-Nitrophenol-d4	14.682	143	55332	17.669	ng/u1	0.00
60) Fluorene-d10	15.470	176	500415	25.923	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.593	200	94042	19.221	ng/u1	0.00
73) Anthracene-d10	17.320	188	873350	26.102	ng/u1	0.00
81) Pyrene-d10	19.624	212	1180323	27.883	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.306	264	1145846	25.658	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.374	149	42754	2.071	ng/u1#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063178.D
Acq On : 6 Nov 2024 22:03
Operator : RC/JU
Sample : P4634-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CC0Q1


Quant Time: Nov 06 22:16:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

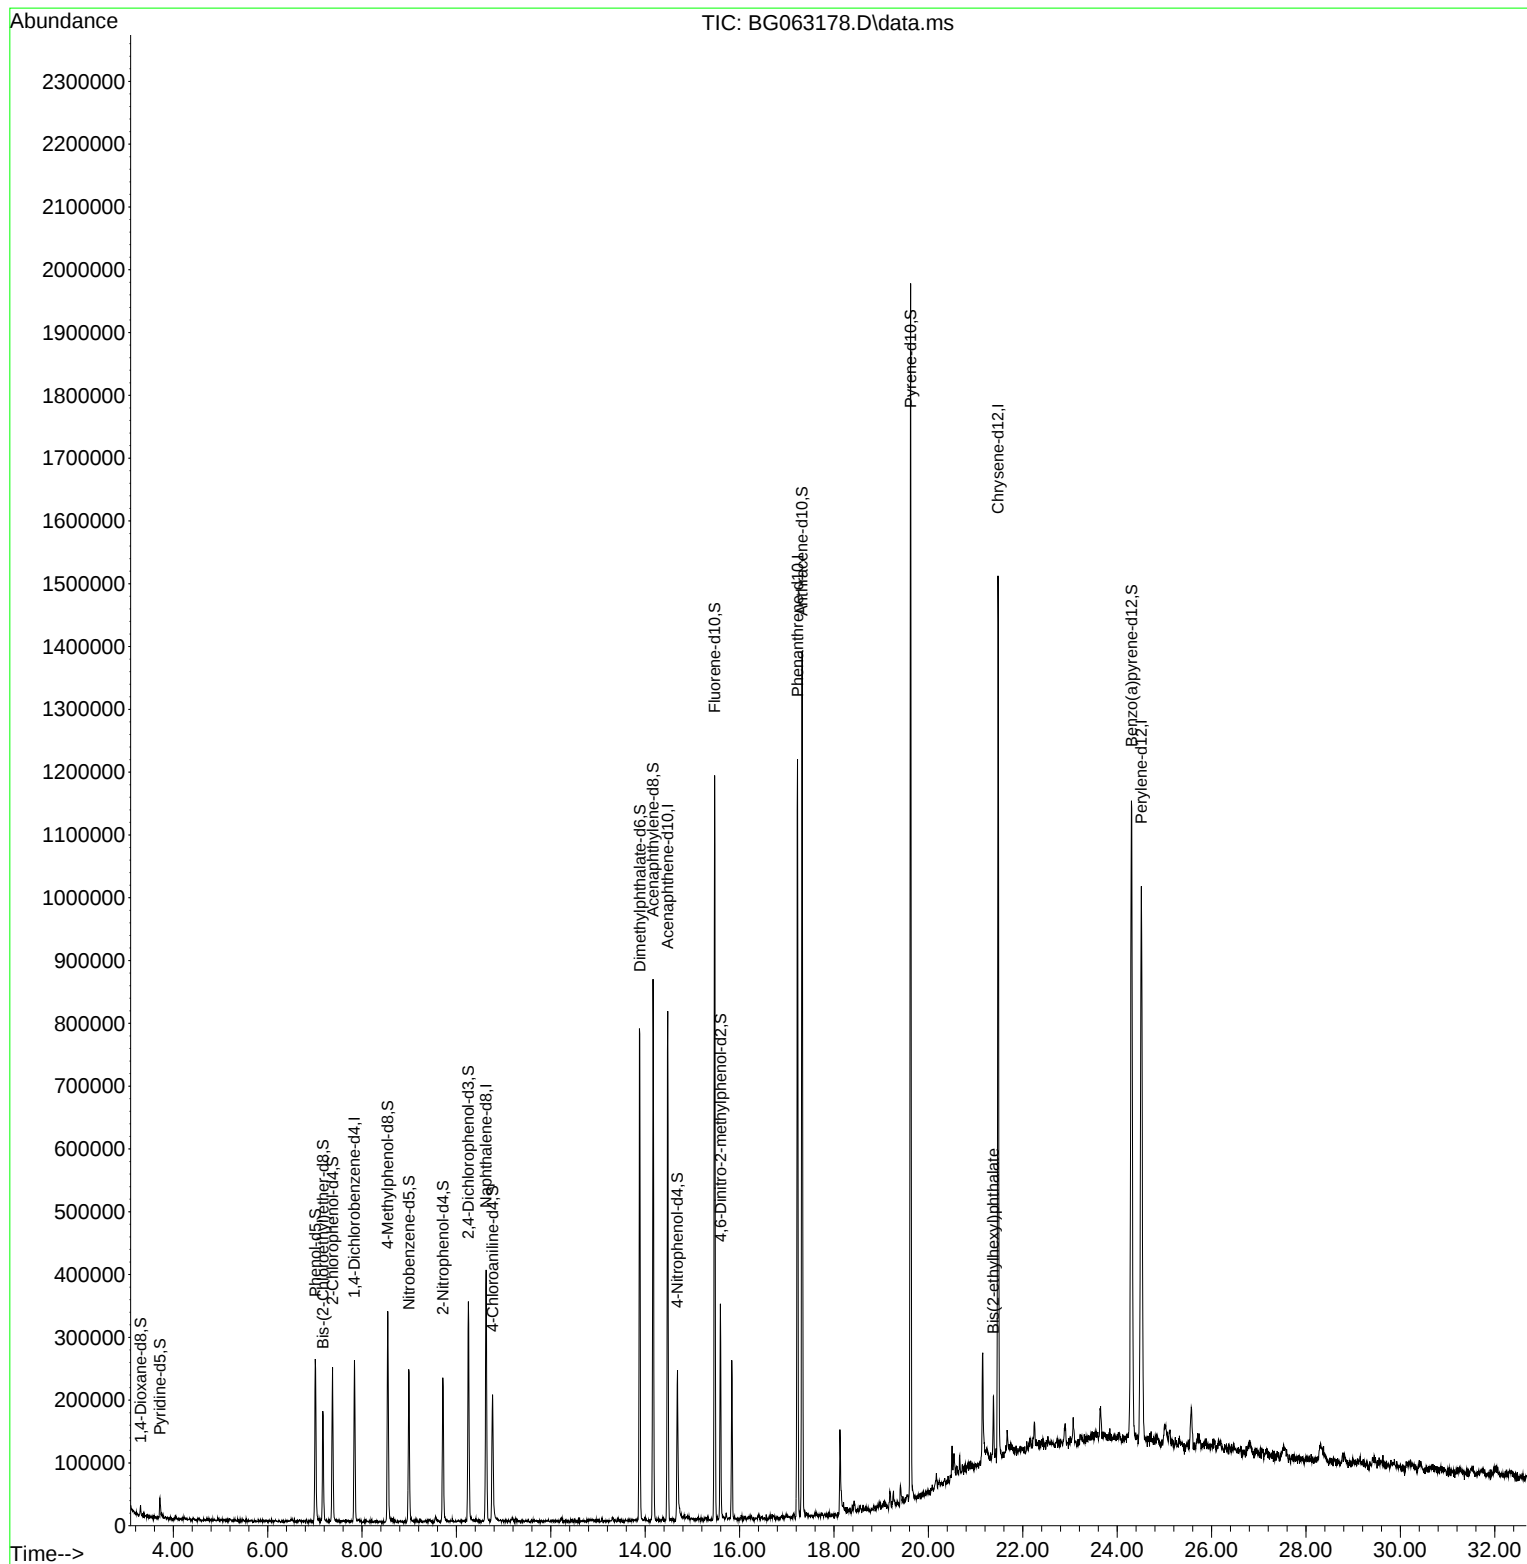

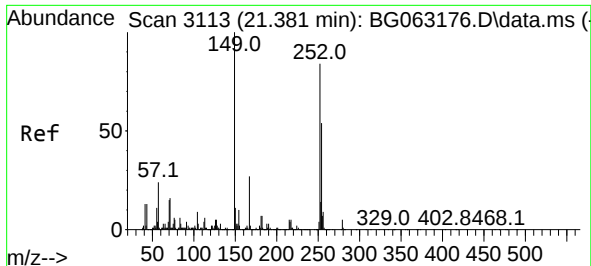

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.071 ng/ul
 RT: 21.374 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BG063178.D
 Acq: 6 Nov 2024 22:03

Instrument :
 BNA_G
 ClientSampleId :
 CC0Q1

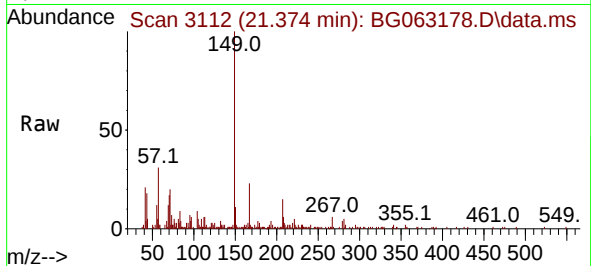

Tgt Ion:149 Resp: 42754
 Ion Ratio Lower Upper
 149 100
 167 22.9 20.6 31.0
 279 4.0 4.2 6.4#

