

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063183.D
 Acq On : 7 Nov 2024 1:13
 Operator : RC/JU
 Sample : P4634-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CC0R4

Quant Time: Nov 07 01:18:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.843	152	79889	20.000	ng/ul	0.00
20) Naphthalene-d8	10.628	136	353133	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.476	164	332106	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.226	188	829483	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	856683	20.000	ng/ul	0.00
88) Perylene-d12	24.517	264	943914	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.313	96	8016	4.537	ng/uL	0.00
4) Pyridine-d5	3.712	84	131039	22.440	ng/ul	0.00
7) Phenol-d5	7.014	99	213368	29.598	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.167	67	124763	29.506	ng/ul	0.00
11) 2-Chlorophenol-d4	7.373	132	151119	32.297	ng/ul	0.00
15) 4-Methylphenol-d8	8.548	113	180233	29.498	ng/ul	0.00
21) Nitrobenzene-d5	8.994	128	82847	33.371	ng/ul	0.00
24) 2-Nitrophenol-d4	9.711	143	103122	32.139	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	205699	32.667	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	238056	29.025	ng/ul	0.00
46) Dimethylphthalate-d6	13.883	166	760977	29.253	ng/ul	0.00
49) Acenaphthylene-d8	14.171	160	831866	32.671	ng/ul	0.00
54) 4-Nitrophenol-d4	14.682	143	86092	24.171	ng/ul	0.00
60) Fluorene-d10	15.469	176	718236	32.714	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	126498	24.265	ng/ul	0.00
73) Anthracene-d10	17.326	188	1192305	33.445	ng/ul	0.00
81) Pyrene-d10	19.623	212	1521861	35.432	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.312	264	1498920	32.890	ng/ul	0.00


Target Compounds					Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.397	149	6503215	310.437	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063183.D
Acq On : 7 Nov 2024 1:13
Operator : RC/JU
Sample : P4634-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CC0R4

Quant Time: Nov 07 01:18:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

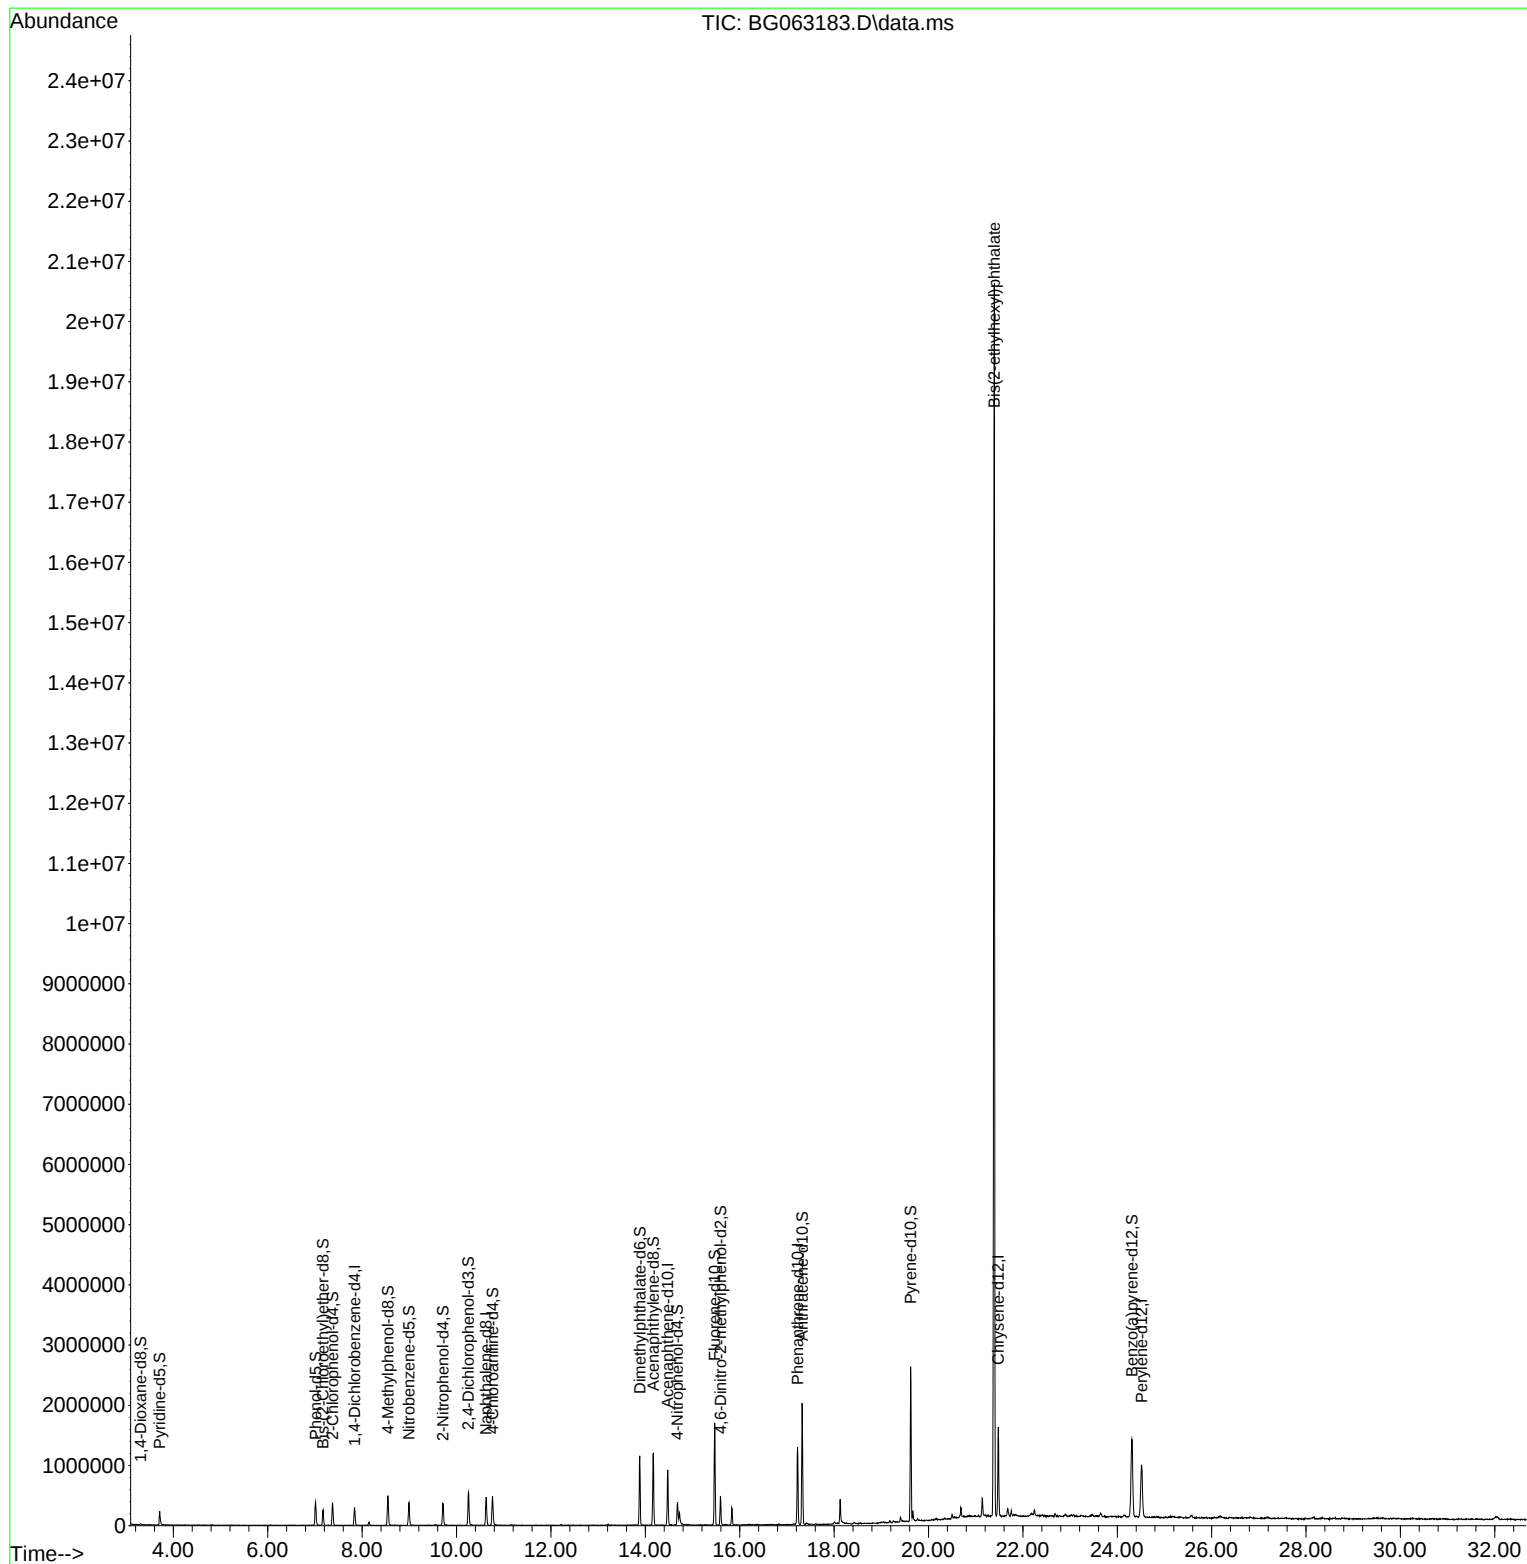

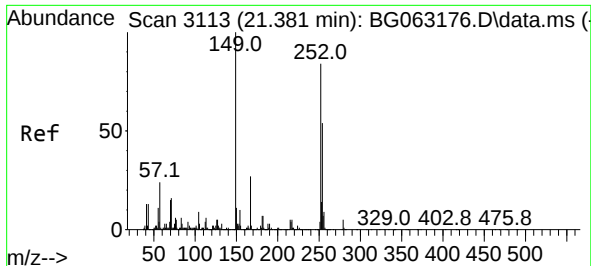

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 310.437 ng/ul
 RT: 21.397 min Scan# 31
 Delta R.T. 0.019 min
 Lab File: BG063183.D
 Acq: 7 Nov 2024 1:13

Instrument :
 BNA_G
 ClientSampleId :
 CC0R4

Tgt Ion:149 Resp: 6503215
 Ion Ratio Lower Upper
 149 100
 167 54.5 20.6 31.0#
 279 13.0 4.2 6.4#

