

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063195.D
 Acq On : 7 Nov 2024 9:27
 Operator : RC/JU
 Sample : P4634-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0P12

Quant Time: Nov 07 10:05:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	88549	20.000	ng/u1	0.00
20) Naphthalene-d8	10.631	136	438952	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.480	164	406337	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.223	188	1017361	20.000	ng/u1	0.00
79) Chrysene-d12	21.477	240	1027350	20.000	ng/u1	0.00
88) Perylene-d12	24.515	264	1091971	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.316	96	3654	1.866	ng/uL	0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.012	99	92230	11.543	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.171	67	55306	11.801	ng/u1	0.00
11) 2-Chlorophenol-d4	7.376	132	67115	12.941	ng/u1	0.00
15) 4-Methylphenol-d8	8.545	113	50905	7.516	ng/u1	0.00
21) Nitrobenzene-d5	8.992	128	37235	12.066	ng/u1	0.00
24) 2-Nitrophenol-d4	9.715	143	46868	11.751	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.255	165	93960	12.004	ng/u1	0.00
31) 4-Chloroaniline-d4	10.766	131	59162	5.803	ng/u1	0.00
46) Dimethylphthalate-d6	13.880	166	381033	11.971	ng/u1	0.00
49) Acenaphthylene-d8	14.168	160	406451	13.047	ng/u1	0.00
54) 4-Nitrophenol-d4	14.685	143	43021	9.872	ng/u1	0.00
60) Fluorene-d10	15.473	176	351401	13.082	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.596	200	64356	10.065	ng/u1	0.00
73) Anthracene-d10	17.323	188	583695	13.349	ng/u1	0.00
81) Pyrene-d10	19.621	212	555563	10.786	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.298	264	344265	6.530	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.657	105	54073	4.959	ng/u1	96
86) Bis(2-ethylhexyl)phtha...	21.377	149	39339	1.566	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063195.D
Acq On : 7 Nov 2024 9:27
Operator : RC/JU
Sample : P4634-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0PI2

Quant Time: Nov 07 10:05:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration




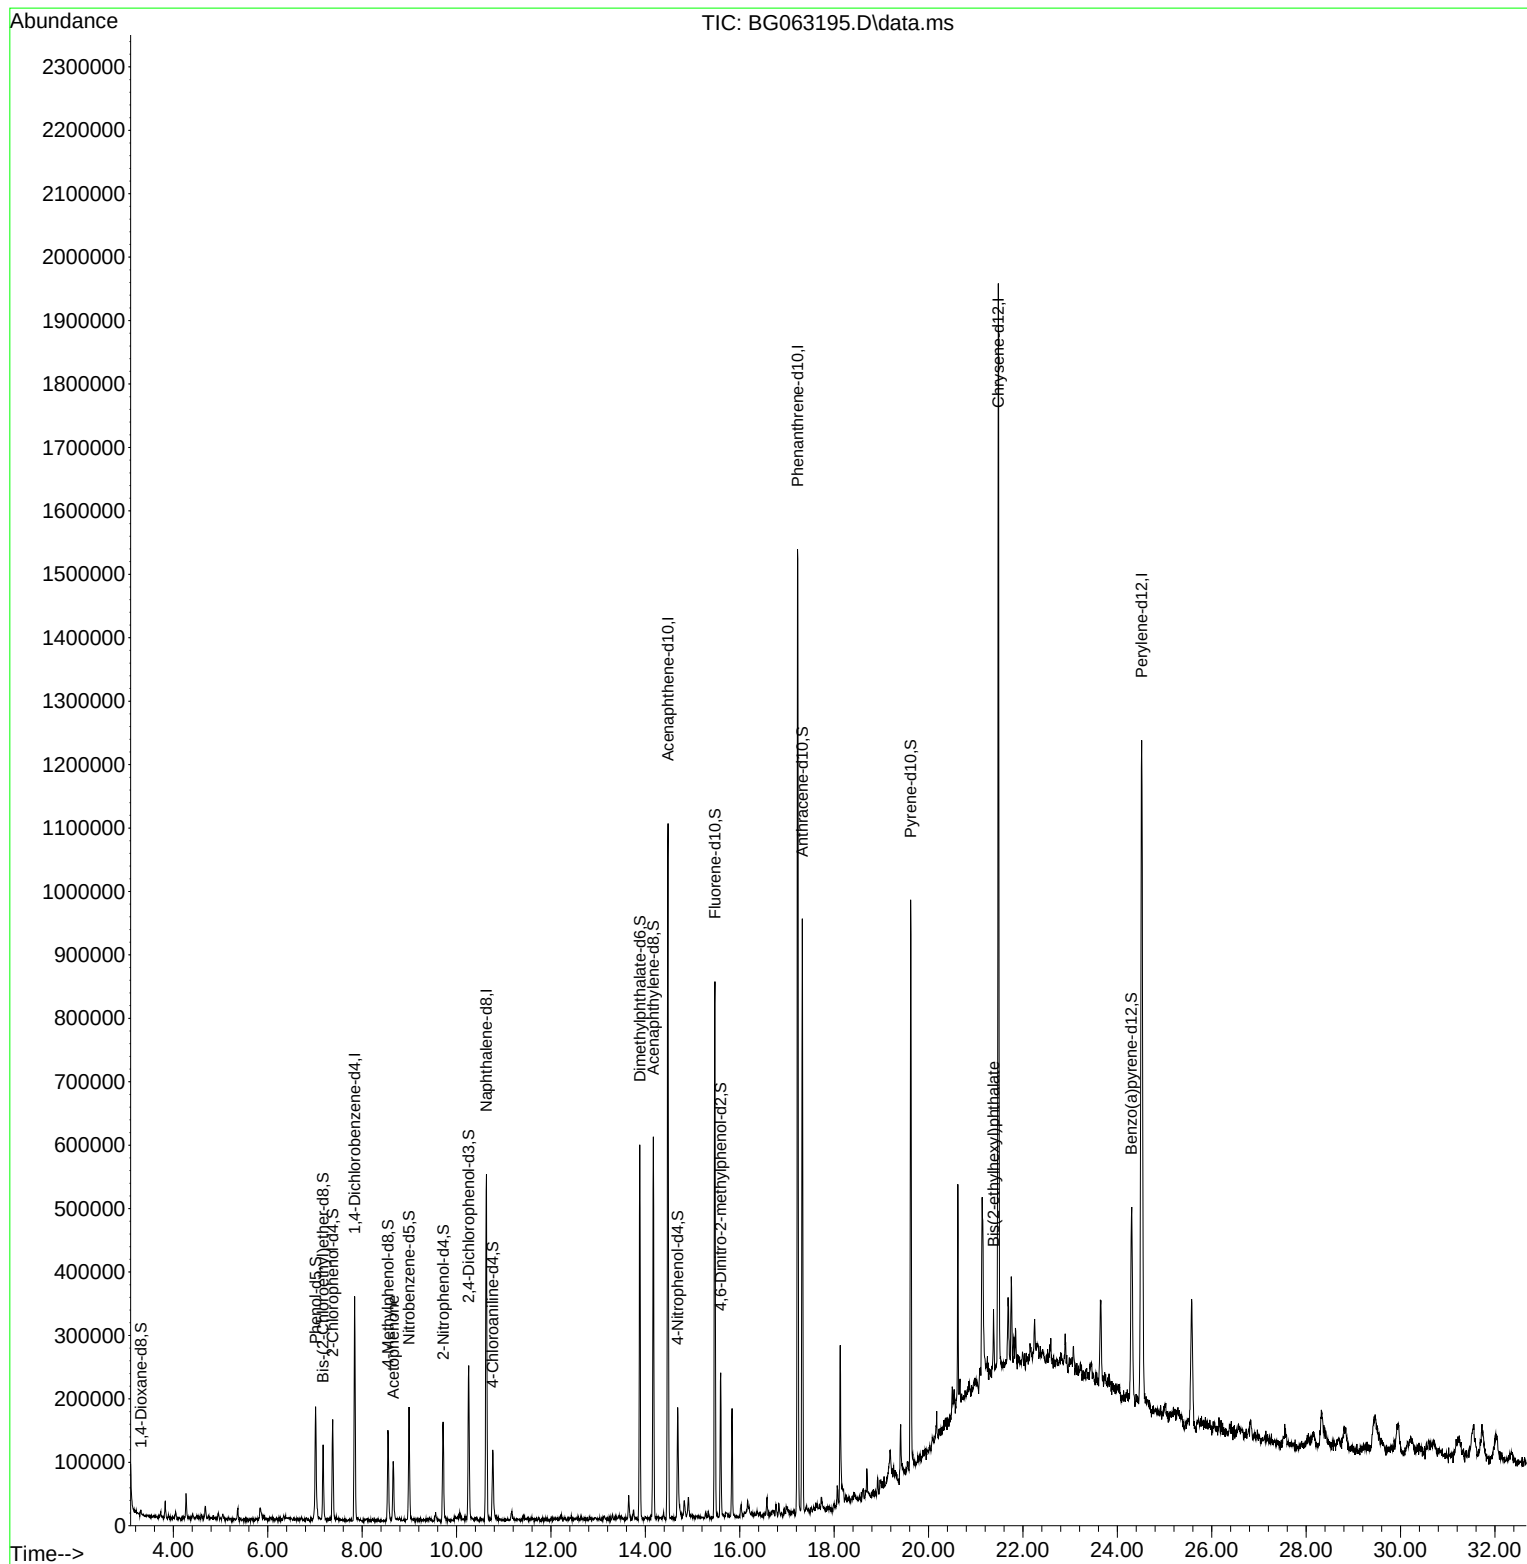


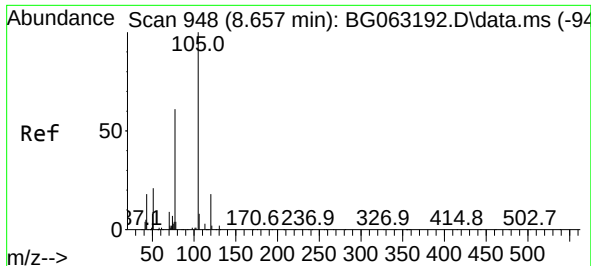

#16
Acetophenone
Concen: 4.959 ng/ul
RT: 8.657 min Scan# 948
Delta R.T. -0.001 min
Lab File: BG063195.D
Acq: 7 Nov 2024 9:27

Instrument :
BNA_G
ClientSampleId :
C0P12

Tgt Ion:105 Resp: 54073
Ion Ratio Lower Upper
105 100
77 83.3 68.0 102.0
51 24.3 24.3 36.5

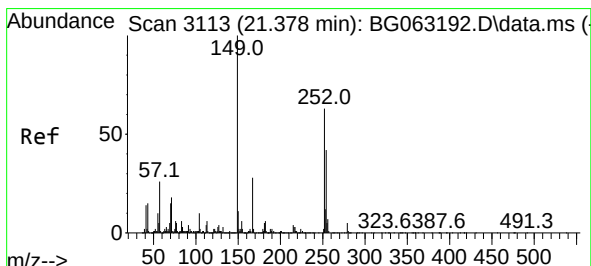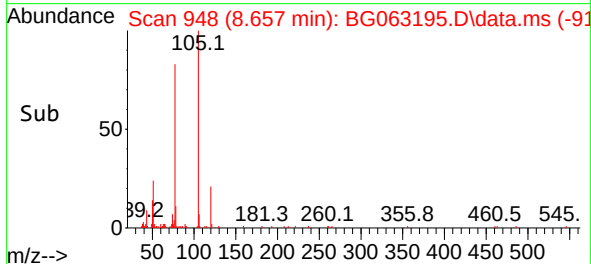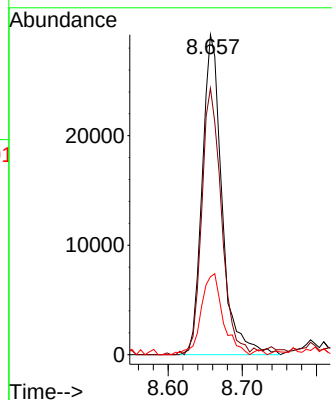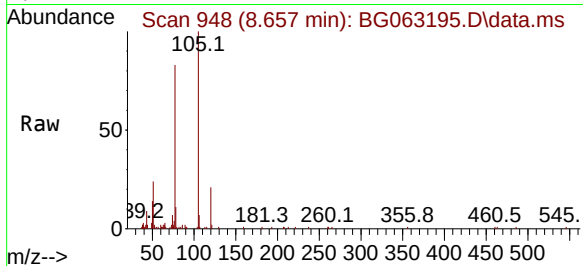

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.566 ng/ul
RT: 21.377 min Scan# 3113
Delta R.T. -0.001 min
Lab File: BG063195.D
Acq: 7 Nov 2024 9:27

Tgt Ion:149 Resp: 39339
Ion Ratio Lower Upper
149 100
167 24.4 20.6 31.0
279 5.6 4.2 6.4

