

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063196.D
 Acq On : 7 Nov 2024 10:05
 Operator : RC/JU
 Sample : P4634-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0P18

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/08/2024
 Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 07 10:16:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.842	152	90982	20.000	ng/u1	0.00
20) Naphthalene-d8	10.633	136	433075	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.476	164	408773	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.225	188	1014114	20.000	ng/u1	0.00
79) Chrysene-d12	21.479	240	1021152	20.000	ng/u1	0.00
88) Perylene-d12	24.511	264	1101260	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	6542	3.251	ng/uL	0.00
4) Pyridine-d5	3.712	84	96950	14.578	ng/u1	0.00
7) Phenol-d5	7.014	99	167952	20.458	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.167	67	89464	18.578	ng/u1	0.00
11) 2-Chlorophenol-d4	7.372	132	114711	21.527	ng/u1	0.00
15) 4-Methylphenol-d8	8.547	113	141004	20.263	ng/u1	0.00
21) Nitrobenzene-d5	8.994	128	58703	19.281	ng/u1	0.00
24) 2-Nitrophenol-d4	9.711	143	83447	21.206	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.257	165	164596	21.314	ng/u1	0.00
31) 4-Chloroaniline-d4	10.762	131	170162	16.917	ng/u1	0.00
46) Dimethylphthalate-d6	13.882	166	605225	18.902	ng/u1	0.00
49) Acenaphthylene-d8	14.170	160	677755	21.626	ng/u1	0.00
54) 4-Nitrophenol-d4	14.687	143	80011m	18.251	ng/u1	0.00
60) Fluorene-d10	15.475	176	565729	20.935	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	111947	17.565	ng/u1	0.00
73) Anthracene-d10	17.325	188	927829	21.288	ng/u1	0.00
81) Pyrene-d10	19.623	212	1155434	22.568	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.311	264	1130336	21.259	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.379	149	28142	1.127	ng/u1	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063196.D
Acq On : 7 Nov 2024 10:05
Operator : RC/JU
Sample : P4634-04
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
COP18

Quant Time: Nov 07 10:16:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/08/2024
Supervised By :mohammad ahmed 11/11/2024

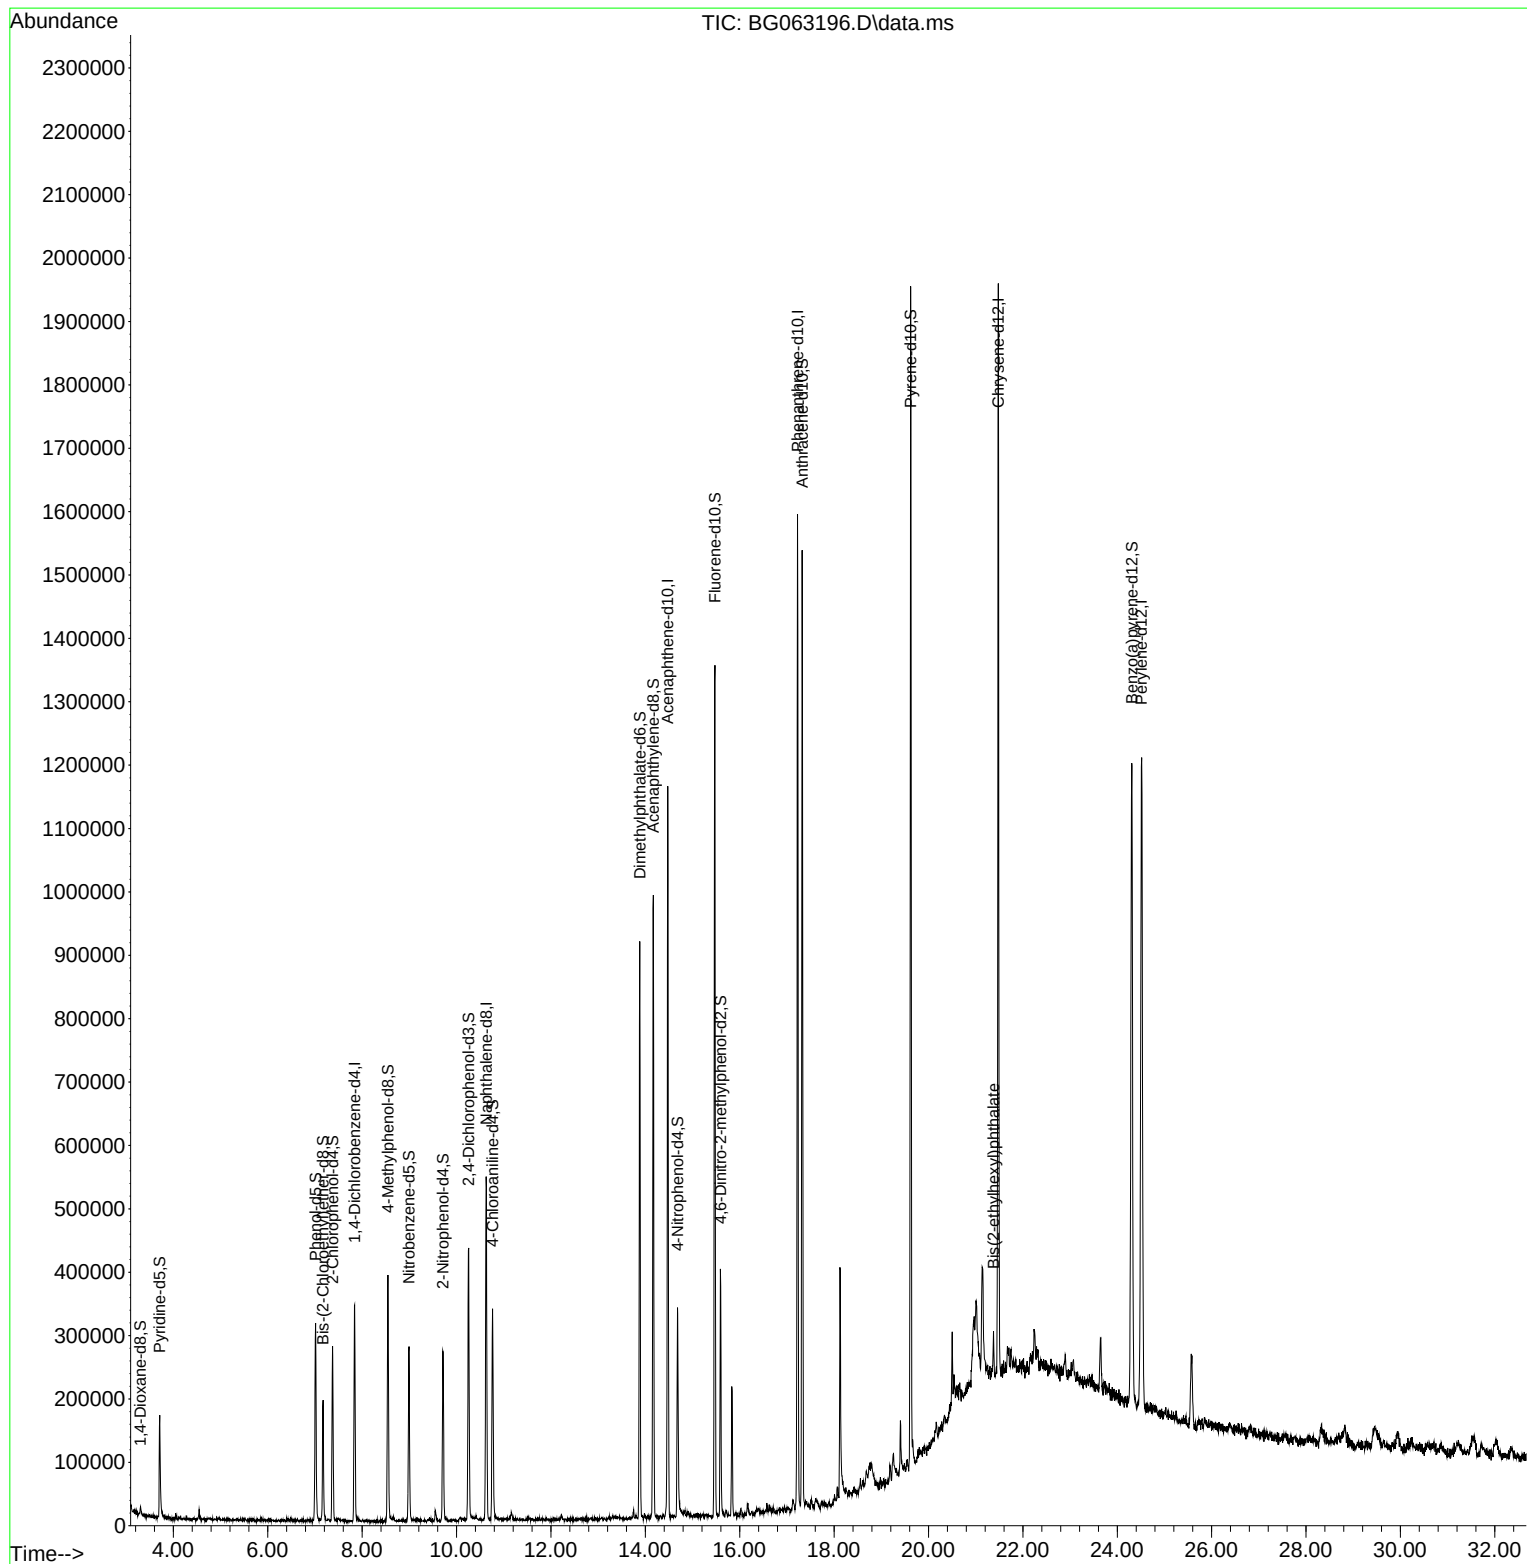

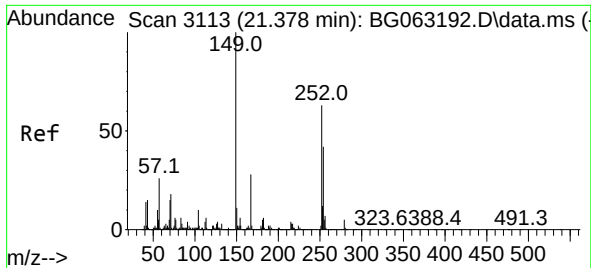

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.127 ng/ul
 RT: 21.379 min Scan# 3113
 Delta R.T. 0.001 min
 Lab File: BG063196.D
 Acq: 7 Nov 2024 10:05

Instrument :
 BNA_G
 ClientSampleId :
 C0PI8

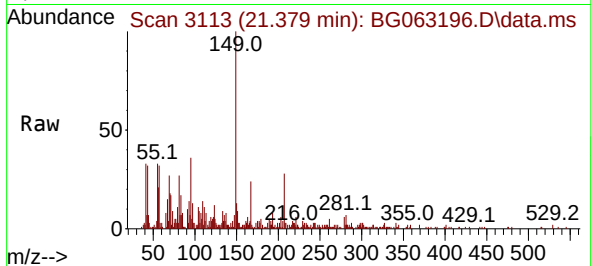

Tgt Ion:149 Resp: 2814
 Ion Ratio Lower Upper
 149 100
 167 23.7 20.6 31.0
 279 5.9 4.2 6.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/08/2024
 Supervised By :mohammad ahmed 11/11/2024

