

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063172.D
 Acq On : 6 Nov 2024 17:35
 Operator : RC/JU
 Sample : PB164608BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK608

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	43	rVB3	15762	26581	0.86%	0.097%
2	3.416	54	56	58	rBV3	7577	5024	0.16%	0.018%
3	3.651	92	96	98	rVB3	6021	5687	0.18%	0.021%
4	3.710	102	106	117	rBV	188357	320936	10.44%	1.172%
5	4.045	158	163	169	rVB2	28541	41248	1.34%	0.151%
6	4.333	209	212	214	rBV3	4718	5218	0.17%	0.019%
7	4.427	226	228	234	rBV4	3723	4308	0.14%	0.016%
8	4.768	282	286	289	rBV2	4462	6299	0.20%	0.023%
9	5.020	326	329	332	rBV3	3760	5215	0.17%	0.019%
10	5.414	395	396	402	rBV4	5273	5864	0.19%	0.021%
11	5.684	439	442	445	rBV	4626	5651	0.18%	0.021%
12	6.483	576	578	582	rVB3	3350	4078	0.13%	0.015%
13	7.006	660	667	677	rBV	236987	430798	14.01%	1.574%
14	7.171	688	695	705	rBV	175382	301652	9.81%	1.102%
15	7.371	721	729	738	rBV	230934	402661	13.10%	1.471%
16	7.835	802	808	816	rBV	239818	413733	13.46%	1.511%
17	8.258	878	880	883	rBV2	4221	4699	0.15%	0.017%
18	8.417	903	907	910	rBV3	3642	4939	0.16%	0.018%
19	8.540	921	928	938	rBV	313566	554186	18.02%	2.024%
20	8.992	998	1005	1015	rBV	242764	420637	13.68%	1.536%
21	9.515	1090	1094	1097	rBV2	3177	5276	0.17%	0.019%
22	9.715	1120	1128	1138	rBV	220646	416850	13.56%	1.523%
23	10.256	1211	1220	1228	rBV	308113	571005	18.57%	2.086%
24	10.455	1251	1254	1258	rBV2	4126	6170	0.20%	0.023%
25	10.626	1276	1283	1291	rBV	377876	657404	21.38%	2.401%
26	10.761	1299	1306	1317	rBV2	324265	624201	20.30%	2.280%
27	11.013	1347	1349	1351	rBV	3487	4088	0.13%	0.015%
28	11.266	1389	1392	1394	rBV2	4136	4292	0.14%	0.016%
29	11.354	1401	1407	1409	rBV	3778	4856	0.16%	0.018%
30	11.577	1444	1445	1450	rBV2	3116	5163	0.17%	0.019%
31	11.642	1452	1456	1459	rVB2	3716	6012	0.20%	0.022%
32	11.677	1459	1462	1467	rBV2	4745	7085	0.23%	0.026%
33	12.100	1530	1534	1537	rBV2	3026	4717	0.15%	0.017%
34	12.735	1638	1642	1644	rVB	4906	5165	0.17%	0.019%
35	13.240	1725	1728	1731	rVB	4194	4414	0.14%	0.016%
36	13.311	1737	1740	1743	rBV2	3589	4859	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063172.D
 Acq On : 6 Nov 2024 17:35
 Operator : RC/JU
 Sample : PB164608BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK608

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	13.481	1767	1769	1772	rVB	4171	4419	0.14%	0.016%
38	13.881	1830	1837	1846	rBV	953807	1353234	44.01%	4.943%
39	14.169	1879	1886	1894	rBV	801816	1268436	41.26%	4.633%
40	14.304	1907	1909	1912	rVB2	6024	7158	0.23%	0.026%
41	14.474	1932	1938	1946	rVB2	796612	1204308	39.17%	4.399%
42	14.680	1966	1973	1990	rBV2	309892	551515	17.94%	2.015%
43	15.109	2043	2046	2048	rBV2	3996	4103	0.13%	0.015%
44	15.173	2054	2057	2059	rBV2	4345	5591	0.18%	0.020%
45	15.285	2075	2076	2080	rBV3	3253	4531	0.15%	0.017%
46	15.402	2093	2096	2097	rBV	4256	4195	0.14%	0.015%
47	15.473	2100	2108	2117	rVV	1159493	1769623	57.56%	6.464%
48	15.590	2122	2128	2134	rBV	394929	603328	19.62%	2.204%
49	15.714	2148	2149	2152	rVB3	9732	7375	0.24%	0.027%
50	16.630	2302	2305	2306	rBV	6135	5996	0.20%	0.022%
51	16.713	2317	2319	2322	rBV2	5353	4622	0.15%	0.017%
52	17.224	2400	2406	2415	rBV	1246346	1845663	60.03%	6.742%
53	17.324	2417	2423	2430	rVV	1523726	2223781	72.33%	8.123%
54	17.394	2433	2435	2439	rVB2	5550	5575	0.18%	0.020%
55	17.523	2454	2457	2458	rBV3	4768	5078	0.17%	0.019%
56	17.711	2488	2489	2494	rVB2	6433	7186	0.23%	0.026%
57	17.888	2517	2519	2522	rBV2	5192	4659	0.15%	0.017%
58	18.111	2555	2557	2559	rBV	4310	4532	0.15%	0.017%
59	18.229	2575	2577	2579	rBV2	5309	4859	0.16%	0.018%
60	18.469	2615	2618	2621	rBV2	4059	5446	0.18%	0.020%
61	18.558	2632	2633	2635	rBV	6735	4319	0.14%	0.016%
62	18.628	2644	2645	2648	rVB	6690	4102	0.13%	0.015%
63	18.740	2661	2664	2666	rBV3	6999	7182	0.23%	0.026%
64	18.863	2683	2685	2688	rBV2	4209	5410	0.18%	0.020%
65	18.998	2706	2708	2710	rBV2	4379	4378	0.14%	0.016%
66	19.186	2736	2740	2747	rVB4	26952	41382	1.35%	0.151%
67	19.257	2747	2752	2757	rBV2	27157	46335	1.51%	0.169%
68	19.357	2766	2769	2771	rBV4	5375	7120	0.23%	0.026%
69	19.451	2783	2785	2788	rVB2	6003	6445	0.21%	0.024%
70	19.539	2797	2800	2802	rBV3	7493	7967	0.26%	0.029%
71	19.621	2807	2814	2823	rBV	2123535	3074609	100.00%	11.231%
72	19.750	2834	2836	2838	rBV3	4609	4428	0.14%	0.016%
73	19.921	2863	2865	2869	rBV4	6780	11017	0.36%	0.040%
74	20.291	2926	2928	2930	rBV3	8428	8260	0.27%	0.030%
75	20.426	2949	2951	2954	rBV4	5498	6066	0.20%	0.022%
76	21.478	3124	3130	3141	rBV	1589881	2469850	80.33%	9.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063172.D
Acq On : 6 Nov 2024 17:35
Operator : RC/JU
Sample : PB164608BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK608

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

77	23.375	3452	3453	3455	rBV2	14313	8007	0.26%	0.029%
78	24.304	3601	3611	3624	rBV	1193889	2992211	97.32%	10.930%
79	24.509	3637	3646	3658	rVB	928772	2461446	80.06%	8.991%




Sum of corrected areas: 27376718

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063172.D
Acq On : 6 Nov 2024 17:35
Operator : RC/JU
Sample : PB164608BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

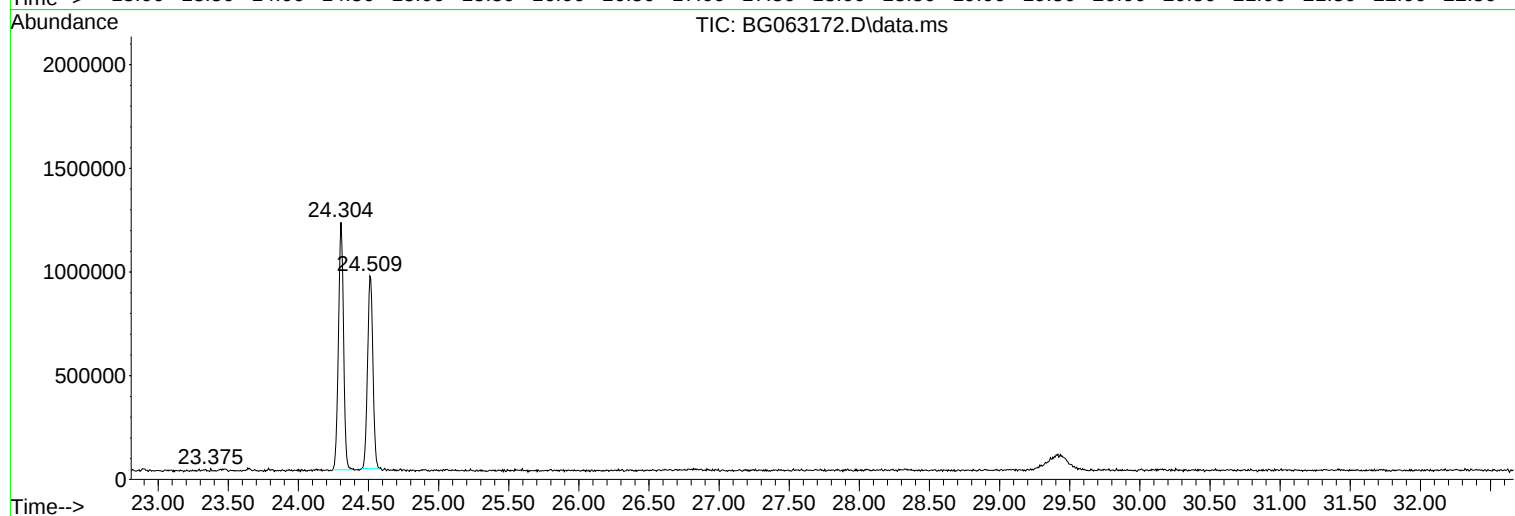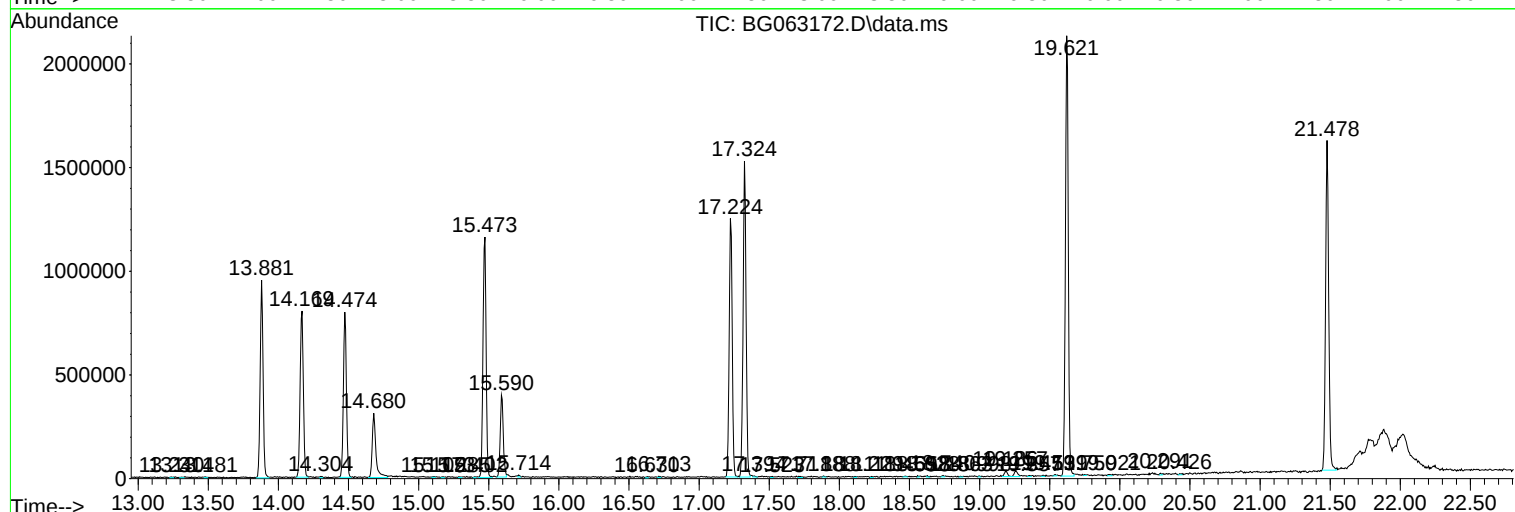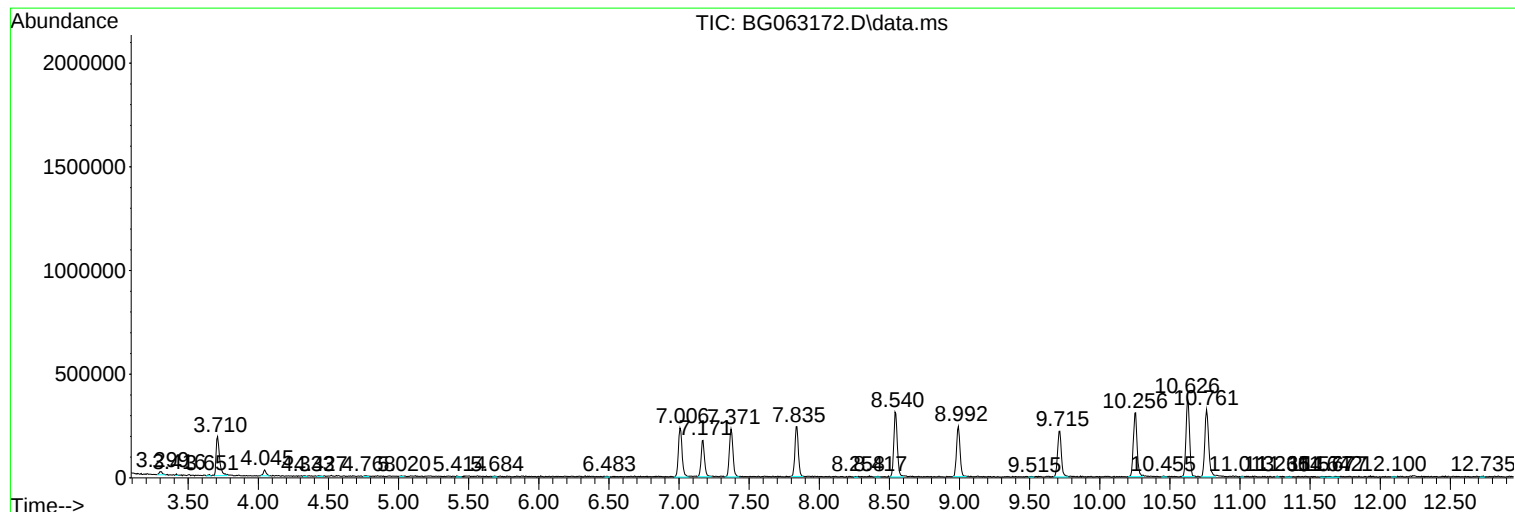

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063172.D
Acq On : 6 Nov 2024 17:35
Operator : RC/JU
Sample : PB164608BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063172.D
Acq On : 6 Nov 2024 17:35
Operator : RC/JU
Sample : PB164608BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------