

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063177.D
 Acq On : 6 Nov 2024 21:24
 Operator : RC/JU
 Sample : PB164608BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK608

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	34	37	42	rVB4	16916	19409	0.59%	0.065%
2	3.711	102	106	116	rBV	210920	342517	10.44%	1.154%
3	4.046	158	163	169	rVB2	32397	54507	1.66%	0.184%
4	5.133	347	348	352	rVB3	4560	4730	0.14%	0.016%
5	6.549	586	589	592	rBV4	5881	4962	0.15%	0.017%
6	7.013	661	668	678	rBV	270547	475000	14.47%	1.601%
7	7.171	688	695	702	rBV	216546	346714	10.56%	1.169%
8	7.371	722	729	737	rBV	265625	470034	14.32%	1.584%
9	7.641	772	775	777	rVB3	6116	4658	0.14%	0.016%
10	7.712	785	787	792	rVB2	5038	5554	0.17%	0.019%
11	7.841	802	809	820	rVB2	281849	483433	14.73%	1.629%
12	8.540	923	928	938	rBV	343096	601340	18.32%	2.027%
13	8.734	958	961	964	rVB	4439	4574	0.14%	0.015%
14	8.993	997	1005	1015	rBV	280510	482996	14.72%	1.628%
15	9.193	1034	1039	1040	rBV	3763	4865	0.15%	0.016%
16	9.451	1082	1083	1090	rVB2	4366	4664	0.14%	0.016%
17	9.715	1120	1128	1136	rBV	255220	462889	14.10%	1.560%
18	10.250	1213	1219	1227	rBV	343496	639937	19.50%	2.157%
19	10.515	1261	1264	1266	rBV	3718	4974	0.15%	0.017%
20	10.626	1277	1283	1292	rBV	405557	728615	22.20%	2.456%
21	10.761	1299	1306	1315	rBV	360003	679290	20.70%	2.289%
22	11.325	1399	1402	1404	rBV	5138	5786	0.18%	0.020%
23	11.560	1441	1442	1447	rBV2	3269	4526	0.14%	0.015%
24	12.224	1551	1555	1559	rBV4	6132	10652	0.32%	0.036%
25	12.677	1629	1632	1637	rBV	4208	5769	0.18%	0.019%
26	12.847	1658	1661	1664	rVB	3800	5221	0.16%	0.018%
27	12.912	1670	1672	1675	rVB	5766	5988	0.18%	0.020%
28	13.881	1830	1837	1844	rBV	988120	1404792	42.80%	4.735%
29	14.169	1878	1886	1893	rBV	880331	1393820	42.47%	4.698%
30	14.475	1931	1938	1947	rVB	861705	1318668	40.18%	4.444%
31	14.680	1962	1973	1986	rBV2	342245	610039	18.59%	2.056%
32	15.003	2024	2028	2030	rBV3	5203	8105	0.25%	0.027%
33	15.209	2060	2063	2066	rVB2	3694	5300	0.16%	0.018%
34	15.468	2100	2107	2114	rBV	1229375	1917738	58.43%	6.464%
35	15.591	2122	2128	2136	rBV2	440465	661757	20.16%	2.230%
36	15.708	2145	2148	2153	rVB5	8799	14391	0.44%	0.049%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063177.D
 Acq On : 6 Nov 2024 21:24
 Operator : RC/JU
 Sample : PB164608BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK608

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	15.896	2177	2180	2184	rVB3	3657	5005	0.15%	0.017%
38	16.308	2248	2250	2255	rVB2	2756	4648	0.14%	0.016%
39	16.543	2286	2290	2291	rVB2	4675	4883	0.15%	0.016%
40	16.560	2291	2293	2297	rBV	5060	5419	0.17%	0.018%
41	16.637	2303	2306	2311	rBV3	5174	7103	0.22%	0.024%
42	17.160	2391	2395	2397	rBV	4011	4590	0.14%	0.015%
43	17.224	2399	2406	2416	rBV	1348000	1999330	60.92%	6.739%
44	17.324	2416	2423	2431	rBV2	1584144	2369380	72.19%	7.986%
45	17.495	2449	2452	2455	rBV2	4499	6745	0.21%	0.023%
46	17.783	2500	2501	2507	rVB4	6453	9152	0.28%	0.031%
47	18.370	2598	2601	2603	rVB3	3713	4548	0.14%	0.015%
48	18.687	2654	2655	2659	rBV3	5589	6313	0.19%	0.021%
49	18.723	2659	2661	2665	rVV4	4521	6695	0.20%	0.023%
50	18.834	2678	2680	2683	rBV3	3702	5078	0.15%	0.017%
51	18.899	2690	2691	2695	rVB2	5528	5433	0.17%	0.018%
52	18.975	2703	2704	2708	rBV3	4073	5963	0.18%	0.020%
53	19.187	2733	2740	2746	rBV3	27482	50941	1.55%	0.172%
54	19.257	2748	2752	2757	rVB2	26038	38735	1.18%	0.131%
55	19.539	2798	2800	2803	rBV3	8030	7248	0.22%	0.024%
56	19.622	2808	2814	2821	rBV	2349038	3282126	100.00%	11.062%
57	20.297	2925	2929	2930	rBV4	7267	7068	0.22%	0.024%
58	20.444	2952	2954	2956	rBV3	7371	4976	0.15%	0.017%
59	21.478	3123	3130	3139	rBV2	1699097	2674908	81.50%	9.015%
60	22.888	3368	3370	3376	rVB6	26586	40375	1.23%	0.136%
61	24.304	3601	3611	3623	rVB	1244263	3174332	96.72%	10.699%
62	24.510	3636	3646	3659	rBV2	991636	2741019	83.51%	9.238%




Sum of corrected areas: 29670227

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063177.D
Acq On : 6 Nov 2024 21:24
Operator : RC/JU
Sample : PB164608BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

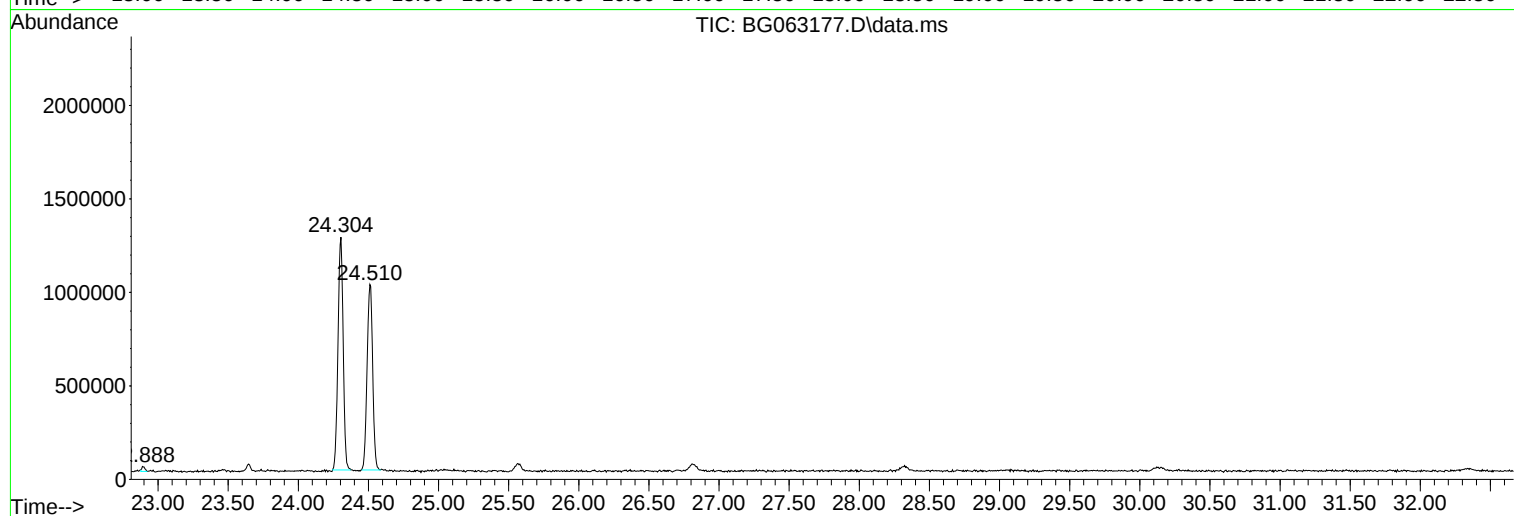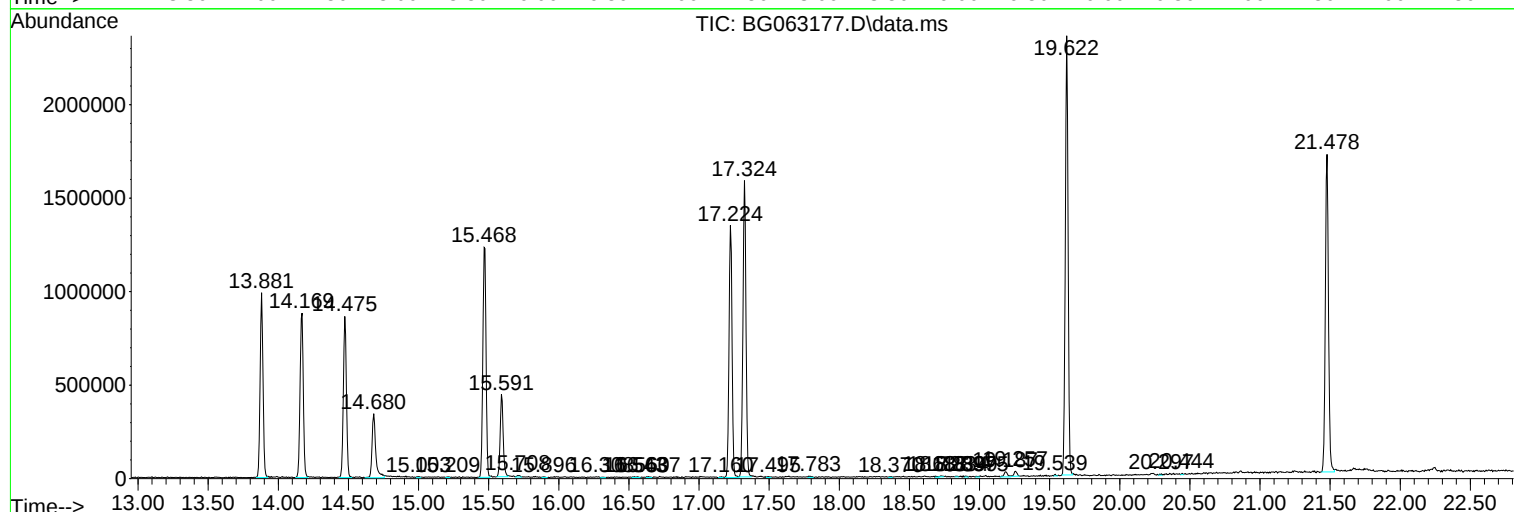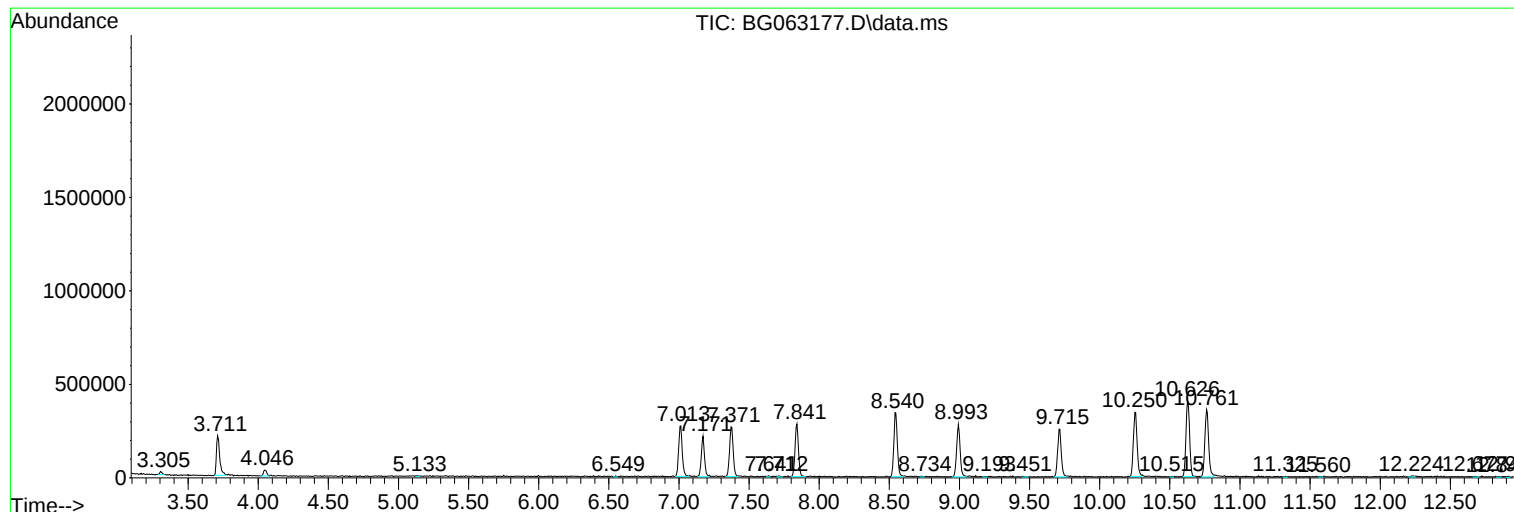

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063177.D
Acq On : 6 Nov 2024 21:24
Operator : RC/JU
Sample : PB164608BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063177.D
Acq On : 6 Nov 2024 21:24
Operator : RC/JU
Sample : PB164608BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK608

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
