

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063201.D
 Acq On : 7 Nov 2024 14:19
 Operator : RC/JU
 Sample : P4634-15DL 10X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CC0R4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.721	104	108	114	rBV2	16018	31455	0.87%	0.205%
2	4.039	160	162	168	rVB5	15888	26311	0.73%	0.172%
3	7.017	663	669	679	rVB2	27994	60727	1.68%	0.397%
4	7.170	690	695	703	rVB	21634	38254	1.06%	0.250%
5	7.370	724	729	739	rVB4	29372	58105	1.61%	0.380%
6	7.840	802	809	819	rBV	266319	462197	12.81%	3.020%
7	8.140	856	860	867	rVB5	8916	14703	0.41%	0.096%
8	8.551	923	930	939	rBV3	41043	76526	2.12%	0.500%
9	8.992	1000	1005	1011	rBV3	31800	58556	1.62%	0.383%
10	9.720	1123	1129	1135	rBV5	29304	58999	1.63%	0.385%
11	10.261	1213	1221	1227	rBV3	45359	91371	2.53%	0.597%
12	10.625	1275	1283	1293	rBV	429056	775584	21.49%	5.067%
13	10.766	1302	1307	1315	rBV3	32584	74474	2.06%	0.487%
14	10.972	1339	1342	1345	rBV2	6407	7862	0.22%	0.051%
15	12.182	1546	1548	1551	rBV2	5660	5724	0.16%	0.037%
16	12.382	1579	1582	1584	rBV2	4537	6066	0.17%	0.040%
17	13.134	1707	1710	1714	rVB2	4250	6473	0.18%	0.042%
18	13.880	1832	1837	1844	rBV2	97802	157704	4.37%	1.030%
19	14.168	1879	1886	1895	rBV2	120200	191587	5.31%	1.252%
20	14.479	1932	1939	1946	rBV	928765	1430296	39.63%	9.344%
21	14.708	1972	1978	1981	rBV4	13457	27573	0.76%	0.180%
22	14.838	1997	2000	2004	rVB3	5512	6445	0.18%	0.042%
23	15.002	2023	2028	2030	rBV2	7619	9081	0.25%	0.059%
24	15.178	2055	2058	2061	rVB	4354	6334	0.18%	0.041%
25	15.378	2089	2092	2095	rBV2	5170	6766	0.19%	0.044%
26	15.472	2100	2108	2117	rBV	182430	286082	7.93%	1.869%
27	15.602	2126	2130	2137	rVB3	19829	30981	0.86%	0.202%
28	15.837	2164	2170	2176	rBV3	22459	39256	1.09%	0.256%
29	16.195	2227	2231	2235	rBV2	5720	10917	0.30%	0.071%
30	16.312	2247	2251	2253	rVB4	5154	6513	0.18%	0.043%
31	16.365	2258	2260	2263	rVB2	4842	5493	0.15%	0.036%
32	16.594	2297	2299	2304	rVB3	5213	7442	0.21%	0.049%
33	16.653	2304	2309	2312	rBV	3814	5806	0.16%	0.038%
34	16.730	2317	2322	2325	rVB6	5696	10020	0.28%	0.065%
35	17.229	2400	2407	2413	rBV	1354930	1944880	53.89%	12.706%
36	17.329	2418	2424	2433	rVB	179771	295936	8.20%	1.933%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063201.D
 Acq On : 7 Nov 2024 14:19
 Operator : RC/JU
 Sample : P4634-15DL 10X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CC0R4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	17.799	2500	2504	2506	rBV4	11446	11480	0.32%	0.075%
38	18.016	2539	2541	2544	rVB3	5567	5546	0.15%	0.036%
39	18.128	2558	2560	2565	rBV5	13616	17447	0.48%	0.114%
40	18.733	2660	2663	2664	rBV3	8071	6837	0.19%	0.045%
41	18.804	2674	2675	2678	rBV2	7188	8072	0.22%	0.053%
42	19.526	2796	2798	2799	rBV2	10023	7603	0.21%	0.050%
43	19.626	2809	2815	2820	rBV	269239	386560	10.71%	2.525%
44	19.667	2820	2822	2825	rVB3	17258	17319	0.48%	0.113%
45	21.383	3109	3114	3123	rVB	2821237	3608728	100.00%	23.576%
46	21.483	3125	3131	3138	rVV2	1470952	2266270	62.80%	14.805%
47	24.309	3609	3612	3619	rVB2	137405	260660	7.22%	1.703%
48	24.520	3639	3648	3659	rVB	890461	2377999	65.90%	15.535%




Sum of corrected areas: 15307020

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063201.D
Acq On : 7 Nov 2024 14:19
Operator : RC/JU
Sample : P4634-15DL 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CC0R4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

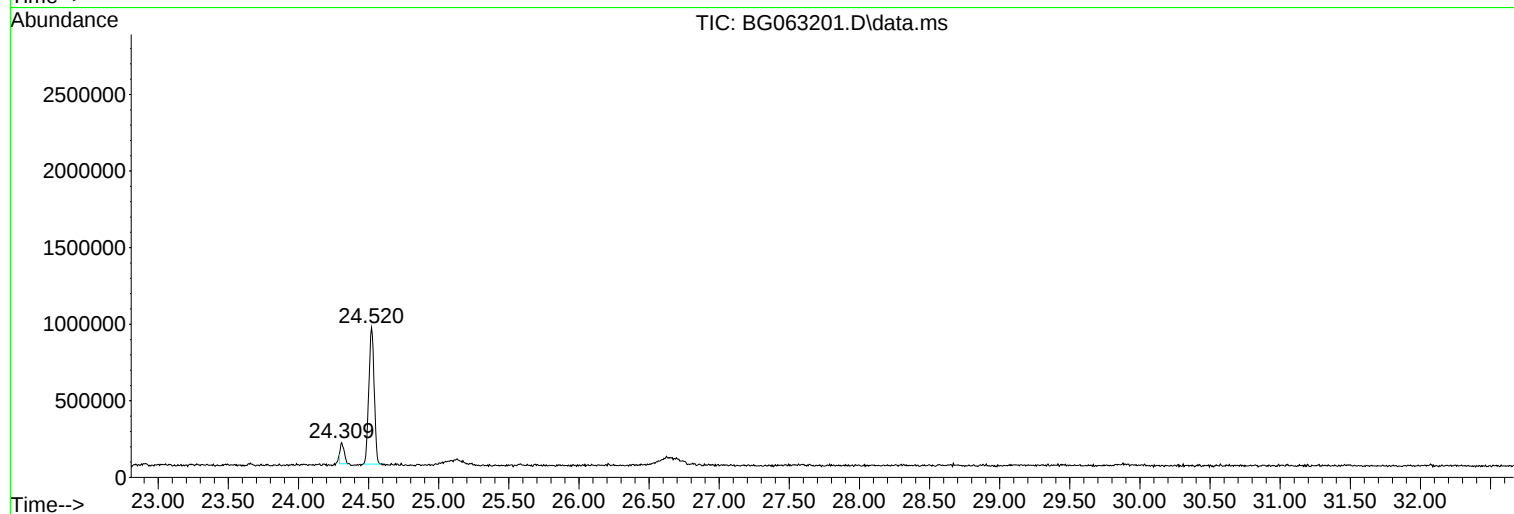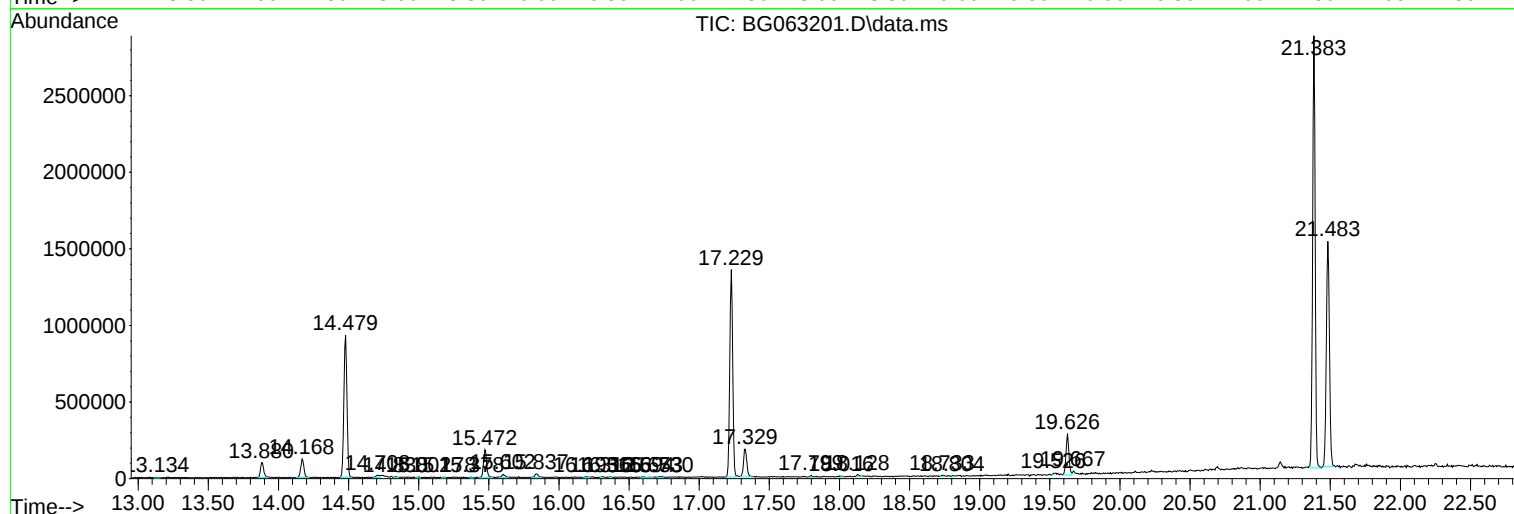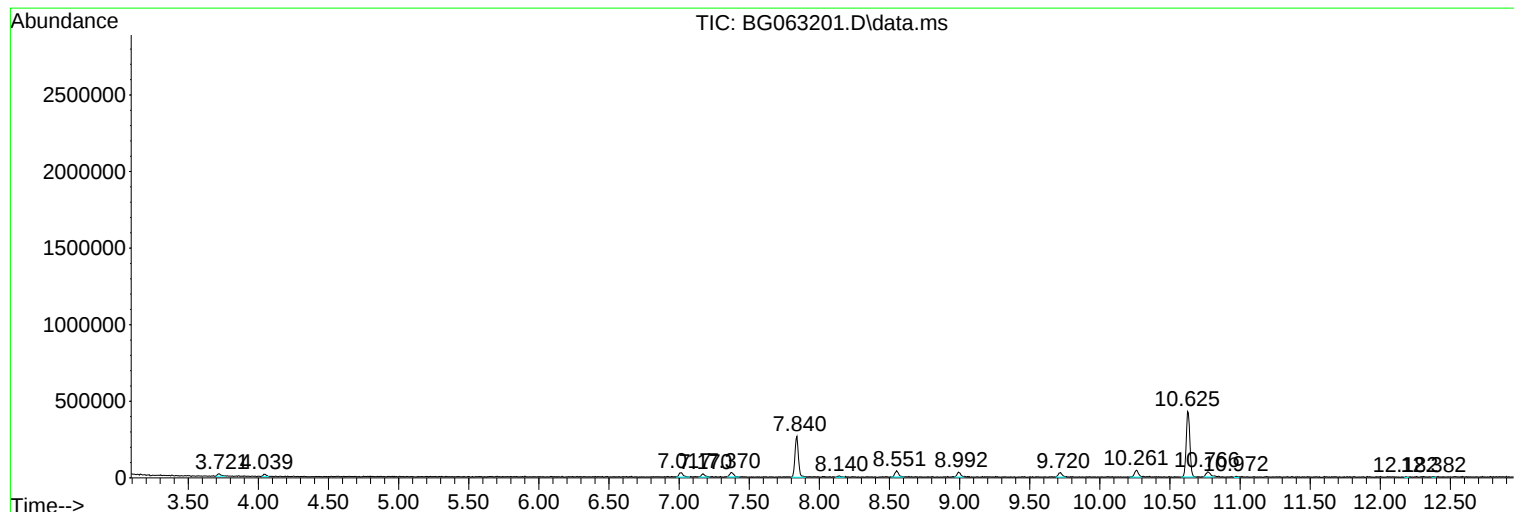

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063201.D
Acq On : 7 Nov 2024 14:19
Operator : RC/JU
Sample : P4634-15DL 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CC0R4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063201.D
Acq On : 7 Nov 2024 14:19
Operator : RC/JU
Sample : P4634-15DL 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CC0R4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc