

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063207.D
Acq On : 7 Nov 2024 18:10
Operator : RC/JU
Sample : PB164682BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK682

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BG063207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	34	37	40	rBV3	15111	18791	0.58%	0.059%
2	3.711	102	106	117	rBV	206647	342368	10.65%	1.076%
3	3.805	121	122	124	rBV2	6224	5026	0.16%	0.016%
4	4.052	159	164	171	rVB	30596	50435	1.57%	0.159%
5	4.140	176	179	183	rVB3	3782	5282	0.16%	0.017%
6	4.240	193	196	199	rBV4	5046	5148	0.16%	0.016%
7	4.974	317	321	324	rVB6	4647	7346	0.23%	0.023%
8	5.003	324	326	329	rBV2	4502	4239	0.13%	0.013%
9	5.127	345	347	350	rVB3	4494	5234	0.16%	0.016%
10	5.180	354	356	358	rVB3	5371	4406	0.14%	0.014%
11	5.197	358	359	362	rBV3	6323	5307	0.17%	0.017%
12	5.350	380	385	386	rBV3	4959	4926	0.15%	0.015%
13	5.955	486	488	492	rBV	3122	4228	0.13%	0.013%
14	6.231	532	535	538	rBV3	4072	4495	0.14%	0.014%
15	6.884	643	646	649	rVB3	5776	4322	0.13%	0.014%
16	7.013	661	668	677	rBV2	328326	562017	17.49%	1.767%
17	7.171	689	695	702	rBV	210834	345989	10.77%	1.088%
18	7.377	723	730	738	rVB	290746	501968	15.62%	1.578%
19	7.718	786	788	792	rVB3	4816	6837	0.21%	0.021%
20	7.841	801	809	819	rBV	302920	523727	16.30%	1.646%
21	8.200	867	870	875	rBV4	4769	8863	0.28%	0.028%
22	8.311	888	889	894	rVB2	5580	5825	0.18%	0.018%
23	8.546	922	929	939	rBV3	440653	749059	23.31%	2.355%
24	8.846	977	980	982	rBV	3895	5581	0.17%	0.018%
25	8.993	998	1005	1013	rBV	314364	560714	17.45%	1.763%
26	9.146	1029	1031	1033	rVB2	5912	4671	0.15%	0.015%
27	9.245	1046	1048	1053	rBV2	3422	4663	0.15%	0.015%
28	9.639	1112	1115	1118	rBV	3996	5424	0.17%	0.017%
29	9.715	1118	1128	1135	rBV	300839	547397	17.03%	1.721%
30	9.821	1143	1146	1148	rBV3	4337	4950	0.15%	0.016%
31	10.256	1212	1220	1229	rBV	462906	866487	26.96%	2.724%
32	10.415	1246	1247	1253	rVB2	4191	6797	0.21%	0.021%
33	10.626	1273	1283	1292	rBV	502534	890530	27.71%	2.799%
34	10.761	1299	1306	1319	rBV	422643	815059	25.36%	2.562%
35	11.343	1404	1405	1408	rBV	4176	4686	0.15%	0.015%
36	11.390	1410	1413	1416	rVB2	3810	5404	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
 Data File : BG063207.D
 Acq On : 7 Nov 2024 18:10
 Operator : RC/JU
 Sample : PB164682BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK682

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	11.837	1488	1489	1493	rVB	5868	4458	0.14%	0.014%
38	12.236	1554	1557	1562	rVB3	8325	12586	0.39%	0.040%
39	12.677	1629	1632	1636	rVB	3193	4623	0.14%	0.015%
40	13.881	1828	1837	1845	rBV	1001126	1435238	44.66%	4.512%
41	13.981	1850	1854	1855	rBV3	3784	4452	0.14%	0.014%
42	13.999	1855	1857	1863	rVB4	4676	8017	0.25%	0.025%
43	14.052	1863	1866	1869	rBV2	3402	4988	0.16%	0.016%
44	14.169	1878	1886	1895	rBV2	1073055	1712166	53.28%	5.382%
45	14.475	1931	1938	1947	rBV	1007656	1618753	50.37%	5.088%
46	14.539	1947	1949	1953	rVB2	4337	5395	0.17%	0.017%
47	14.686	1967	1974	1988	rBV	347709	655695	20.40%	2.061%
48	14.892	2005	2009	2010	rBV2	6698	6774	0.21%	0.021%
49	14.909	2010	2012	2014	rVB3	7191	5929	0.18%	0.019%
50	15.015	2029	2030	2033	rVB3	5109	4531	0.14%	0.014%
51	15.473	2100	2108	2115	rBV	1530885	2265215	70.48%	7.121%
52	15.597	2123	2129	2139	rBV	397481	613122	19.08%	1.927%
53	15.708	2145	2148	2154	rVB4	12209	18767	0.58%	0.059%
54	15.932	2182	2186	2188	rBV4	6520	7364	0.23%	0.023%
55	15.979	2193	2194	2199	rVB4	4172	4844	0.15%	0.015%
56	16.049	2204	2206	2209	rVB3	5747	6297	0.20%	0.020%
57	16.255	2238	2241	2243	rBV2	6523	5725	0.18%	0.018%
58	16.343	2251	2256	2257	rBV4	4996	6448	0.20%	0.020%
59	16.555	2289	2292	2294	rVB2	5299	5169	0.16%	0.016%
60	16.613	2299	2302	2305	rBV4	6080	8087	0.25%	0.025%
61	16.672	2311	2312	2315	rBV2	4049	4674	0.15%	0.015%
62	16.719	2318	2320	2323	rVB3	5998	6770	0.21%	0.021%
63	16.848	2338	2342	2343	rBV2	5406	7212	0.22%	0.023%
64	16.931	2355	2356	2361	rVB2	6571	5305	0.17%	0.017%
65	16.983	2361	2365	2368	rBV2	4950	8306	0.26%	0.026%
66	17.142	2389	2392	2394	rBV2	4276	5448	0.17%	0.017%
67	17.230	2399	2407	2415	rBV	1411024	2158283	67.16%	6.784%
68	17.324	2417	2423	2435	rVB2	1695044	2579470	80.26%	8.108%
69	17.465	2445	2447	2451	rVB3	4878	5194	0.16%	0.016%
70	17.518	2451	2456	2457	rBV3	6577	7704	0.24%	0.024%
71	17.965	2530	2532	2536	rBV4	4129	4225	0.13%	0.013%
72	18.282	2584	2586	2589	rVB4	6938	4715	0.15%	0.015%
73	18.311	2589	2591	2593	rBV2	4015	4226	0.13%	0.013%
74	18.523	2625	2627	2630	rVB2	8521	5704	0.18%	0.018%
75	18.652	2648	2649	2651	rBV2	7004	4710	0.15%	0.015%
76	18.728	2659	2662	2664	rBV4	7649	7925	0.25%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063207.D
Acq On : 7 Nov 2024 18:10
Operator : RC/JU
Sample : PB164682BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK682

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

77	18.787	2671	2672	2675	rBV3	4360	4961	0.15%	0.016%
78	18.946	2697	2699	2704	rBV4	6286	9575	0.30%	0.030%
79	19.034	2711	2714	2715	rBV2	6373	4982	0.16%	0.016%
80	19.193	2737	2741	2745	rVB2	23822	32555	1.01%	0.102%
81	19.257	2748	2752	2756	rBV2	29274	38891	1.21%	0.122%
82	19.316	2760	2762	2763	rVB2	7009	4347	0.14%	0.014%
83	19.539	2797	2800	2801	rBV3	10673	11301	0.35%	0.036%
84	19.627	2809	2815	2824	rBV	2199030	3213798	100.00%	10.102%
85	21.478	3124	3130	3139	rVB	1595708	2567331	79.88%	8.070%
86	24.310	3603	3612	3624	rVB	1220740	3105527	96.63%	9.762%
87	24.516	3638	3647	3659	rVB	1001491	2676131	83.27%	8.412%




Sum of corrected areas: 31812114

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063207.D
Acq On : 7 Nov 2024 18:10
Operator : RC/JU
Sample : PB164682BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK682

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

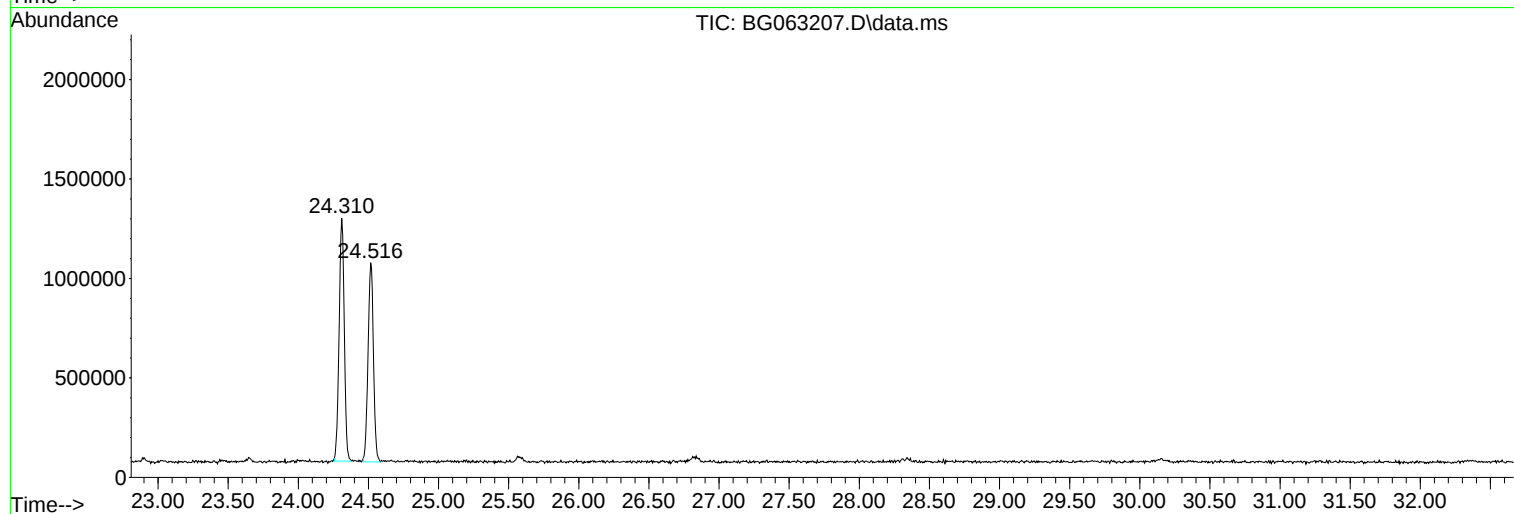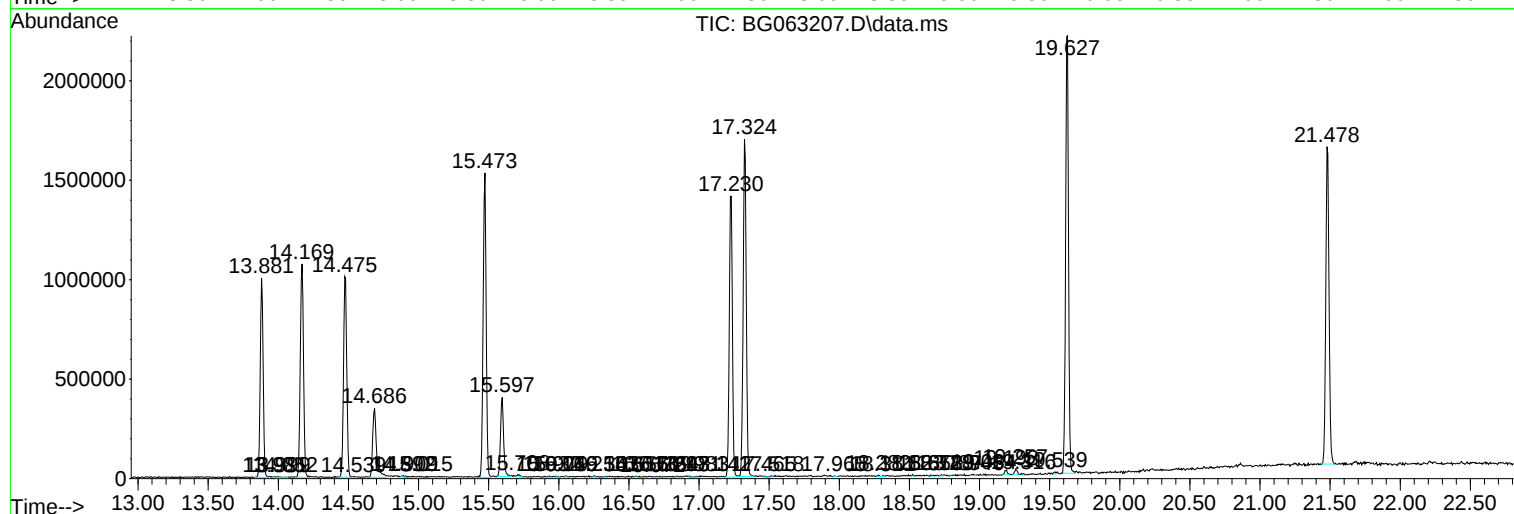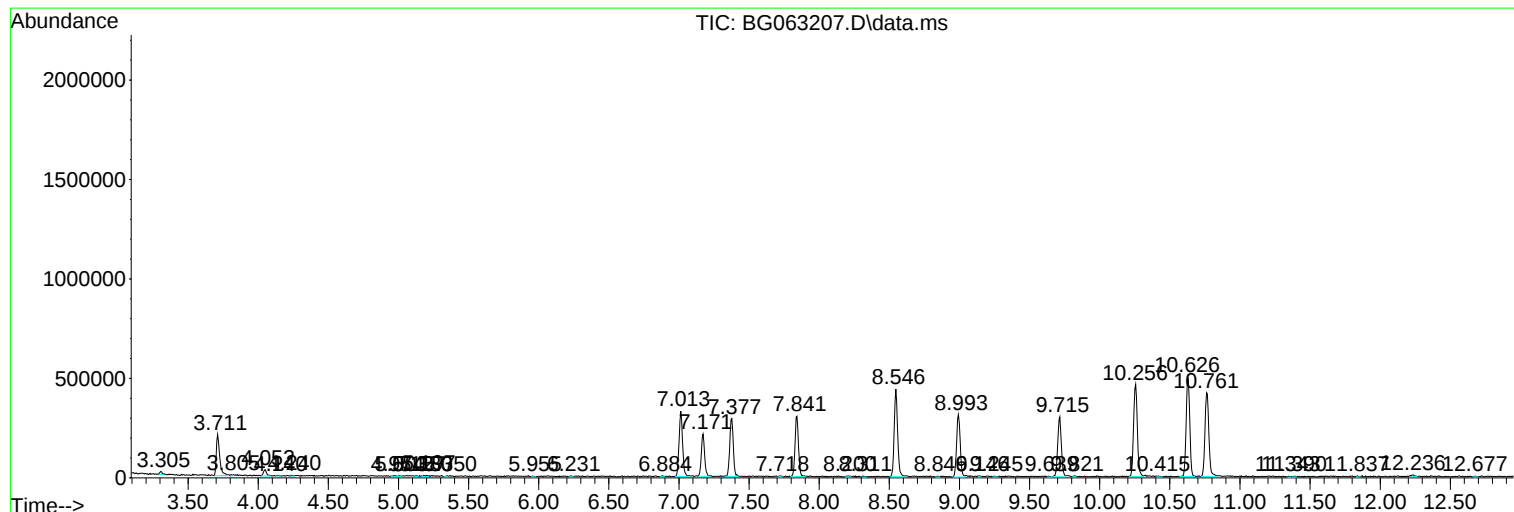

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063207.D
Acq On : 7 Nov 2024 18:10
Operator : RC/JU
Sample : PB164682BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK682

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110624\
Data File : BG063207.D
Acq On : 7 Nov 2024 18:10
Operator : RC/JU
Sample : PB164682BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK682

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------