

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110716\
 Data File : BG024736.D
 Acq On : 7 Nov 2016 19:45
 Operator : UM/SJ
 Sample : H5544-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GW-110-10.3-22.0

Quant Time: Nov 08 00:03:45 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.26	152	111973	20.00	ng	0.00
21) Naphthalene-d8	11.09	136	407546	20.00	ng	-0.02
38) Acenaphthene-d10	14.88	164	329408	20.00	ng	0.00
63) Phenanthrene-d10	17.62	188	740364	20.00	ng	0.00
75) Chrysene-d12	21.91	240	1044277	20.00	ng	-0.02
86) Perylene-d12	25.34	264	1097760	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.79	112	522683	76.51	ng	0.00
7) Phenol-d6	7.40	99	498595	53.20	ng	0.00
23) Nitrobenzene-d5	9.43	82	888728	99.29	ng	-0.02
41) 2,4,6-Tribromophenol	16.36	330	772107	156.89	ng	0.00
44) 2-Fluorobiphenyl	13.50	172	1906945	96.22	ng	-0.02
78) Terphenyl-d14	20.20	244	3114052	89.11	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.32	163	140859	6.02	ng	Qvalue # 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110716\
Data File : BG024736.D
Acq On : 7 Nov 2016 19:45
Operator : UM/SJ
Sample : H5544-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GW-110-10.3-22.0

Quant Time: Nov 08 00:03:45 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

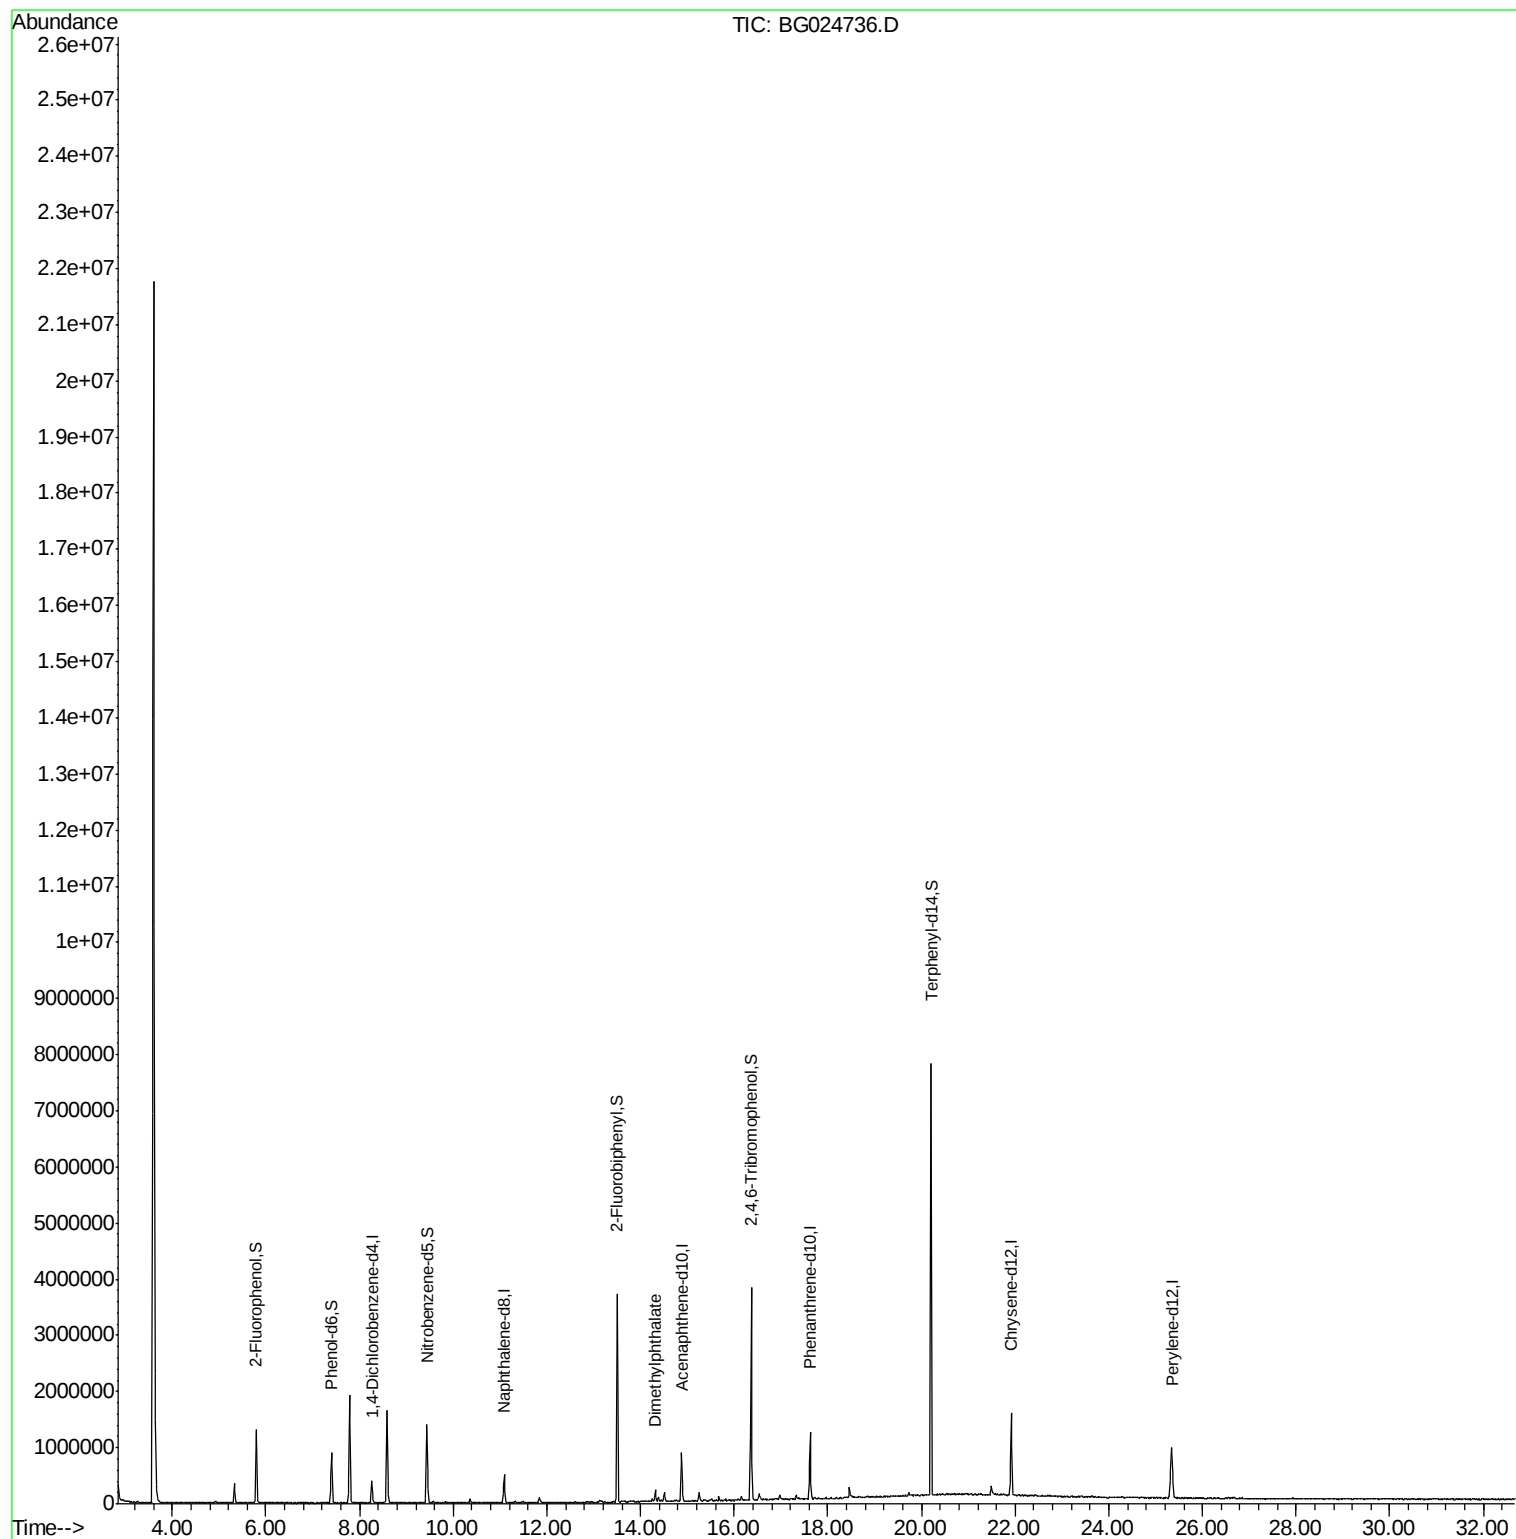

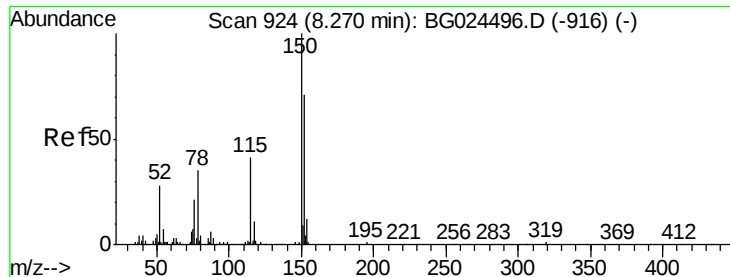

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.26 min Scan# 923

Delta R.T. -0.01 min

Lab File: BG024736.D

Acq: 7 Nov 2016 19:45

Instrument :

BNA_G

ClientSampleId :

GW-110-10.3-22.0


Tgt Ion:152 Resp: 111973

Ion Ratio Lower Upper

152 100

150 154.2 114.0 171.0

115 62.1 48.1 72.1

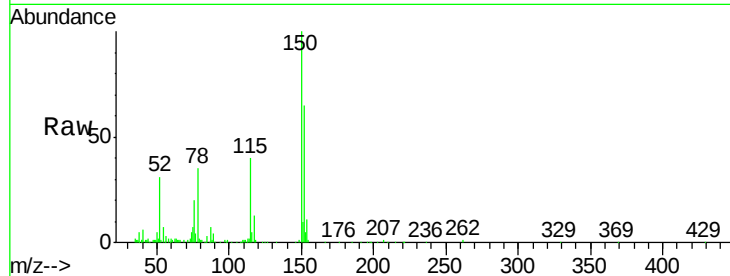

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

120000

100000

80000

60000



40000

20000

0

8.20 8.25 8.30

Time-->

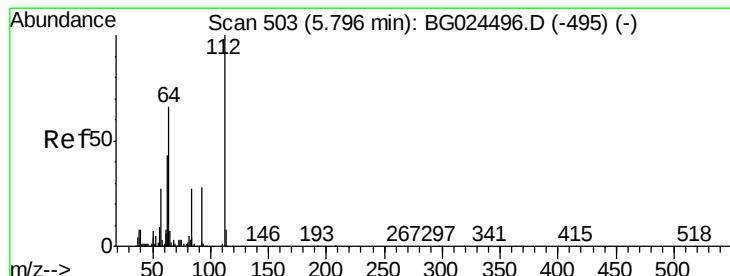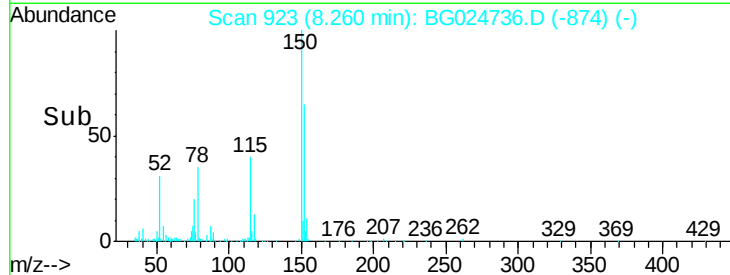

#5

2-Fluorophenol

Concen: 76.51 ng

RT: 5.79 min Scan# 503

Delta R.T. -0.00 min

Lab File: BG024736.D

Acq: 7 Nov 2016 19:45


Tgt Ion:112 Resp: 522683

Ion Ratio Lower Upper

112 100

64 74.3 61.8 92.6

63 45.2 37.2 55.8

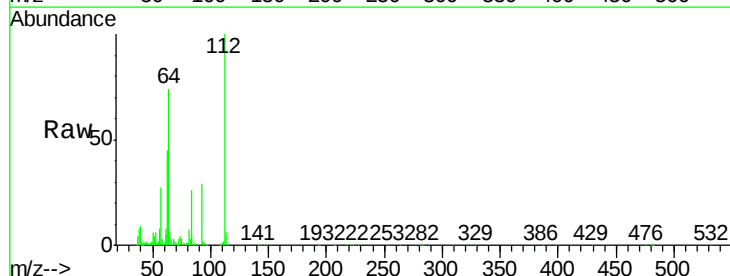

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

400000

300000


200000

100000

0

5.70 5.75 5.80 5.85 5.90

Time-->

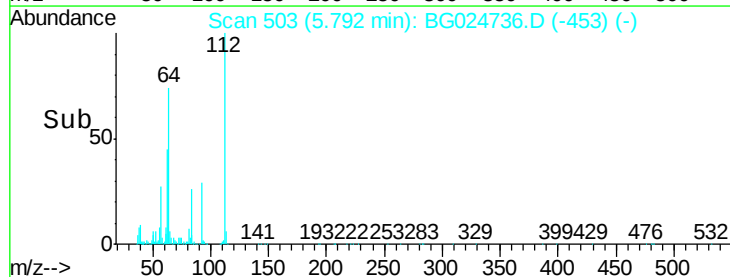



#7

Phenol-d6

Concen: 53.20 ng

RT: 7.40 min Scan# 776

Delta R.T. -0.00 min

Lab File: BG024736.D

Acq: 7 Nov 2016 19:45

Instrument :

BNA_G

ClientSampleId :

GW-110-10.3-22.0


Tgt Ion: 99 Resp: 498595

Ion Ratio Lower Upper

99 100

42 22.6 20.5 30.7




71 48.5 37.6 56.4

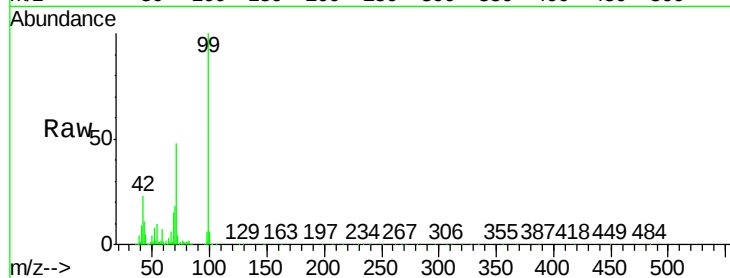

Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

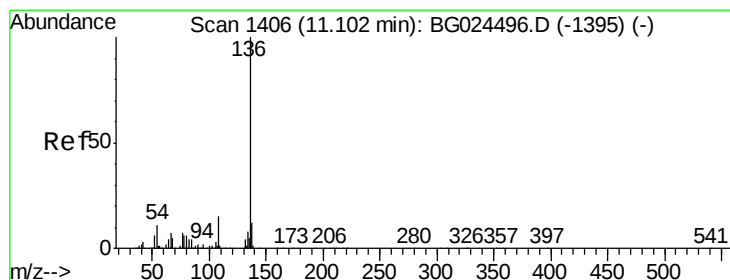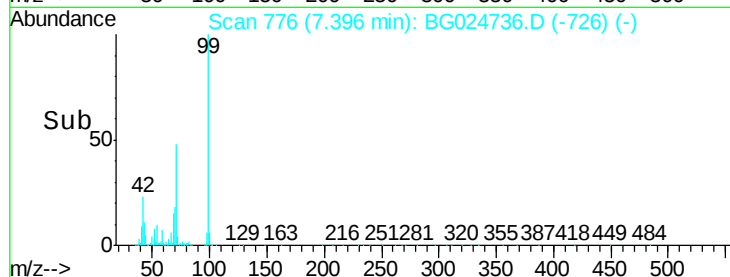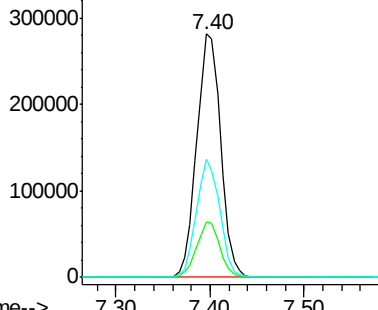

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.09 min Scan# 1404

Delta R.T. -0.02 min

Lab File: BG024736.D

Acq: 7 Nov 2016 19:45

Tgt Ion: 136 Resp: 407546


Ion Ratio Lower Upper

136 100

137 11.6 8.9 13.3

54 10.0 9.3 13.9

68 4.9 5.1 7.7#


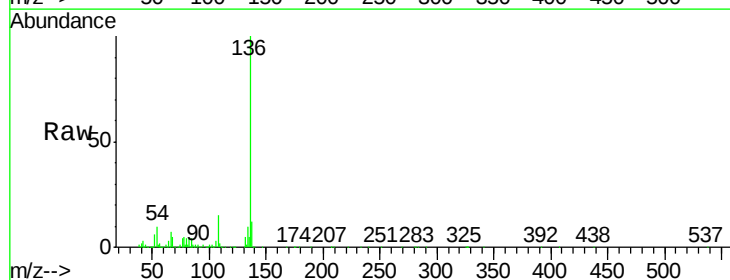



Abundance Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



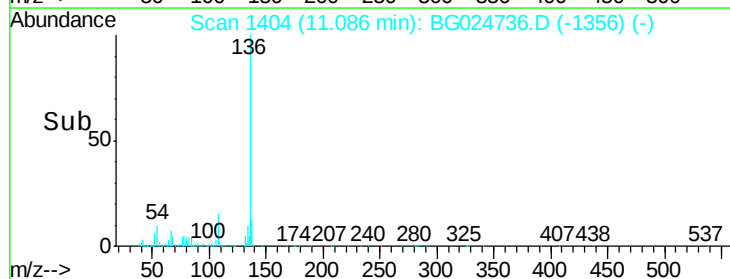
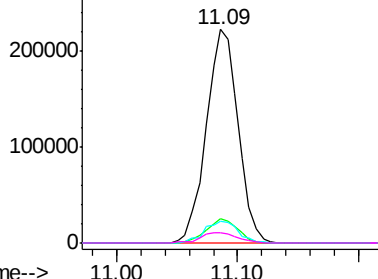


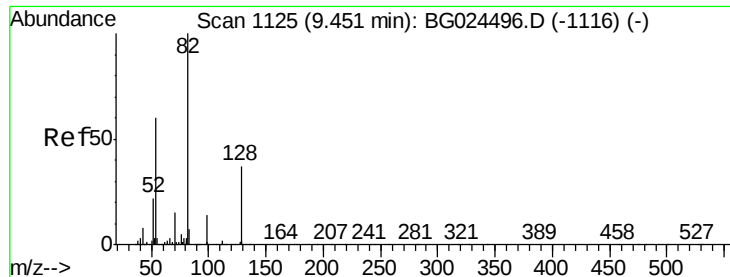

#23
Nitrobenzene-d5
Concen: 99.29 ng
RT: 9.43 min Scan# 1123
Delta R.T. -0.02 min
Lab File: BG024736.D
Acq: 7 Nov 2016 19:45

Instrument :
BNA_G
ClientSampleId :
GW-110-10.3-22.0

Tgt Ion: 82 Resp: 888728
Ion Ratio Lower Upper
82 100
128 36.9 26.4 39.6
54 56.2 49.4 74.2

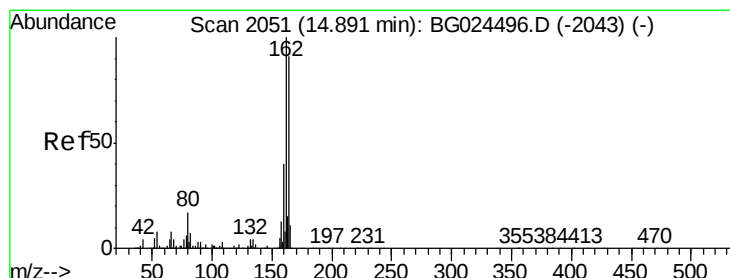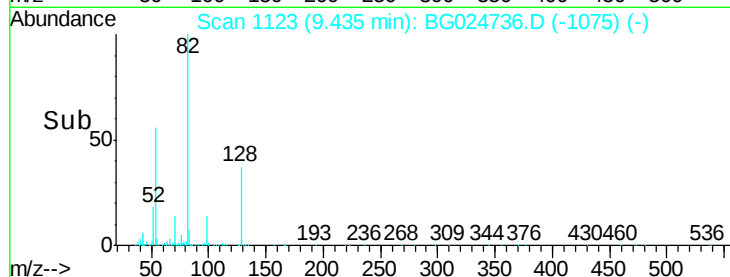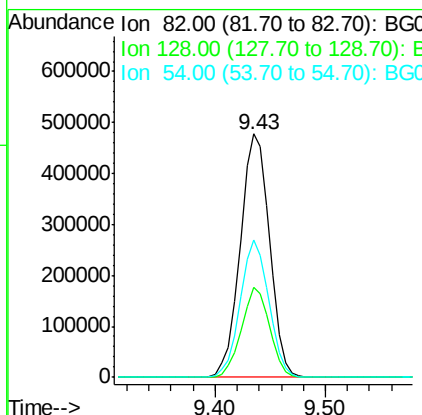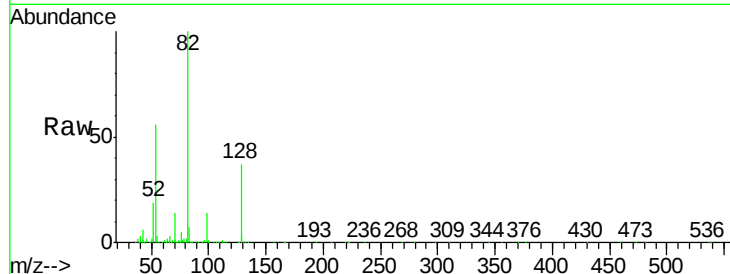

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.88 min Scan# 2050
Delta R.T. -0.01 min
Lab File: BG024736.D
Acq: 7 Nov 2016 19:45

Tgt Ion: 164 Resp: 329408
Ion Ratio Lower Upper
164 100
162 106.4 85.1 127.7
160 43.6 34.7 52.1

