

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110716\
 Data File : BG024737.D
 Acq On : 7 Nov 2016 20:24
 Operator : UM/SJ
 Sample : H5544-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GW-111-10.5-21.0

Quant Time: Nov 08 00:03:56 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.26	152	98668	20.00	ng	0.00
21) Naphthalene-d8	11.09	136	400266	20.00	ng	-0.02
38) Acenaphthene-d10	14.88	164	308985	20.00	ng	-0.02
63) Phenanthrene-d10	17.62	188	702295	20.00	ng	0.00
75) Chrysene-d12	21.91	240	987335	20.00	ng	-0.02
86) Perylene-d12	25.34	264	1071055	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.79	112	402135	66.80	ng	0.00
7) Phenol-d6	7.40	99	361132	43.73	ng	0.00
23) Nitrobenzene-d5	9.44	82	844027	96.01	ng	-0.02
41) 2,4,6-Tribromophenol	16.36	330	724904	157.04	ng	0.00
44) 2-Fluorobiphenyl	13.50	172	1807661	97.24	ng	-0.02
78) Terphenyl-d14	20.20	244	2776122	84.02	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.59	79	16393	2.13	ng	Qvalue # 57
49) Dimethylphthalate	14.32	163	167241	7.62	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110716\
Data File : BG024737.D
Acq On : 7 Nov 2016 20:24
Operator : UM/SJ
Sample : H5544-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GW-111-10.5-21.0

Quant Time: Nov 08 00:03:56 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

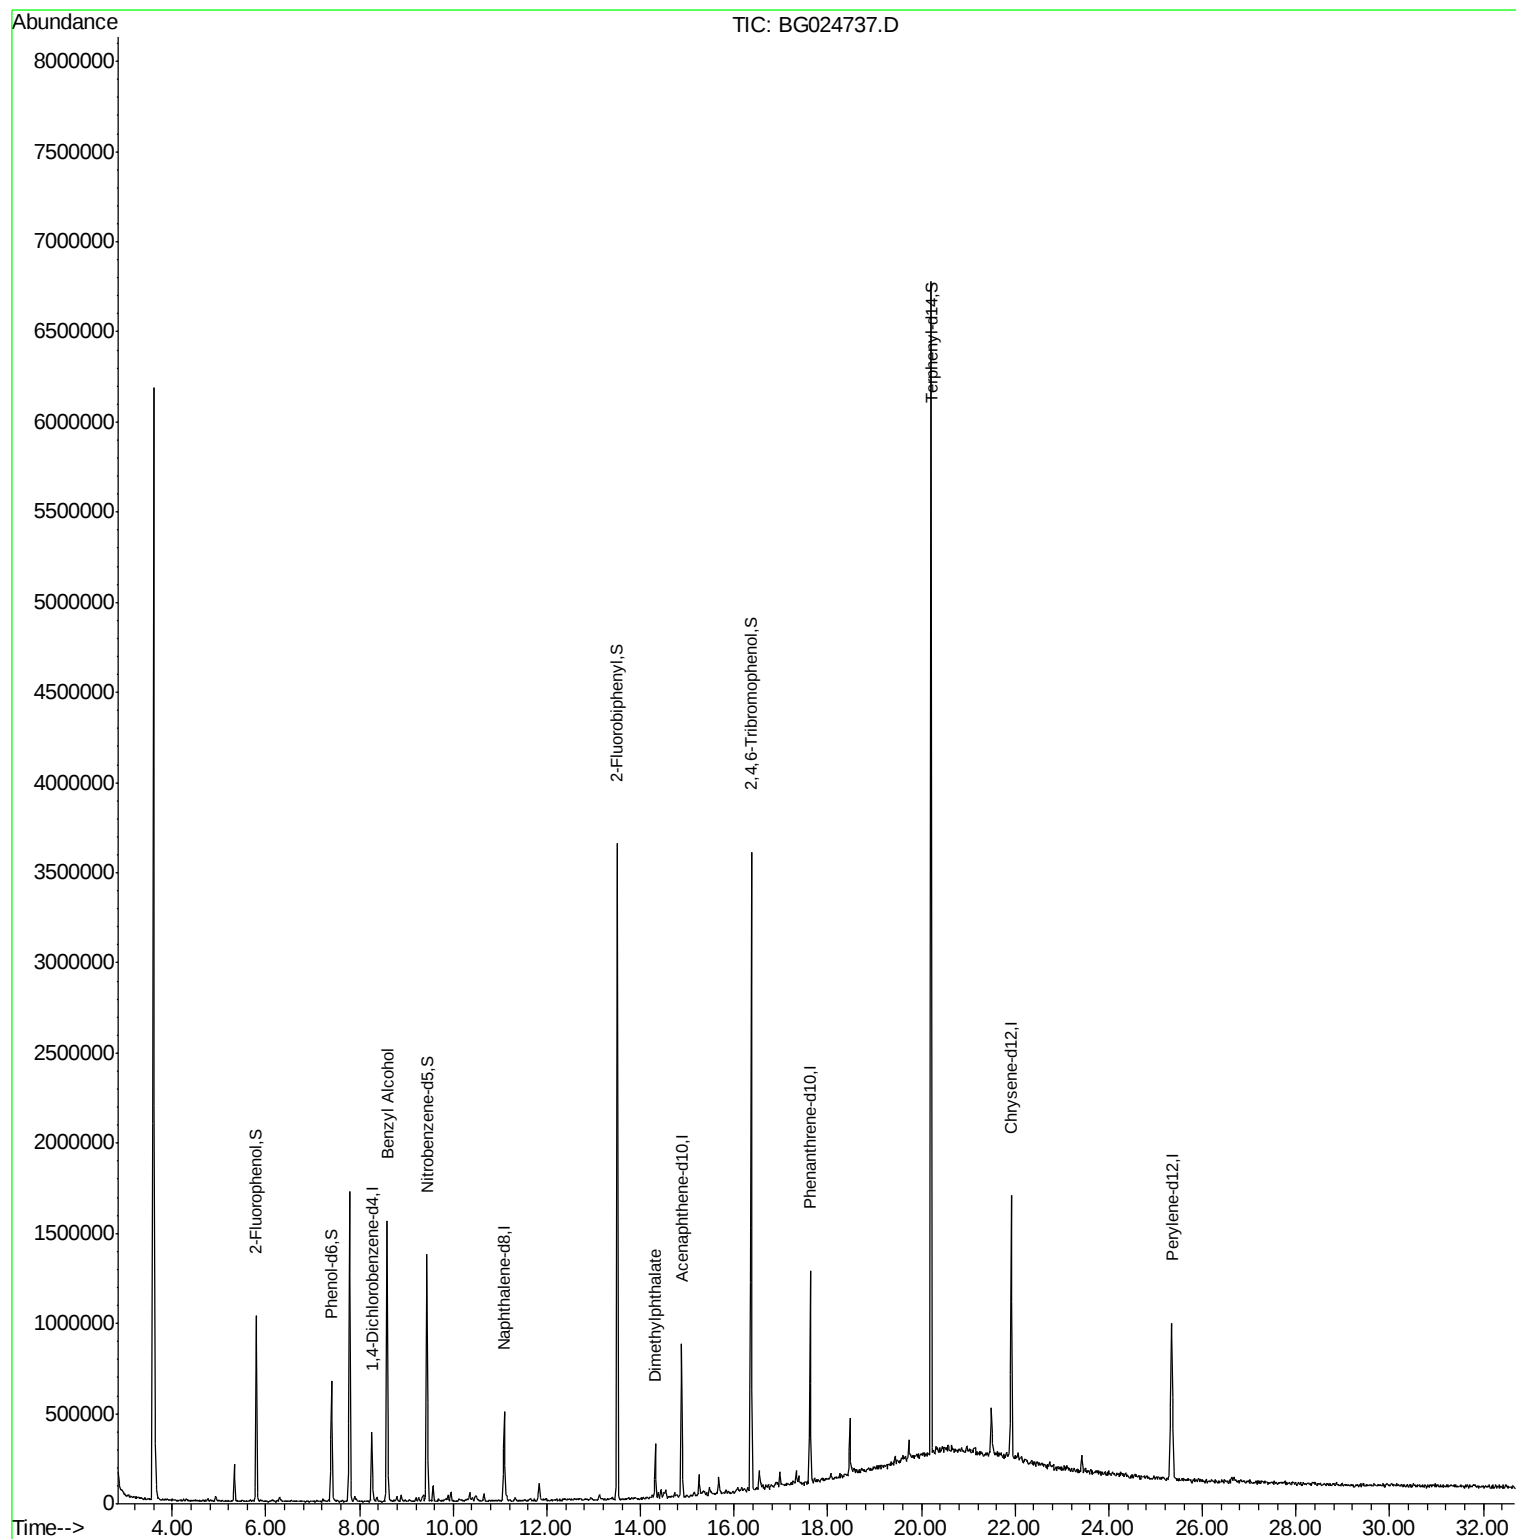

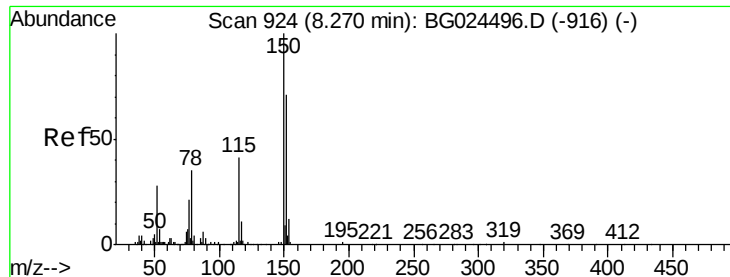

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.26 min Scan# 923

Delta R.T. -0.01 min

Lab File: BG024737.D

Acq: 7 Nov 2016 20:24

Instrument :

BNA_G

ClientSampleId :

GW-111-10.5-21.0


Tgt Ion:152 Resp: 98668

Ion Ratio Lower Upper

152 100

150 137.5 114.0 171.0




115 62.6 48.1 72.1

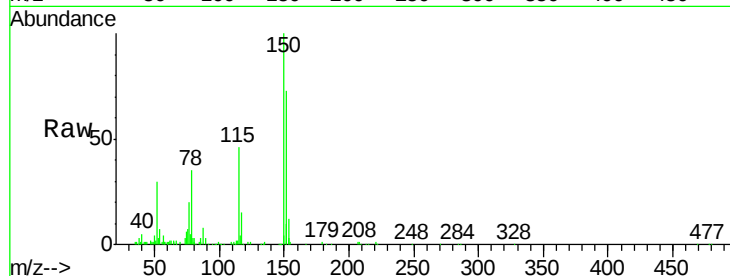

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

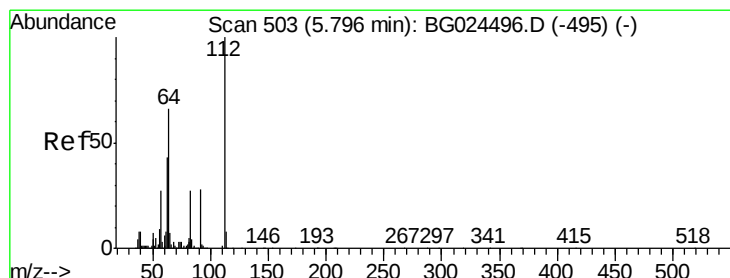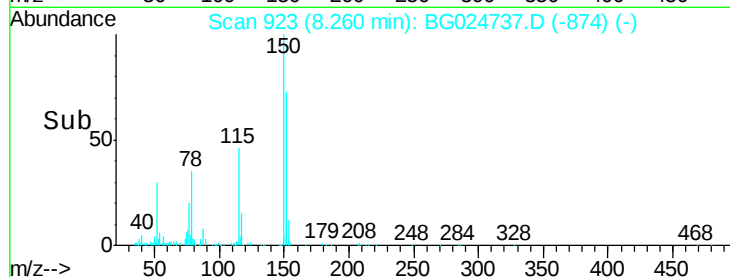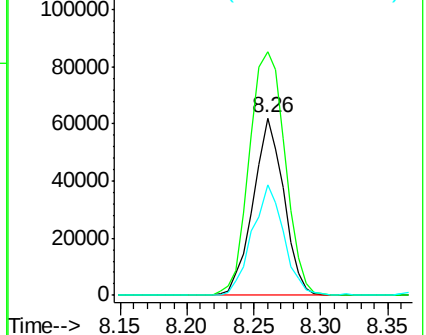

#5

2-Fluorophenol

Concen: 66.80 ng

RT: 5.79 min Scan# 503

Delta R.T. -0.00 min

Lab File: BG024737.D

Acq: 7 Nov 2016 20:24


Tgt Ion:112 Resp: 402135

Ion Ratio Lower Upper

112 100

64 76.2 61.8 92.6



63 45.7 37.2 55.8

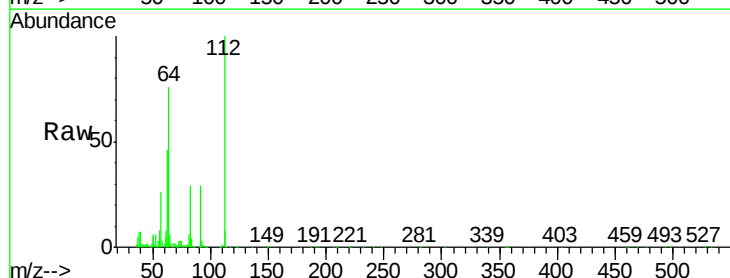

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

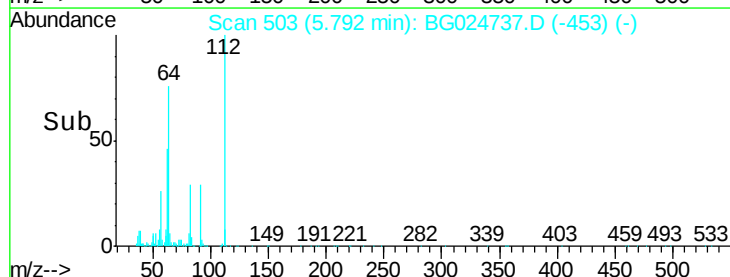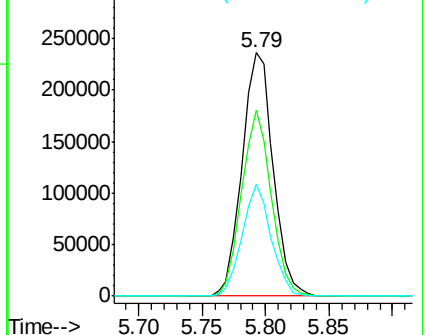



#7

Phenol-d6

Concen: 43.73 ng

RT: 7.40 min Scan# 776

Delta R.T. -0.00 min

Lab File: BG024737.D

Acq: 7 Nov 2016 20:24

Instrument :

BNA_G

ClientSampleId :

GW-111-10.5-21.0


Tgt Ion: 99 Resp: 361132

Ion Ratio Lower Upper




99 100

42 20.3 20.5 30.7#

71 41.6 37.6 56.4

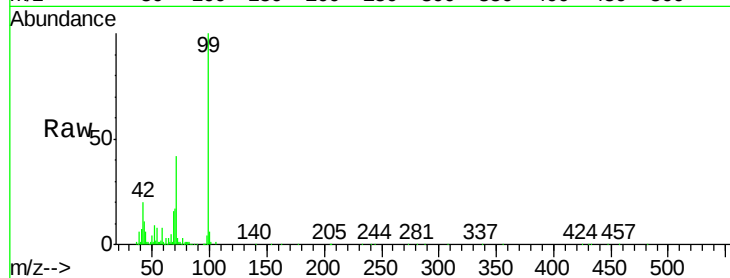

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

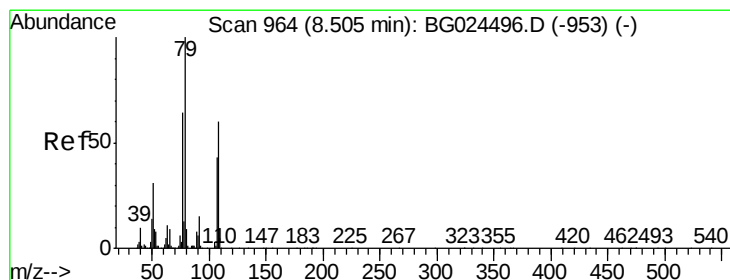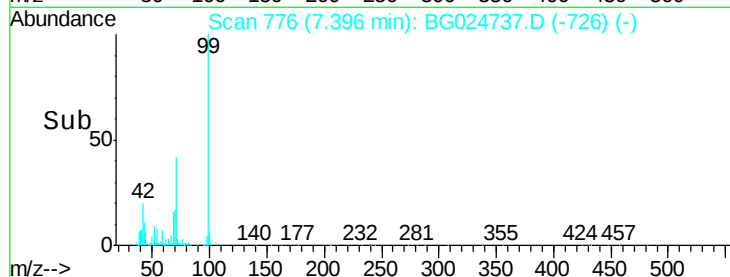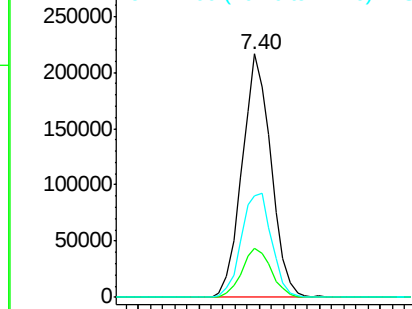

#15

Benzyl Alcohol

Concen: 2.13 ng

RT: 8.59 min Scan# 979

Delta R.T. 0.08 min

Lab File: BG024737.D

Acq: 7 Nov 2016 20:24


Tgt Ion: 79 Resp: 16393

Ion Ratio Lower Upper



79 100

108 28.8 45.5 68.3#

77 105.9 54.3 81.5#

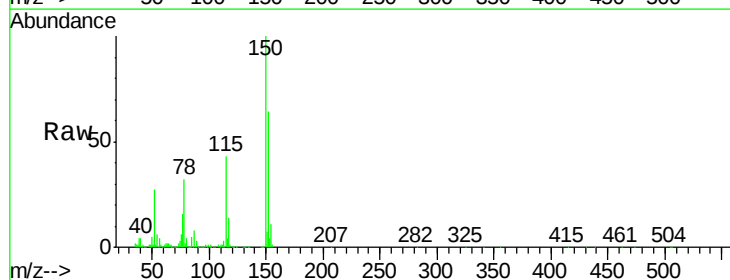

Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC



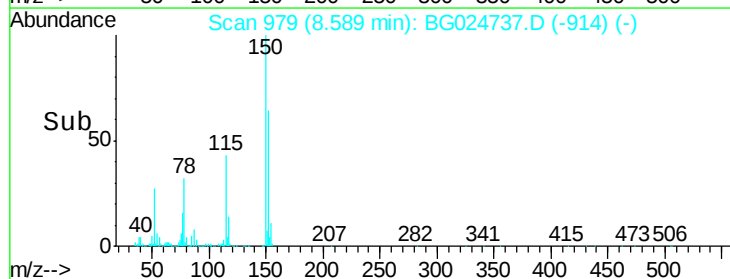
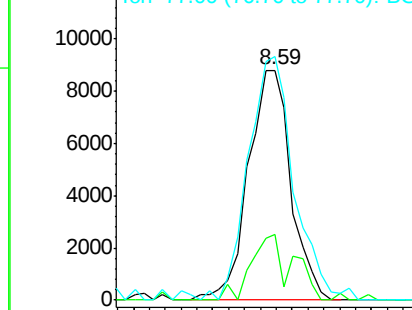




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.09 min Scan# 1404
Delta R.T. -0.02 min
Lab File: BG024737.D
Acq: 7 Nov 2016 20:24




Instrument :
BNA_G
ClientSampleId :
GW-111-10.5-21.0


Tgt Ion:	136	Resp:	400266
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.9	13.3
54	10.6	9.3	13.9
68	6.3	5.1	7.7

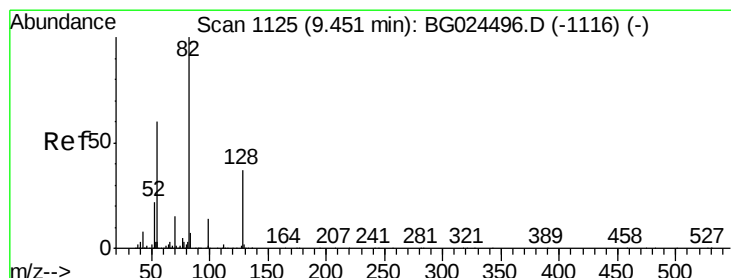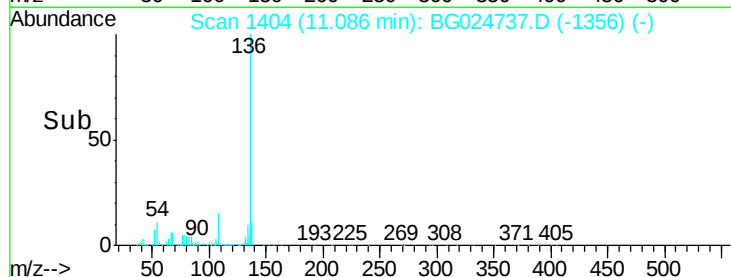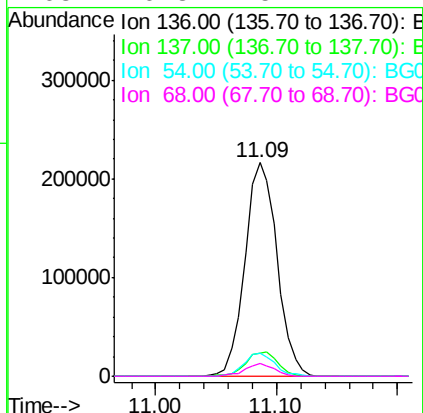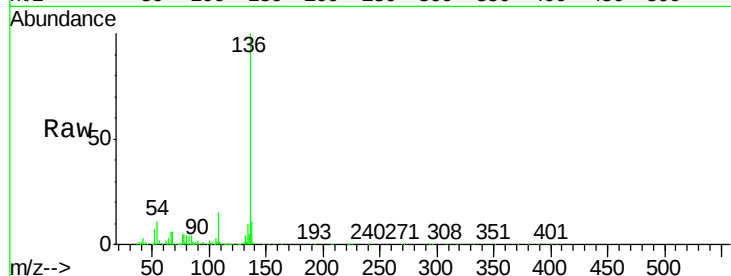

#23
Nitrobenzene-d5
Concen: 96.01 ng
RT: 9.44 min Scan# 1123
Delta R.T. -0.02 min
Lab File: BG024737.D
Acq: 7 Nov 2016 20:24

Tgt Ion:	82	Resp:	844027
Ion	Ratio	Lower	Upper
82	100		
128	35.5	26.4	39.6
54	59.1	49.4	74.2


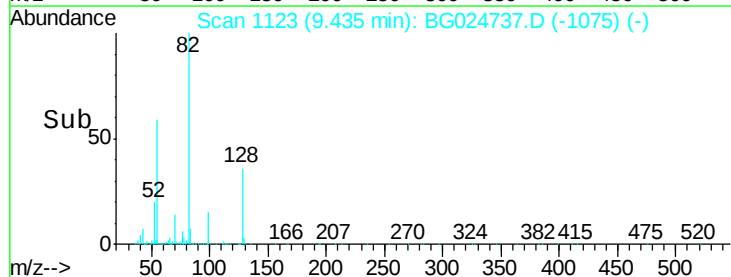
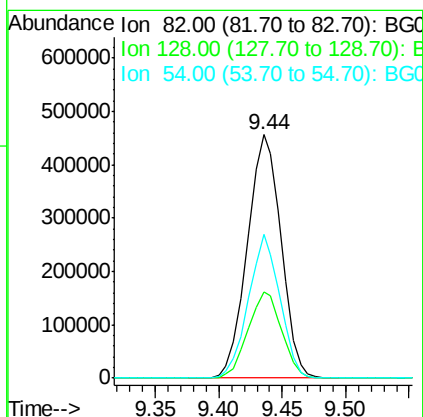
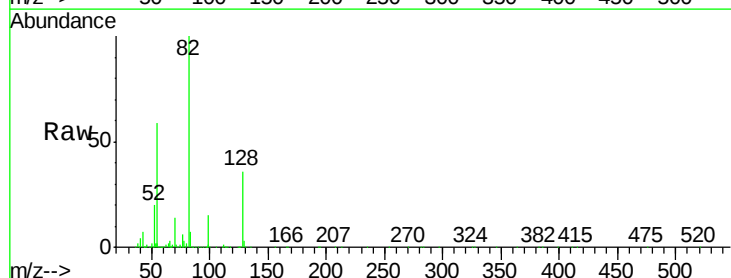


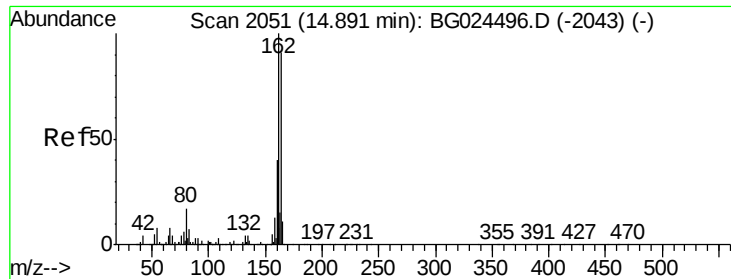

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.88 min Scan# 2049
Delta R.T. -0.02 min
Lab File: BG024737.D
Acq: 7 Nov 2016 20:24




Instrument :
BNA_G
ClientSampleId :
GW-111-10.5-21.0


Tgt Ion:164 Resp: 308985
Ion Ratio Lower Upper
164 100
162 101.6 85.1 127.7
160 44.1 34.7 52.1

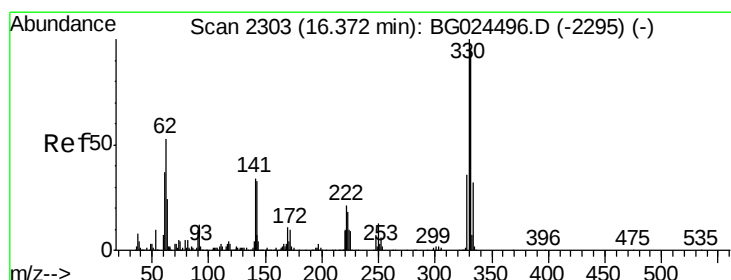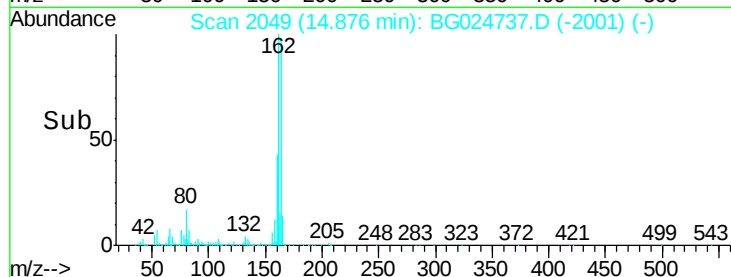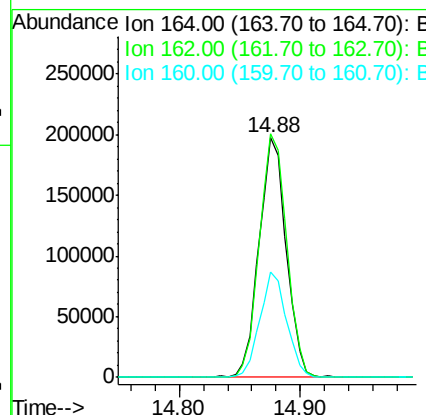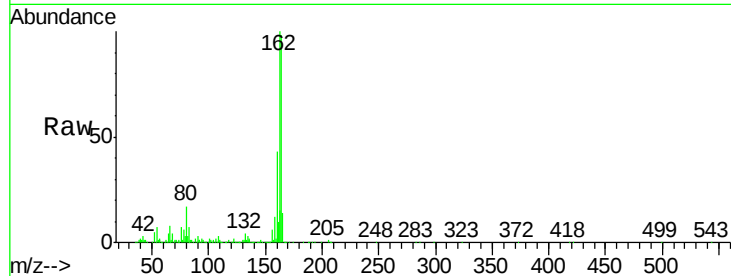

#41
2,4,6-Tribromophenol
Concen: 157.04 ng
RT: 16.36 min Scan# 2302
Delta R.T. -0.01 min
Lab File: BG024737.D
Acq: 7 Nov 2016 20:24

Tgt Ion:330 Resp: 724904
Ion Ratio Lower Upper
330 100
332 95.7 77.3 115.9
141 32.8 32.1 48.1


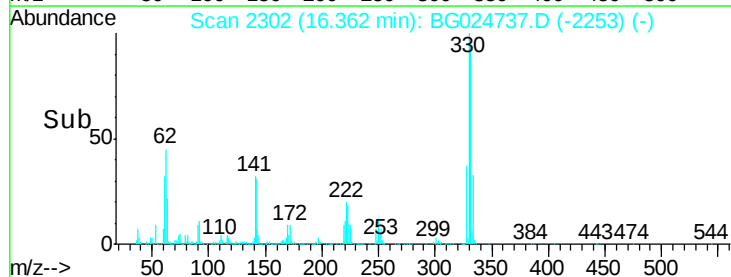
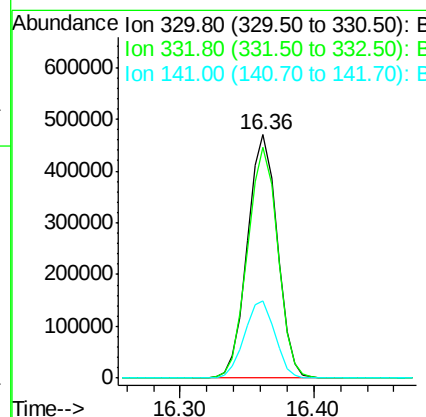
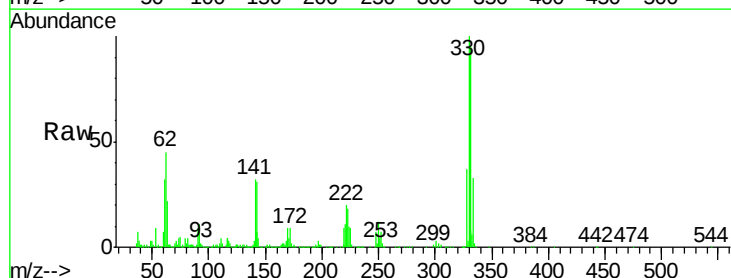


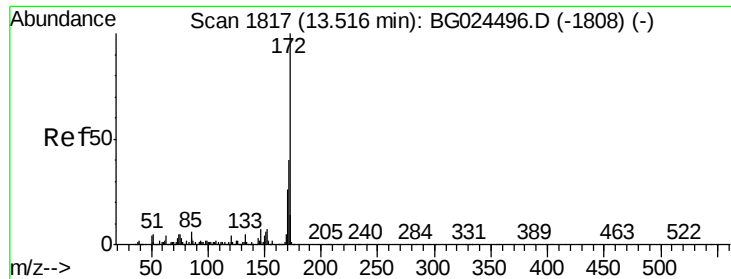

#44
2-Fluorobiphenyl
Concen: 97.24 ng
RT: 13.50 min Scan# 1815
Delta R.T. -0.02 min
Lab File: BG024737.D
Acq: 7 Nov 2016 20:24




Instrument :
BNA_G
ClientSampleId :
GW-111-10.5-21.0


Tgt Ion:172 Resp: 1807661
Ion Ratio Lower Upper
172 100
171 38.2 32.2 48.2
170 26.4 21.8 32.6

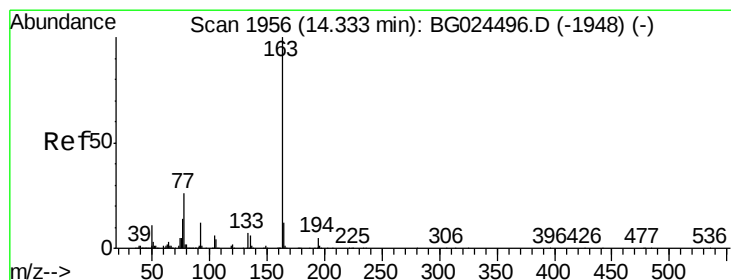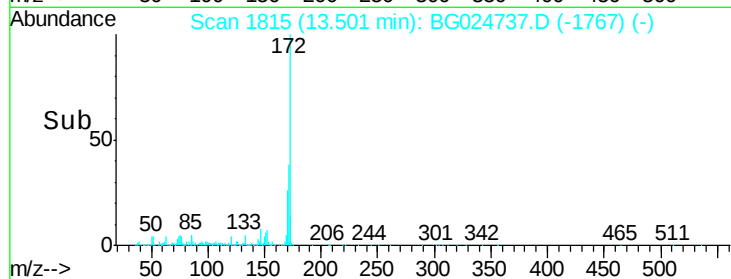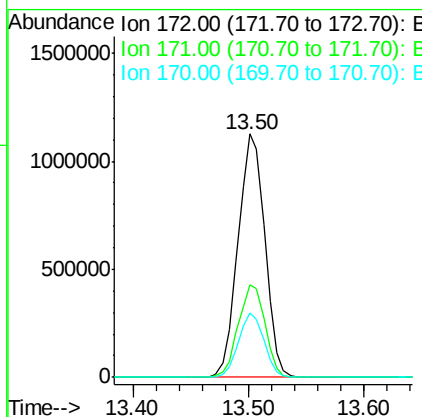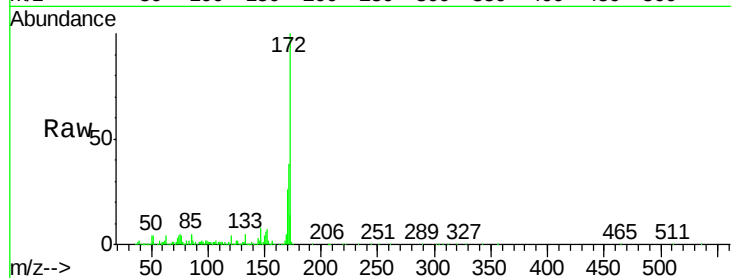

#49
Dimethylphthalate
Concen: 7.62 ng
RT: 14.32 min Scan# 1954
Delta R.T. -0.02 min
Lab File: BG024737.D
Acq: 7 Nov 2016 20:24

Tgt Ion:163 Resp: 167241
Ion Ratio Lower Upper
163 100
194 5.0 3.8 5.6
164 11.8 9.3 13.9

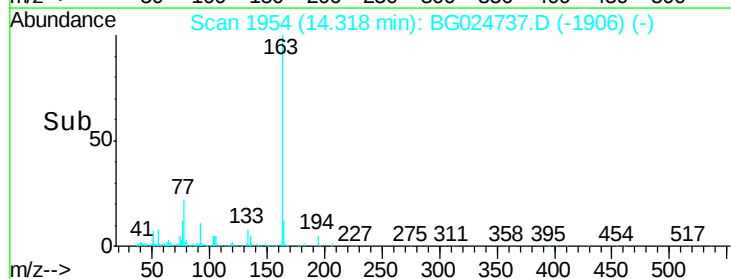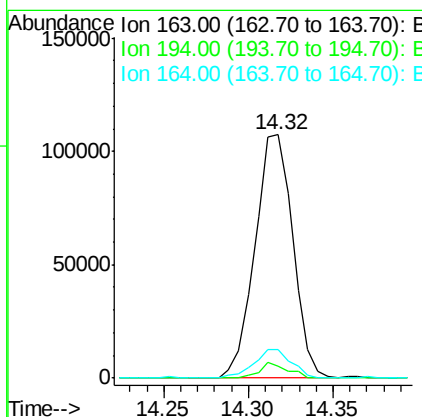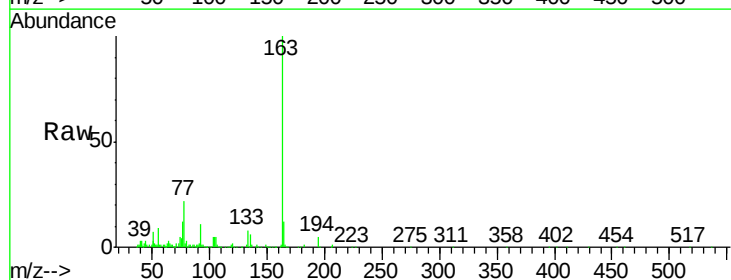

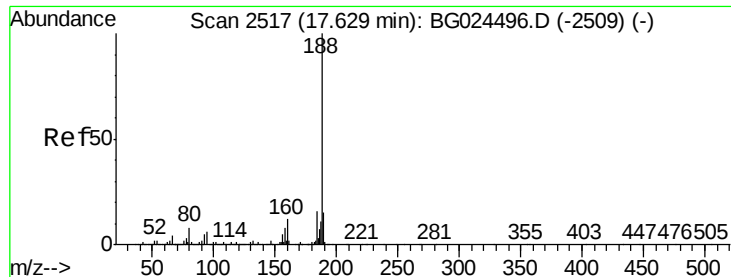

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.62 min Scan# 2516

Delta R.T. -0.01 min

Lab File: BG024737.D

Acq: 7 Nov 2016 20:24

Instrument :

BNA_G

ClientSampleId :

GW-111-10.5-21.0


Tgt Ion:188 Resp: 702295

Ion Ratio Lower Upper

188 100

94 7.7 5.8 8.8


80 7.5 7.5 11.3#

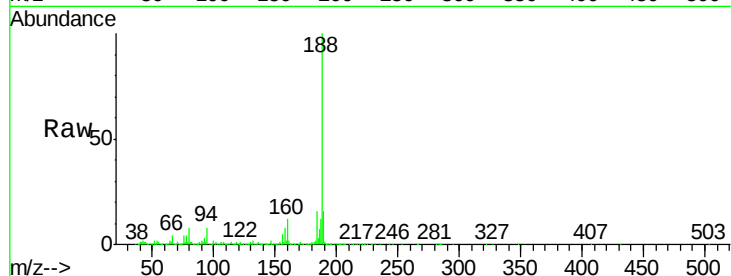



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

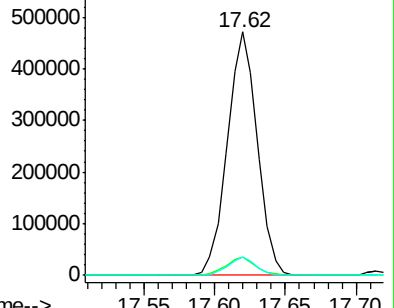

Time-->

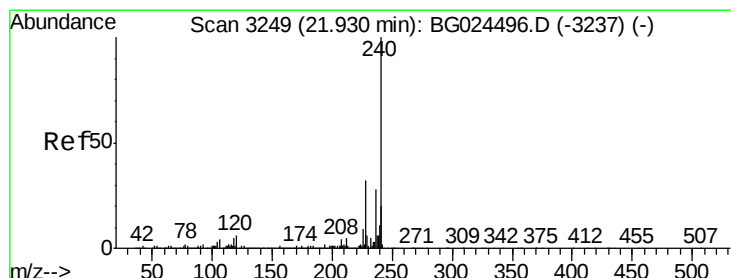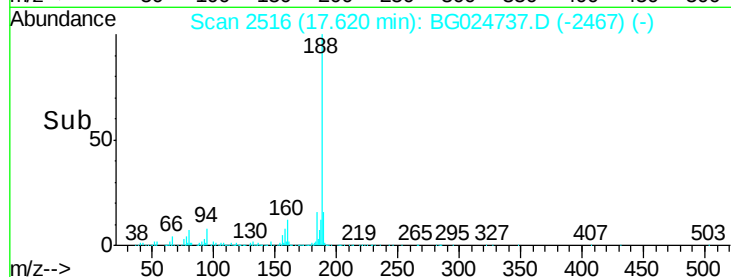

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.91 min Scan# 3247

Delta R.T. -0.02 min

Lab File: BG024737.D

Acq: 7 Nov 2016 20:24


Tgt Ion:240 Resp: 987335

Ion Ratio Lower Upper

240 100

120 5.6 5.7 8.5#


236 25.8 22.2 33.4

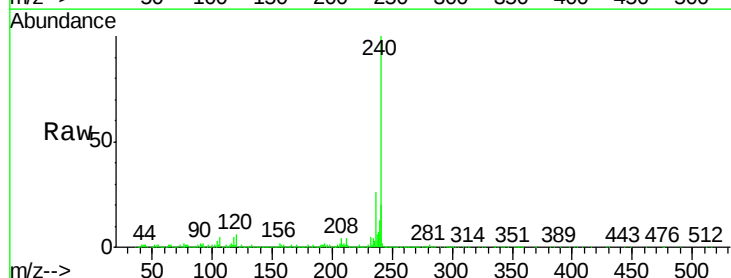

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

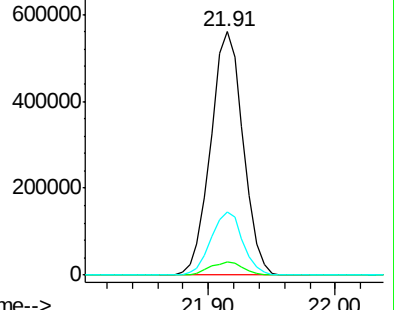

Time-->

