
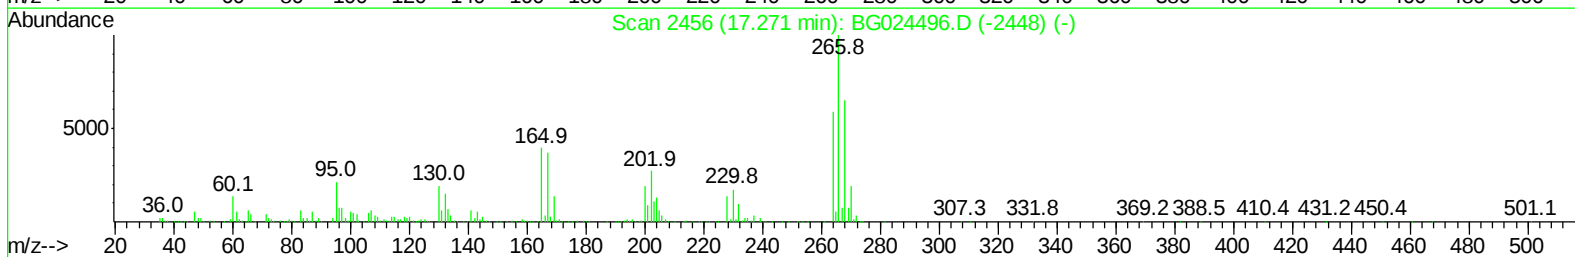
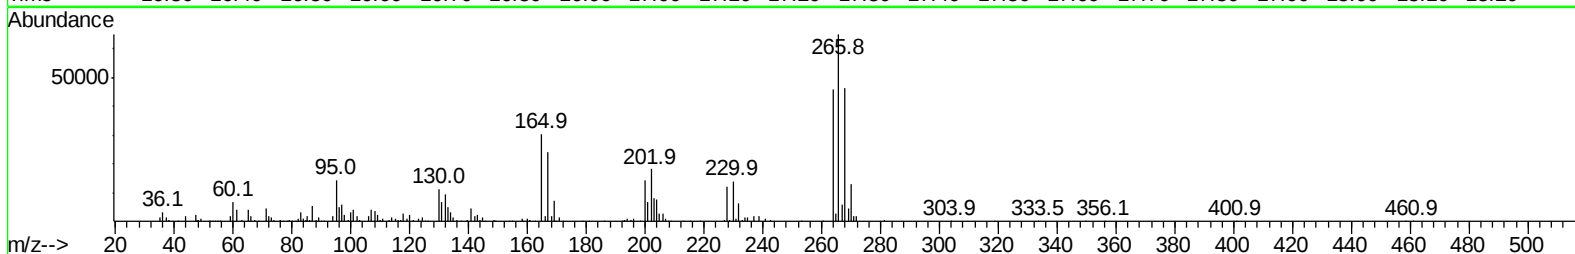


Data Path : Z:\HPCHEM1\BNA G\DATA\BG110716\
Data File : BG024722.D
Acq On : 7 Nov 2016 10:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 17:45:26 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

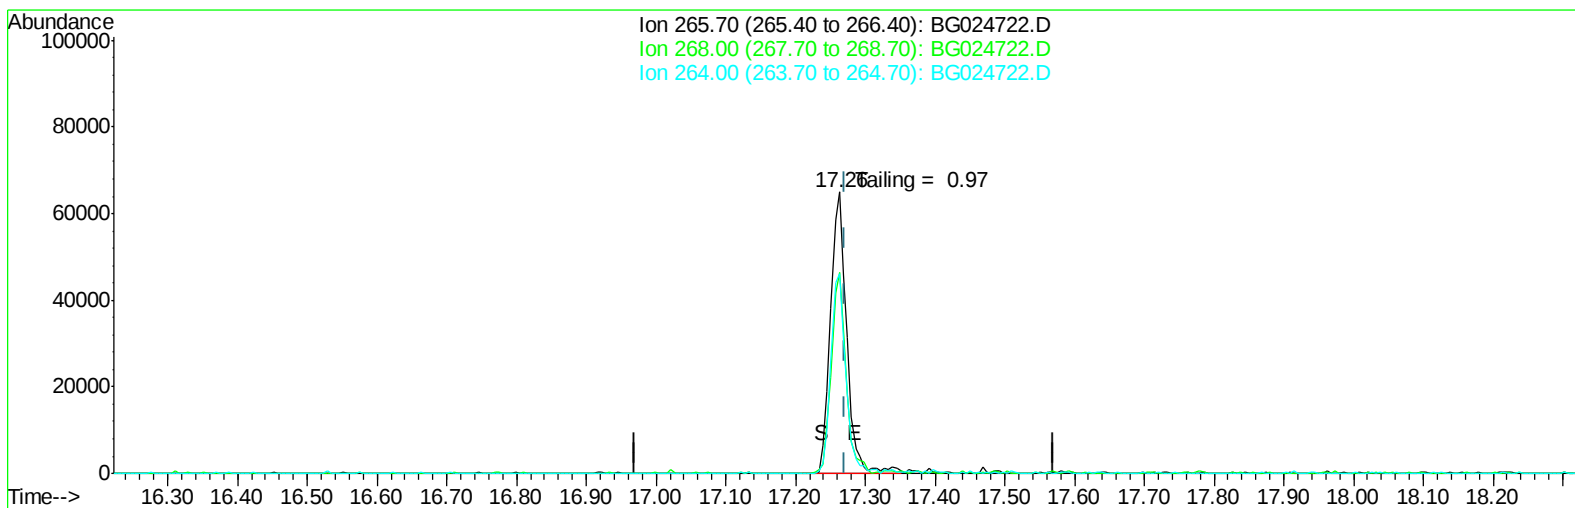

TIC: BG024722.D

(69) Pentachlorophenol (C)




17.263min (-0.008) 135695.14ng

response 102092

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	71.25
264.00	62.60	70.74
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110716\
Data File : BG024722.D
Acq On : 7 Nov 2016 10:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 07 17:45:26 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

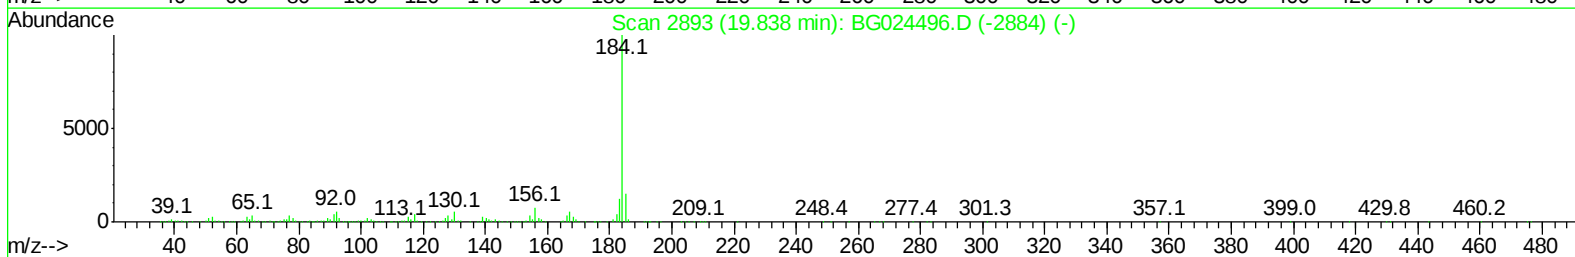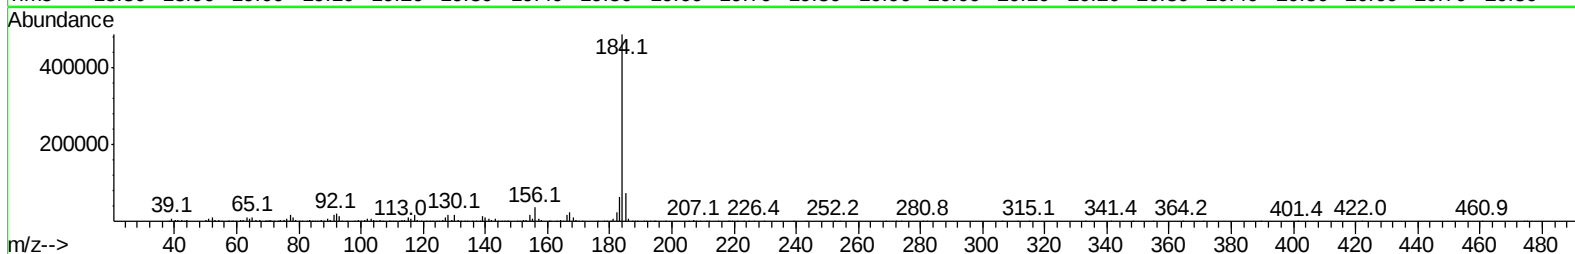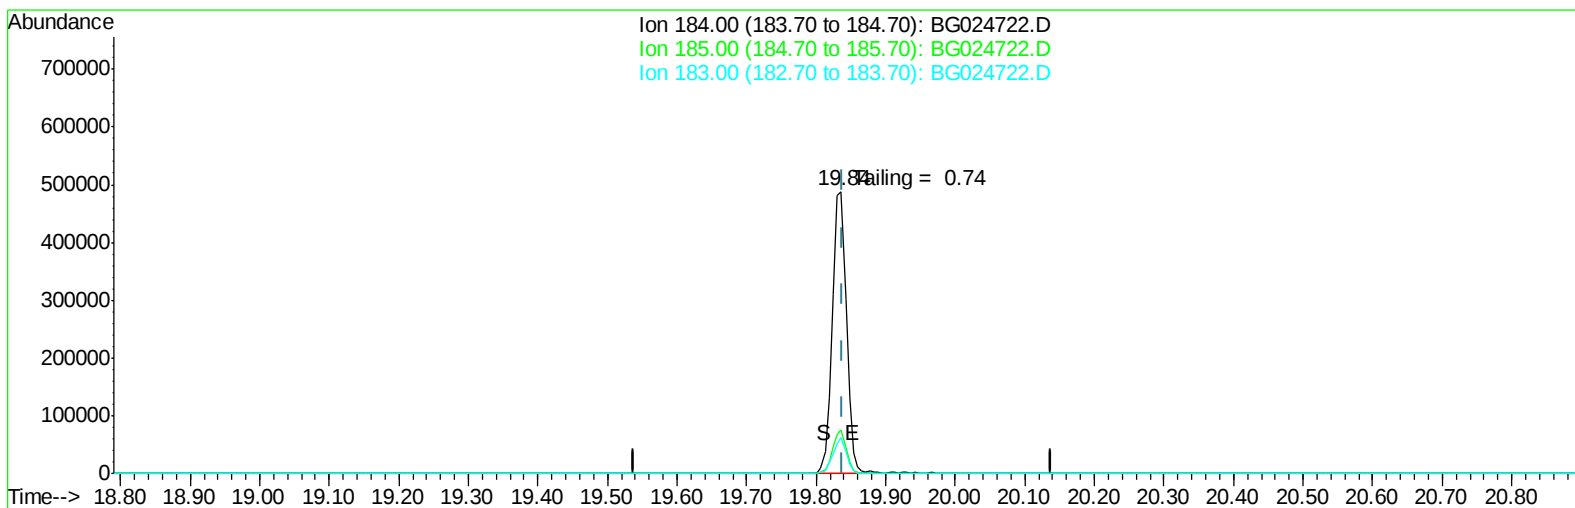

TIC: BG024722.D

(76) Benzidine

19.836min (-0.002) 471912.37ng

response 689366

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.25
183.00	13.80	12.82
0.00	0.00	0.00