
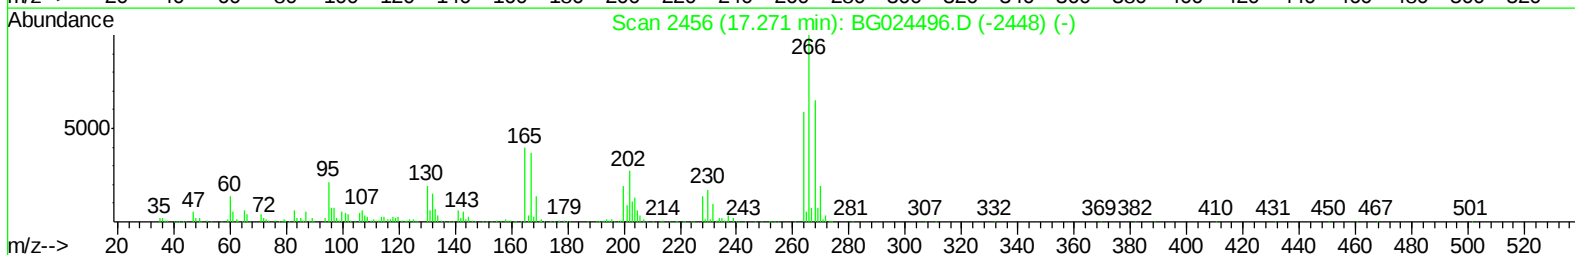
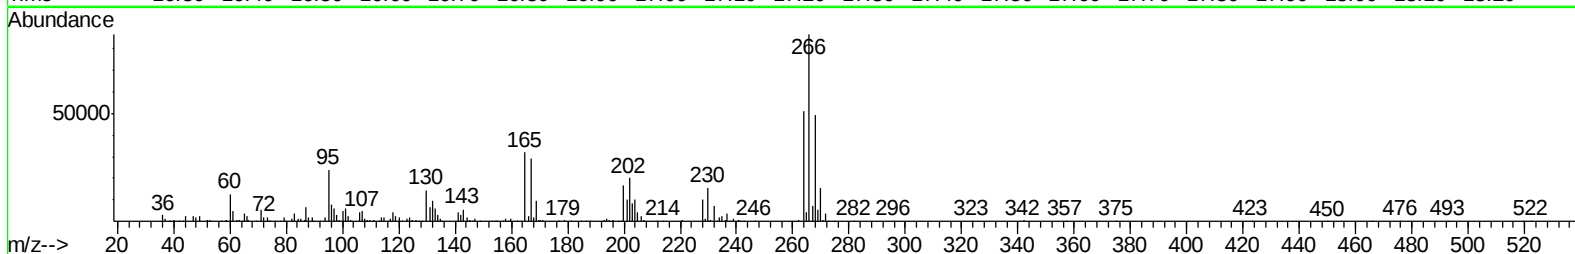


Data Path : Z:\HPCHEM1\BNA_G\Data\BG110716\
Data File : BG024731.D
Acq On : 7 Nov 2016 16:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 07:15:58 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

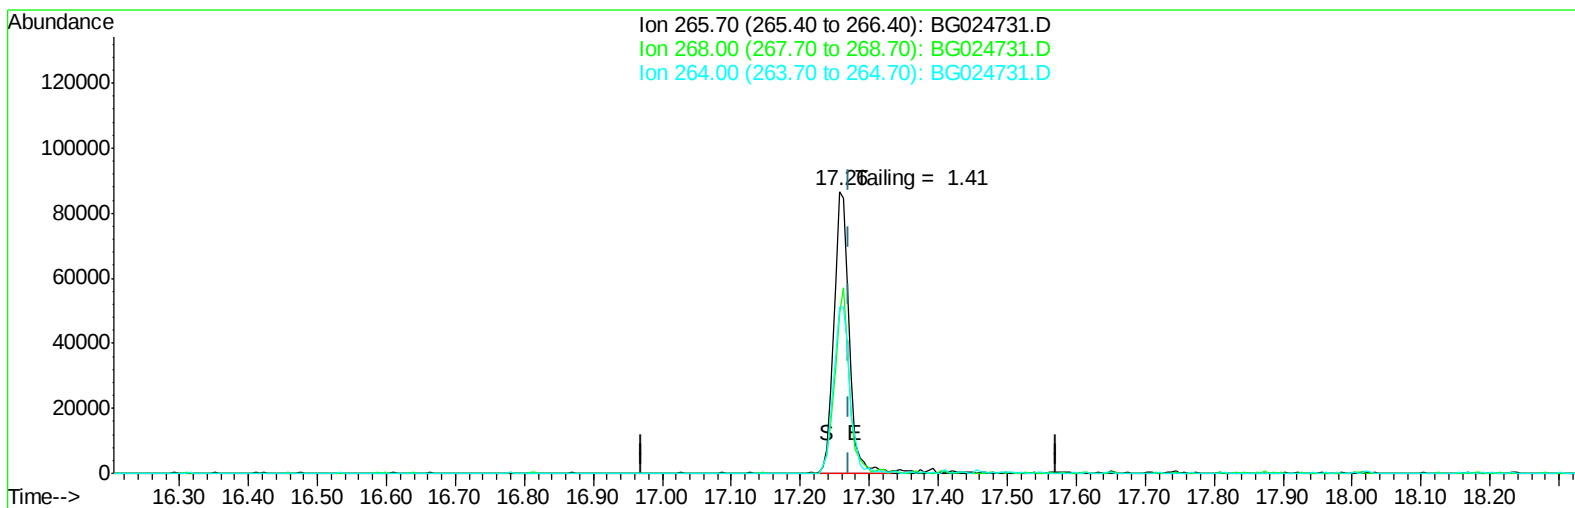

TIC: BG024731.D

(69) Pentachlorophenol (C)




17.256min (-0.014) 232710.82ng

response 133887

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	56.96
264.00	62.60	59.17
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG110716\
Data File : BG024731.D
Acq On : 7 Nov 2016 16:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 07:15:58 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

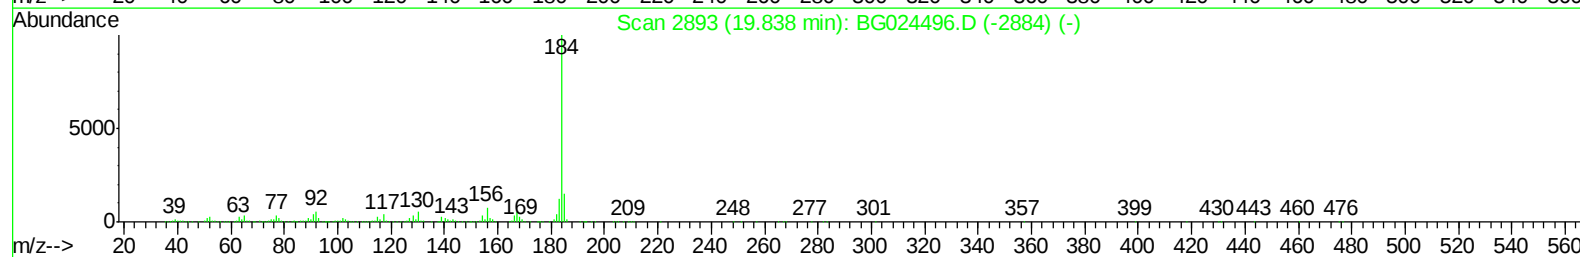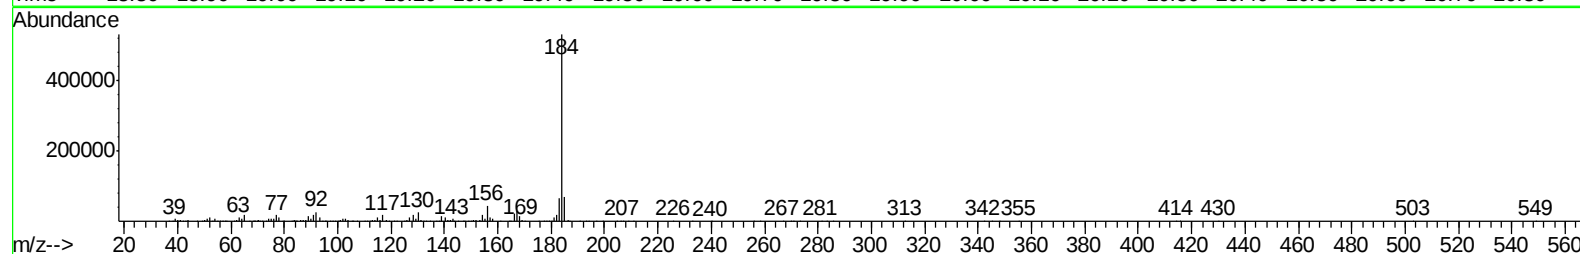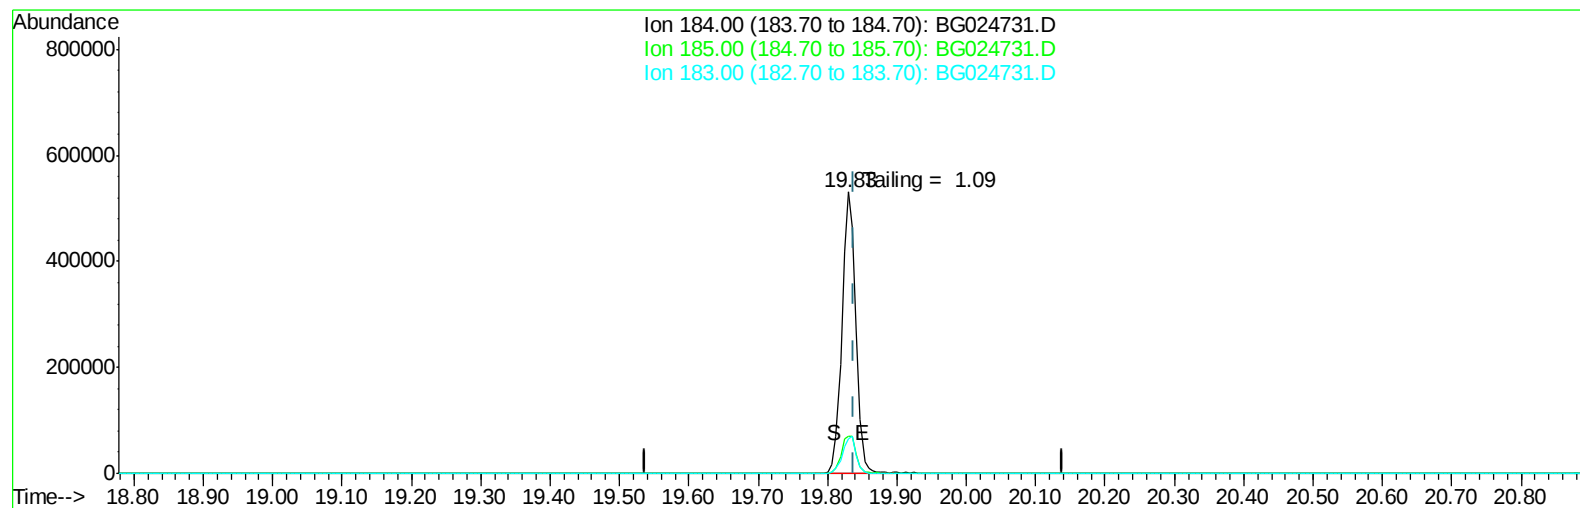

TIC: BG024731.D

(76) Benzidine

19.830min (-0.009) 148658.99ng

response 749552

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.16
183.00	13.80	12.18
0.00	0.00	0.00