
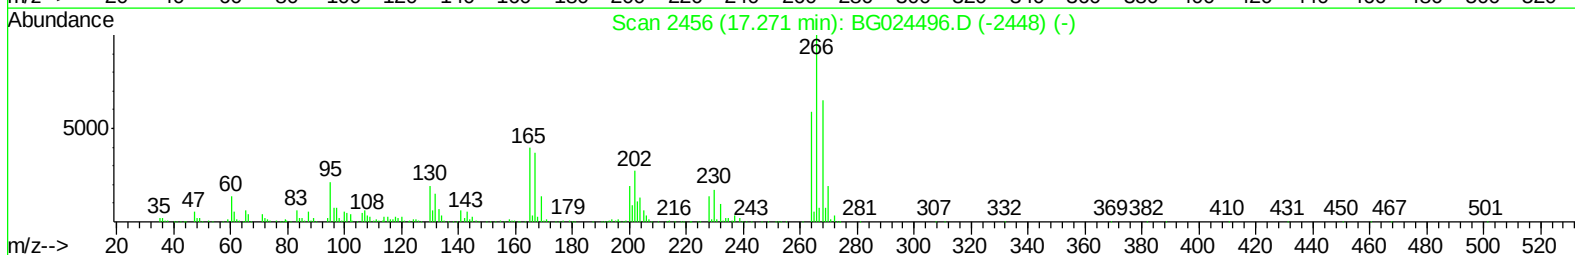
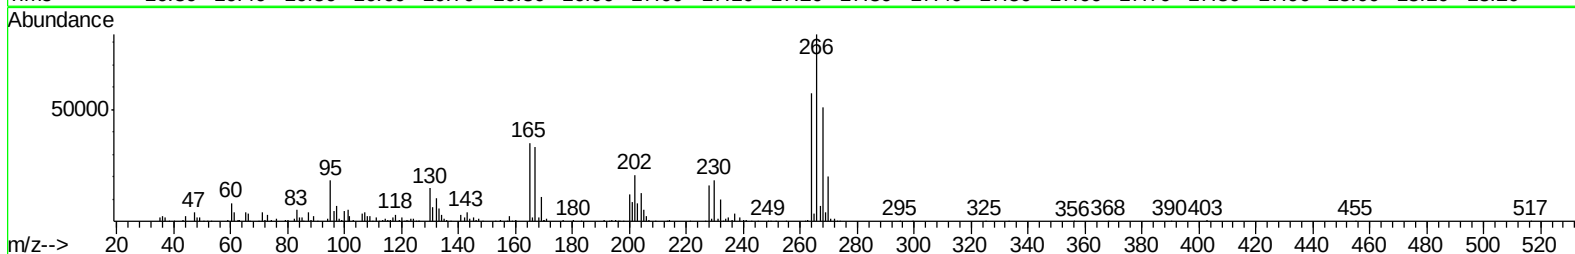


Data Path : Z:\HPCHEM1\BNA_G\Data\BG110716\
Data File : BG024749.D
Acq On : 8 Nov 2016 5:35
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 07:16:55 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

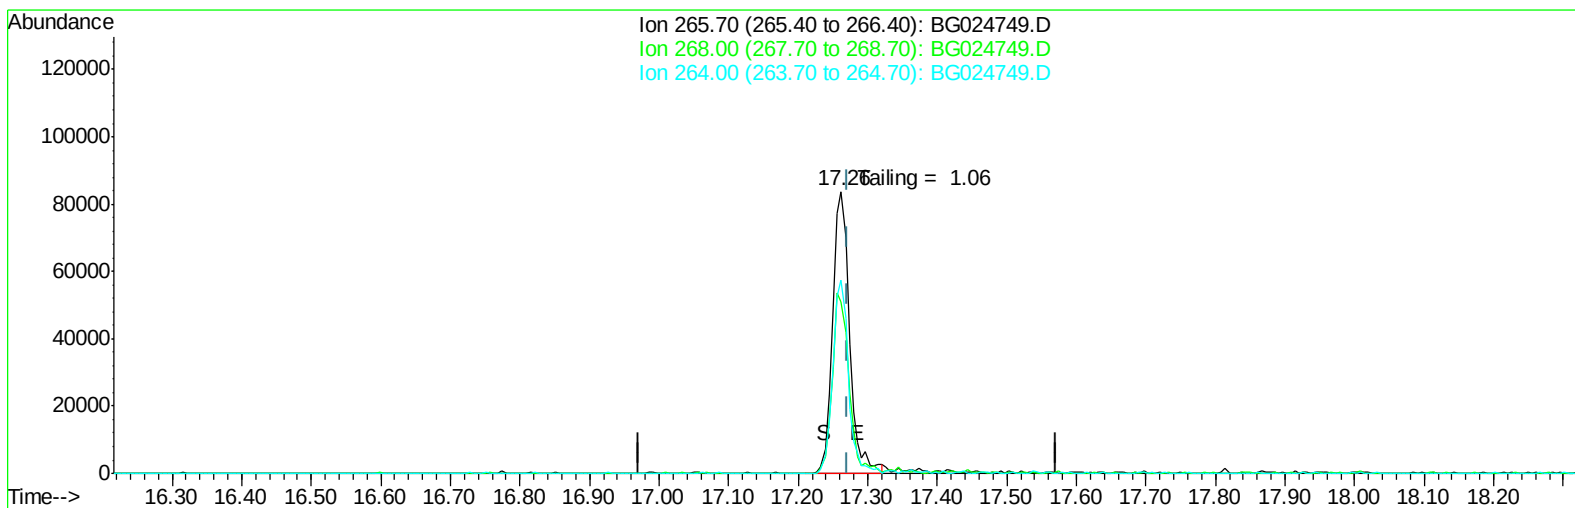

TIC: BG024749.D

(69) Pentachlorophenol (C)




17.262min (-0.009) 249226.32ng

response 138977

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	60.89
264.00	62.60	68.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG110716\
Data File : BG024749.D
Acq On : 8 Nov 2016 5:35
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 07:16:55 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

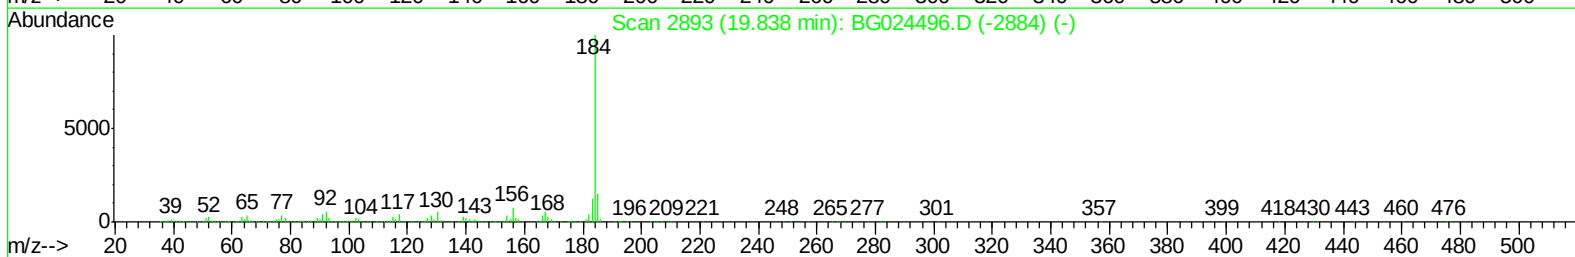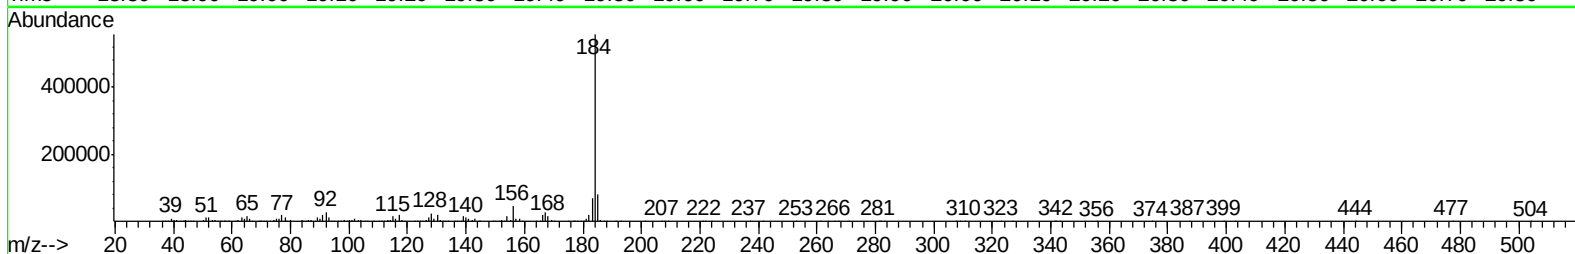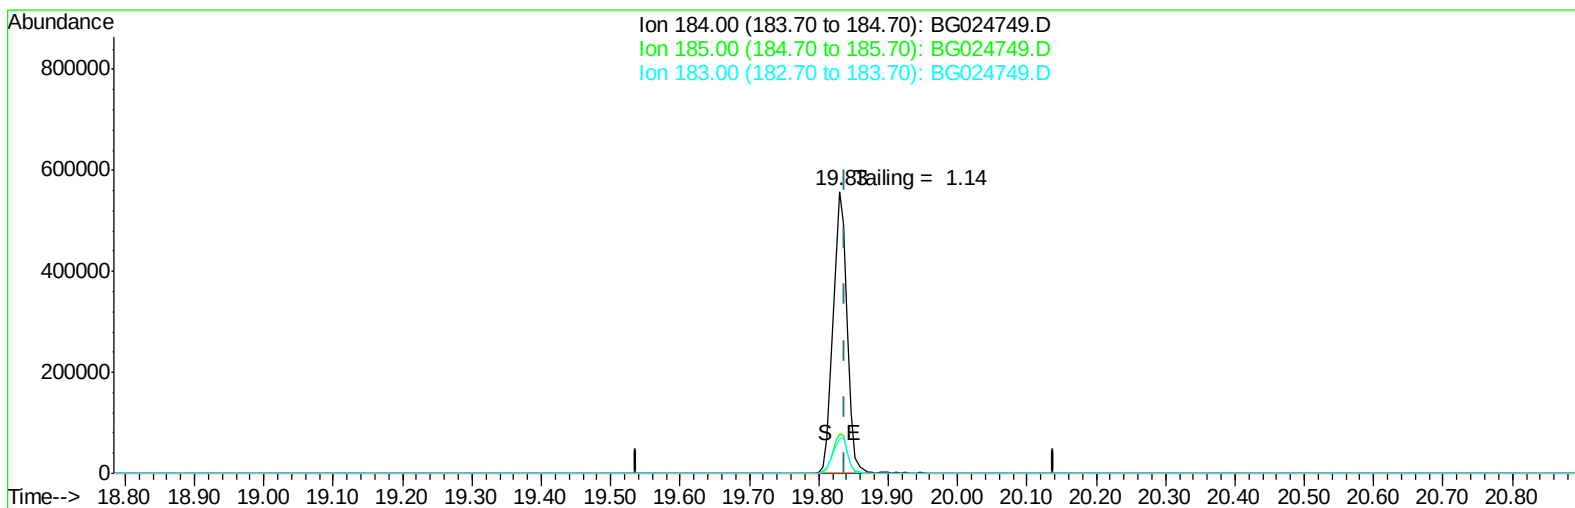

TIC: BG024749.D

(76) Benzidine

19.829min (-0.009) 188751.40ng

response 787155

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.10
183.00	13.80	12.43
0.00	0.00	0.00