

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110716\
 Data File : BG024730.D
 Acq On : 7 Nov 2016 15:54
 Operator : UM/SJ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC040

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.660	134	140	149	rVB	221345	340804	2.86%	0.128%
2	3.983	188	195	204	rBV	274464	481013	4.04%	0.181%
3	4.066	204	209	222	rVV	592142	1098547	9.23%	0.414%
4	5.793	495	503	513	rVB	1311154	2217606	18.63%	0.835%
5	7.403	769	777	789	rVB3	1886400	4720223	39.65%	1.778%
6	7.585	799	808	816	rBV	743027	1382472	11.61%	0.521%
7	7.673	816	823	831	rVB	533835	886019	7.44%	0.334%
8	7.791	834	843	846	rBV	1364301	2610649	21.93%	0.983%
9	8.149	895	904	911	rBV	847745	1468363	12.33%	0.553%
10	8.267	914	924	925	rVV	415003	686410	5.77%	0.258%
11	8.296	925	929	939	rVB	847985	1538166	12.92%	0.579%
12	8.496	955	963	971	rBV	969679	1686177	14.16%	0.635%
13	8.590	971	979	983	rBV	1506487	3214924	27.00%	1.211%
14	8.690	990	996	1004	rVB	911457	1605813	13.49%	0.605%
15	8.778	1004	1011	1018	rBV2	514674	1257380	10.56%	0.473%
16	9.024	1045	1053	1056	rBV	860856	1676650	14.08%	0.631%
17	9.089	1056	1064	1073	rVB2	993250	2936710	24.67%	1.106%
18	9.353	1100	1109	1116	rBV2	712098	1299945	10.92%	0.490%
19	9.442	1116	1124	1128	rVV	1259588	2553626	21.45%	0.962%
20	9.483	1128	1131	1138	rVB	743188	1206348	10.13%	0.454%
21	9.994	1210	1218	1226	rVB	999048	1829616	15.37%	0.689%
22	10.194	1244	1252	1255	rBV2	633556	1214364	10.20%	0.457%
23	10.235	1255	1259	1266	rVV	1042192	1825672	15.33%	0.688%
24	10.370	1266	1282	1291	rVV2	377739	1482409	12.45%	0.558%
25	10.476	1293	1300	1307	rVB	693713	1139907	9.57%	0.429%
26	10.722	1334	1342	1351	rBV	912365	1677635	14.09%	0.632%
27	10.946	1371	1380	1389	rVB	1070626	1894299	15.91%	0.713%
28	11.087	1394	1404	1408	rBV	524089	1016186	8.54%	0.383%
29	11.140	1408	1413	1423	rVB	1163788	2151316	18.07%	0.810%
30	11.245	1423	1431	1439	rBV2	904101	1691785	14.21%	0.637%
31	11.404	1449	1458	1467	rVB	1151283	2042074	17.15%	0.769%
32	12.021	1554	1563	1579	rBV	499752	1290193	10.84%	0.486%
33	12.338	1609	1617	1627	rBV2	1165314	1970834	16.55%	0.742%
34	12.726	1672	1683	1692	rVB	1583343	2618264	21.99%	0.986%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110716\
 Data File : BG024730.D
 Acq On : 7 Nov 2016 15:54
 Operator : UM/SJ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC040

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.943	1710	1720	1727	rVV	1517483	2659348	22.34%	1.001%
36	13.055	1730	1739	1740	rVV	958645	1336104	11.22%	0.503%
37	13.079	1740	1743	1755	rVB	1488806	2616433	21.98%	0.985%
38	13.314	1776	1783	1790	rBV	1253510	2115638	17.77%	0.797%
39	13.390	1790	1796	1804	rVV	1251733	2041517	17.15%	0.769%
40	13.502	1808	1815	1823	rBV	3647470	5715166	48.00%	2.152%
41	13.713	1845	1851	1856	rBV	1997426	3210354	26.96%	1.209%
42	13.766	1856	1860	1872	rVB	1622547	2549444	21.41%	0.960%
43	13.972	1885	1895	1901	rBV	1045550	1751697	14.71%	0.660%
44	14.248	1936	1942	1948	rBV	761010	1260621	10.59%	0.475%
45	14.324	1948	1955	1961	rVV	1787462	2649500	22.25%	0.998%
46	14.395	1961	1967	1972	rVV	876863	1434421	12.05%	0.540%
47	14.453	1972	1977	1983	rVB	1230554	1882356	15.81%	0.709%
48	14.559	1989	1995	1999	rBV	785831	1305114	10.96%	0.491%
49	14.606	1999	2003	2013	rVB	1660063	2716194	22.81%	1.023%
50	14.788	2026	2034	2042	rBV	1177469	1882126	15.81%	0.709%
51	14.882	2042	2050	2055	rVV	980493	1557074	13.08%	0.586%
52	14.947	2055	2061	2065	rVV	2036623	3453082	29.00%	1.300%
53	14.988	2065	2068	2075	rVV	939309	1327777	11.15%	0.500%
54	15.076	2075	2083	2090	rVB	978849	1570643	13.19%	0.591%
55	15.235	2097	2110	2113	rBV	1259746	2018572	16.95%	0.760%
56	15.276	2113	2117	2126	rVB	1944267	2977230	25.01%	1.121%
57	15.411	2133	2140	2147	rBV	1582345	2404815	20.20%	0.906%
58	15.493	2147	2154	2163	rVB	1558465	2434973	20.45%	0.917%
59	15.670	2177	2184	2191	rVB	2038098	2960948	24.87%	1.115%
60	15.911	2217	2225	2235	rBV3	3001229	8579609	72.06%	3.231%
61	15.993	2235	2239	2250	rVV	1134819	1641779	13.79%	0.618%
62	16.122	2253	2261	2267	rVV	2309804	3528403	29.64%	1.329%
63	16.198	2267	2274	2286	rVB	1829644	2734748	22.97%	1.030%
64	16.363	2295	2302	2311	rBV	2433843	3797463	31.90%	1.430%
65	16.798	2369	2376	2383	rVB	2139469	3007747	25.26%	1.133%
66	16.921	2388	2397	2403	rBV	2102429	3234414	27.17%	1.218%
67	17.056	2413	2420	2431	rVB	1913412	2714529	22.80%	1.022%
68	17.262	2445	2455	2464	rBV	1561254	2437570	20.47%	0.918%
69	17.620	2509	2516	2519	rBV	1344170	2073161	17.41%	0.781%
70	17.667	2519	2524	2530	rVV	2702717	4324122	36.32%	1.628%
71	17.755	2532	2539	2546	rVB	2804140	4230826	35.54%	1.593%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110716\
Data File : BG024730.D
Acq On : 7 Nov 2016 15:54
Operator : UM/SJ
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTDCCC040

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	18.026	2577	2585	2593	rBV	2421125	3911868	32.86%	1.473%
73	18.549	2668	2674	2680	rBV	2788865	3651322	30.67%	1.375%
74	18.807	2713	2718	2724	rVB4	101707	150325	1.26%	0.057%
75	19.659	2856	2863	2870	rVB	3473306	5177594	43.49%	1.950%
76	19.829	2886	2892	2901	rBV	1638171	2390119	20.07%	0.900%
77	20.017	2914	2924	2931	rBV	3537748	5275864	44.31%	1.987%
78	20.200	2949	2955	2962	rBV	7383961	10205151	85.71%	3.843%
79	20.881	3066	3071	3075	rBV	3132148	3978073	33.41%	1.498%
80	20.928	3075	3079	3085	rVB	3700568	4307257	36.18%	1.622%
81	21.751	3213	3219	3224	rBV	3089766	4645994	39.02%	1.750%
82	21.804	3224	3228	3235	rVV	2645737	4141957	34.79%	1.560%
83	21.898	3236	3244	3251	rVV2	3508810	8719082	73.23%	3.283%
84	21.968	3251	3256	3264	rVB	3495278	6018979	50.55%	2.267%
85	23.026	3424	3436	3444	rBV	2378571	5042471	42.35%	1.899%
86	24.248	3628	3644	3650	rBV	2228455	6237090	52.39%	2.349%
87	24.324	3650	3657	3668	rVB	2276258	5829240	48.96%	2.195%
88	24.694	3715	3720	3730	rVB	46417	119666	1.01%	0.045%
89	25.188	3790	3804	3813	rBV	1927614	5950129	49.98%	2.241%
90	25.346	3816	3831	3843	rVB3	880739	2870787	24.11%	1.081%
91	26.486	4018	4025	4033	rVB3	51818	146132	1.23%	0.055%
92	29.348	4482	4512	4528	rVB3	1544046	11906014	100.00%	4.484%
93	30.529	4691	4713	4731	rVB2	1130263	6027538	50.63%	2.270%


Sum of corrected areas: 265550569

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110716\
Data File : BG024730.D
Acq On : 7 Nov 2016 15:54
Operator : UM/SJ
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_G
LabSampleId :
SSTDCCC040

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

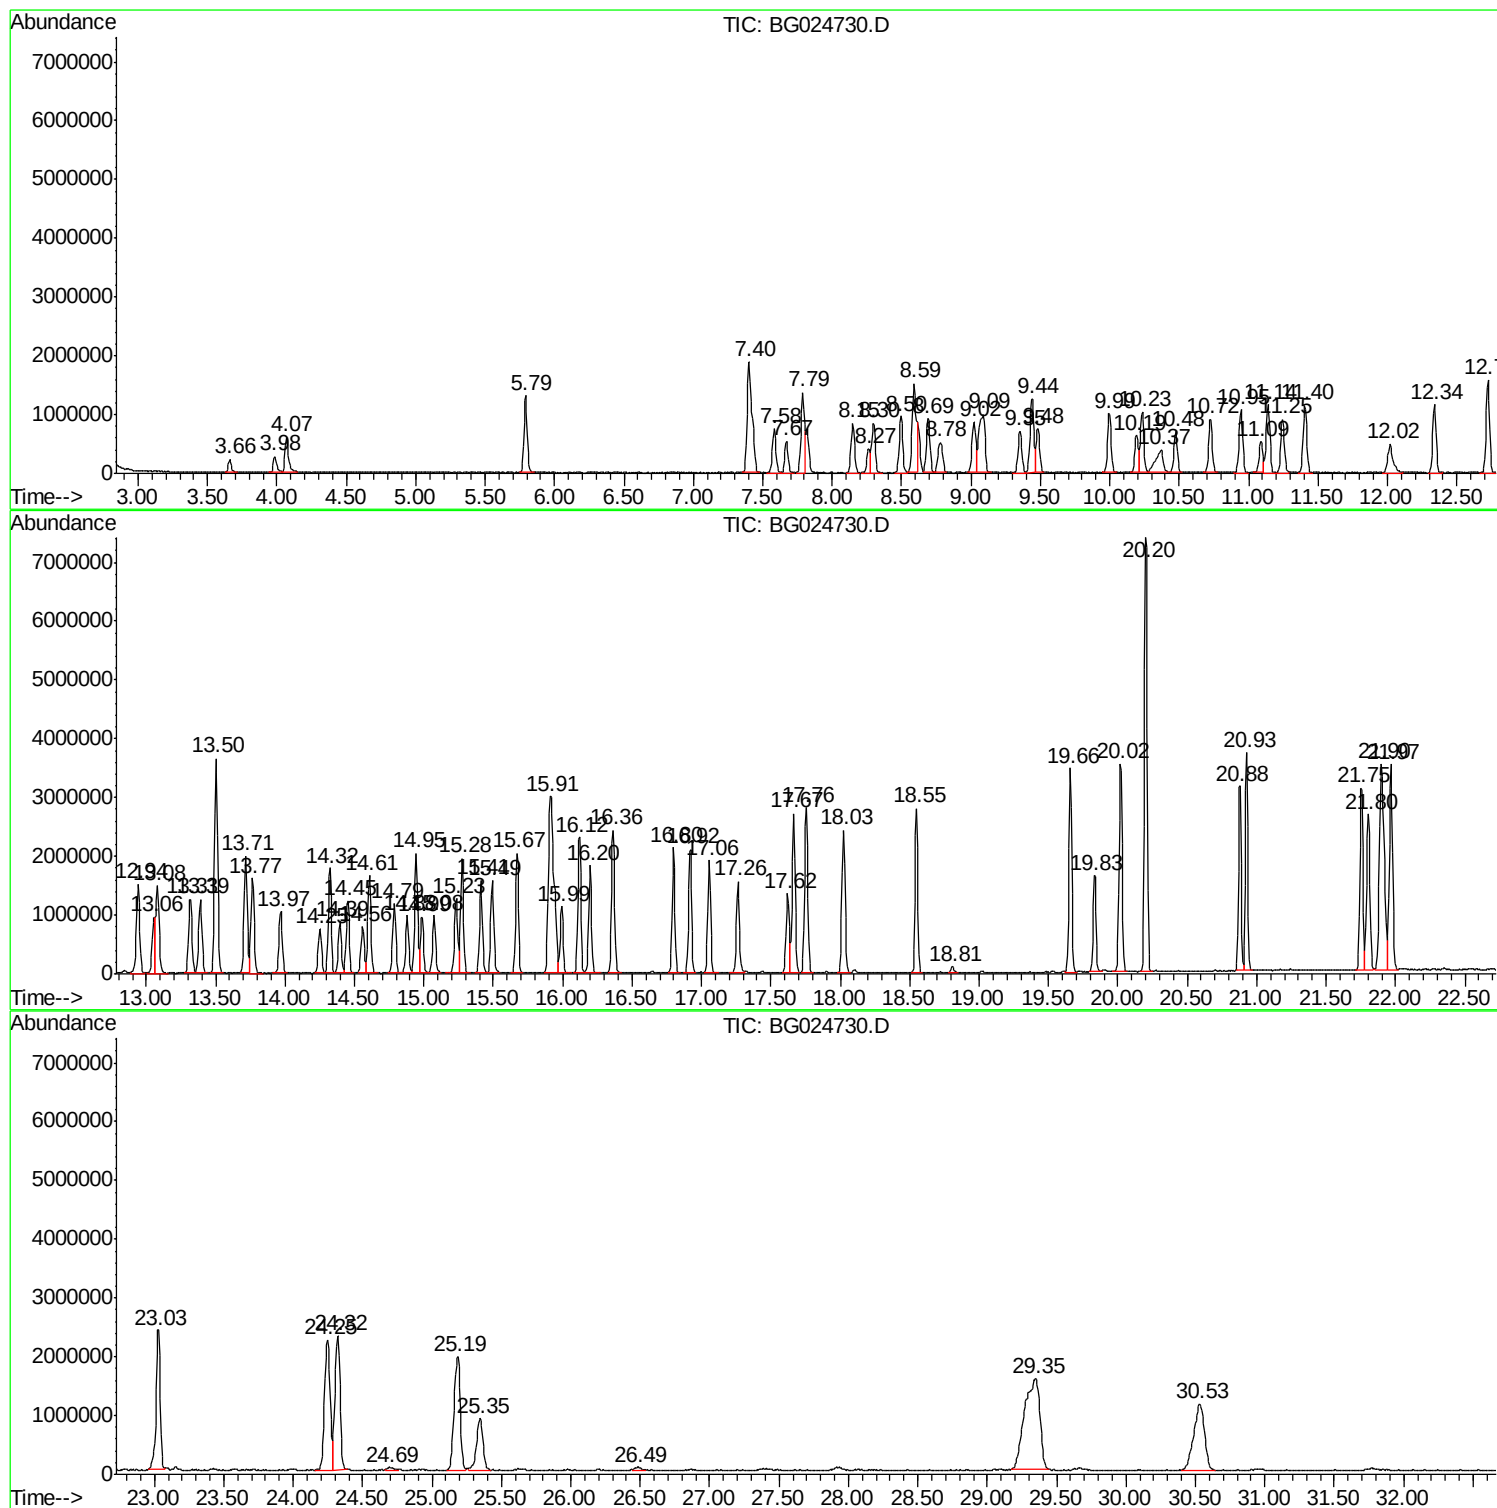

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG110716\
Data_File : BG024730.D
Acq_On : 7 Nov 2016 15:544
Operator : UM/SJJ
Sample : SSTDCCC0400
Misc :
ALS_Vial : 2 Sample_Multiplier: 11

Instrument :
BNA_G
LabSampleId :
SSTDCCC040

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
