


Data Path : Z:\HPCHEM1\BNA G\DATA\BG110716\
Data File : BG024722.D
Acq On : 7 Nov 2016 10:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 26 11:14:13 2016

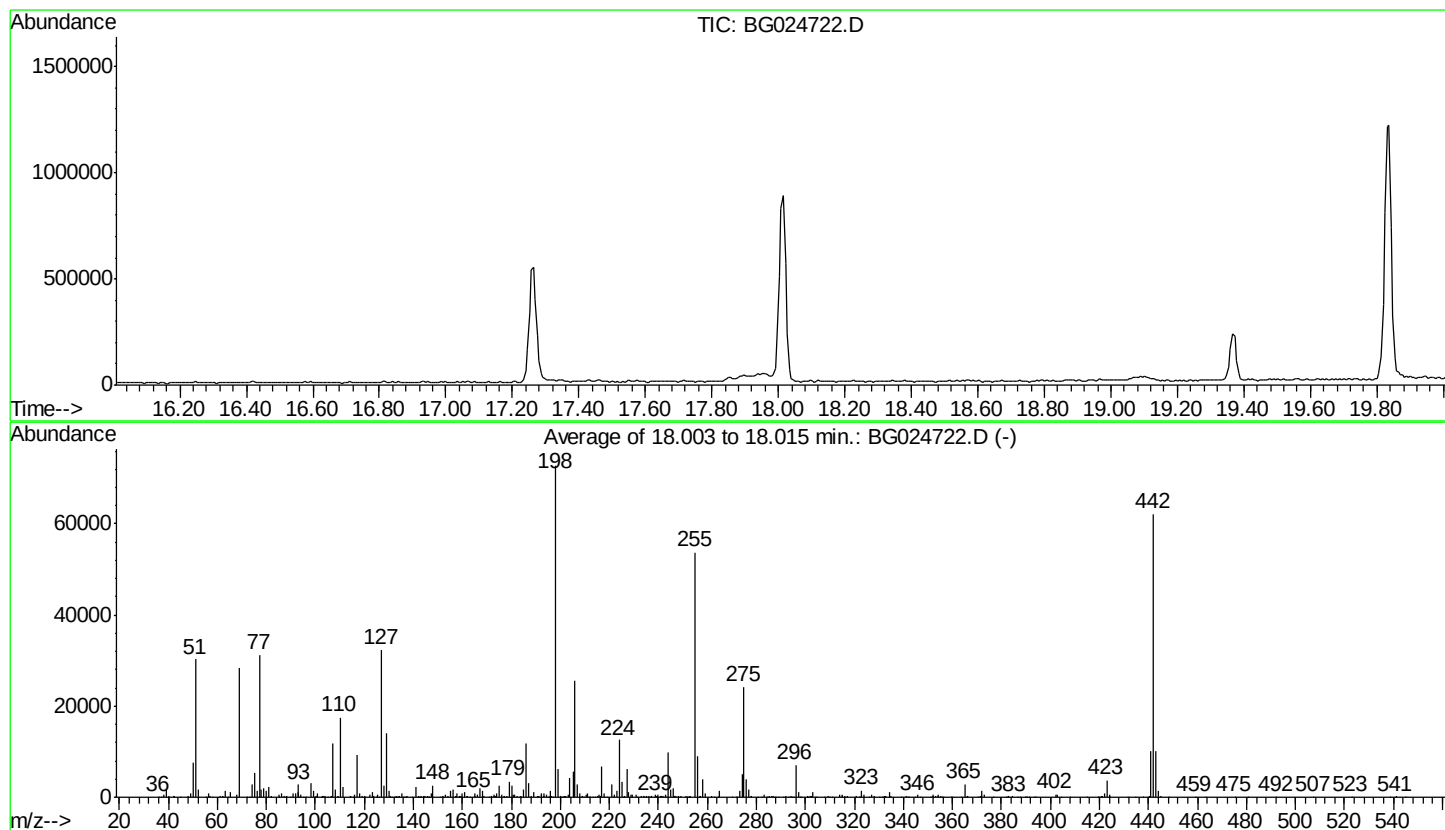

AutoFind: Scans 2581, 2582, 2583; Background Corrected with Scan 2574

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	30288	PASS
68	69	0.00	2	1.7	477	PASS
69	198	0.00	100	39.1	28486	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.6	32440	PASS
197	198	0.00	2	0.2	141	PASS
198	198	100	100	100.0	72784	PASS
199	198	5	9	8.5	6180	PASS
275	198	10	60	33.2	24170	PASS
365	198	1	100	3.9	2845	PASS
441	442	0.01	24	16.3	10111	PASS
442	198	50	100	85.5	62197	PASS
443	442	15	24	16.3	10163	PASS