


Data Path : Z:\HPCHEM1\BNA G\DATA\BG110716\
 Data File : BG024731.D
 Acq On : 7 Nov 2016 16:32
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 11:14:13 2016

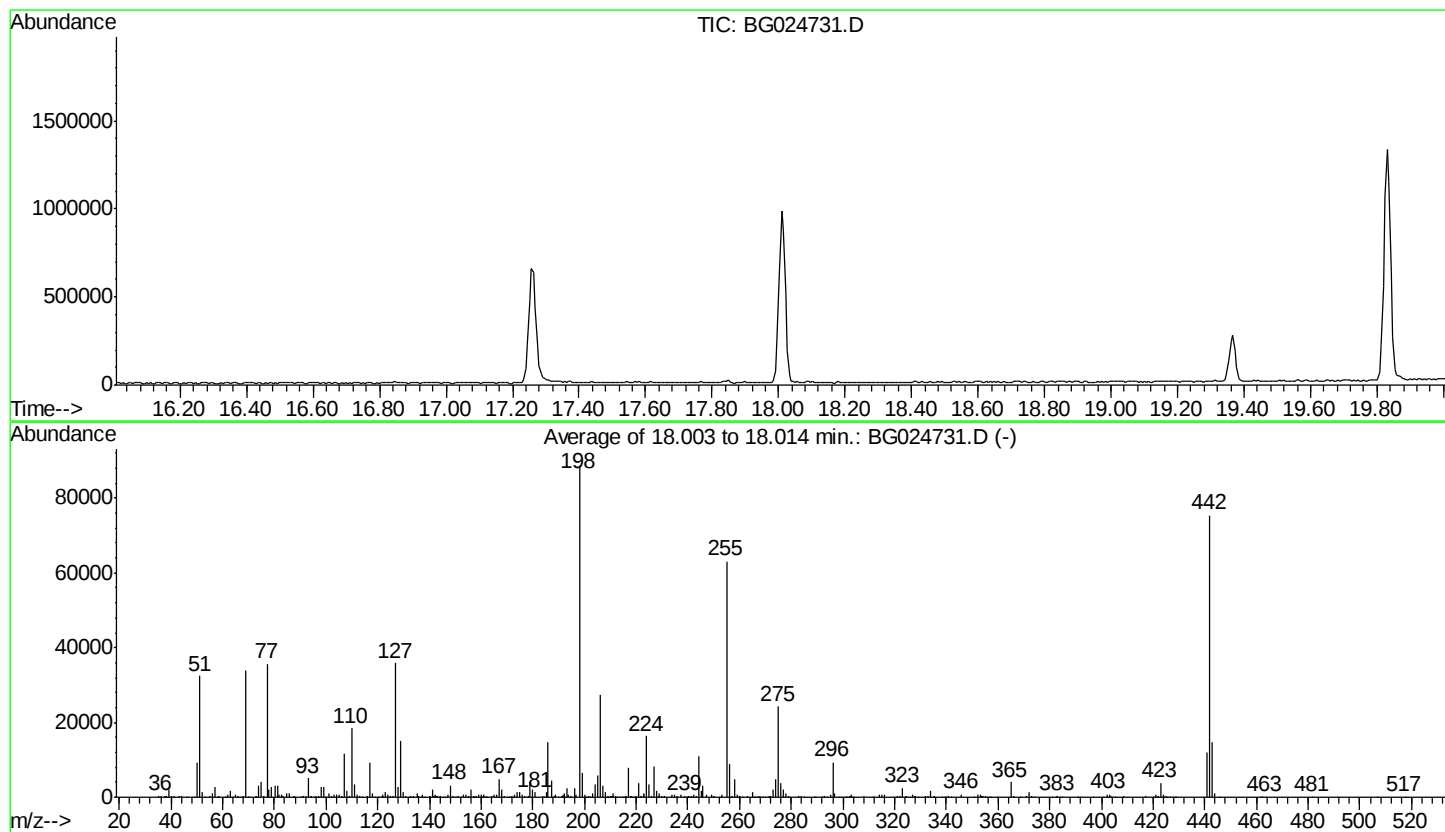

AutoFind: Scans 2581, 2582, 2583; Background Corrected with Scan 2574

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	32491	PASS
68	69	0.00	2	0.6	219	PASS
69	198	0.00	100	38.1	33762	PASS
70	69	0.00	2	0.5	159	PASS
127	198	10	80	40.4	35850	PASS
197	198	0.00	2	0.9	774	PASS
198	198	100	100	100.0	88682	PASS
199	198	5	9	7.5	6629	PASS
275	198	10	60	27.3	24192	PASS
365	198	1	100	4.5	3985	PASS
441	442	0.01	24	15.8	11893	PASS
442	198	50	100	85.1	75450	PASS
443	442	15	24	19.7	14879	PASS