

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110717\
 Data File : BG030828.D
 Acq On : 8 Nov 2017 3:54
 Operator : SJ/JU
 Sample : I6222-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 08 04:34:35 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 08 04:22:00 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	67545	20.00	ng/ul	0.00
18) Naphthalene-d8	10.97	136	336176	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.77	164	227343	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	541372	20.00	ng/ul	0.00
75) Chrysene-d12	21.78	240	571157	20.00	ng/ul	0.00
83) Perylene-d12	25.09	264	586479	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	8994	5.41	ng/uL	0.00
5) Phenol-d5	7.31	99	183150	28.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.46	67	108289	26.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	149556	32.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	124509	23.78	ng/ul	0.00
19) Nitrobenzene-d5	9.31	128	79128	32.79	ng/ul	0.00
22) 2-Nitrophenol-d4	10.04	143	98933	40.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	170089	30.19	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	187912	28.70	ng/ul	0.00
43) Dimethylphthalate-d6	14.17	166	612438	31.51	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	744101	31.48	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	98775	27.53	ng/ul	0.00
57) Fluorene-d10	15.75	176	560760	35.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.88	200	98313	37.20	ng/ul	0.00
70) Anthracene-d10	17.61	188	830966	32.45	ng/ul	0.00
76) Pyrene-d10	19.88	212	978675	33.10	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.87	264	961930	34.63	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	7.33	94	10925	1.629	ng/ul 91
44) Dimethylphthalate	14.21	163	196301	10.355	ng/ul 99
74) Fluoranthene	19.55	202	86725	2.652	ng/ul 98
77) Pyrene	19.91	202	88057	2.300	ng/ul 98
80) Benzo(a)anthracene	21.83	228	57542	1.608	ng/ul 96
82) Chrysene	21.83	228	57806	1.777	ng/ul 98
85) Benzo(b)fluoranthene	24.03	252	82473	2.342	ng/ul 97
86) Benzo(k)fluoranthene	24.03	252	82473	2.423	ng/ul 98
88) Benzo(a)pyrene	24.93	252	56116	1.637	ng/ul# 91
89) Indeno(1,2,3-cd)pyrene	28.87	276	45690	1.178	ng/ul 96
91) Benzo(g,h,i)perylene	30.06	276	40290	1.254	ng/ul 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG110717\
Data File : BG030828.D
Acq On : 8 Nov 2017 3:54
Operator : SJ/JU
Sample : I6222-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 08 04:34:35 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 08 04:22:00 2017
Response via : Initial Calibration

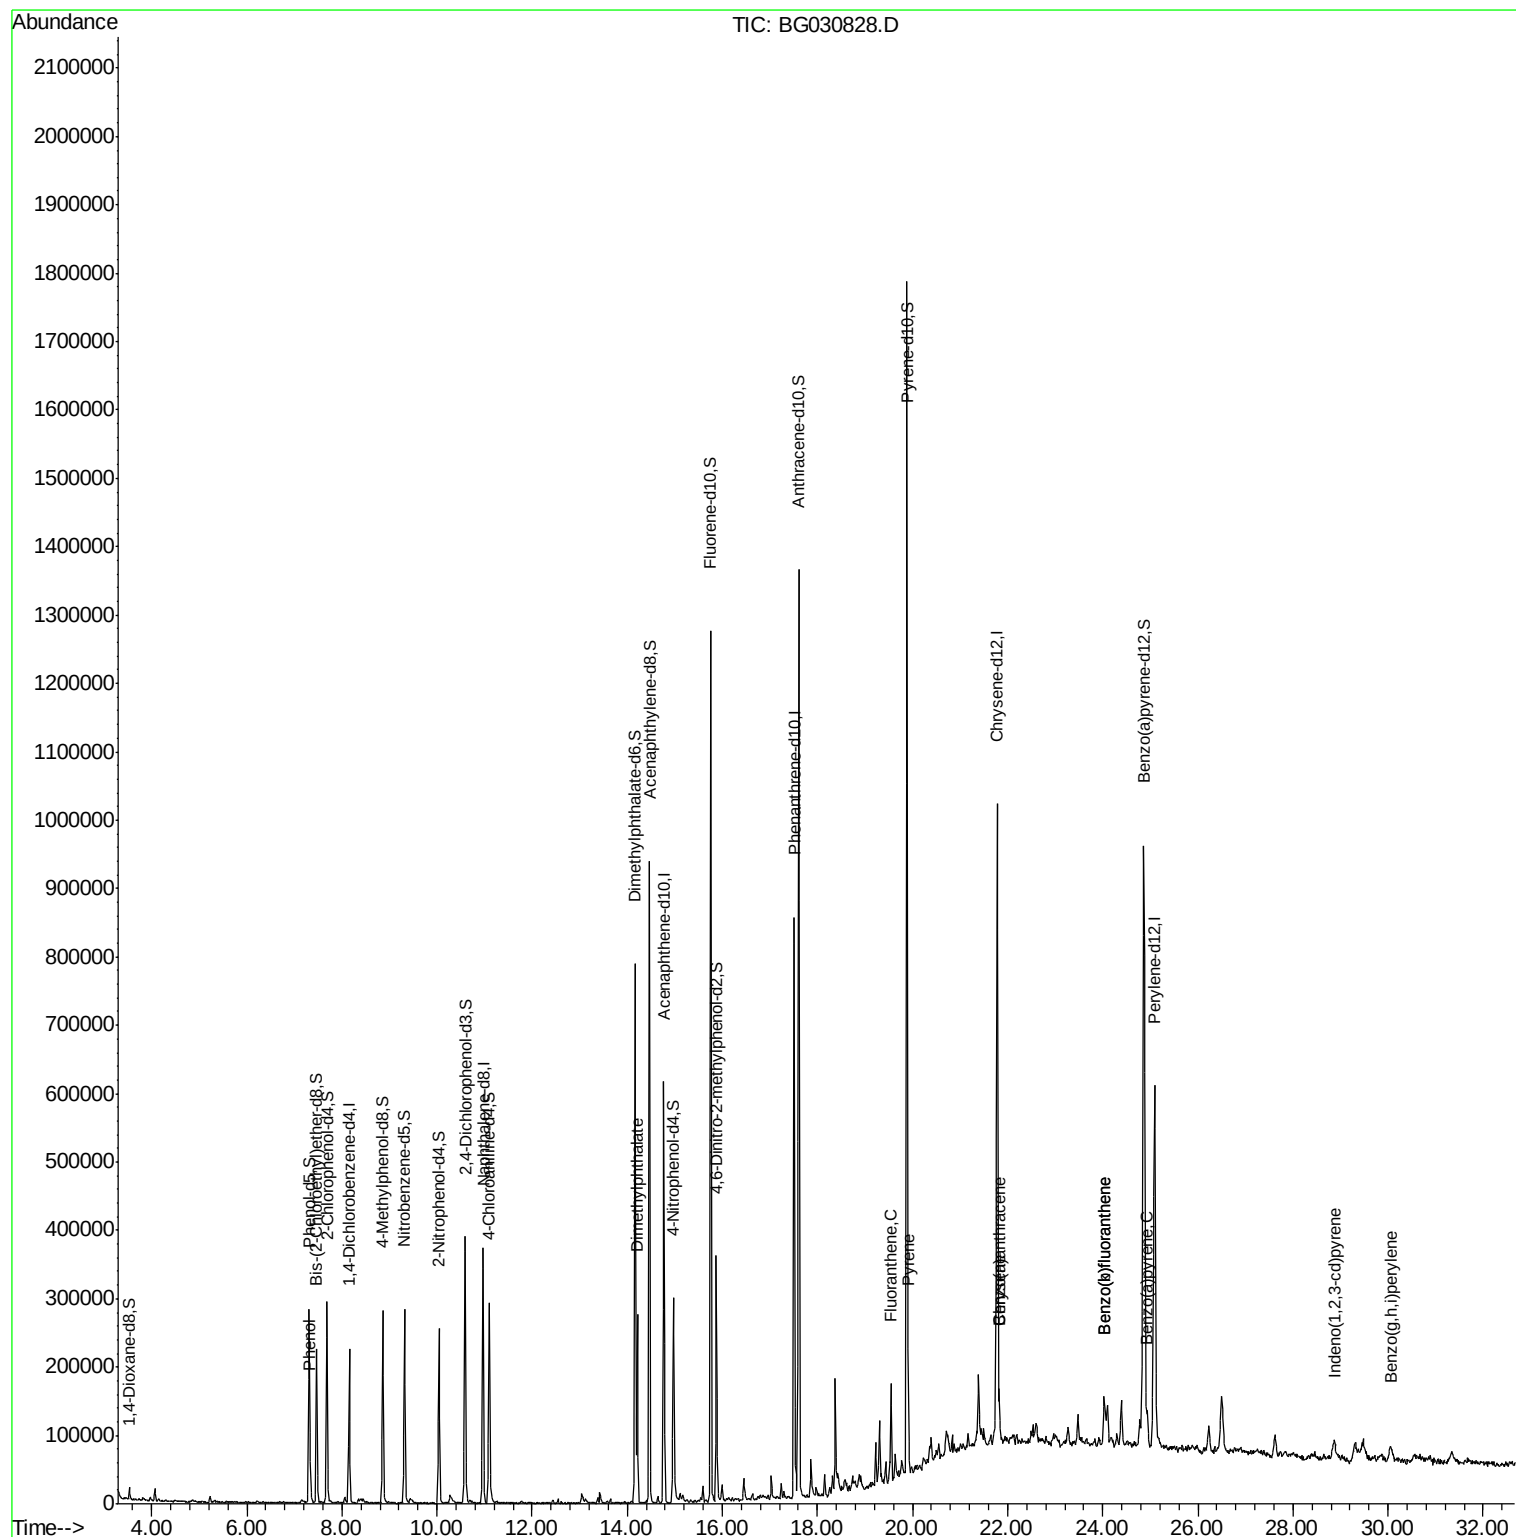

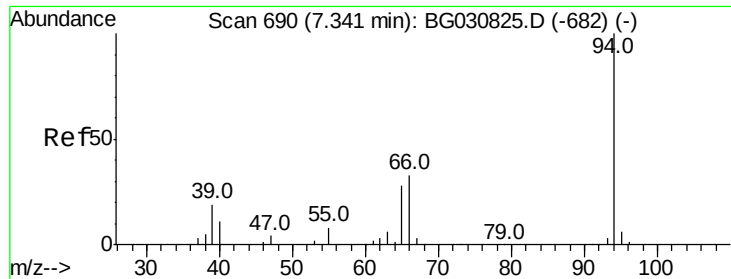


#6

Phenol




Concen: 1.629 ng/ul
 RT: 7.33 min Scan# 689
 Delta R.T. -0.01 min
 Lab File: BG030828.D
 Acq: 8 Nov 2017 3:54

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion: 94 Resp: 10925
 Ion Ratio Lower Upper
 94 100
 65 28.3 27.1 40.7
 66 38.5 34.6 52.0

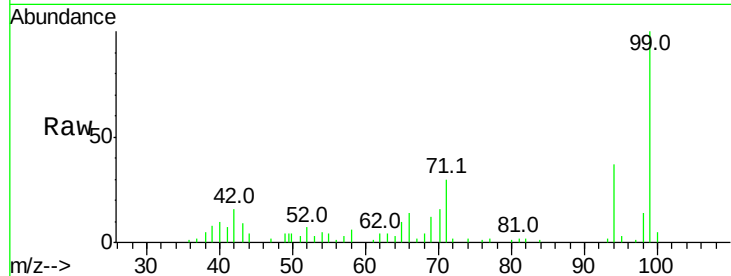

Abundance Ion 94.00 (93.70 to 94.70): BGC
 Ion 65.00 (64.70 to 65.70): BGC
 Ion 66.00 (65.70 to 66.70): BGC

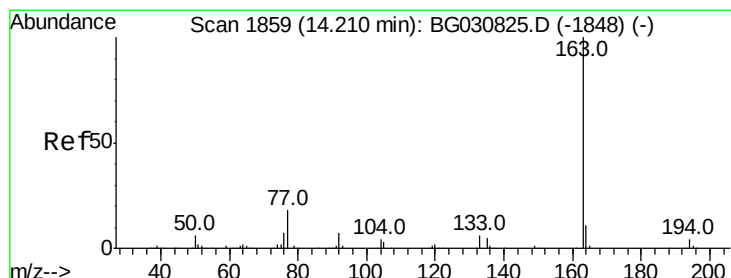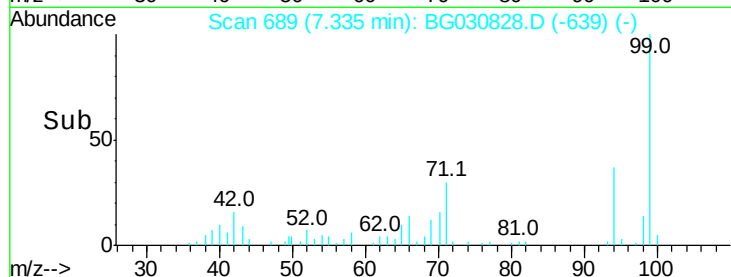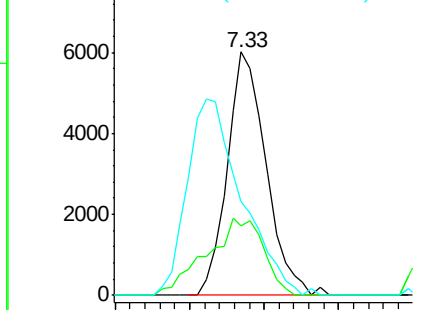


#44



Dimethylphthalate


Concen: 10.355 ng/ul
 RT: 14.21 min Scan# 1859
 Delta R.T. -0.00 min
 Lab File: BG030828.D
 Acq: 8 Nov 2017 3:54

Tgt Ion:163 Resp: 196301
 Ion Ratio Lower Upper
 163 100
 194 4.4 3.5 5.3
 164 9.9 7.6 11.4

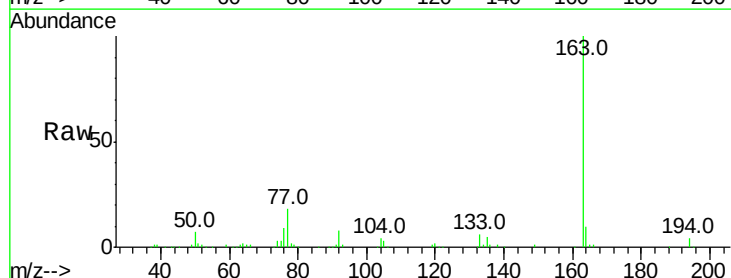

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

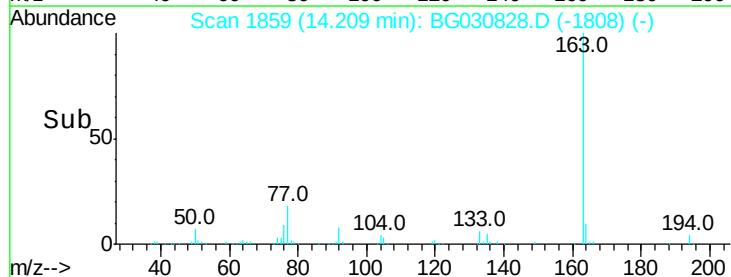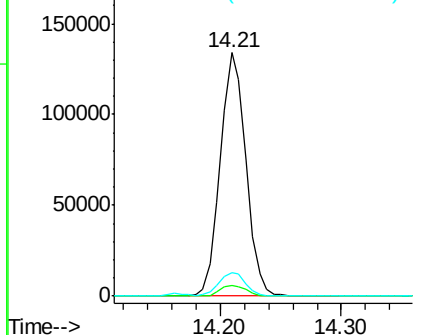

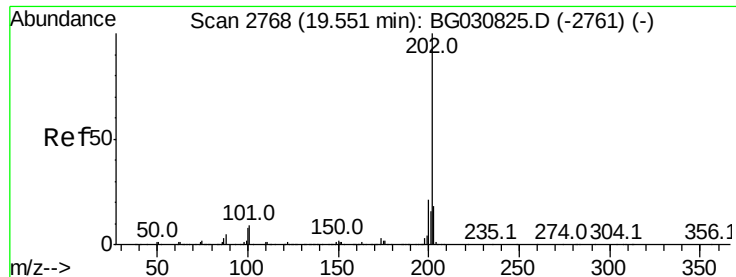

#74

Fluoranthene

Concen: 2.652 ng/ul

RT: 19.55 min Scan# 2768

Delta R.T. -0.00 min

Lab File: BG030828.D

Acq: 8 Nov 2017 3:54

Instrument :

BNA_G

ClientSampleId :


Tot Ion:202 Resp: 86725

Ion Ratio Lower Upper

202 100

101 10.0 7.4 11.2




100 7.5 5.6 8.4

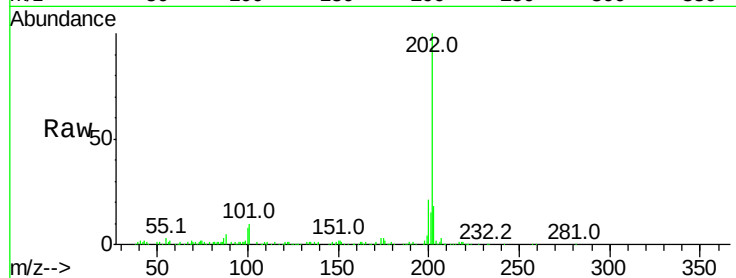

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

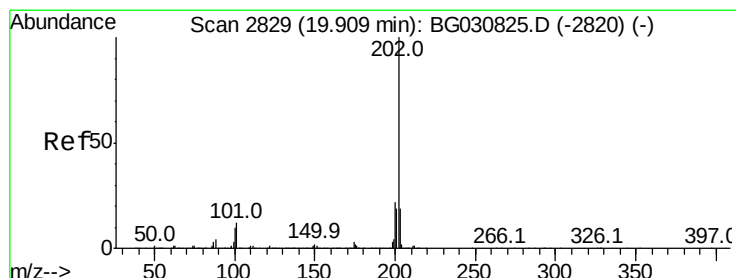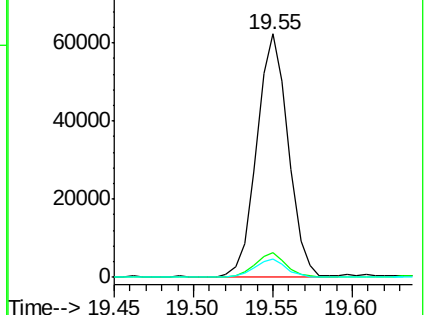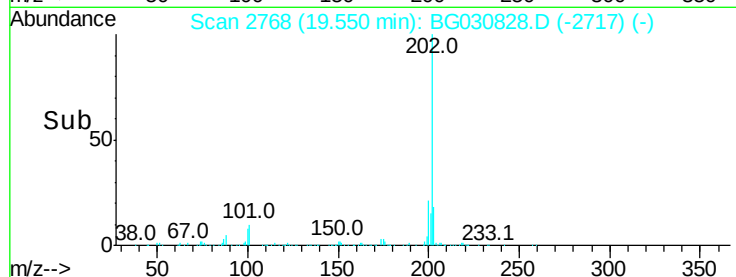

#77

Pyrene

Concen: 2.300 ng/ul

RT: 19.91 min Scan# 2830

Delta R.T. 0.01 min

Lab File: BG030828.D

Acq: 8 Nov 2017 3:54


Tgt Ion:202 Resp: 88057

Ion Ratio Lower Upper

202 100

101 9.5 8.4 12.6



100 8.5 7.0 10.6

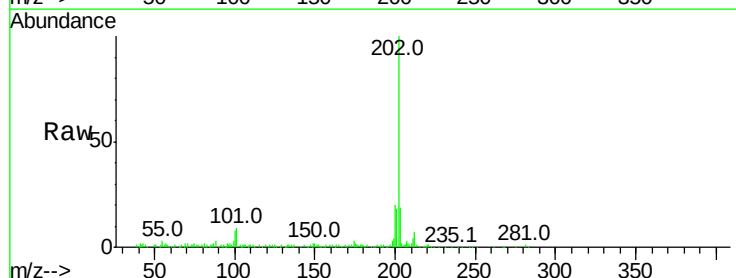


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

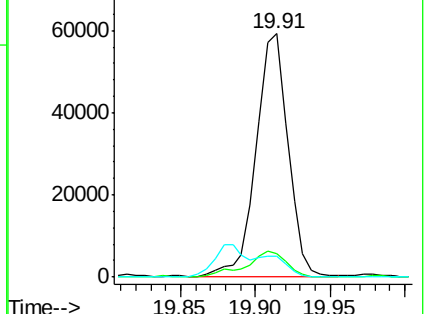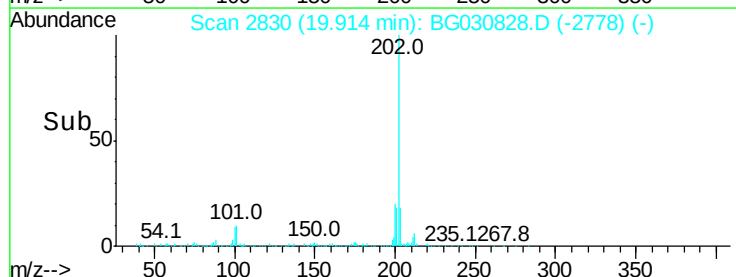

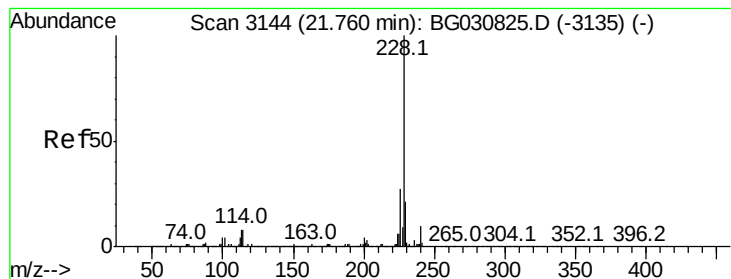

#80

Benzo(a)anthracene

Concen: 1.608 ng/ul

RT: 21.83 min Scan# 3156

Delta R.T. 0.07 min

Lab File: BG030828.D

Acq: 8 Nov 2017 3:54


Instrument :

BNA_G

ClientSampleId :

Tot Ion:228 Resp: 57542



Ion	Ratio	Lower	Upper
228	100		
229	20.6	16.2	24.4
226	31.0	22.2	33.2

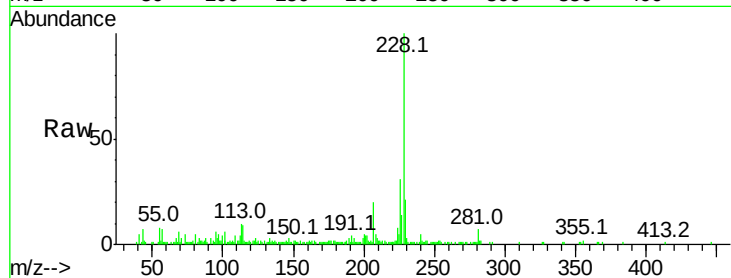

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

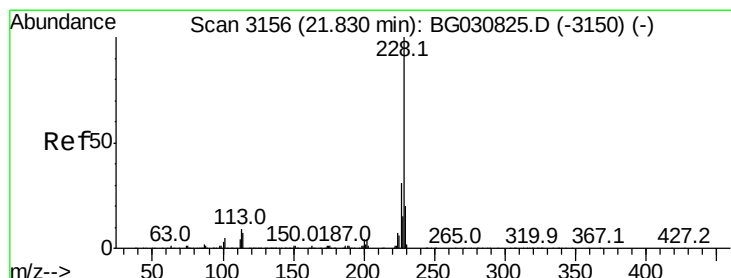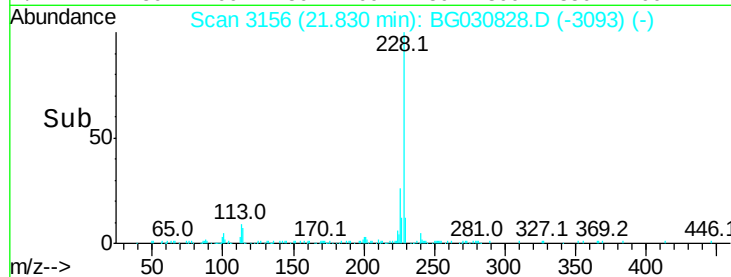

#82

Chrysene

Concen: 1.777 ng/ul

RT: 21.83 min Scan# 3156



Delta R.T. -0.00 min


Lab File: BG030828.D

Acq: 8 Nov 2017 3:54

Tgt Ion:228 Resp: 57806

Ion	Ratio	Lower	Upper
228	100		
226	31.0	24.2	36.2
229	20.6	15.2	22.8

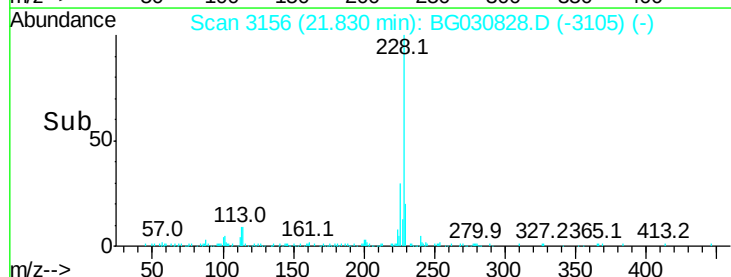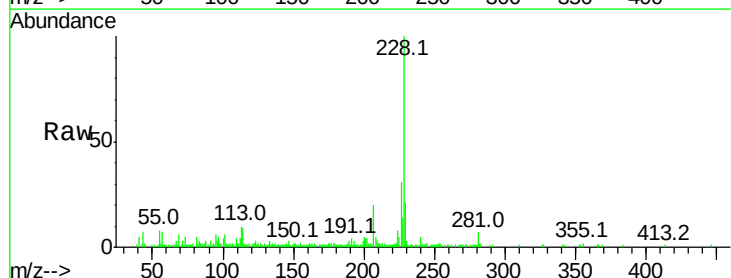

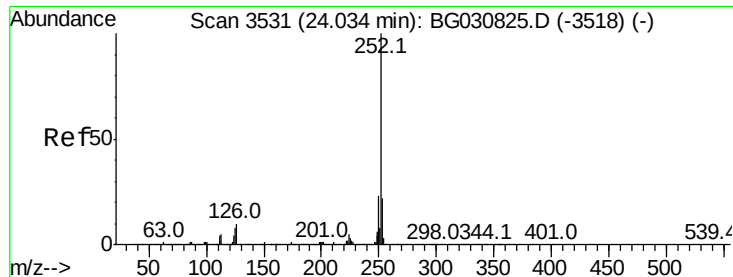

#85

Benzo(b)fluoranthene

Concen: 2.342 ng/ul

RT: 24.03 min Scan# 3531

Delta R.T. -0.00 min

Lab File: BG030828.D





Acq: 8 Nov 2017 3:54

Instrument :

BNA_G

ClientSampleId :

Tot Ion:	252	Resp:	82473
Ion Ratio	Lower	Upper	
252	100		
253	23.0	17.0	25.4
125	10.1	7.5	11.3

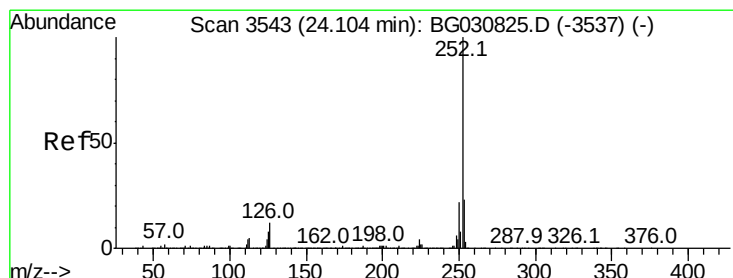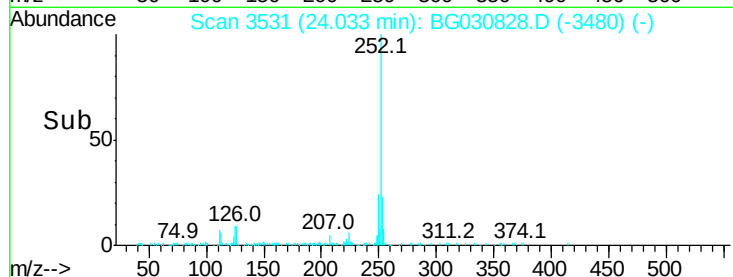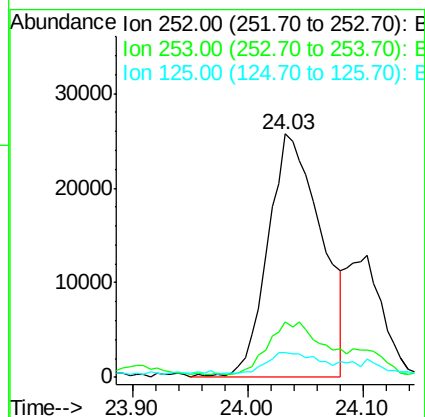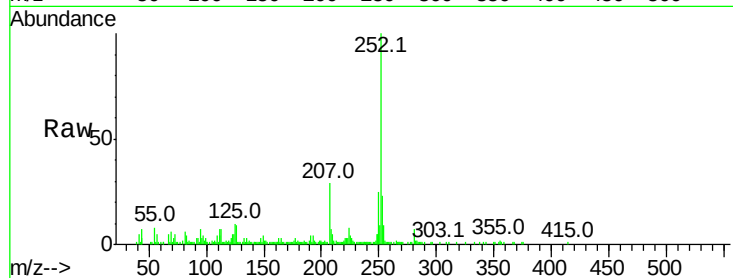

#86

Benzo(k)fluoranthene

Concen: 2.423 ng/ul




RT: 24.03 min Scan# 3531


Delta R.T. -0.07 min

Lab File: BG030828.D

Acq: 8 Nov 2017 3:54

Tgt Ion:	252	Resp:	82473
Ion Ratio	Lower	Upper	
252	100		
253	23.0	17.2	25.8
125	10.1	7.8	11.8

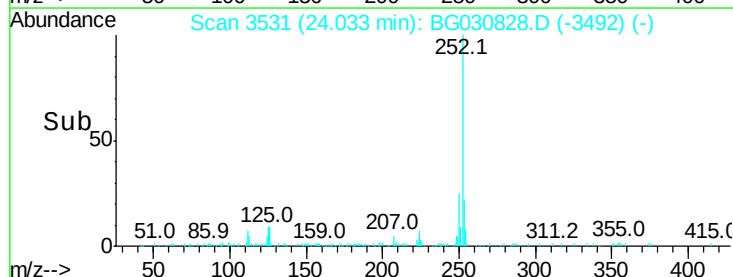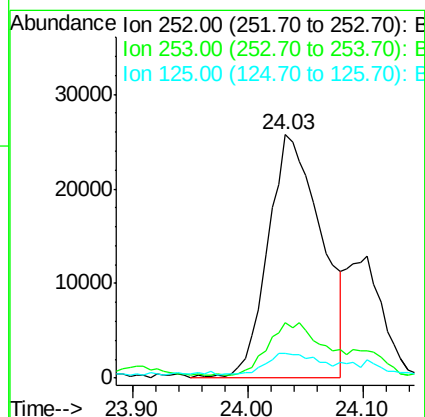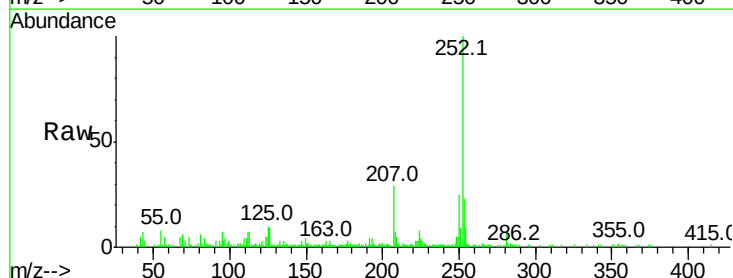

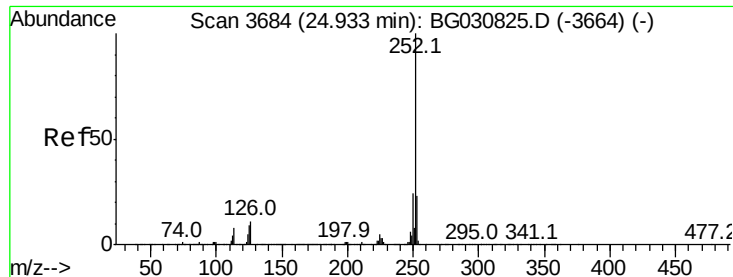

#88

Benzo(a)pyrene

Concen: 1.637 ng/ul

RT: 24.93 min Scan# 3684

Delta R.T. -0.00 min

Lab File: BG030828.D

Acq: 8 Nov 2017 3:54

Instrument :

BNA_G

ClientSampleId :


Tot Ion:252 Resp: 56116

Ion Ratio Lower Upper

252 100

253 27.0 17.1 25.7#




125 9.3 7.8 11.8

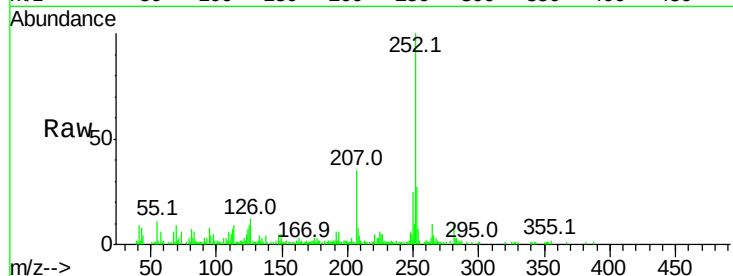

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

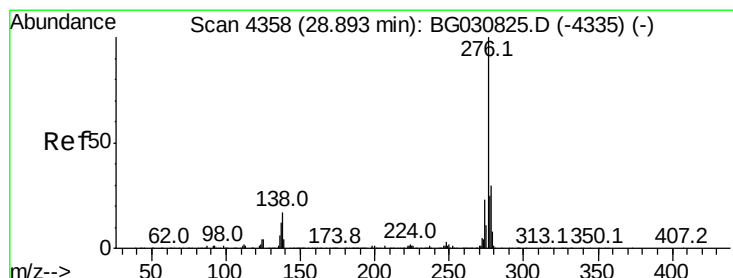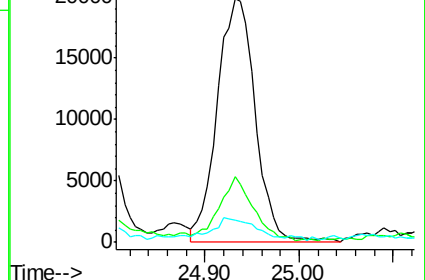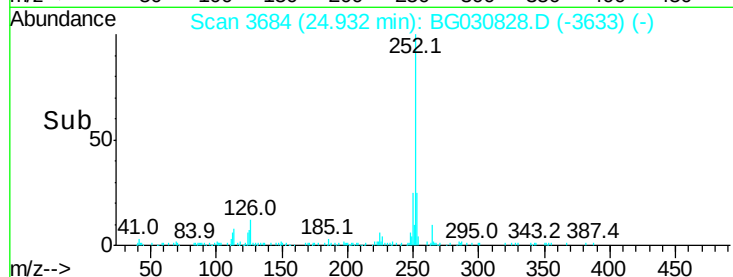

#89

Indeno(1,2,3-cd)pyrene

Concen: 1.178 ng/ul

RT: 28.87 min Scan# 4354

Delta R.T. -0.02 min

Lab File: BG030828.D

Acq: 8 Nov 2017 3:54


Tgt Ion:276 Resp: 45690

Ion Ratio Lower Upper

276 100

138 15.0 13.4 20.0



277 21.2 18.6 28.0

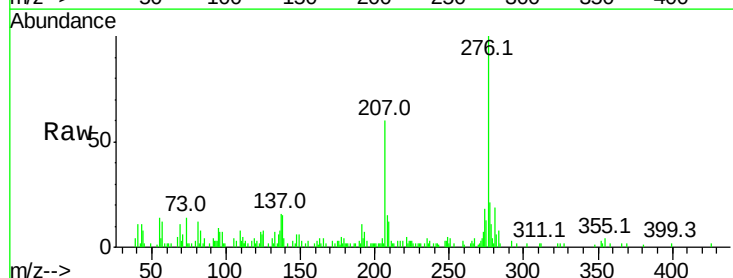


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

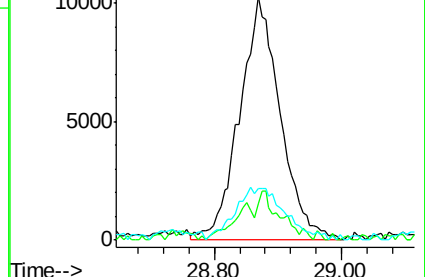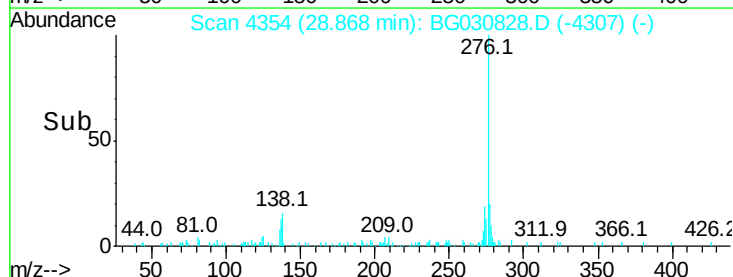

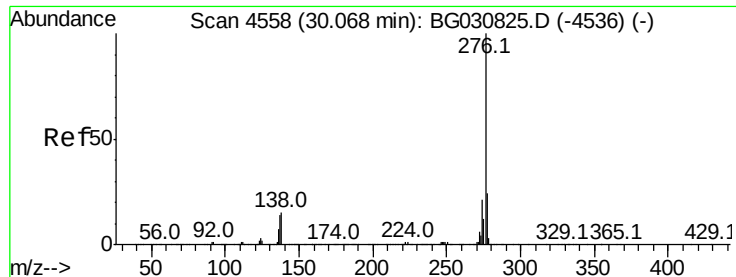

#91

Benzo(a,h,i)perylene

Concen: 1.254 ng/ul

RT: 30.06 min Scan# 4556

Delta R.T. -0.01 min

Lab File: BG030828.D

Acq: 8 Nov 2017 3:54

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 276 Resp: 40290

Ion Ratio Lower Upper

276 100

138 17.6 12.1 18.1

277 25.3 17.7 26.5

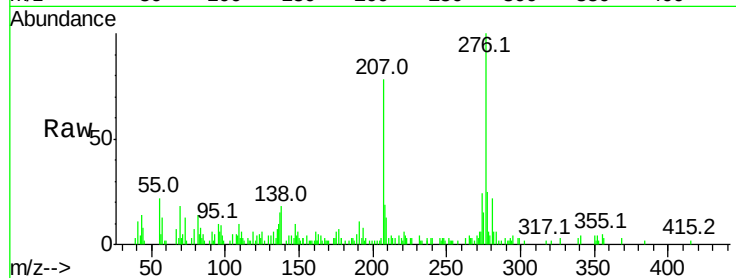

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

