

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110717\
 Data File : BG030828.D
 Acq On : 8 Nov 2017 3:54
 Operator : SJ/JU
 Sample : I6222-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B0EP8

Manual Integrations
 APPROVED

Sohil
 11/8/2017 5:29:58 PM

Quant Time: Nov 08 04:49:46 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 08 04:22:00 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	67545	20.00	ng/ul	0.00
18) Naphthalene-d8	10.97	136	336176	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.77	164	227343	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	541372	20.00	ng/ul	0.00
75) Chrysene-d12	21.78	240	571157	20.00	ng/ul	0.00
83) Perylene-d12	25.09	264	586479	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	8994	5.41	ng/uL	0.00
5) Phenol-d5	7.31	99	183150	28.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.46	67	108289	26.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	149556	32.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	124509	23.78	ng/ul	0.00
19) Nitrobenzene-d5	9.31	128	79128	32.79	ng/ul	0.00
22) 2-Nitrophenol-d4	10.04	143	98933	40.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	170089	30.19	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	187912	28.70	ng/ul	0.00
43) Dimethylphthalate-d6	14.17	166	612438	31.51	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	744101	31.48	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	98775	27.53	ng/ul	0.00
57) Fluorene-d10	15.75	176	560760	35.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.88	200	98313	37.20	ng/ul	0.00
70) Anthracene-d10	17.61	188	830966	32.45	ng/ul	0.00
76) Pyrene-d10	19.88	212	978675	33.10	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.87	264	961930	34.63	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	7.33	94	10925	1.629 ng/ul	91
44) Dimethylphthalate	14.21	163	196301	10.355 ng/ul	99
74) Fluoranthene	19.55	202	86725	2.652 ng/ul	98
77) Pyrene	19.91	202	88057	2.300 ng/ul	98
80) Benzo(a)anthracene	21.76	228	56438m	1.577 ng/ul	
82) Chrysene	21.83	228	57806	1.777 ng/ul	98
85) Benzo(b)fluoranthene	24.03	252	82473	2.342 ng/ul	97
88) Benzo(a)pyrene	24.93	252	56116	1.637 ng/ul#	91
89) Indeno(1,2,3-cd)pyrene	28.87	276	45690	1.178 ng/ul	96
91) Benzo(g,h,i)perylene	30.06	276	40290	1.254 ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG110717\
Data File : BG030828.D
Acq On : 8 Nov 2017 3:54
Operator : SJ/JU
Sample : I6222-01
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampled :
B0EP8

Manual Integrations
APPROVED

Sohil
11/8/2017 5:29:58 PM

Quant Time: Nov 08 04:49:46 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 08 04:22:00 2017
Response via : Initial Calibration

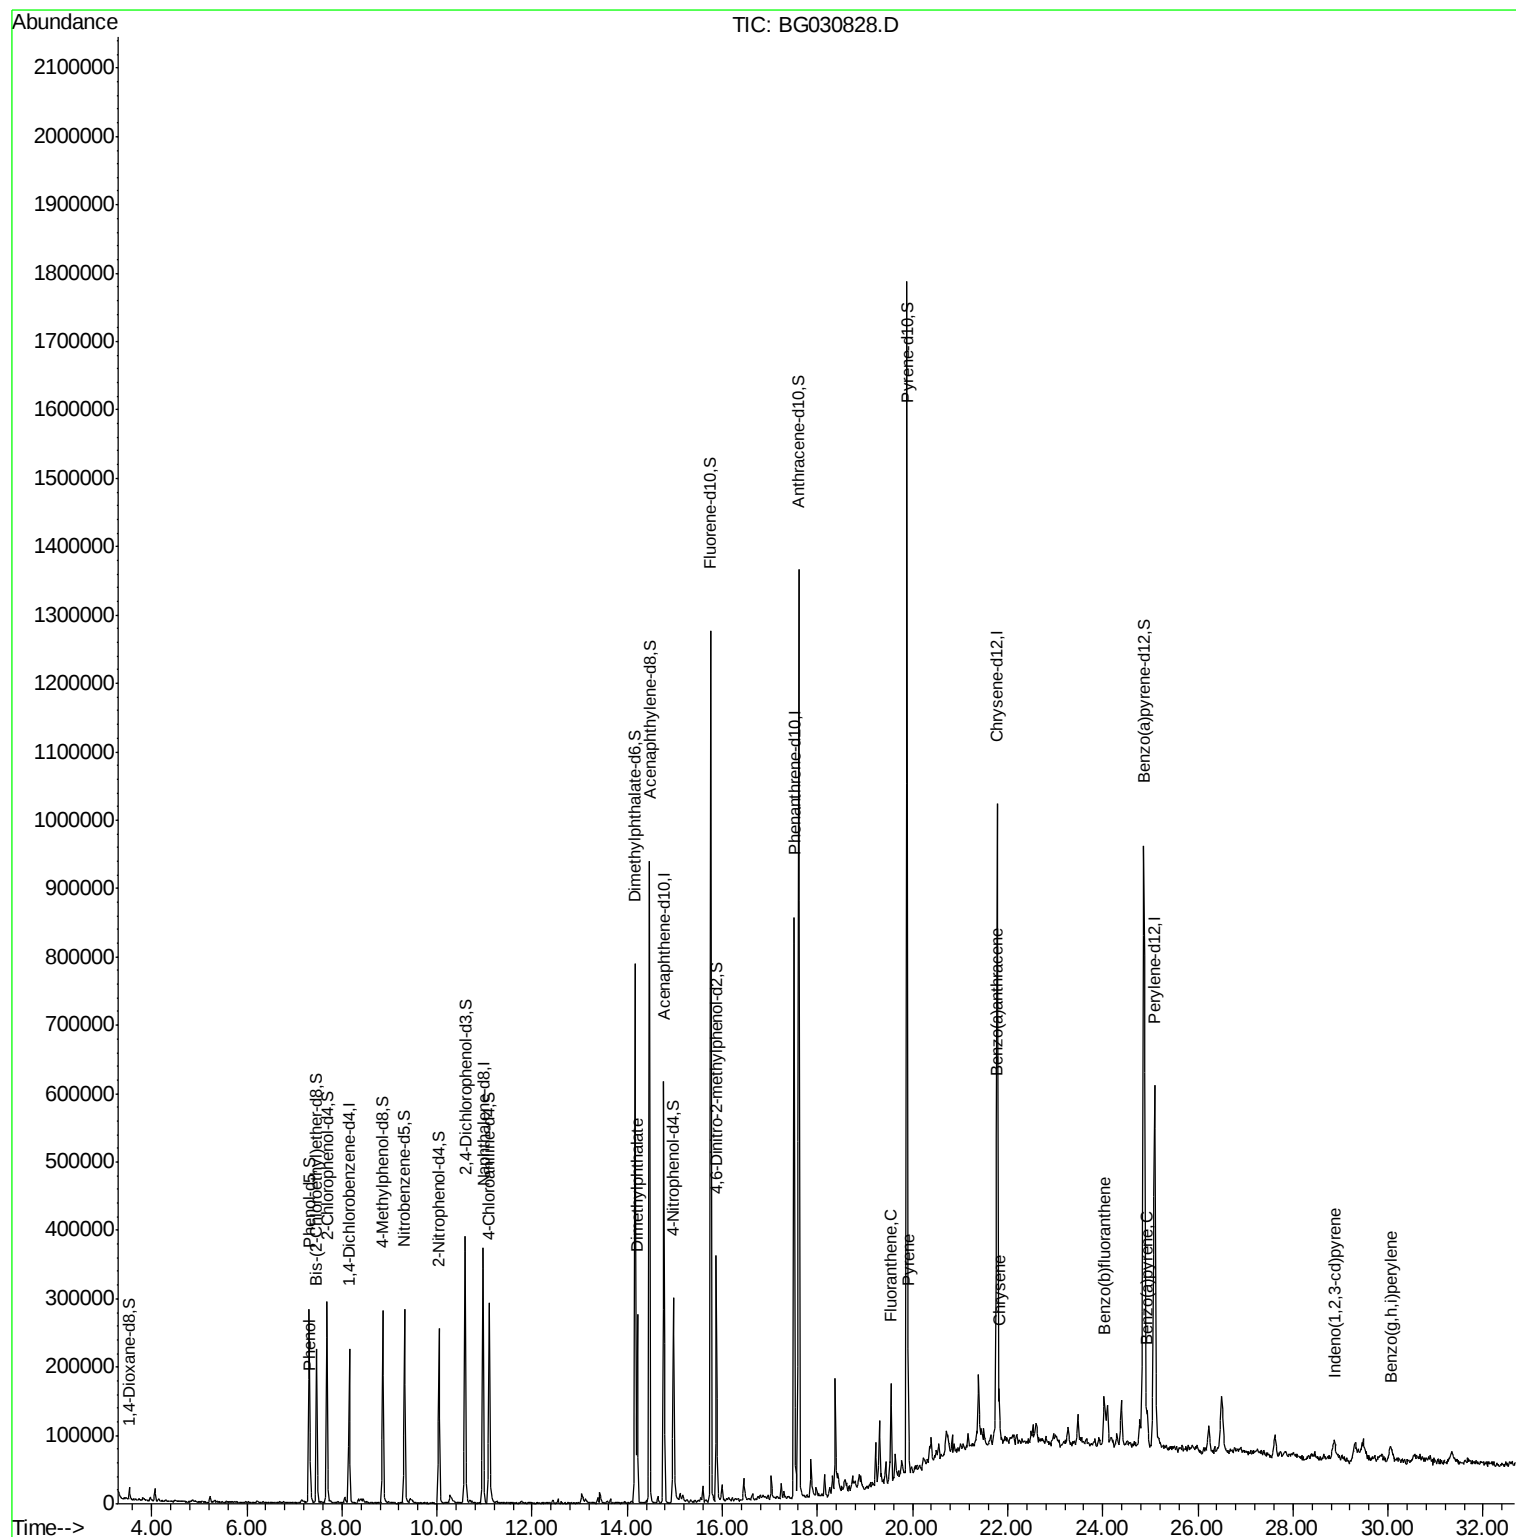

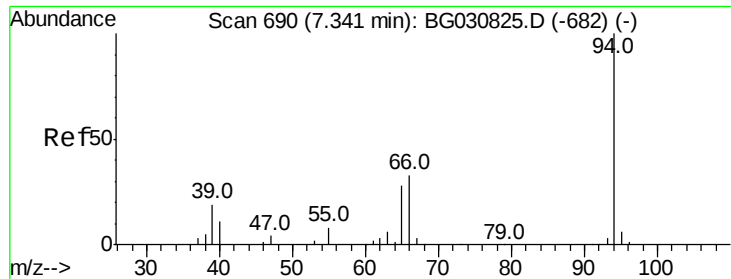

#6

Phenol





Concen: 1.629 ng/ul
 RT: 7.33 min Scan# 689
 Delta R.T. -0.01 min
 Lab File: BG030828.D
 Acq: 8 Nov 2017 3:54

Instrument :
 BNA_G
 ClientSampled :
 B0EP8

Tot Ion	Ratio	Lower	Upper
94	100		
65	28.3	27.1	40.7
66	38.5	34.6	52.0

Manual Integrations
 APPROVED

Sohil
 11/8/2017 5:29:58 PM

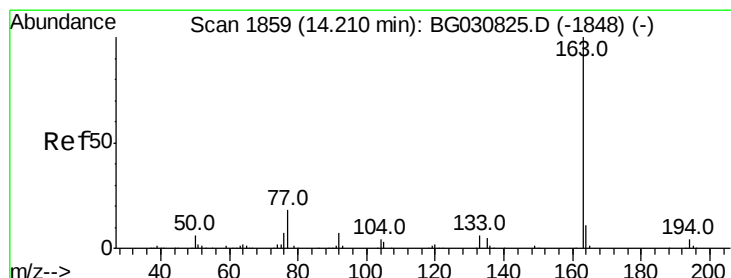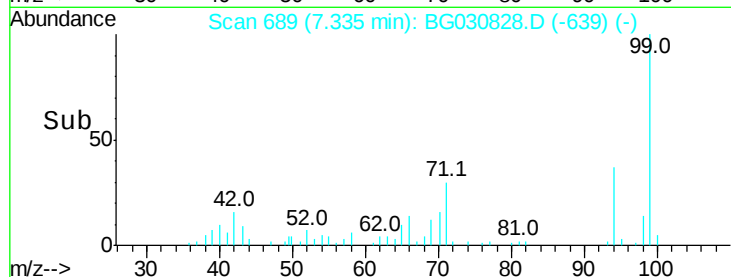
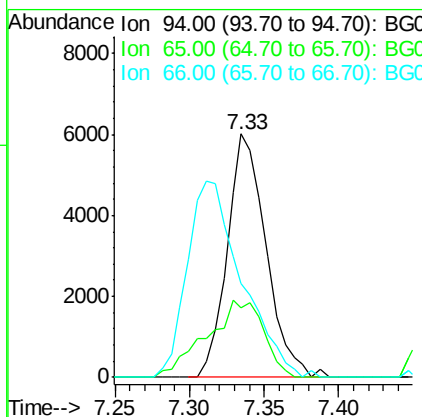
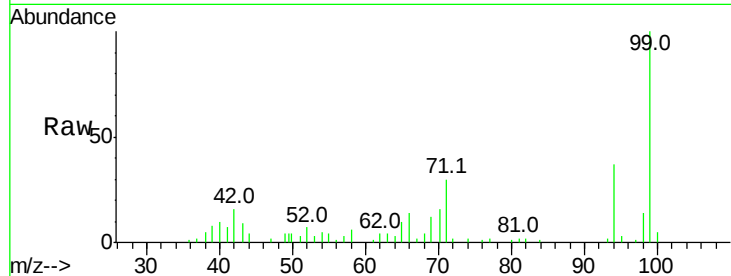



#44

Dimethylphthalate

Concen: 10.355 ng/ul
 RT: 14.21 min Scan# 1859
 Delta R.T. -0.00 min
 Lab File: BG030828.D
 Acq: 8 Nov 2017 3:54

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.5	5.3
164	9.9	7.6	11.4

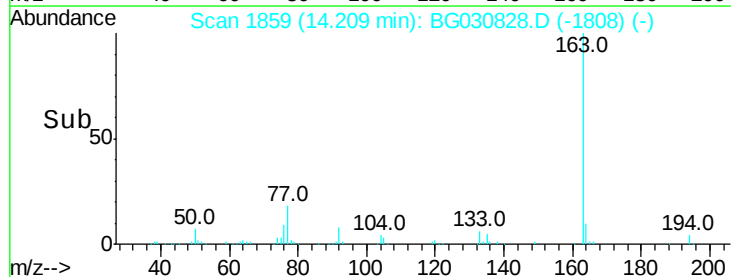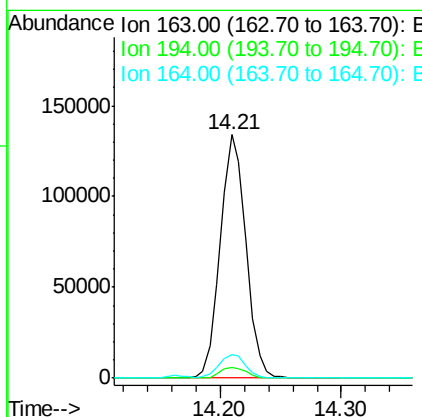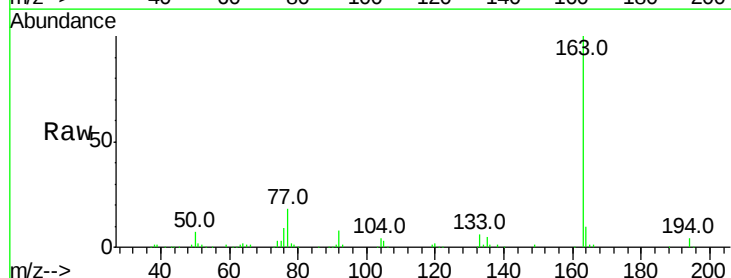

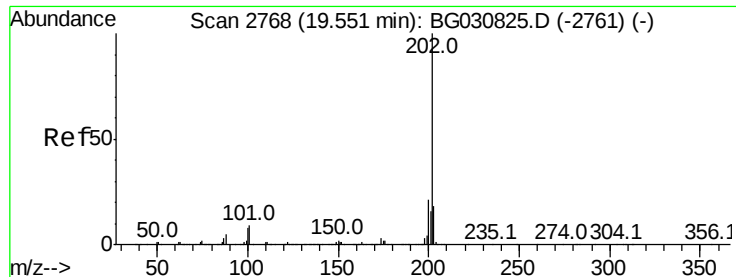

#74

Fluoranthene

Concen: 2.652 ng/ul

RT: 19.55 min Scan# 2768

Delta R.T. -0.00 min

Lab File: BG030828.D

Acq: 8 Nov 2017 3:54

Instrument :

BNA_G





ClientSampleId :

B0EP8

Tot Ion:	202	Resp:	86725
Ion Ratio	Lower	Upper	
202	100		
101	10.0	7.4	11.2
100	7.5	5.6	8.4

Manual Integrations
APPROVED

Sohil
11/8/2017 5:29:58 PM

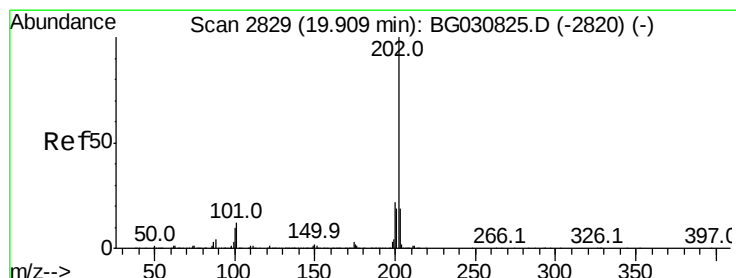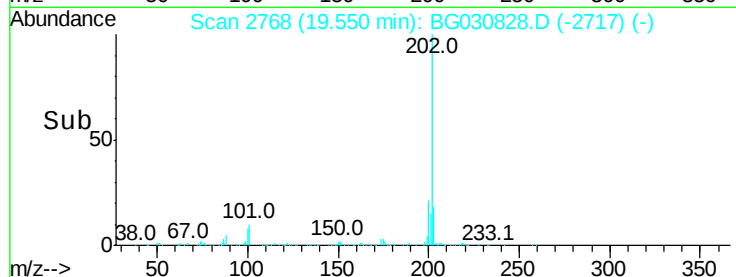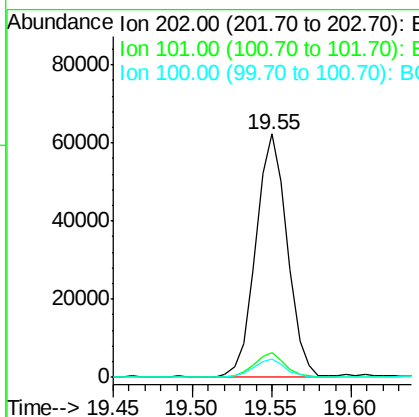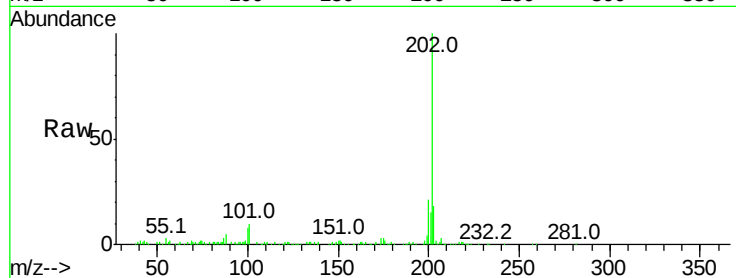

#77

Pyrene

Concen: 2.300 ng/ul




RT: 19.91 min Scan# 2830


Delta R.T. 0.01 min

Lab File: BG030828.D

Acq: 8 Nov 2017 3:54

Tgt Ion:	202	Resp:	88057
Ion Ratio	Lower	Upper	
202	100		
101	9.5	8.4	12.6
100	8.5	7.0	10.6

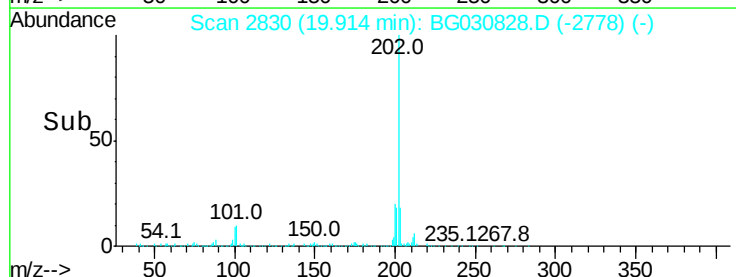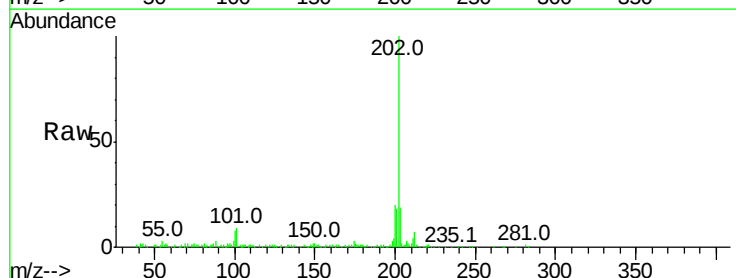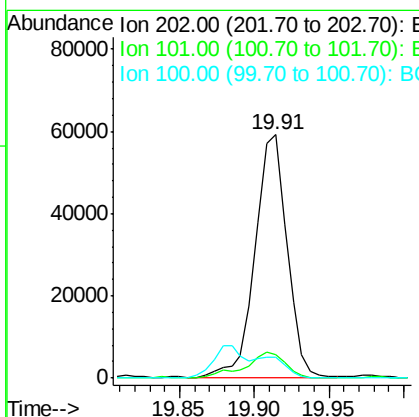

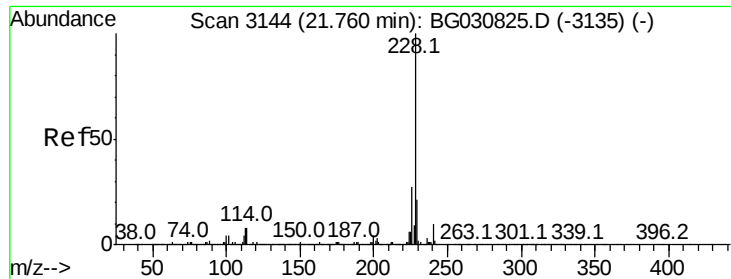





#80
Benzo(a)anthracene
Concen: 1.577 ng/ul m
RT: 21.76 min Scan# 3144
Delta R.T. -0.00 min
Lab File: BG030828.D
Acq: 8 Nov 2017 3:54

Instrument :
BNA_G
ClientSampleId :
B0EP8

Tot Ion	Ratio	Lower	Upper
228	100		
229	24.9	16.2	24.4#
226	29.0	22.2	33.2




Manual Integrations
APPROVED


Sohil
11/8/2017 5:29:58 PM

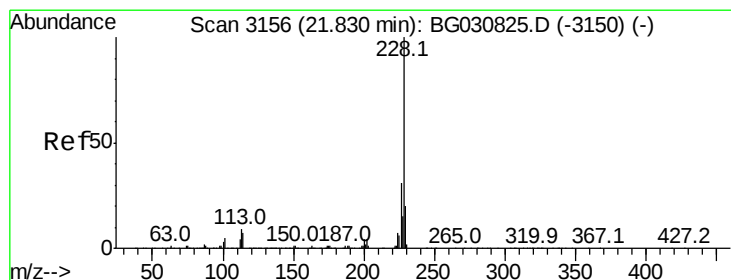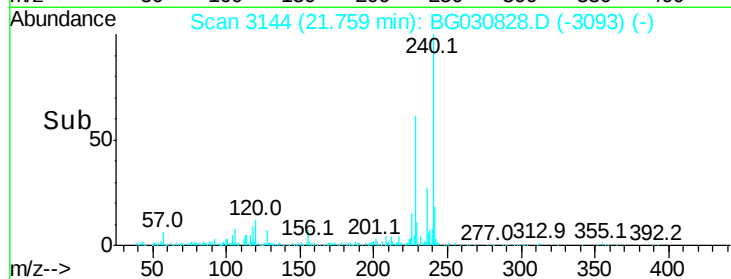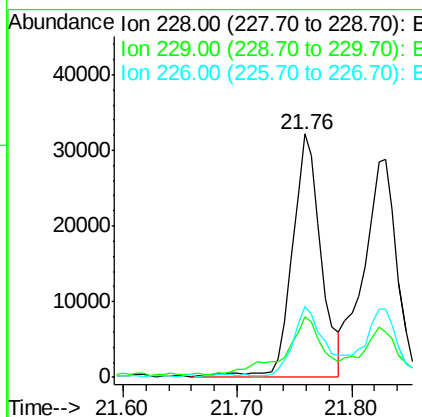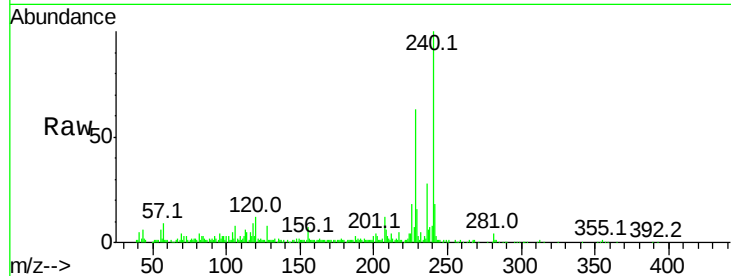

#82
Chrysene
Concen: 1.777 ng/ul
RT: 21.83 min Scan# 3156
Delta R.T. -0.00 min
Lab File: BG030828.D
Acq: 8 Nov 2017 3:54

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.0	24.2	36.2
229	20.6	15.2	22.8

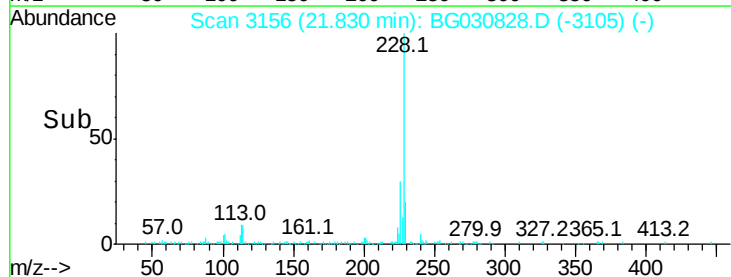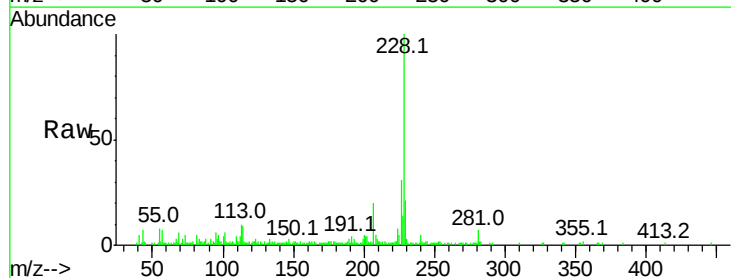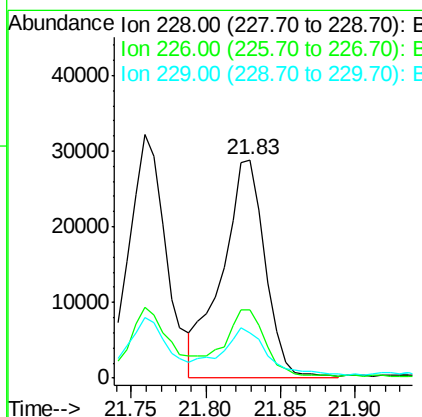

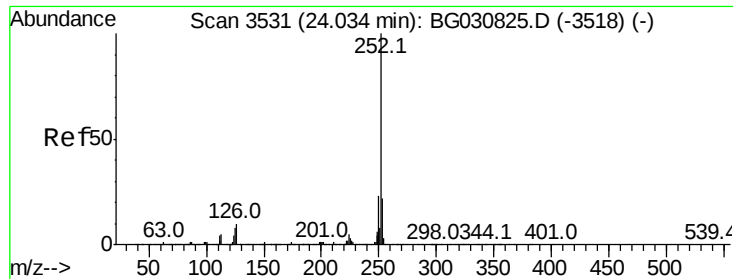

#85

Benzo(b)fluoranthene

Concen: 2.342 ng/ul

RT: 24.03 min Scan# 3531

Delta R.T. -0.00 min

Lab File: BG030828.D

Acq: 8 Nov 2017 3:54

Instrument :

BNA_G





ClientSampleId :

B0EP8

Tot Ion:	252	Resp:	82473
Ion Ratio	Lower	Upper	
252	100		
253	23.0	17.0	25.4
125	10.1	7.5	11.3

Manual Integrations
APPROVED

Sohil
11/8/2017 5:29:58 PM

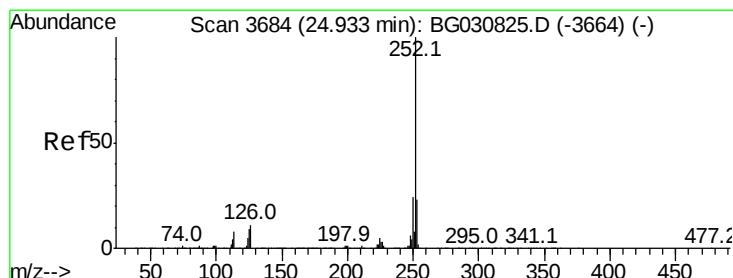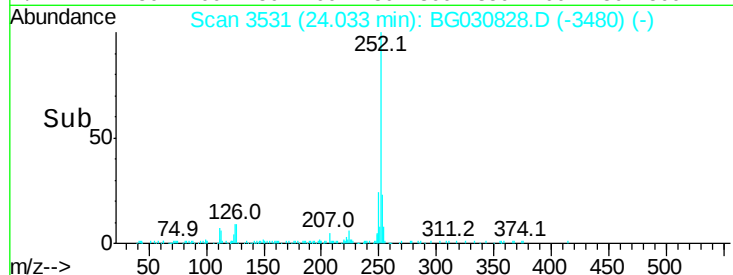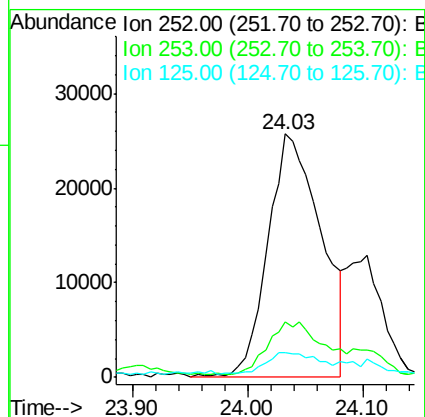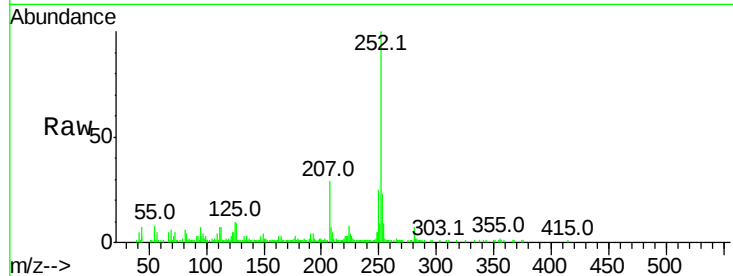

#88

Benzo(a)pyrene

Concen: 1.637 ng/ul




RT: 24.93 min Scan# 3684


Delta R.T. -0.00 min

Lab File: BG030828.D

Acq: 8 Nov 2017 3:54

Tgt Ion:	252	Resp:	56116
Ion Ratio	Lower	Upper	
252	100		
253	27.0	17.1	25.7#
125	9.3	7.8	11.8

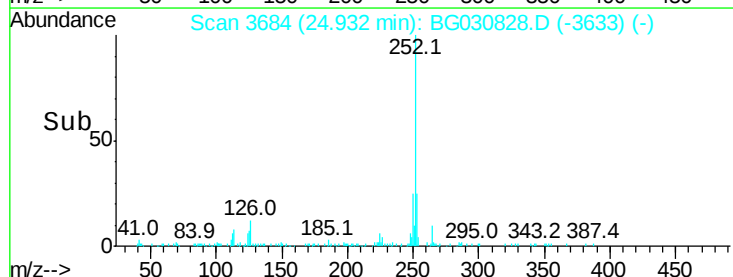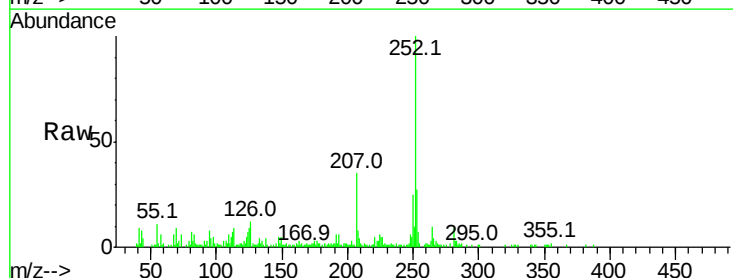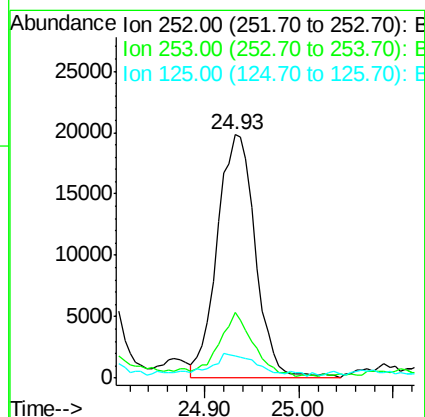

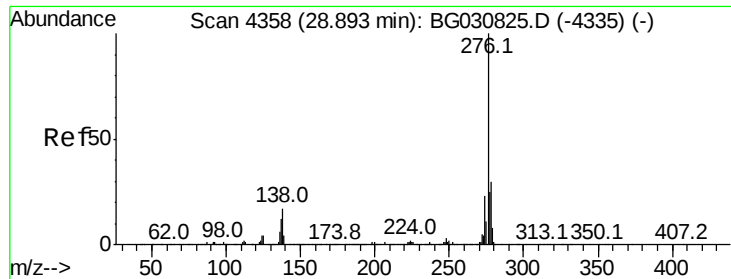





#89
 Indeno(1,2,3-cd)pyrene
 Concen: 1.178 ng/ul
 RT: 28.87 min Scan# 4354
 Delta R.T. -0.02 min
 Lab File: BG030828.D
 Acq: 8 Nov 2017 3:54

Instrument :
 BNA_G
 ClientSampled :
 B0EP8

Tot Ion	Ratio	Lower	Upper
276	100		
138	15.0	13.4	20.0
277	21.2	18.6	28.0

Manual Integrations
 APPROVED

Sohil
 11/8/2017 5:29:58 PM

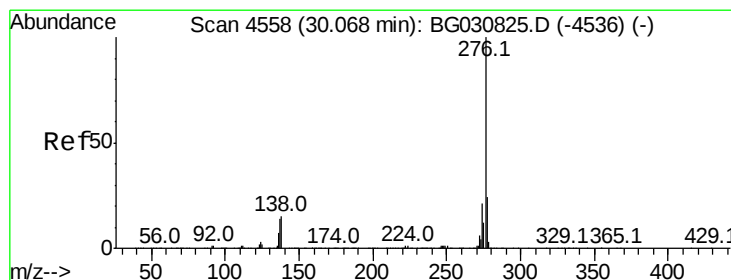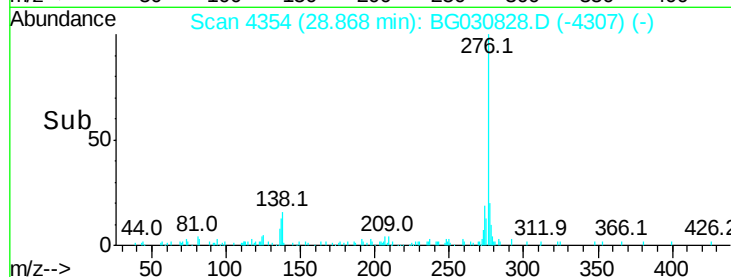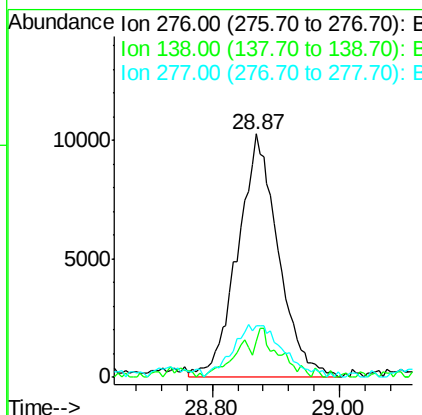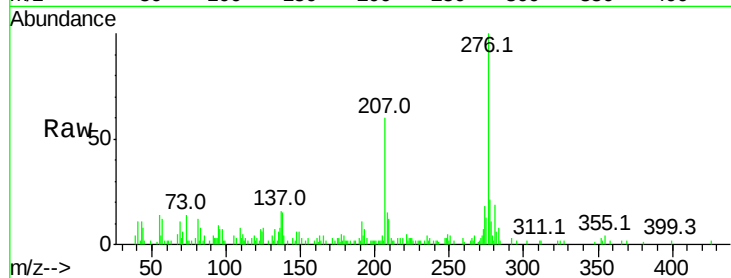

#91
 Benzo(g,h,i)perylene
 Concen: 1.254 ng/ul
 RT: 30.06 min Scan# 4556
 Delta R.T. -0.01 min
 Lab File: BG030828.D
 Acq: 8 Nov 2017 3:54

Tgt Ion	Ratio	Lower	Upper
276	100		
138	17.6	12.1	18.1
277	25.3	17.7	26.5

