




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063273.D
Acq On : 9 Nov 2024 20:33
Operator : RC/JU
Sample : P4744-06
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCP60

Manual IntegrationsAPPROVED

Quant Time: Nov 10 00:43:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/11/2024

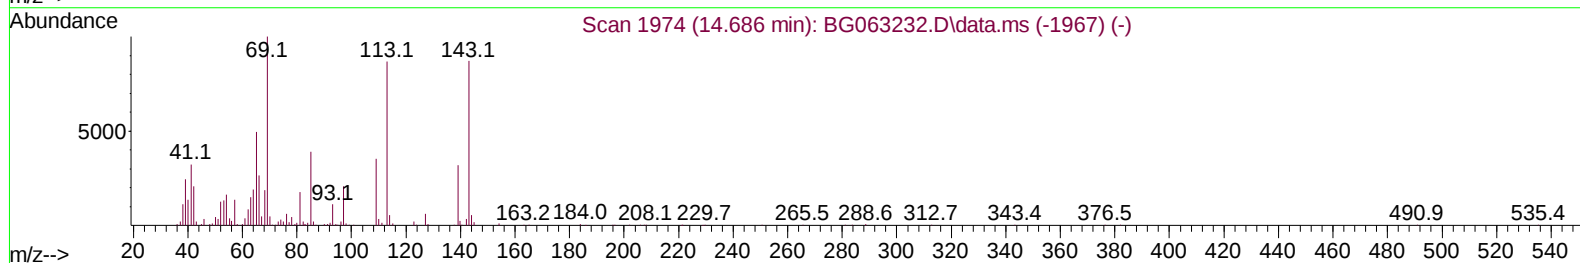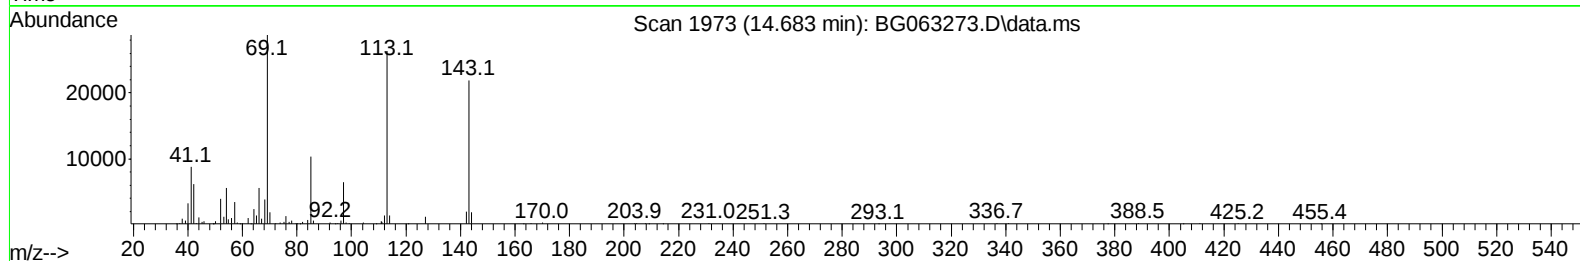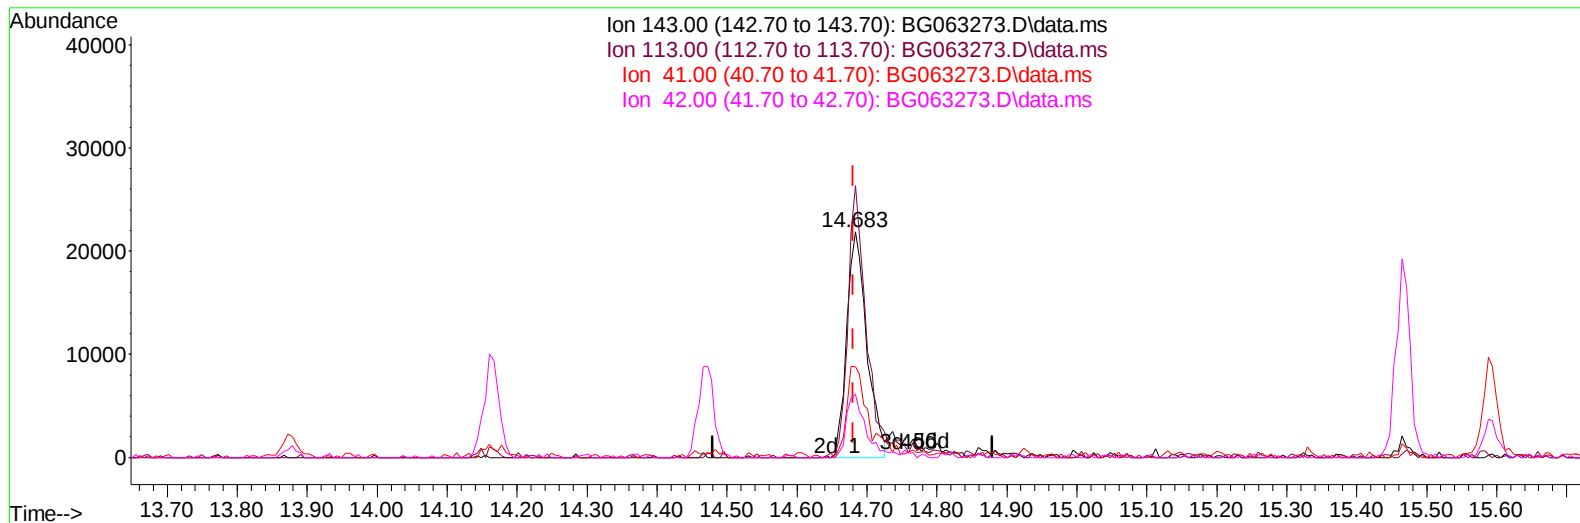

TIC: BG063273.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.683min (+ 0.003) 7.65 ng/u1

response 43397

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	123.00	120.17
41.00	42.60	40.08
42.00	30.90	28.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063273.D
Acq On : 9 Nov 2024 20:33
Operator : RC/JU
Sample : P4744-06
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCP60

Manual IntegrationsAPPROVED

Quant Time: Nov 10 00:43:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/11/2024

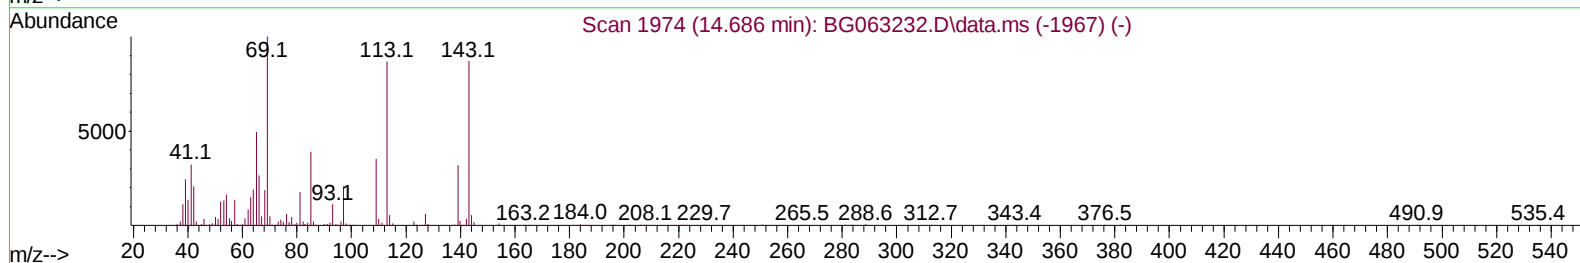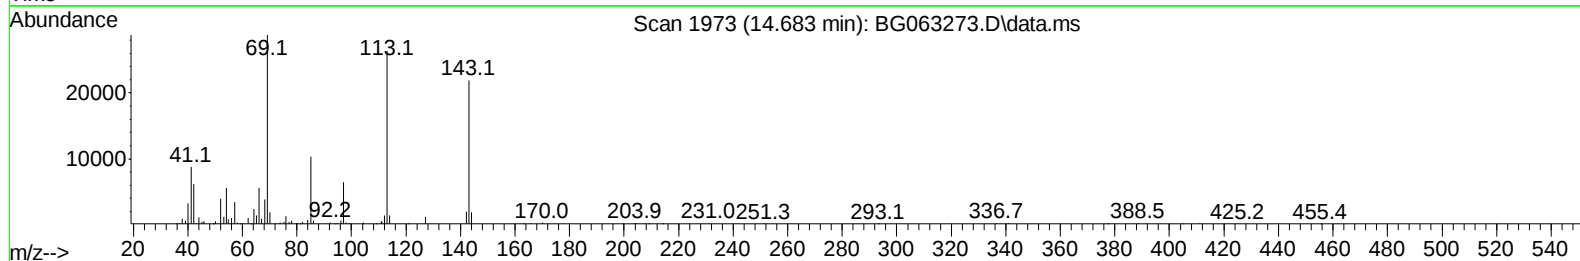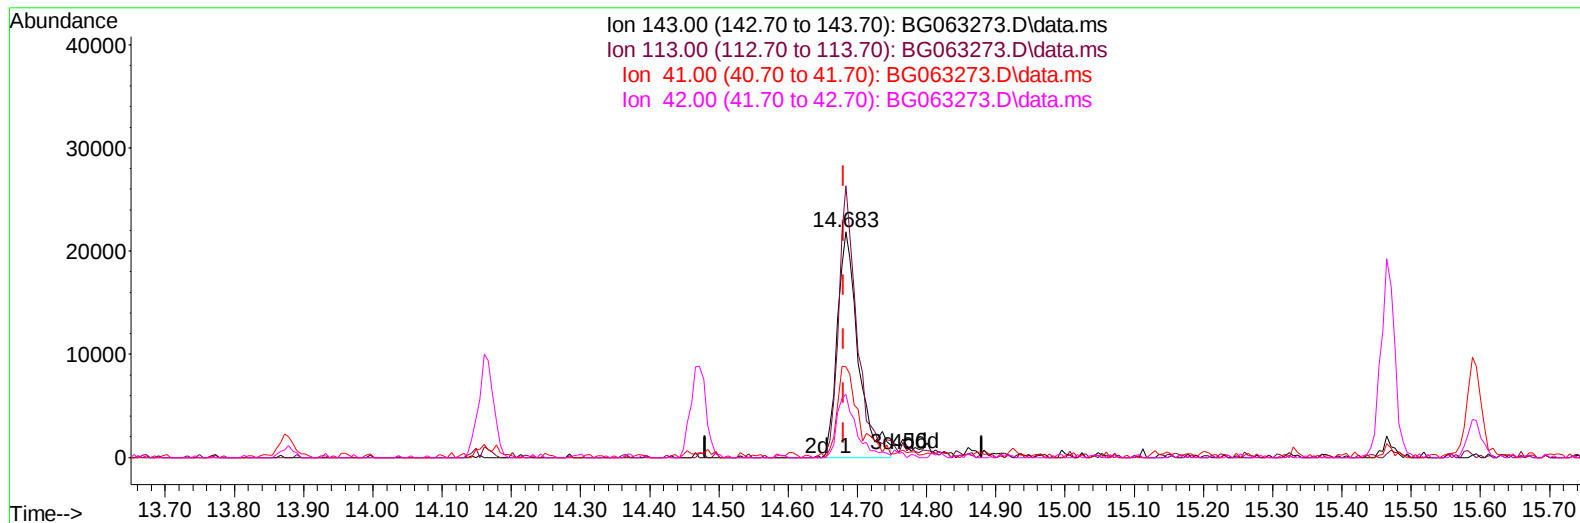

TIC: BG063273.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.683min (+ 0.003) 8.10 ng/ul m

response 45953

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	123.00	120.17
41.00	42.60	40.08
42.00	30.90	28.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
 Data File : BG063273.D
 Acq On : 9 Nov 2024 20:33
 Operator : RC/JU
 Sample : P4744-06
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCP60

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/10/2024
 Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 10 00:43:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.833	152	125940	20.000	ng/ul	0.00
20) Naphthalene-d8	10.624	136	588356	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.472	164	528766	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.222	188	1222135	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.475	240	1246781	20.000	ng/ul	# 0.00
88) Perylene-d12	24.507	264	1352626	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.303	96	13767	4.943	ng/uL	0.00
4) Pyridine-d5	3.708	84	73584	7.993	ng/ul	0.00
7) Phenol-d5	7.010	99	112166	9.870	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.163	67	213635	32.050	ng/ul	0.00
11) 2-Chlorophenol-d4	7.368	132	240398	32.591	ng/ul	0.00
15) 4-Methylphenol-d8	8.538	113	226947	23.561	ng/ul	0.00
21) Nitrobenzene-d5	8.990	128	145952	35.285	ng/ul	0.00
24) 2-Nitrophenol-d4	9.707	143	189675	35.480	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.247	165	357841	34.108	ng/ul	0.00
31) 4-Chloroaniline-d4	10.759	131	393851	28.822	ng/ul	0.00
46) Dimethylphthalate-d6	13.879	166	1288770	31.116	ng/ul	0.00
49) Acenaphthylene-d8	14.166	160	1404004	34.633	ng/ul	0.00
54) 4-Nitrophenol-d4	14.683	143	45953m	8.103	ng/ul	0.00
60) Fluorene-d10	15.465	176	1173057	33.558	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.594	200	227894	29.671	ng/ul	0.00
73) Anthracene-d10	17.322	188	1923399	36.618	ng/ul	0.00
81) Pyrene-d10	19.619	212	2354038	37.658	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.307	264	2400055	36.751	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063273.D
Acq On : 9 Nov 2024 20:33
Operator : RC/JU
Sample : P4744-06
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCP60

Manual IntegrationsAPPROVED

Quant Time: Nov 10 00:43:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/10/2024
Supervised By :mohammad ahmed 11/11/2024

