

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
 Data File : BG063230.D
 Acq On : 8 Nov 2024 16:05
 Operator : RC/JU
 Sample : P4636-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CC0P2

Quant Time: Nov 08 15:38:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.836	152	103581	20.000	ng/u1	0.00
20) Naphthalene-d8	10.627	136	493031	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.475	164	426078	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.225	188	1044044	20.000	ng/u1	0.00
79) Chrysene-d12	21.479	240	1046189	20.000	ng/u1	0.00
88) Perylene-d12	24.516	264	1119272	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.300	96	6083	2.655	ng/uL	0.00
4) Pyridine-d5	3.711	84	87942	11.615	ng/u1	0.00
7) Phenol-d5	7.007	99	153003	16.370	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.166	67	90917	16.584	ng/u1	0.00
11) 2-Chlorophenol-d4	7.372	132	108142	17.826	ng/u1	0.00
15) 4-Methylphenol-d8	8.541	113	135965	17.163	ng/u1	0.00
21) Nitrobenzene-d5	8.988	128	61162	17.645	ng/u1	0.00
24) 2-Nitrophenol-d4	9.710	143	76948	17.177	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	157571	17.923	ng/u1	0.00
31) 4-Chloroaniline-d4	10.756	131	168825	14.743	ng/u1	0.00
46) Dimethylphthalate-d6	13.882	166	580225	17.385	ng/u1	0.00
49) Acenaphthylene-d8	14.164	160	631557	19.333	ng/u1	0.00
54) 4-Nitrophenol-d4	14.687	143	69082	15.118	ng/u1	0.00
60) Fluorene-d10	15.468	176	539460	19.152	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.597	200	105630	16.098	ng/u1	0.00
73) Anthracene-d10	17.325	188	842450	18.775	ng/u1	0.00
81) Pyrene-d10	19.622	212	1143084	21.792	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.311	264	1087111	20.117	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.379	149	195422	7.639	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063230.D
Acq On : 8 Nov 2024 16:05
Operator : RC/JU
Sample : P4636-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CC0P2


Quant Time: Nov 08 15:38:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

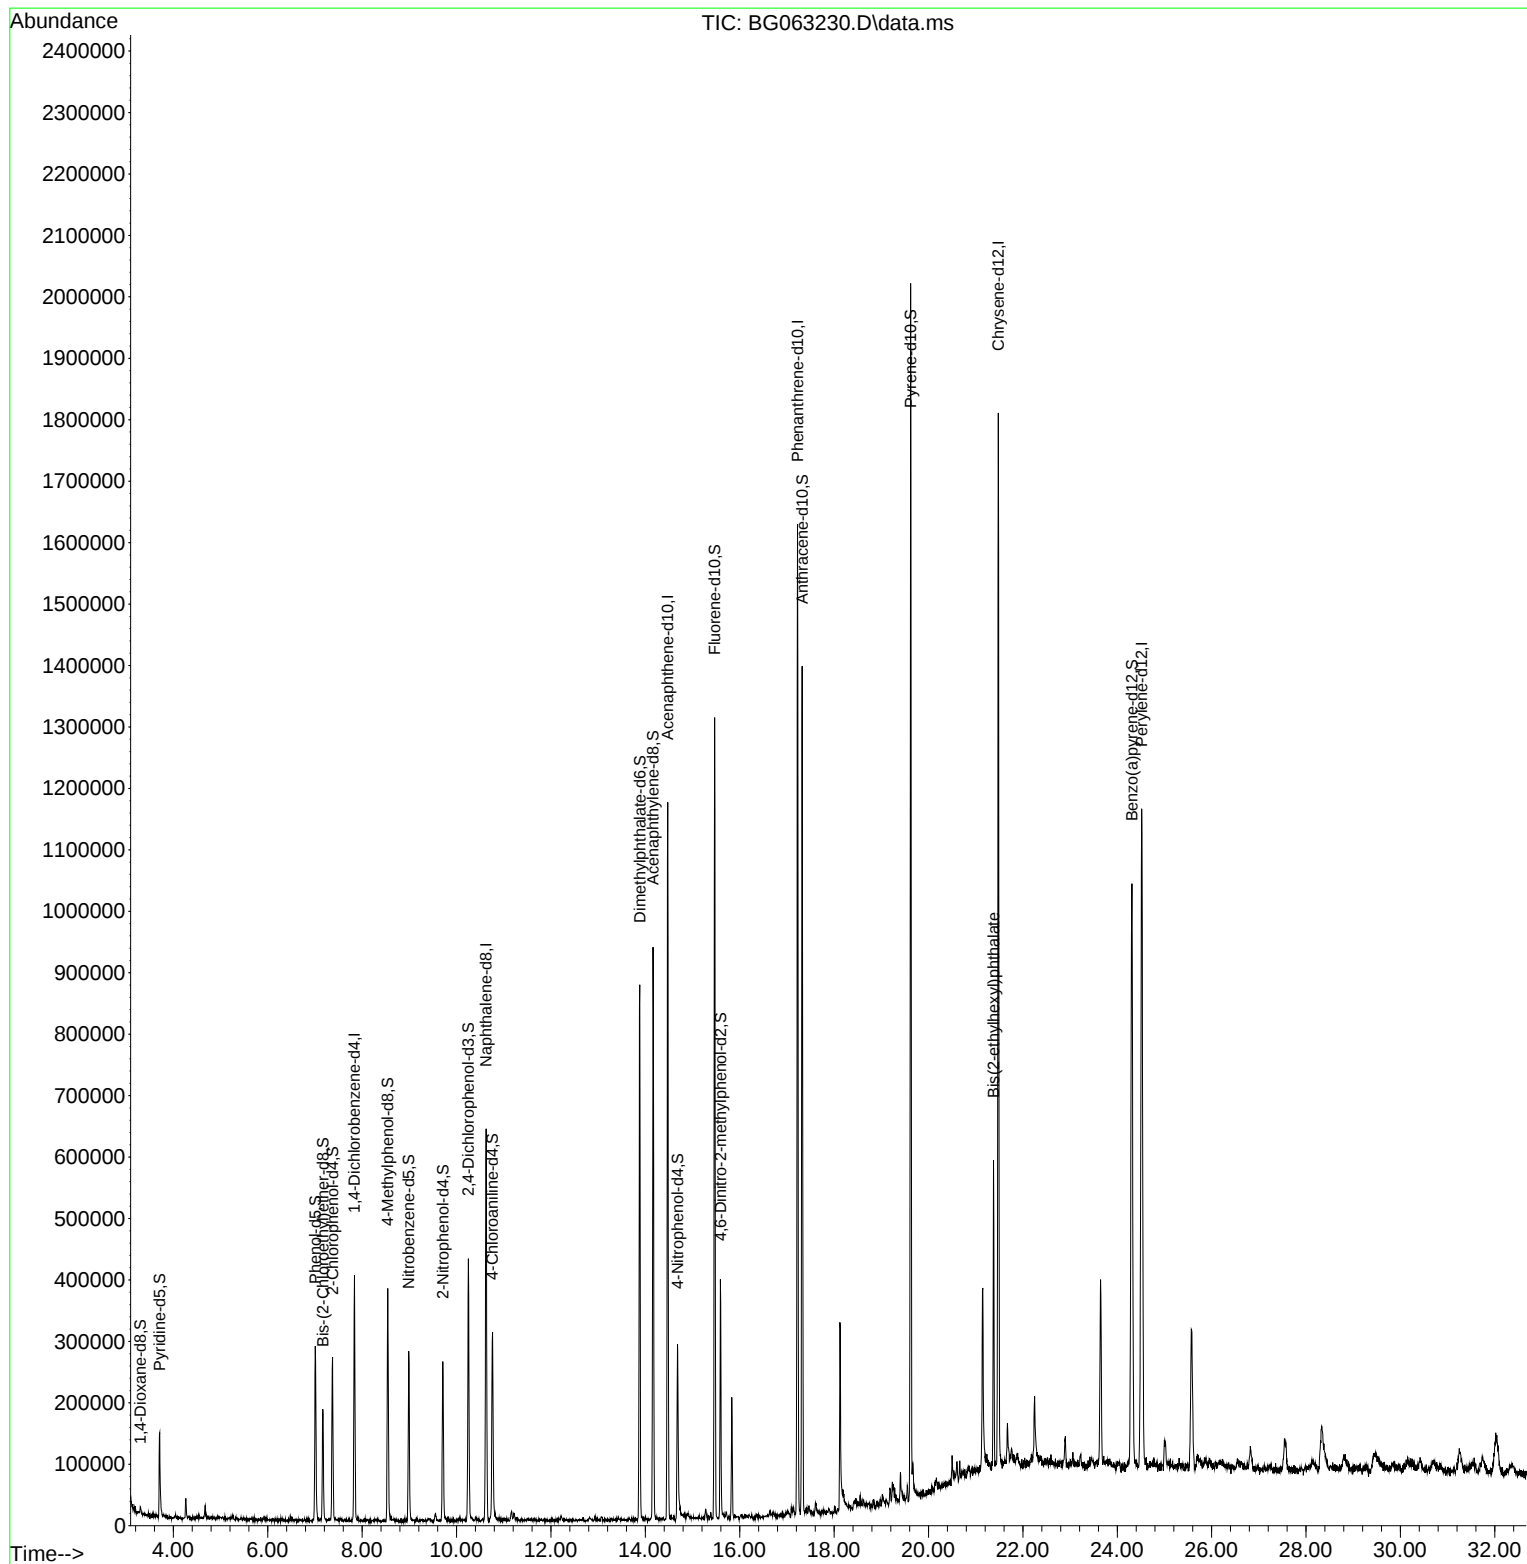

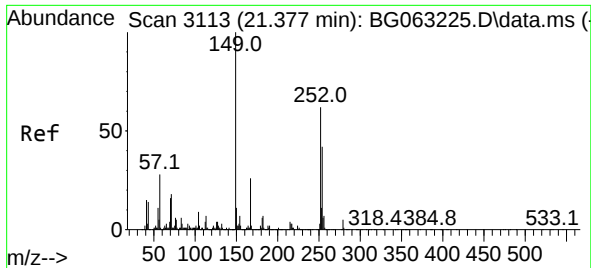

#86
Bis(2-ethylhexyl)phthalate
Concen: 7.639 ng/ul
RT: 21.379 min Scan# 3113
Delta R.T. 0.001 min
Lab File: BG063230.D
Acq: 8 Nov 2024 16:05

Instrument :
BNA_G
ClientSampleId :
CC0P2

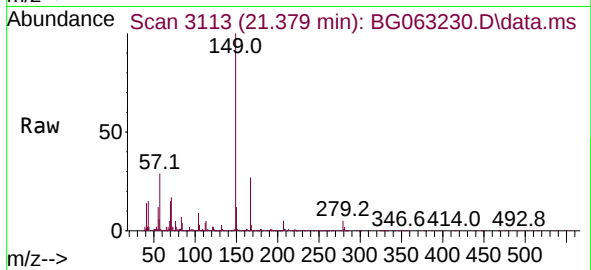

Tgt Ion:149 Resp: 195422
Ion Ratio Lower Upper
149 100
167 26.7 20.6 31.0
279 5.0 4.2 6.4

