

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
 Data File : BG063231.D
 Acq On : 8 Nov 2024 16:43
 Operator : RC/JU
 Sample : P4636-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CC0P4

Quant Time: Nov 08 16:16:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 15:45:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	100470	20.000	ng/ul	0.00
20) Naphthalene-d8	10.625	136	451732	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.474	164	399937	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.223	188	977018	20.000	ng/ul	0.00
79) Chrysene-d12	21.477	240	956069	20.000	ng/ul	0.00
88) Perylene-d12	24.515	264	1031223	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.304	96	7228	3.253	ng/uL	0.00
4) Pyridine-d5	3.710	84	96073	13.082	ng/ul	0.00
7) Phenol-d5	7.012	99	165274	18.230	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.165	67	92763	17.444	ng/ul	0.00
11) 2-Chlorophenol-d4	7.370	132	112119	19.054	ng/ul	0.00
15) 4-Methylphenol-d8	8.545	113	142166	18.501	ng/ul	0.00
21) Nitrobenzene-d5	8.986	128	62830	19.784	ng/ul	0.00
24) 2-Nitrophenol-d4	9.715	143	81859	19.943	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.249	165	161926	20.102	ng/ul	0.00
31) 4-Chloroaniline-d4	10.760	131	177601	16.928	ng/ul	0.00
46) Dimethylphthalate-d6	13.880	166	608570	19.426	ng/ul	0.00
49) Acenaphthylene-d8	14.162	160	650363	21.210	ng/ul	0.00
54) 4-Nitrophenol-d4	14.685	143	71312	16.626	ng/ul	0.00
60) Fluorene-d10	15.467	176	546960	20.687	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.596	200	108322	17.641	ng/ul	0.00
73) Anthracene-d10	17.323	188	887354	21.132	ng/ul	0.00
81) Pyrene-d10	19.621	212	1156545	24.127	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.309	264	1112331	22.341	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.377	149	25990	1.112	ng/ul#	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063231.D
Acq On : 8 Nov 2024 16:43
Operator : RC/JU
Sample : P4636-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CC0P4

Quant Time: Nov 08 16:16:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 15:45:52 2024
Response via : Initial Calibration

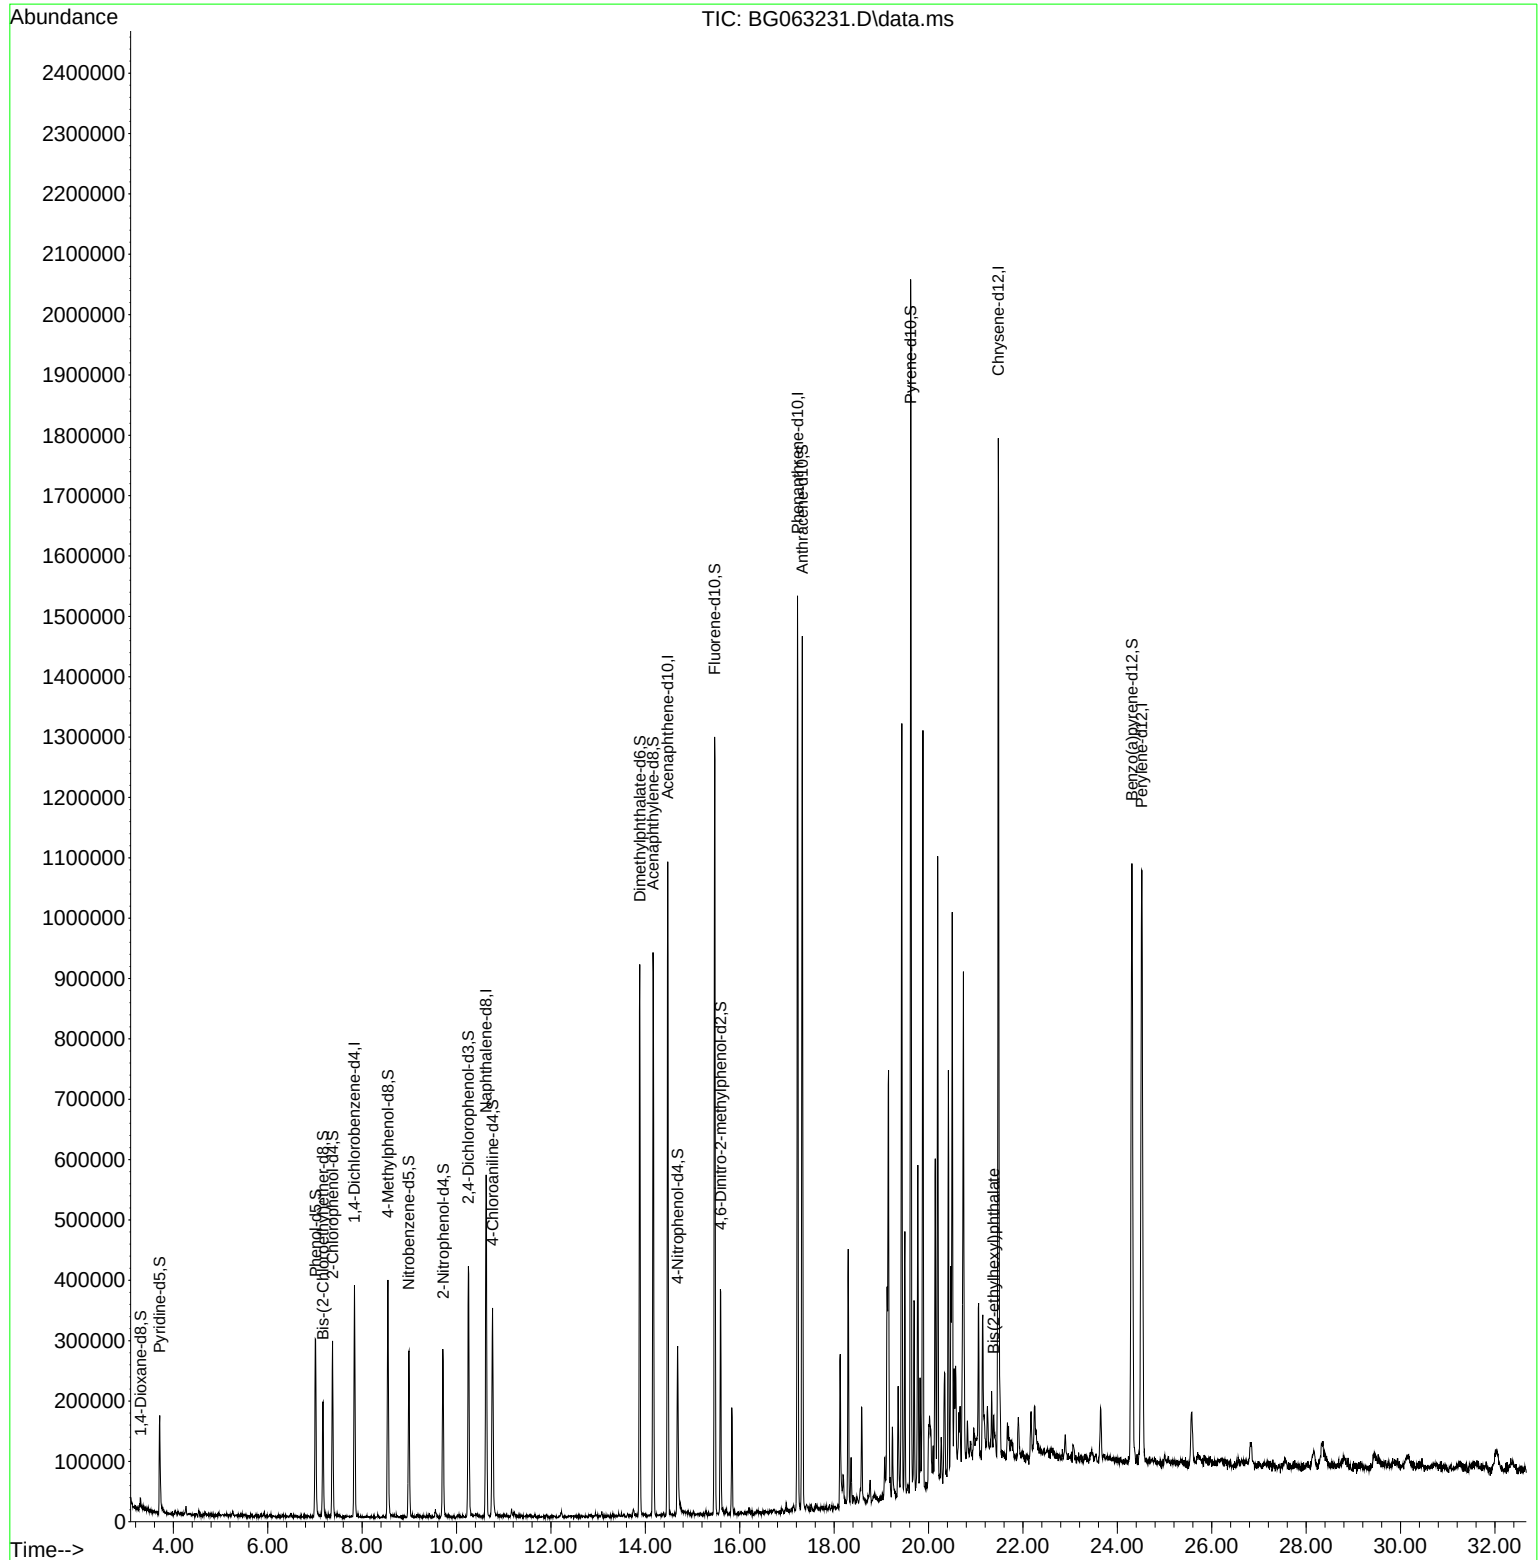

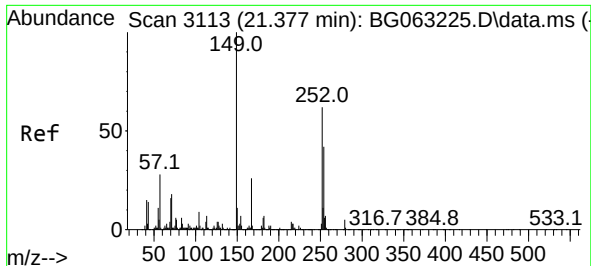

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.112 ng/ul
 RT: 21.377 min Scan# 3113
 Delta R.T. -0.001 min
 Lab File: BG063231.D
 Acq: 8 Nov 2024 16:43

Instrument :
 BNA_G
 ClientSampleId :
 CC0P4

Tgt Ion:149 Resp: 25990
 Ion Ratio Lower Upper
 149 100
 167 27.9 20.6 31.0
 279 7.3 4.2 6.4#

