

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
 Data File : BG063226.D
 Acq On : 8 Nov 2024 13:32
 Operator : RC/JU
 Sample : PB164721BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.296	32	35	42	rVB2	23462	34382	0.97%	0.099%
2	3.707	100	105	117	rBV	265959	450225	12.69%	1.301%
3	4.442	229	230	234	rBV2	5924	6049	0.17%	0.017%
4	5.082	335	339	340	rBV2	6259	5046	0.14%	0.015%
5	5.123	344	346	350	rBV3	3932	6039	0.17%	0.017%
6	5.311	375	378	379	rBV3	4905	4881	0.14%	0.014%
7	5.540	414	417	418	rBV2	6254	5604	0.16%	0.016%
8	6.210	530	531	536	rVB4	3929	5644	0.16%	0.016%
9	6.633	600	603	605	rBV2	5384	5543	0.16%	0.016%
10	7.009	660	667	676	rBV	376281	657697	18.54%	1.900%
11	7.162	686	693	703	rBV	279624	467086	13.17%	1.349%
12	7.368	722	728	735	rBV	378997	618271	17.43%	1.786%
13	7.832	799	807	816	rBV	372791	643455	18.14%	1.859%
14	8.032	840	841	844	rBV3	5423	6476	0.18%	0.019%
15	8.543	921	928	941	rVB	501307	836463	23.58%	2.416%
16	8.660	945	948	951	rBV4	5232	6415	0.18%	0.019%
17	8.989	996	1004	1010	rBV	364032	646689	18.23%	1.868%
18	9.271	1049	1052	1055	rVB2	3516	4890	0.14%	0.014%
19	9.706	1119	1126	1137	rVB	342926	611685	17.25%	1.767%
20	10.123	1193	1197	1198	rBV3	5457	7088	0.20%	0.020%
21	10.247	1212	1218	1226	rBV	500057	904708	25.51%	2.613%
22	10.623	1275	1282	1289	rBV	552314	986304	27.81%	2.849%
23	10.758	1298	1305	1321	rBV	513819	948536	26.74%	2.740%
24	11.328	1400	1402	1407	rVB3	4841	6248	0.18%	0.018%
25	12.221	1549	1554	1555	rBV4	8880	12559	0.35%	0.036%
26	12.344	1573	1575	1578	rVB2	6822	5986	0.17%	0.017%
27	12.450	1587	1593	1594	rBV5	5967	7040	0.20%	0.020%
28	12.820	1655	1656	1665	rBV3	4956	8077	0.23%	0.023%
29	13.196	1717	1720	1722	rVB3	4607	4964	0.14%	0.014%
30	13.554	1779	1781	1784	rBV3	4602	5651	0.16%	0.016%
31	13.725	1808	1810	1814	rBV2	3482	4874	0.14%	0.014%
32	13.878	1830	1836	1844	rBV	1131802	1620004	45.67%	4.680%
33	14.165	1878	1885	1896	rVB2	1158273	1797082	50.67%	5.191%
34	14.324	1909	1912	1915	rBV3	3775	5494	0.15%	0.016%
35	14.477	1930	1938	1947	rVB	1051158	1646395	46.42%	4.756%
36	14.683	1967	1973	1984	rBV	417323	723879	20.41%	2.091%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
 Data File : BG063226.D
 Acq On : 8 Nov 2024 13:32
 Operator : RC/JU
 Sample : PB164721BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	14.912	2010	2012	2016	rVB5	4575	5062	0.14%	0.015%
38	15.006	2027	2028	2032	rBV4	6212	5647	0.16%	0.016%
39	15.294	2075	2077	2081	rBV2	5057	6679	0.19%	0.019%
40	15.470	2100	2107	2114	rBV	1600487	2364874	66.67%	6.831%
41	15.593	2122	2128	2139	rBV	500232	767167	21.63%	2.216%
42	15.711	2146	2148	2154	rVB6	11111	14958	0.42%	0.043%
43	16.104	2212	2215	2219	rBV4	6446	9576	0.27%	0.028%
44	16.157	2219	2224	2227	rVB5	4265	7425	0.21%	0.021%
45	16.245	2238	2239	2241	rBV2	6741	5429	0.15%	0.016%
46	16.316	2249	2251	2254	rBV	4713	5306	0.15%	0.015%
47	16.868	2344	2345	2348	rBV3	4661	5133	0.14%	0.015%
48	17.021	2369	2371	2375	rVB4	7828	7311	0.21%	0.021%
49	17.227	2399	2406	2414	rBV	1555911	2270095	64.00%	6.558%
50	17.326	2416	2423	2436	rVB2	1928373	2869457	80.90%	8.289%
51	17.444	2442	2443	2445	rBV2	7405	5485	0.15%	0.016%
52	17.691	2484	2485	2488	rBV2	5179	6174	0.17%	0.018%
53	17.844	2509	2511	2515	rVB2	4786	5254	0.15%	0.015%
54	18.190	2568	2570	2577	rVB	23277	31880	0.90%	0.092%
55	18.290	2585	2587	2590	rBV3	5663	5866	0.17%	0.017%
56	18.343	2594	2596	2599	rBV3	5062	5133	0.14%	0.015%
57	18.737	2661	2663	2668	rBV5	4814	5954	0.17%	0.017%
58	19.036	2711	2714	2715	rBV3	6436	7784	0.22%	0.022%
59	19.189	2736	2740	2744	rVB6	32377	48619	1.37%	0.140%
60	19.260	2748	2752	2756	rVB2	31614	40508	1.14%	0.117%
61	19.365	2769	2770	2772	rBV2	6948	5181	0.15%	0.015%
62	19.453	2782	2785	2786	rBV3	8418	9093	0.26%	0.026%
63	19.624	2808	2814	2821	rBV	2540862	3546972	100.00%	10.246%
64	20.670	2988	2992	2995	rBV4	28980	40515	1.14%	0.117%
65	21.151	3071	3074	3079	rVB4	77300	102485	2.89%	0.296%
66	21.480	3124	3130	3138	rBV2	1713977	2633347	74.24%	7.607%
67	21.674	3159	3163	3169	rBV6	68080	91315	2.57%	0.264%
68	24.312	3602	3612	3622	rBV	1260272	3284978	92.61%	9.489%
69	24.518	3639	3647	3657	rVB	1015848	2679449	75.54%	7.740%




Sum of corrected areas: 34617540

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063226.D
Acq On : 8 Nov 2024 13:32
Operator : RC/JU
Sample : PB164721BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

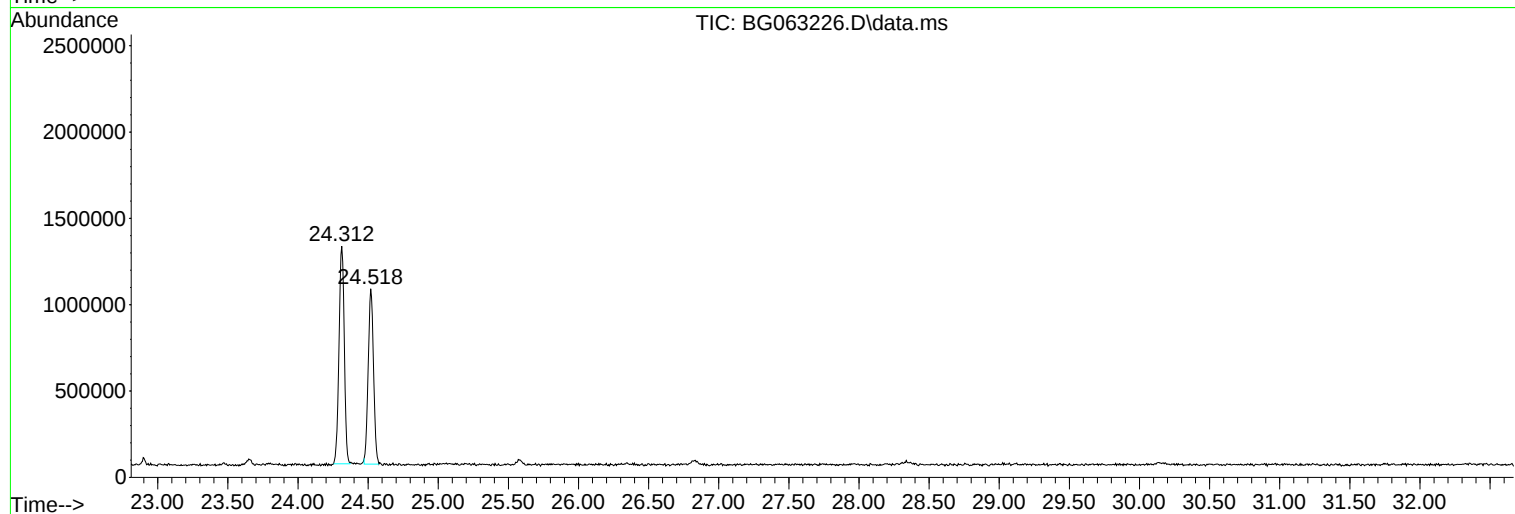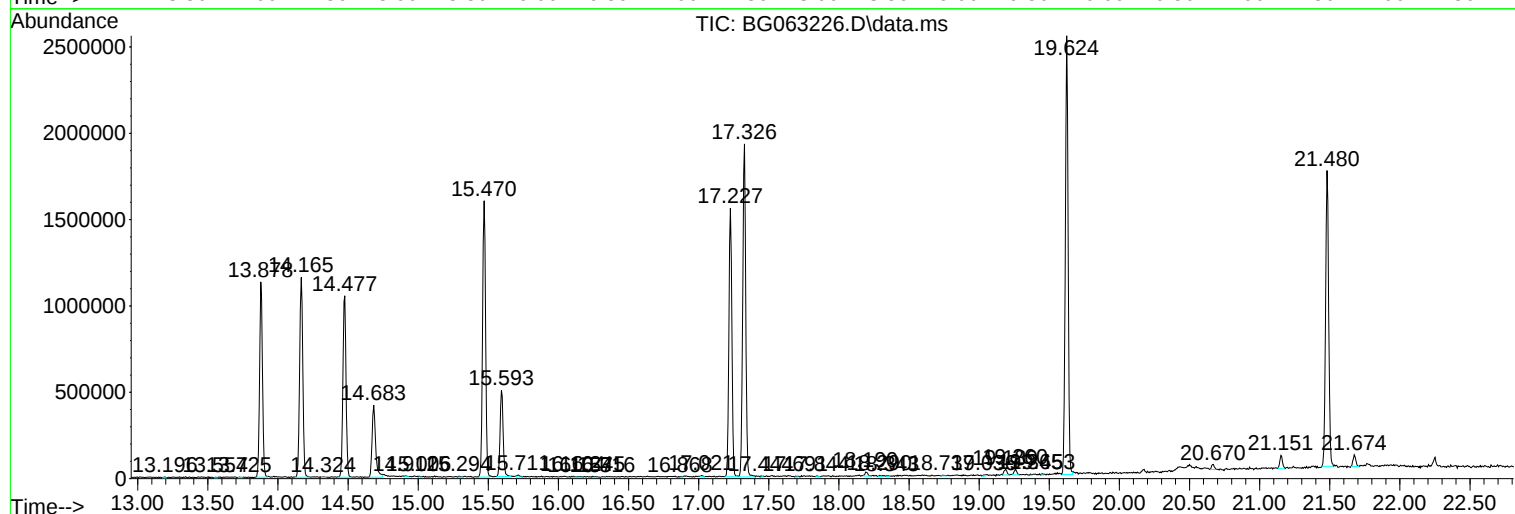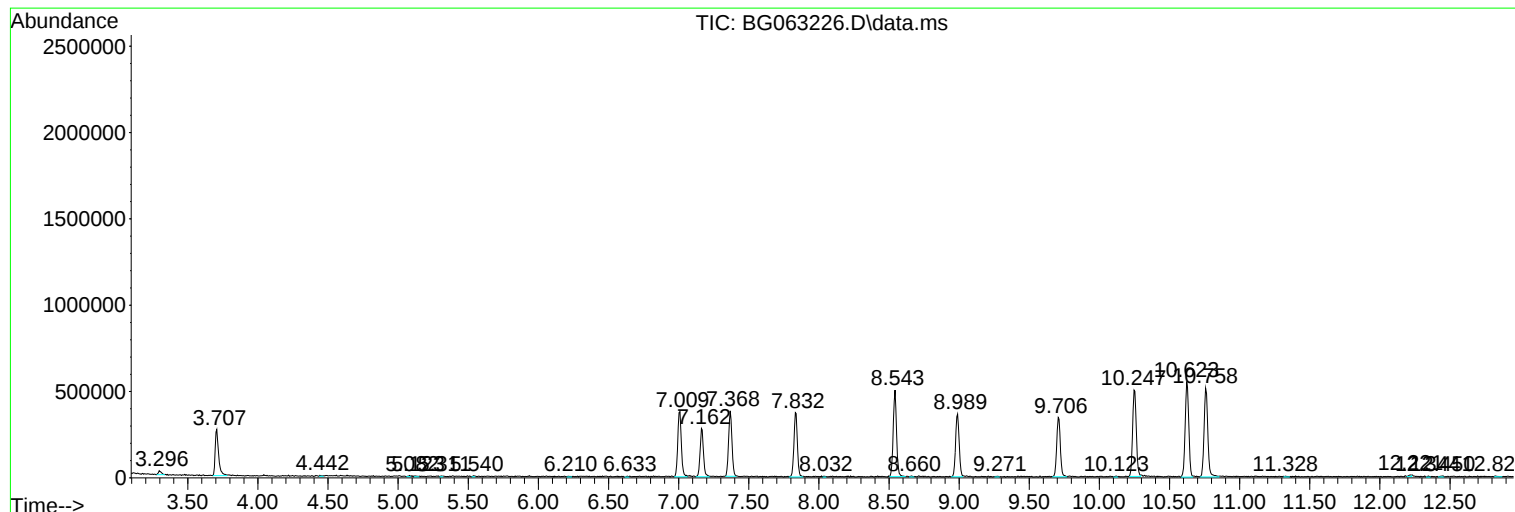

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063226.D
Acq On : 8 Nov 2024 13:32
Operator : RC/JU
Sample : PB164721BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063226.D
Acq On : 8 Nov 2024 13:32
Operator : RC/JU
Sample : PB164721BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc