

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
 Data File : BG063236.D
 Acq On : 8 Nov 2024 19:53
 Operator : RC/JU
 Sample : P4627-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0CD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	45	rVB5	23038	44104	1.01%	0.117%
2	3.710	102	106	116	rBV	69825	126083	2.89%	0.335%
3	4.856	299	301	304	rBV4	6557	6594	0.15%	0.018%
4	6.437	566	570	573	rVB4	3750	6217	0.14%	0.017%
5	6.478	573	577	581	rBV3	5830	7082	0.16%	0.019%
6	7.007	659	667	679	rVB	114199	223581	5.12%	0.594%
7	7.165	688	694	702	rVB	298476	479224	10.98%	1.272%
8	7.371	721	729	738	rBV2	360169	590428	13.52%	1.567%
9	7.770	793	797	802	rBV3	6317	8519	0.20%	0.023%
10	7.835	802	808	816	rVV	386397	656358	15.03%	1.743%
11	7.894	816	818	824	rBV4	5191	10021	0.23%	0.027%
12	8.070	845	848	853	rBV2	4011	7521	0.17%	0.020%
13	8.546	919	929	936	rBV2	336470	590922	13.53%	1.569%
14	8.987	995	1004	1012	rBV	399233	716354	16.41%	1.902%
15	9.427	1073	1079	1082	rBV5	7336	14996	0.34%	0.040%
16	9.639	1111	1115	1118	rVB2	3671	6885	0.16%	0.018%
17	9.709	1118	1127	1138	rBV2	382612	701806	16.07%	1.863%
18	9.980	1171	1173	1178	rVB2	4695	6076	0.14%	0.016%
19	10.250	1212	1219	1230	rBV	587054	1033962	23.68%	2.745%
20	10.626	1275	1283	1292	rBV	607410	1081664	24.77%	2.872%
21	10.761	1298	1306	1319	rBV2	467854	869538	19.92%	2.308%
22	11.108	1362	1365	1369	rBV3	4562	6341	0.15%	0.017%
23	11.202	1379	1381	1385	rBV3	4684	6668	0.15%	0.018%
24	11.919	1500	1503	1505	rBV2	6776	6170	0.14%	0.016%
25	12.218	1551	1554	1557	rBV	9305	11805	0.27%	0.031%
26	13.305	1738	1739	1744	rVB4	6611	7667	0.18%	0.020%
27	13.423	1757	1759	1762	rBV	7007	9034	0.21%	0.024%
28	13.881	1829	1837	1845	rBV	1268276	1873060	42.90%	4.973%
29	14.163	1875	1885	1894	rBV	1289930	2038597	46.69%	5.412%
30	14.292	1904	1907	1912	rVB4	6491	9242	0.21%	0.025%
31	14.339	1912	1915	1918	rBV2	6647	6443	0.15%	0.017%
32	14.392	1918	1924	1927	rVV4	5421	9162	0.21%	0.024%
33	14.474	1930	1938	1945	rVB	1139273	1780963	40.79%	4.728%
34	14.686	1966	1974	1984	rBV2	105980	225113	5.16%	0.598%
35	14.903	2007	2011	2013	rBV4	6178	7201	0.16%	0.019%
36	15.285	2074	2076	2081	rVB5	7066	9534	0.22%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
 Data File : BG063236.D
 Acq On : 8 Nov 2024 19:53
 Operator : RC/JU
 Sample : P4627-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0CD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	15.467	2099	2107	2120	rBV	1927530	2850096	65.28%	7.567%
38	15.591	2122	2128	2136	rBV	682173	993791	22.76%	2.638%
39	15.708	2145	2148	2153	rVB6	12269	18653	0.43%	0.050%
40	15.832	2165	2169	2174	rBV2	102469	147579	3.38%	0.392%
41	16.155	2221	2224	2233	rBV8	8491	16557	0.38%	0.044%
42	16.372	2257	2261	2262	rBV2	6720	6837	0.16%	0.018%
43	16.619	2301	2303	2304	rBV2	7553	6000	0.14%	0.016%
44	16.907	2350	2352	2356	rVB2	6924	8343	0.19%	0.022%
45	16.948	2356	2359	2361	rBV2	7031	6676	0.15%	0.018%
46	17.007	2367	2369	2375	rVB6	5155	6309	0.14%	0.017%
47	17.089	2380	2383	2385	rBV3	5689	7527	0.17%	0.020%
48	17.224	2399	2406	2414	rBV	1586683	2352481	53.88%	6.245%
49	17.324	2416	2423	2431	rVV	2437113	3587361	82.16%	9.524%
50	17.582	2463	2467	2477	rVB7	10639	20351	0.47%	0.054%
51	18.123	2555	2559	2563	rBV5	30851	48879	1.12%	0.130%
52	18.188	2566	2570	2573	rVV3	12950	16407	0.38%	0.044%
53	18.617	2639	2643	2644	rBV3	8977	8304	0.19%	0.022%
54	19.186	2736	2740	2744	rBV3	41241	63506	1.45%	0.169%
55	19.257	2748	2752	2757	rVV2	30580	45750	1.05%	0.121%
56	19.621	2808	2814	2822	rBV	3101116	4366216	100.00%	11.592%
57	19.850	2851	2853	2857	rVB3	10608	9445	0.22%	0.025%
58	20.597	2976	2980	2982	rBV5	14566	18904	0.43%	0.050%
59	21.149	3071	3074	3079	rBV6	41992	50593	1.16%	0.134%
60	21.478	3124	3130	3140	rBV2	1735585	2655731	60.82%	7.051%
61	23.640	3495	3498	3507	rVB8	51609	107889	2.47%	0.286%
62	24.304	3600	3611	3622	rBV	1664121	4279284	98.01%	11.361%
63	24.516	3638	3647	3660	rVB	1037696	2772459	63.50%	7.360%




Sum of corrected areas: 37666863

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063236.D
Acq On : 8 Nov 2024 19:53
Operator : RC/JU
Sample : P4627-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

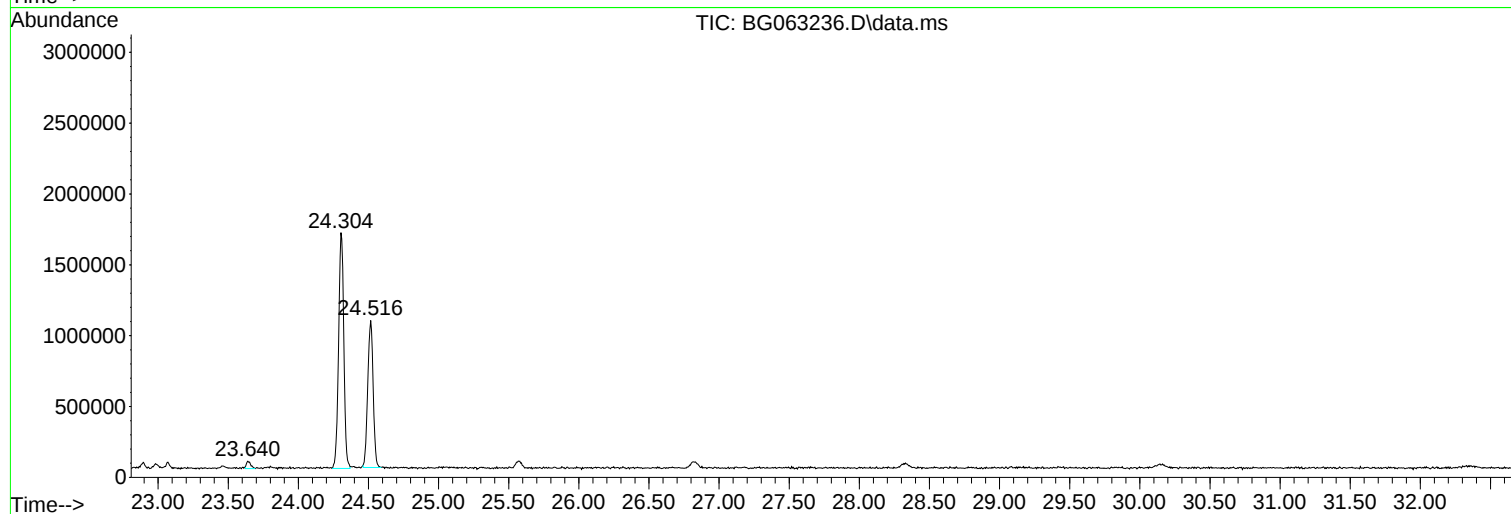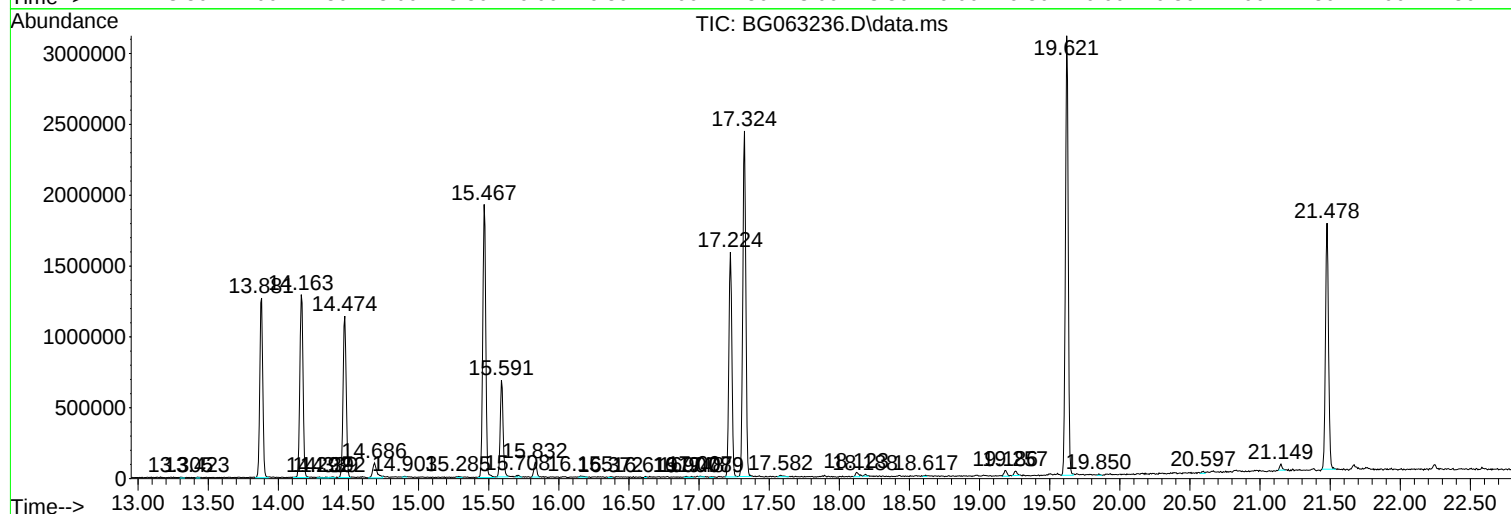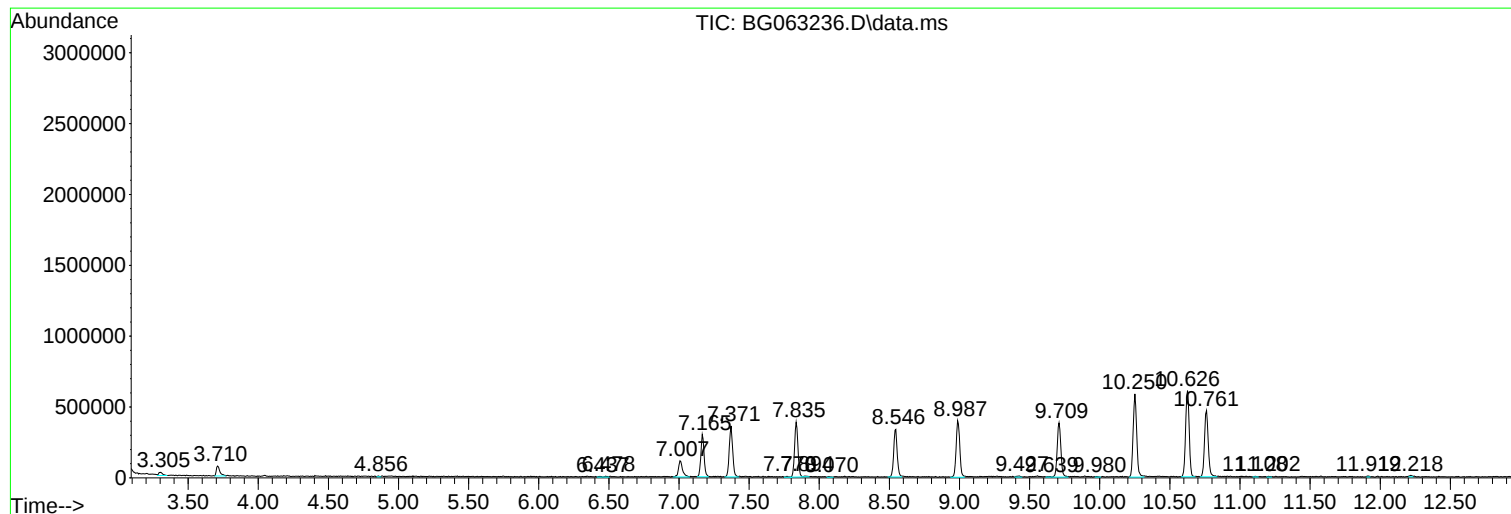

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063236.D
Acq On : 8 Nov 2024 19:53
Operator : RC/JU
Sample : P4627-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063236.D
Acq On : 8 Nov 2024 19:53
Operator : RC/JU
Sample : P4627-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc