

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
 Data File : BG063242.D
 Acq On : 8 Nov 2024 23:41
 Operator : RC/JU
 Sample : P4627-18
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0CF6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	41	rBV4	19798	26464	0.59%	0.069%
2	3.710	102	106	114	rBV	77925	134493	3.00%	0.350%
3	5.861	467	472	474	rVB4	4296	7027	0.16%	0.018%
4	6.531	582	586	588	rBV2	5549	6188	0.14%	0.016%
5	7.006	660	667	675	rBV2	105714	198466	4.43%	0.517%
6	7.165	688	694	701	rBV	321689	513711	11.47%	1.337%
7	7.371	721	729	737	rBV2	363611	613076	13.69%	1.596%
8	7.582	762	765	771	rBV4	5456	7745	0.17%	0.020%
9	7.835	800	808	816	rBV	387505	640480	14.30%	1.667%
10	8.540	922	928	938	rBV	331228	574289	12.82%	1.495%
11	8.986	996	1004	1011	rBV	433553	746463	16.67%	1.943%
12	9.063	1015	1017	1022	rVV4	6844	7626	0.17%	0.020%
13	9.286	1053	1055	1060	rVB3	5390	6701	0.15%	0.017%
14	9.709	1118	1127	1137	rBV2	412427	739404	16.51%	1.925%
15	10.250	1212	1219	1232	rBV	618466	1103604	24.64%	2.873%
16	10.391	1240	1243	1247	rBV6	5861	7989	0.18%	0.021%
17	10.626	1275	1283	1290	rBV	618934	1056713	23.59%	2.751%
18	10.761	1299	1306	1320	rBV	502990	911838	20.36%	2.374%
19	11.266	1390	1392	1396	rBV3	4821	6299	0.14%	0.016%
20	12.218	1550	1554	1559	rVB3	10193	14773	0.33%	0.038%
21	12.817	1655	1656	1661	rBV2	5243	8324	0.19%	0.022%
22	13.469	1764	1767	1769	rBV2	5011	6476	0.14%	0.017%
23	13.881	1830	1837	1845	rBV	1434513	2026270	45.24%	5.275%
24	14.163	1877	1885	1892	rBV	1369479	2178496	48.64%	5.672%
25	14.474	1931	1938	1945	rVB	1156043	1746968	39.01%	4.548%
26	14.580	1952	1956	1957	rBV4	5824	6302	0.14%	0.016%
27	14.686	1968	1974	1984	rBV2	101902	189791	4.24%	0.494%
28	15.467	2100	2107	2120	rBV	1980414	3016554	67.35%	7.854%
29	15.591	2122	2128	2136	rBV	708426	1043240	23.29%	2.716%
30	15.708	2144	2148	2153	rVB6	14325	24379	0.54%	0.063%
31	15.831	2165	2169	2174	rVB	54549	75508	1.69%	0.197%
32	15.890	2178	2179	2184	rVB3	4954	6151	0.14%	0.016%
33	15.949	2184	2189	2194	rBV5	5544	10861	0.24%	0.028%
34	16.155	2220	2224	2225	rBV3	7903	8508	0.19%	0.022%
35	16.172	2225	2227	2231	rVB5	6008	8776	0.20%	0.023%
36	16.666	2308	2311	2314	rBV4	5103	6380	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
 Data File : BG063242.D
 Acq On : 8 Nov 2024 23:41
 Operator : RC/JU
 Sample : P4627-18
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0CF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	16.760	2324	2327	2328	rBV3	6382	7865	0.18%	0.020%
38	17.083	2379	2382	2384	rBV2	5385	7351	0.16%	0.019%
39	17.142	2388	2392	2397	rBV4	8576	11881	0.27%	0.031%
40	17.224	2399	2406	2416	rVV	1570583	2300005	51.35%	5.988%
41	17.324	2416	2423	2433	rBV	2488174	3636306	81.19%	9.467%
42	17.518	2450	2456	2459	rBV2	8067	12925	0.29%	0.034%
43	17.588	2464	2468	2470	rBV4	21756	29150	0.65%	0.076%
44	17.641	2475	2477	2480	rVB4	10393	9511	0.21%	0.025%
45	17.853	2511	2513	2517	rBV4	5603	7681	0.17%	0.020%
46	17.894	2517	2520	2523	rBV4	8875	12771	0.29%	0.033%
47	18.123	2555	2559	2563	rBV3	29091	49792	1.11%	0.130%
48	18.187	2568	2570	2574	rVB	14367	15549	0.35%	0.040%
49	18.422	2607	2610	2612	rBV3	7184	7533	0.17%	0.020%
50	18.499	2620	2623	2625	rVB2	7726	7199	0.16%	0.019%
51	18.611	2638	2642	2645	rBV6	13613	23416	0.52%	0.061%
52	18.781	2670	2671	2674	rBV3	6918	6803	0.15%	0.018%
53	18.881	2687	2688	2692	rVB4	6597	7725	0.17%	0.020%
54	18.922	2692	2695	2698	rBV4	6196	9907	0.22%	0.026%
55	19.028	2710	2713	2717	rVB6	12101	17141	0.38%	0.045%
56	19.186	2735	2740	2744	rBV2	46866	60800	1.36%	0.158%
57	19.257	2748	2752	2760	rVV	35772	62155	1.39%	0.162%
58	19.404	2775	2777	2780	rVB4	8927	7702	0.17%	0.020%
59	19.462	2785	2787	2789	rBV3	7066	8276	0.18%	0.022%
60	19.504	2790	2794	2799	rVV2	21052	36488	0.81%	0.095%
61	19.621	2808	2814	2825	rBV	3163470	4478741	100.00%	11.660%
62	21.149	3072	3074	3078	rVB5	46413	51624	1.15%	0.134%
63	21.478	3124	3130	3137	rBV	1721394	2638279	58.91%	6.869%
64	23.646	3495	3499	3504	rVB4	51729	85626	1.91%	0.223%
65	24.310	3602	3612	3624	rVB	1669625	4318075	96.41%	11.242%
66	24.509	3637	3646	3660	rVB	1041670	2795220	62.41%	7.277%




Sum of corrected areas: 38409830

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063242.D
Acq On : 8 Nov 2024 23:41
Operator : RC/JU
Sample : P4627-18
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

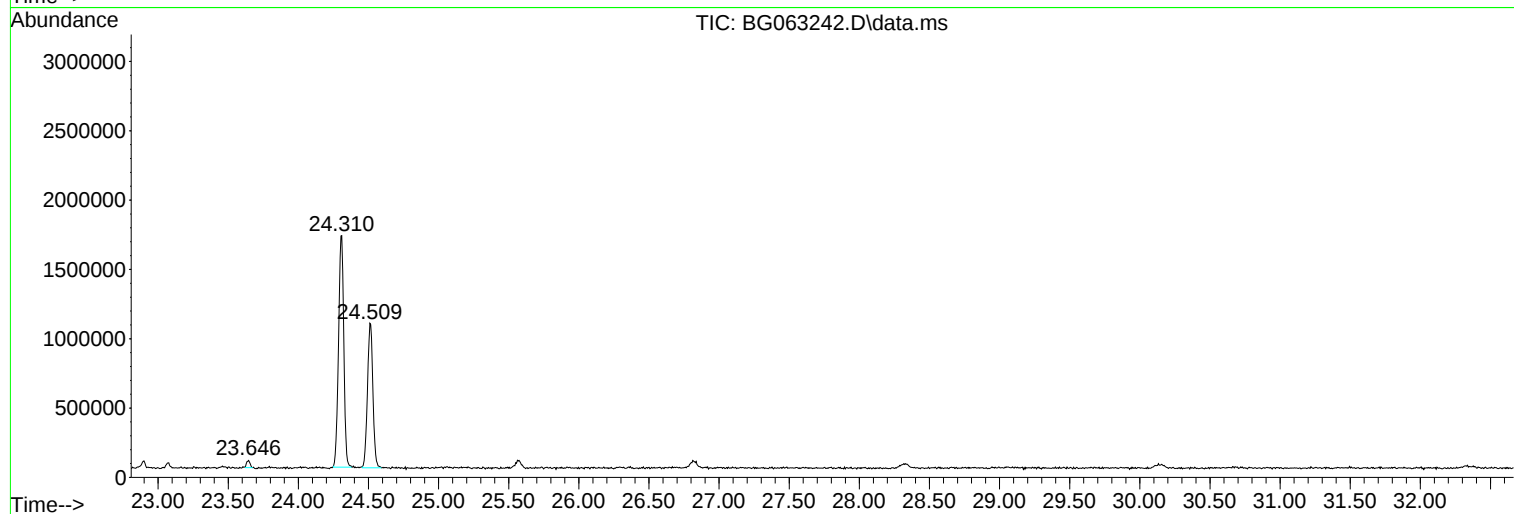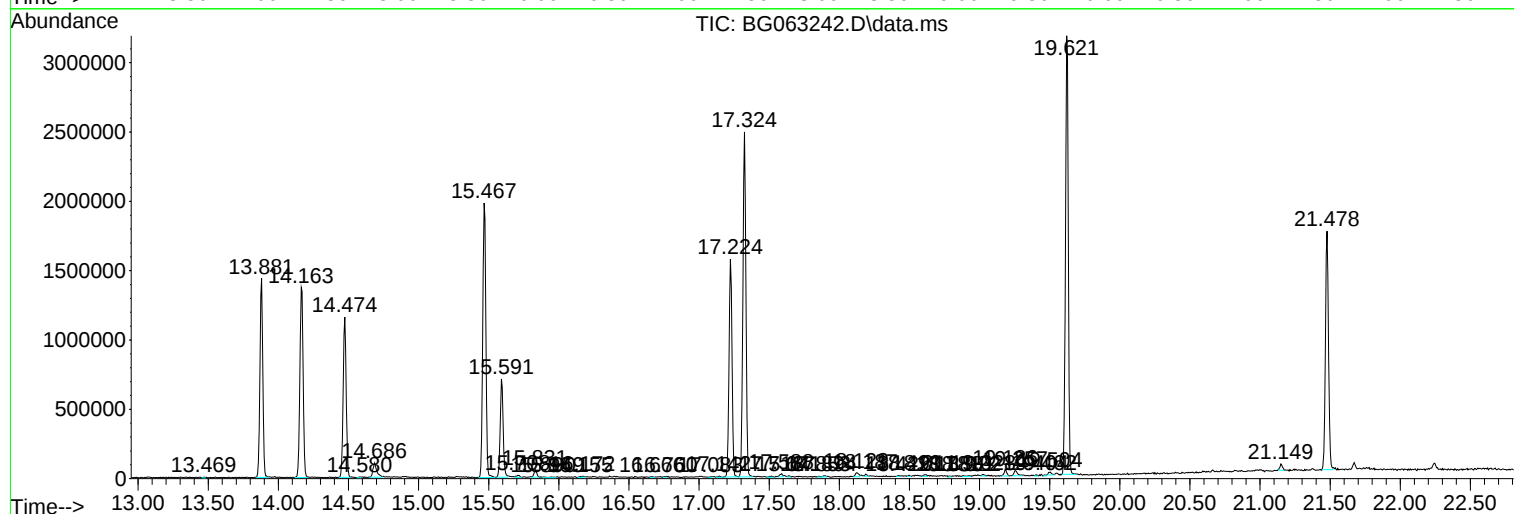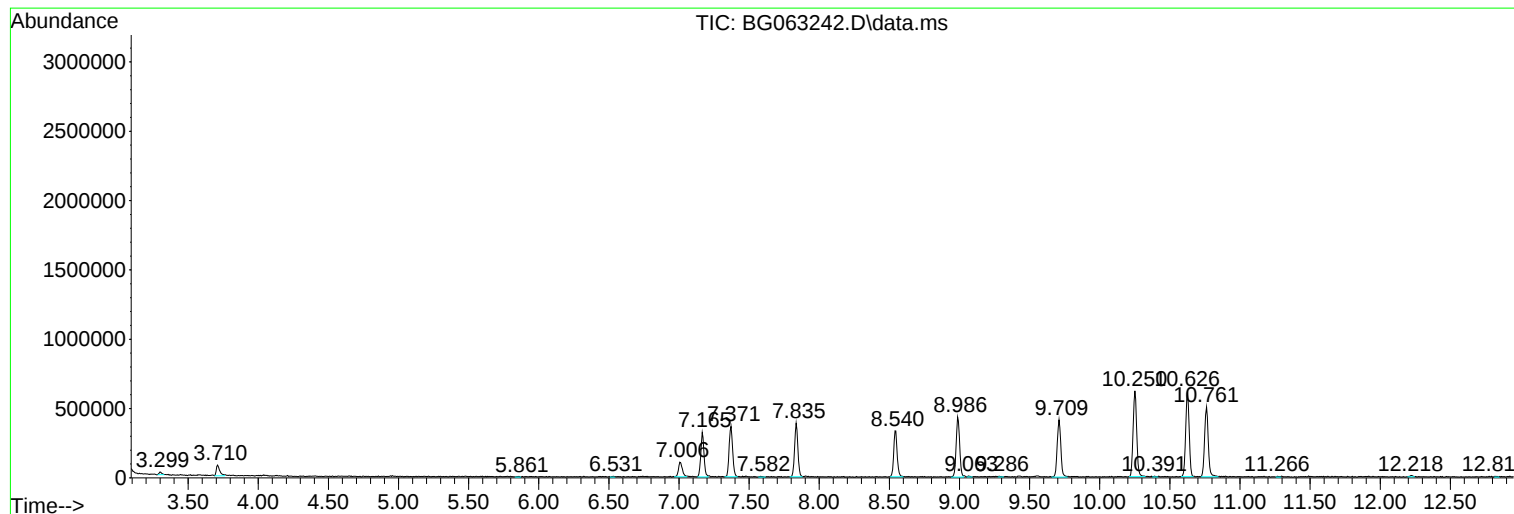

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063242.D
Acq On : 8 Nov 2024 23:41
Operator : RC/JU
Sample : P4627-18
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063242.D
Acq On : 8 Nov 2024 23:41
Operator : RC/JU
Sample : P4627-18
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc