

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063249.D
Acq On : 9 Nov 2024 4:46
Operator : RC/JU
Sample : PB164571BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK571

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BG063249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.300	32	36	41	rVB5	34537	47495	0.99%	0.106%
2	3.705	100	105	116	rBV	405609	661358	13.76%	1.475%
3	7.007	658	667	677	rBV	533303	886865	18.45%	1.978%
4	7.166	687	694	703	rBV	378083	596165	12.40%	1.330%
5	7.371	722	729	742	rVB	496375	863460	17.97%	1.926%
6	7.836	801	808	815	rBV	407441	682069	14.19%	1.521%
7	8.541	920	928	938	rBV	683366	1153033	23.99%	2.572%
8	8.987	996	1004	1012	rBV	518069	887984	18.48%	1.981%
9	9.710	1118	1127	1134	rBV	508418	865126	18.00%	1.930%
10	10.250	1212	1219	1228	rBV	731778	1290748	26.86%	2.879%
11	10.626	1274	1283	1291	rVB	646491	1157135	24.08%	2.581%
12	10.756	1298	1305	1315	rBV	686831	1294245	26.93%	2.887%
13	11.461	1419	1425	1427	rBV	4658	6564	0.14%	0.015%
14	12.219	1549	1554	1560	rBV4	10847	20928	0.44%	0.047%
15	13.875	1829	1836	1846	rBV	1535880	2233249	46.47%	4.981%
16	14.163	1878	1885	1893	rBV	1673185	2586437	53.82%	5.769%
17	14.475	1928	1938	1947	rBV	1221985	1939549	40.36%	4.326%
18	14.680	1966	1973	1988	rBV2	541531	978934	20.37%	2.184%
19	14.880	2004	2007	2009	rBV4	6284	6899	0.14%	0.015%
20	15.103	2042	2045	2050	rVB6	4763	7579	0.16%	0.017%
21	15.186	2056	2059	2062	rBV4	5403	7357	0.15%	0.016%
22	15.291	2075	2077	2082	rVB4	6835	6538	0.14%	0.015%
23	15.468	2100	2107	2114	rBV	2360147	3405499	70.86%	7.596%
24	15.591	2122	2128	2138	rBV	681108	1025149	21.33%	2.287%
25	15.709	2144	2148	2153	rVB7	15318	24319	0.51%	0.054%
26	15.820	2166	2167	2173	rVB3	6037	6440	0.13%	0.014%
27	16.038	2200	2204	2207	rBV3	4206	7290	0.15%	0.016%
28	16.895	2346	2350	2354	rBV4	5956	10199	0.21%	0.023%
29	17.225	2399	2406	2415	rBV	1713347	2585768	53.80%	5.768%
30	17.324	2415	2423	2432	rBV	2656015	3909991	81.36%	8.722%
31	17.477	2445	2449	2453	rBV3	4375	6870	0.14%	0.015%
32	17.595	2465	2469	2471	rVB5	4549	6817	0.14%	0.015%
33	17.818	2504	2507	2509	rVB2	7138	7924	0.16%	0.018%
34	18.194	2568	2571	2574	rVB5	5644	6982	0.15%	0.016%
35	18.740	2660	2664	2666	rVB4	5904	7438	0.15%	0.017%
36	19.187	2735	2740	2746	rVB	44448	70131	1.46%	0.156%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063249.D
Acq On : 9 Nov 2024 4:46
Operator : RC/JU
Sample : PB164571BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK571

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Title : SVOA CALIBRATION

37	19.257	2746	2752	2758	rBV2	41088	74639	1.55%	0.166%
38	19.551	2799	2802	2805	rVB4	12372	13239	0.28%	0.030%
39	19.622	2807	2814	2825	rBV	3357755	4805931	100.00%	10.720%
40	19.927	2863	2866	2870	rBV4	6198	11440	0.24%	0.026%
41	20.174	2906	2908	2911	rVB4	9255	6717	0.14%	0.015%
42	21.478	3123	3130	3138	rBV	1875938	2971766	61.84%	6.629%
43	24.304	3601	3611	3620	rBV	1780420	4619049	96.11%	10.303%
44	24.510	3637	3646	3657	rVB	1182176	3067700	63.83%	6.843%




Sum of corrected areas: 44831015

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063249.D
Acq On : 9 Nov 2024 4:46
Operator : RC/JU
Sample : PB164571BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

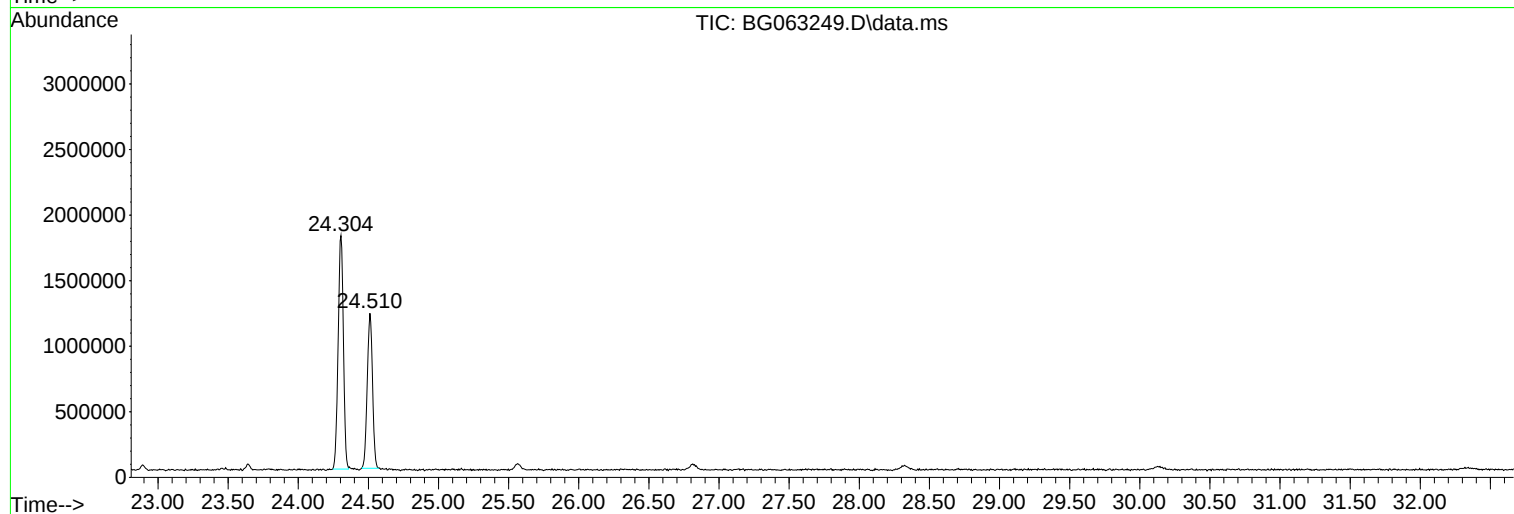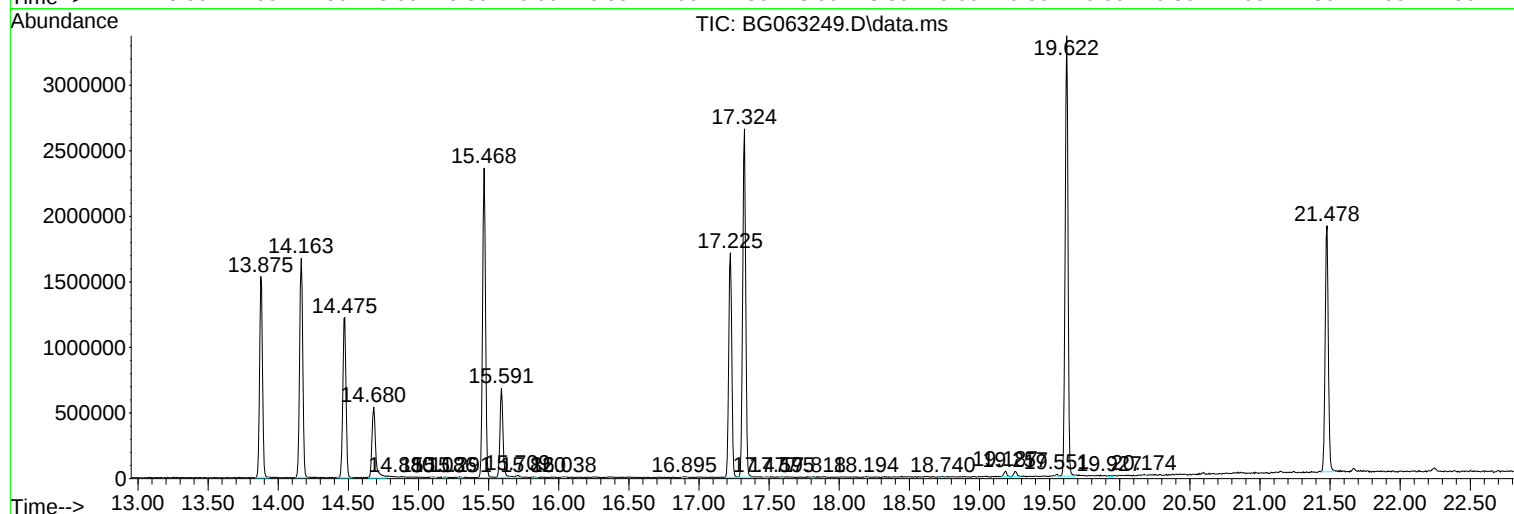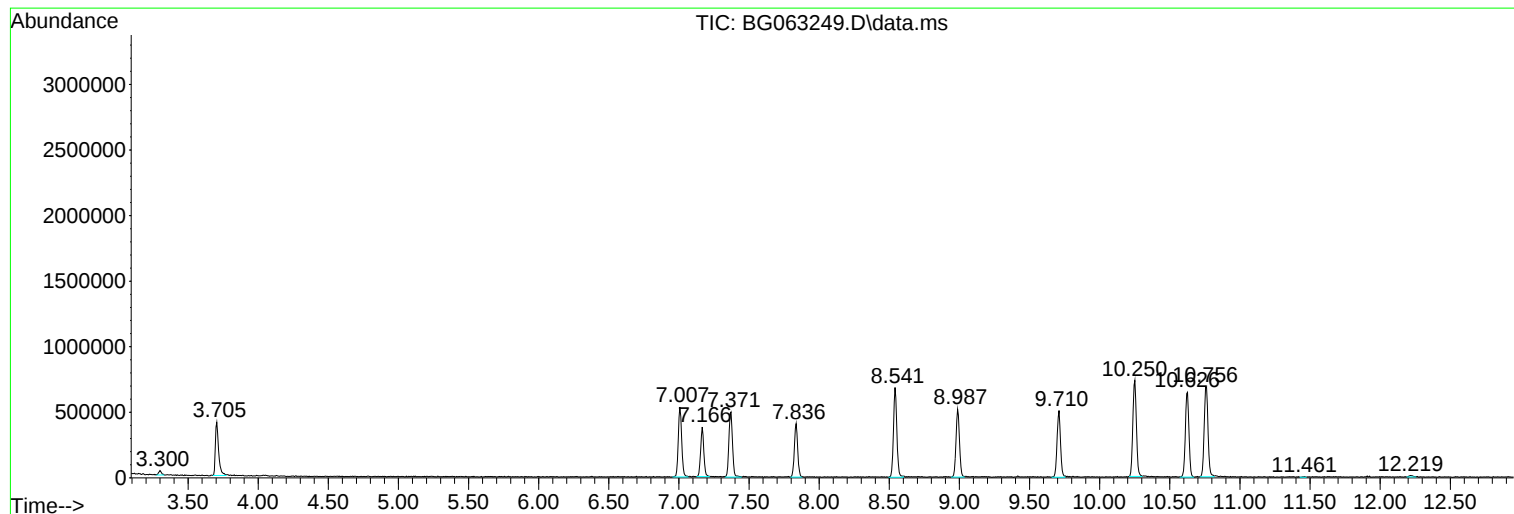

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063249.D
Acq On : 9 Nov 2024 4:46
Operator : RC/JU
Sample : PB164571BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063249.D
Acq On : 9 Nov 2024 4:46
Operator : RC/JU
Sample : PB164571BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc