

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
 Data File : BG063269.D
 Acq On : 9 Nov 2024 18:01
 Operator : RC/JU
 Sample : P4744-02
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCP56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.300	32	36	42	rVB4	23349	33486	0.67%	0.073%
2	3.447	57	61	64	rBV5	7450	12134	0.24%	0.027%
3	3.711	102	106	114	rBV	68205	120180	2.40%	0.263%
4	5.139	340	349	356	rVB3	27268	47864	0.96%	0.105%
5	6.649	602	606	609	rVB4	5365	8117	0.16%	0.018%
6	6.684	609	612	615	rBV4	5851	6939	0.14%	0.015%
7	7.007	656	667	676	rBV2	197122	365934	7.32%	0.800%
8	7.166	688	694	703	rBV	446040	711751	14.24%	1.556%
9	7.372	721	729	737	rBV	539117	919326	18.39%	2.010%
10	7.466	742	745	751	rVB5	6277	10233	0.20%	0.022%
11	7.836	801	808	819	rBV2	455481	780762	15.62%	1.707%
12	8.541	922	928	937	rBV	580507	988090	19.77%	2.161%
13	8.987	996	1004	1012	rBV	663299	1121740	22.44%	2.453%
14	9.264	1048	1051	1054	rBV2	4765	7421	0.15%	0.016%
15	9.416	1072	1077	1083	rVB2	41774	55465	1.11%	0.121%
16	9.710	1119	1127	1135	rBV	600838	1058997	21.19%	2.316%
17	10.251	1209	1219	1228	rBV	898538	1639882	32.81%	3.586%
18	10.621	1273	1282	1291	rBV	704888	1280689	25.62%	2.800%
19	10.756	1298	1305	1316	rBV	375898	707275	14.15%	1.547%
20	11.908	1496	1501	1505	rVB4	19026	28794	0.58%	0.063%
21	12.207	1550	1552	1553	rBV	11136	7845	0.16%	0.017%
22	12.801	1649	1653	1655	rBV2	4965	7483	0.15%	0.016%
23	13.089	1699	1702	1707	rBV4	12489	19729	0.39%	0.043%
24	13.365	1745	1749	1755	rVB5	11453	17533	0.35%	0.038%
25	13.447	1758	1763	1765	rBV4	5415	7513	0.15%	0.016%
26	13.876	1829	1836	1844	rBV	1692156	2472058	49.46%	5.406%
27	14.164	1878	1885	1893	rVB	1866991	2918805	58.40%	6.383%
28	14.469	1928	1937	1947	rBV	1320791	2062170	41.26%	4.509%
29	14.681	1966	1973	1983	rBV3	152130	307510	6.15%	0.672%
30	14.892	2006	2009	2014	rVB7	9892	16930	0.34%	0.037%
31	15.274	2071	2074	2075	rBV2	6417	7234	0.14%	0.016%
32	15.292	2075	2077	2079	rVB2	9825	6898	0.14%	0.015%
33	15.468	2099	2107	2117	rBV	2545106	3838879	76.80%	8.394%
34	15.591	2121	2128	2137	rBV2	757781	1140199	22.81%	2.493%
35	15.703	2145	2147	2152	rVB4	16335	23113	0.46%	0.051%
36	15.832	2164	2169	2174	rVB4	21005	39685	0.79%	0.087%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
 Data File : BG063269.D
 Acq On : 9 Nov 2024 18:01
 Operator : RC/JU
 Sample : P4744-02
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GCP56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
 Title : SVOA CALIBRATION

37	15.885	2174	2178	2181	rBV4	5882	9789	0.20%	0.021%
38	15.985	2194	2195	2199	rVB3	6322	7405	0.15%	0.016%
39	16.026	2199	2202	2203	rBV	8531	8015	0.16%	0.018%
40	16.379	2253	2262	2263	rBV6	5809	11453	0.23%	0.025%
41	16.649	2304	2308	2309	rBV3	6601	8375	0.17%	0.018%
42	16.896	2346	2350	2355	rBV6	8573	15323	0.31%	0.034%
43	17.225	2399	2406	2413	rVV	1732607	2555052	51.12%	5.587%
44	17.319	2415	2422	2433	rVV	2678483	4085376	81.74%	8.933%
45	17.407	2435	2437	2440	rVB3	7989	7774	0.16%	0.017%
46	17.601	2469	2470	2474	rBV3	6686	9387	0.19%	0.021%
47	17.707	2485	2488	2489	rBV2	6283	7268	0.15%	0.016%
48	17.889	2515	2519	2525	rVB3	108811	149854	3.00%	0.328%
49	18.059	2546	2548	2552	rVB5	8041	11391	0.23%	0.025%
50	18.100	2552	2555	2556	rBV4	6396	6938	0.14%	0.015%
51	18.124	2556	2559	2566	rVV6	16900	32963	0.66%	0.072%
52	18.335	2590	2595	2607	rBV2	88024	177337	3.55%	0.388%
53	18.547	2629	2631	2634	rBV4	9532	11423	0.23%	0.025%
54	18.611	2640	2642	2648	rVB5	21506	23205	0.46%	0.051%
55	19.181	2735	2739	2743	rVB3	51072	70562	1.41%	0.154%
56	19.258	2747	2752	2755	rBV2	39346	58451	1.17%	0.128%
57	19.375	2770	2772	2774	rBV3	6825	7358	0.15%	0.016%
58	19.622	2808	2814	2821	rBV	3495560	4998230	100.00%	10.930%
59	21.473	3123	3129	3142	rBV2	1827781	2955082	59.12%	6.462%
60	24.305	3600	3611	3622	rBV	1856136	4760994	95.25%	10.411%
61	24.510	3637	3646	3657	rVB	1110225	2943617	58.89%	6.437%




Sum of corrected areas: 45731285

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063269.D
Acq On : 9 Nov 2024 18:01
Operator : RC/JU
Sample : P4744-02
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCP56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

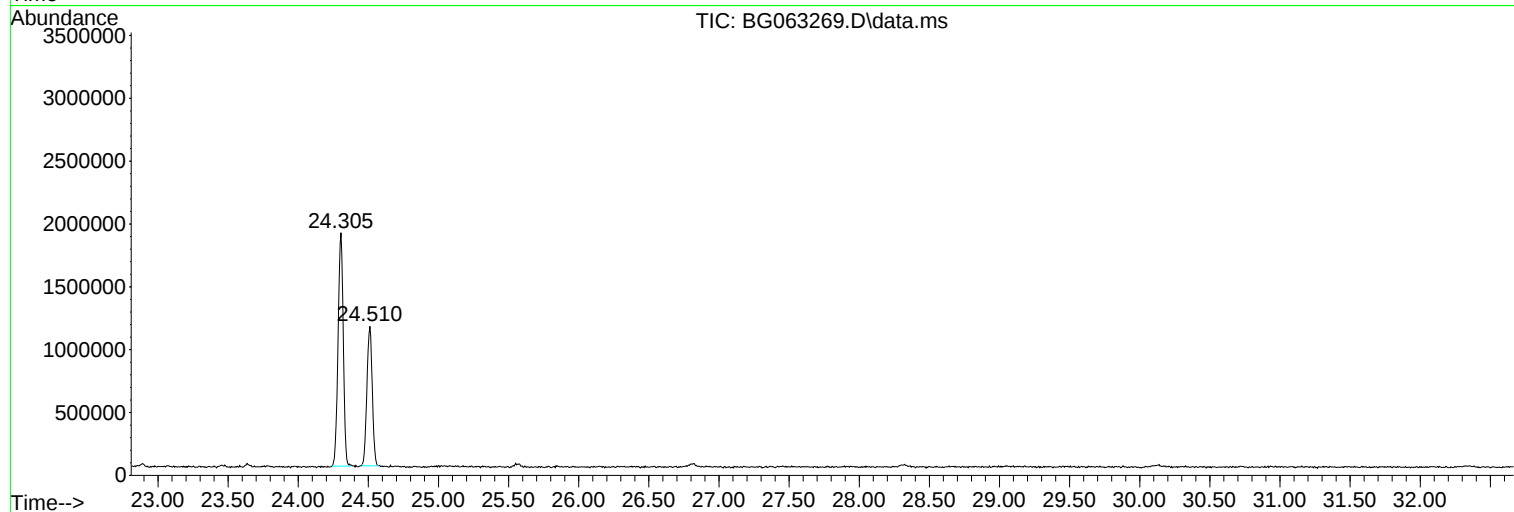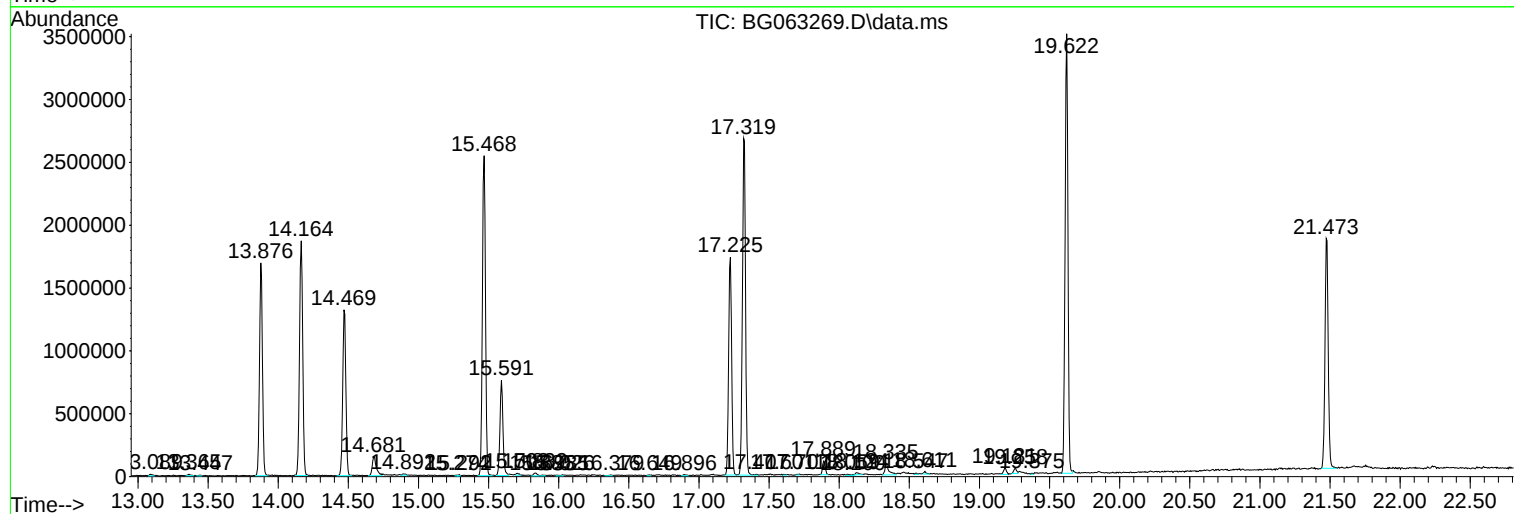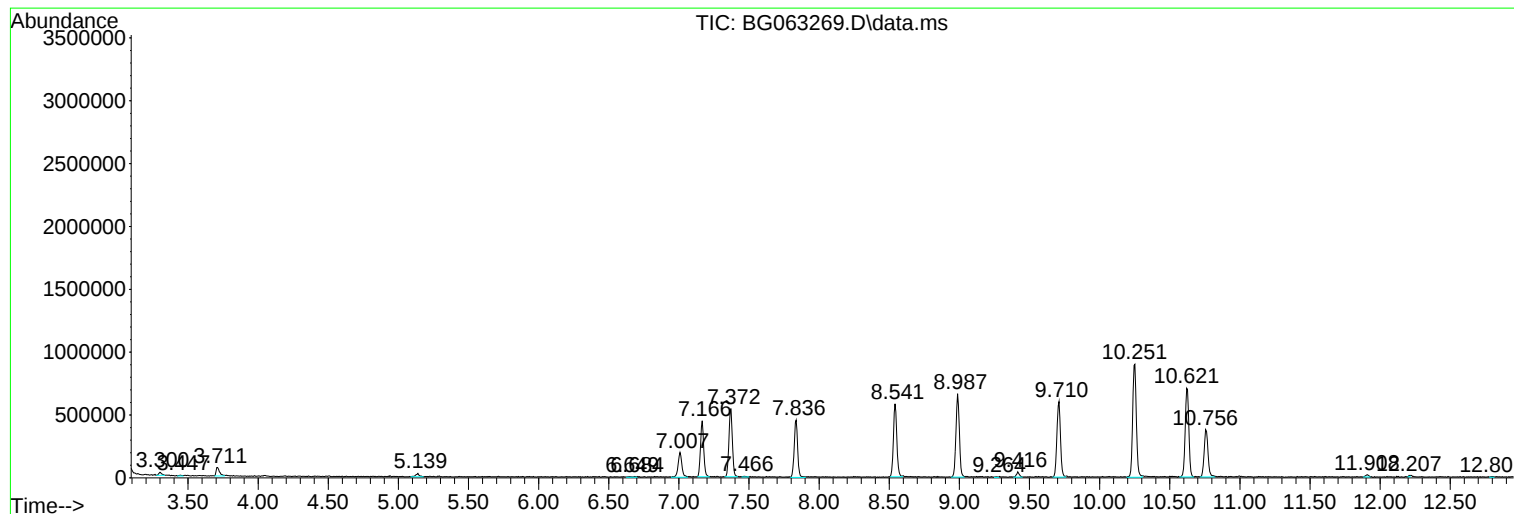

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063269.D
Acq On : 9 Nov 2024 18:01
Operator : RC/JU
Sample : P4744-02
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCP56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110824\
Data File : BG063269.D
Acq On : 9 Nov 2024 18:01
Operator : RC/JU
Sample : P4744-02
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GCP56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc