

Data Path : Z:\HPCHEM1\BNA_G\Data\BG110915\
 Data File : BG019536.D
 Acq On : 9 Nov 2015 17:09
 Operator : UM/NP
 Sample : G4245-18DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCY53DL

Quant Time: Nov 23 07:10:43 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 10 00:14:14 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/10/2015 1:04:21 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	31138	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	132514	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.81	164	103520	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	278228	20.00	ng/ul	0.00
78) Chrysene-d12	21.82	240	393420	20.00	ng/ul	0.00
86) Perylene-d12	25.17	264	378697	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	235	0.36	ng/uL	0.00
5) Phenol-d5	7.32	99	8208	2.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	14953	8.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	10966	6.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	10570	4.64	ng/ul	0.00
19) Nitrobenzene-d5	9.34	128	8380	8.60	ng/ul	0.00
22) 2-Nitrophenol-d4	10.07	143	8380	7.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.62	165	16129	6.43	ng/ul	0.00
29) 4-Chloroaniline-d4	11.15	131	14210	5.60	ng/ul	0.01
44) Dimethylphthalate-d6	14.20	166	75923	8.90	ng/ul	0.00
47) Acenaphthylene-d8	14.50	160	78658	8.32	ng/ul	0.00
52) 4-Nitrophenol-d4	14.98	143	4211	3.11	ng/ul	0.00
58) Fluorene-d10	15.80	176	65546	8.30	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.90	200	12176	6.76	ng/ul	0.00
71) Anthracene-d10	17.65	188	111527	8.79	ng/ul	0.00
79) Pyrene-d10	19.92	212	137535	7.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.93	264	156291	8.22	ng/ul	-0.02

Target Compounds

					Qvalue
28) Naphthalene	11.08	128	5126687	773.22 ng/ul#	64
34) 2-Methylnaphthalene	12.65	142	179324	33.66 ng/ul	97
41) 1,1'-Biphenyl	13.64	154	185786	25.39 ng/ul#	95
48) Acenaphthylene	14.53	152	23988	2.48 ng/ul#	86
50) Acenaphthene	14.87	153	507350	77.58 ng/ul	98
54) Dibenzofuran	15.20	168	521689	54.17 ng/ul	95
59) Fluorene	15.85	166	325522	38.75 ng/ul	98
70) Phenanthrene	17.59	178	534244	38.05 ng/ul	97
72) Anthracene	17.68	178	34735m-9	2.43 ng/ul	
75) Carbazole	17.95	167	716604	62.74 ng/ul	94
77) Fluoranthene	19.58	202	54080	2.98 ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M
 11/10/15


```
Data Path   : Z:\HPCHEM1\BNA G\Data\BG110915\  
Data File  : BG019536.D  
Acq On     : 9 Nov 2015 17:09  
Operator   : UM/NP  
Sample     : G4245-18DL 5X  
Misc       :  
ALS Vial   : 8      Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
BCY53DL

Quant Time: Nov 10 02:20:03 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 10 00:14:14 2015
Response via : Initial Calibration

Manual Integrations

Mmdadoda
11/10/2015 1:04:21 PM

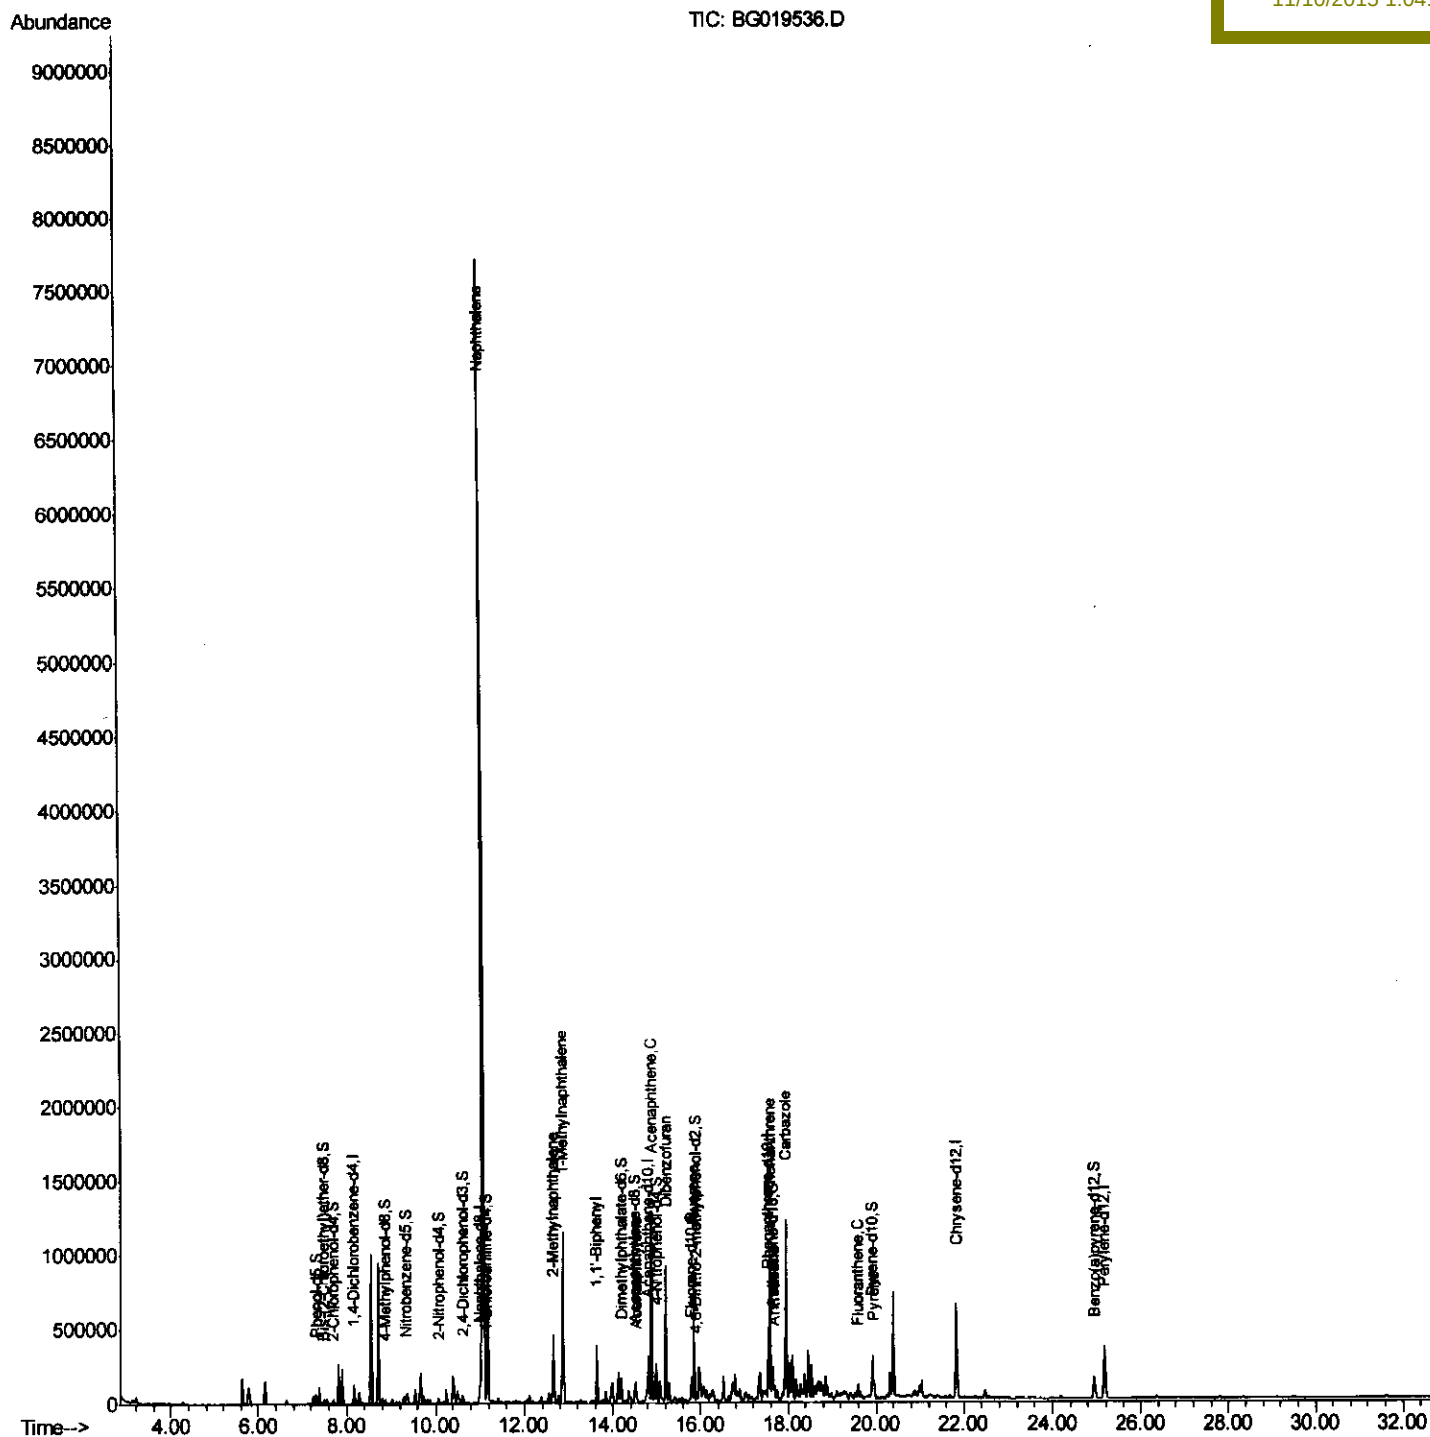

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA G\Data\BG110915\
 Data File : BG019536.D
 Acq On : 9 Nov 2015 17:09
 Operator : UM/NP
 Sample : G4245-18DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCY53DL

Quant Time: Nov 10 00:17:38 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 10 00:14:14 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Mmdadoda
 11/10/2015 1:04:21 PM

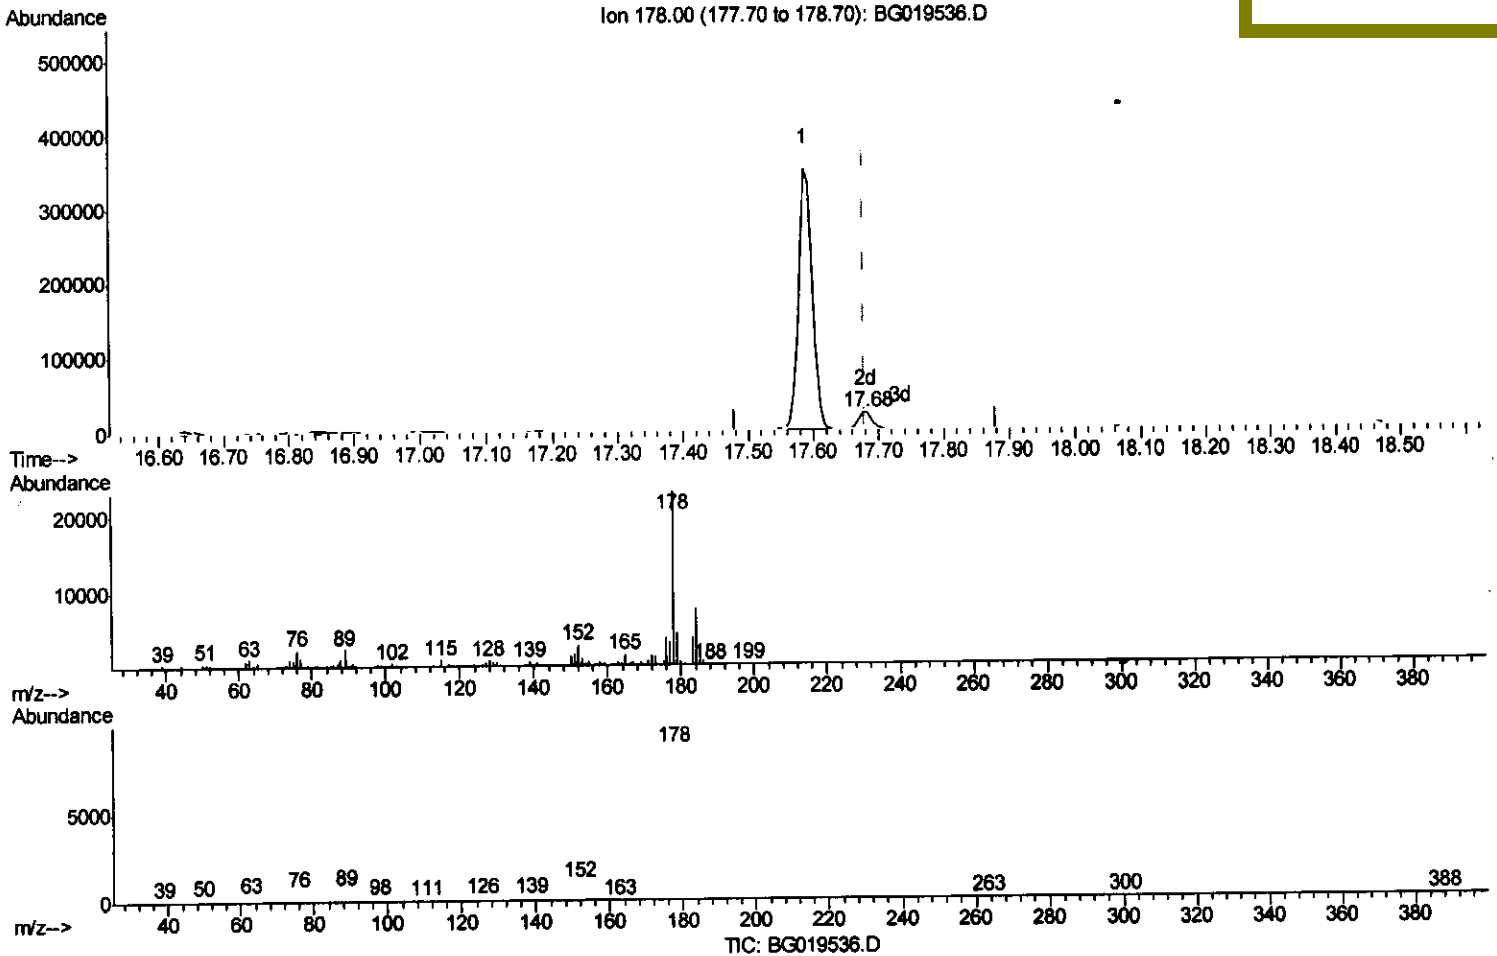

(72) Anthracene

17.681min (+0.002) 2.43ng/ul m

response 34735

Ion	Exp%	Act%
178.00	100	100
179.00	14.50	18.92#
176.00	17.80	16.51
0.00	0.00	0.00

U.M.
11/10/15

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA G\Data\BG110915\
Data File : BG019536.D
Acq On : 9 Nov 2015 17:09
Operator : UM/NP
Sample : G4245-18DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Nov 10 00:17:38 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 10 00:14:14 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
BCY53DL

Manual Integrations
APPROVED

Mmdadoda
11/10/2015 1:04:21 PM

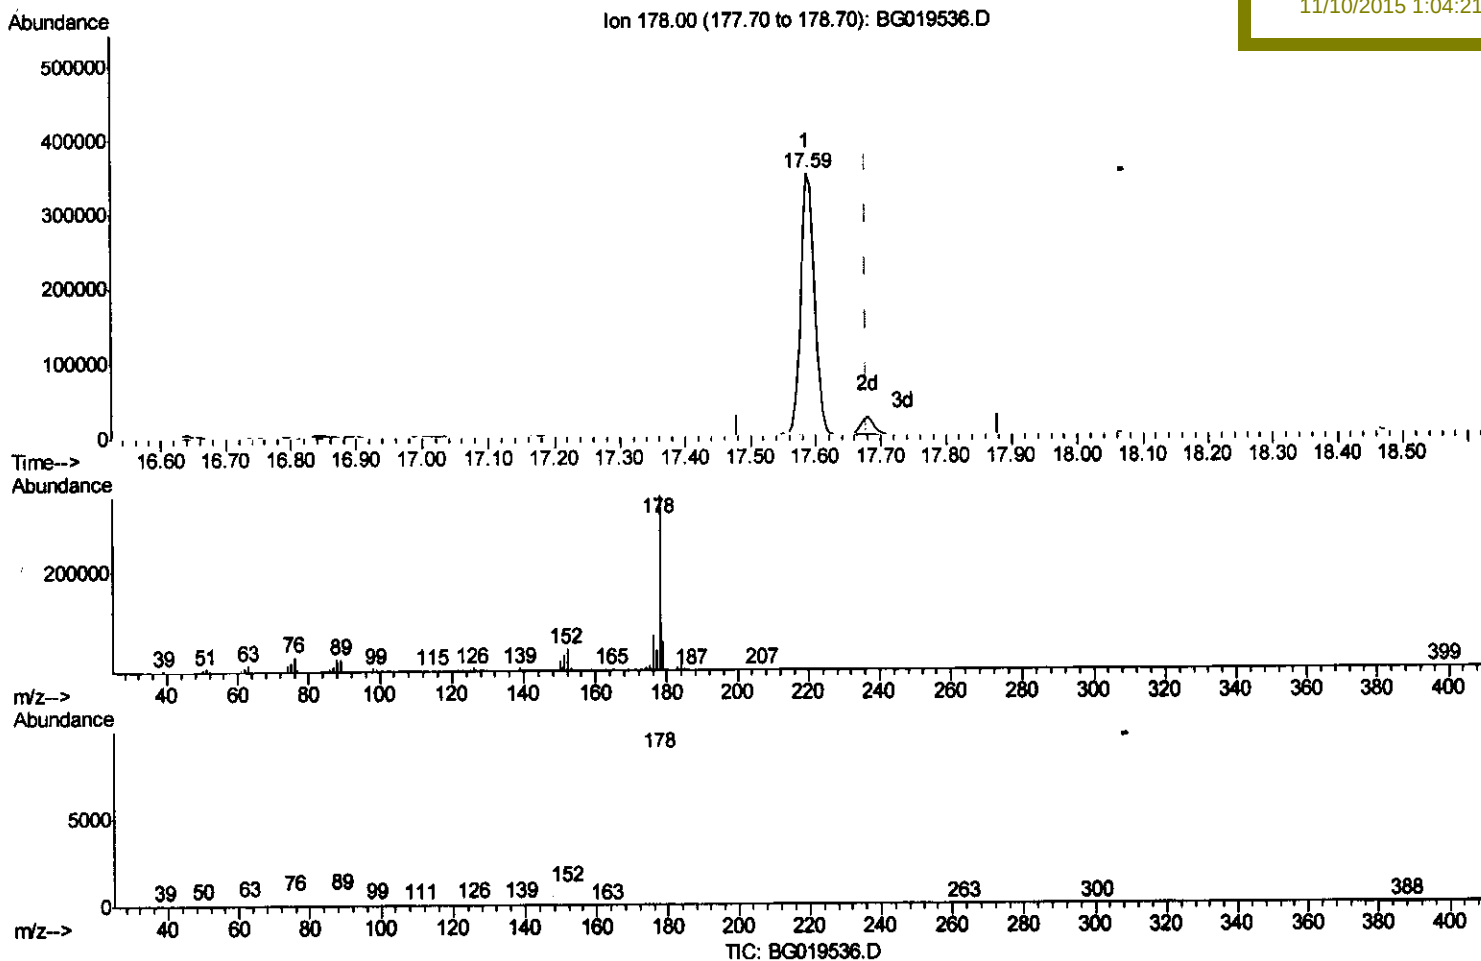

(72) Anthracene

17.587min (-0.092) 37.33ng/ul

response 534244

Ion	Exp%	Act%
178.00	100	100
179.00	14.50	16.35
176.00	17.80	19.77
0.00	0.00	0.00