

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110917\
 Data File : BG030884.D
 Acq On : 9 Nov 2017 17:41
 Operator : SJ/JU
 Sample : I6286-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 10 01:22:34 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 01:20:10 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	63591	20.00	ng/ul	0.00
18) Naphthalene-d8	10.97	136	300346	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.77	164	196980	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	480014	20.00	ng/ul	0.00
75) Chrysene-d12	21.78	240	525095	20.00	ng/ul	0.00
83) Perylene-d12	25.09	264	521932	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	6009	3.84	ng/uL	0.00
5) Phenol-d5	7.31	99	116885	19.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	70777	18.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	98749	22.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	91800	18.62	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	53664	24.89	ng/ul	0.00
22) 2-Nitrophenol-d4	10.04	143	65669	29.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	114257	22.70	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	118948	20.34	ng/ul	0.00
43) Dimethylphthalate-d6	14.16	166	391498	23.25	ng/ul	0.00
46) Acenaphthylene-d8	14.46	160	486167	23.74	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	54743	17.61	ng/ul	0.00
57) Fluorene-d10	15.76	176	355778	25.79	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.88	200	62835	26.82	ng/ul	0.00
70) Anthracene-d10	17.61	188	557519	24.56	ng/ul	0.00
76) Pyrene-d10	19.88	212	658023	24.21	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.86	264	628441	25.42	ng/ul	0.00

Target Compounds


					Ovalue	
6) Phenol	7.34	94	8703	1.38	ng/ul#	88
44) Dimethylphthalate	14.21	163	58611	3.57	ng/ul	98
69) Phenanthrene	17.55	178	146113	5.63	ng/ul	99
74) Fluoranthene	19.55	202	227647	7.85	ng/ul	99
77) Pyrene	19.91	202	300127	8.53	ng/ul	98
80) Benzo(a)anthracene	21.76	228	135586	4.12	ng/ul	96
82) Chrysene	21.83	228	183427	6.13	ng/ul	97
85) Benzo(b)fluoranthene	24.03	252	193698	6.18	ng/ul#	95
88) Benzo(a)pyrene	24.93	252	134995	4.43	ng/ul	97
89) Indeno(1,2,3-cd)pyrene	28.87	276	90009	2.61	ng/ul	99
91) Benzo(g,h,i)perylene	30.06	276	80967	2.83	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110917\
Data File : BG030884.D
Acq On : 9 Nov 2017 17:41
Operator : SJ/JU
Sample : I6286-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :

Quant Time: Nov 10 01:22:34 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 01:20:10 2017
Response via : Initial Calibration

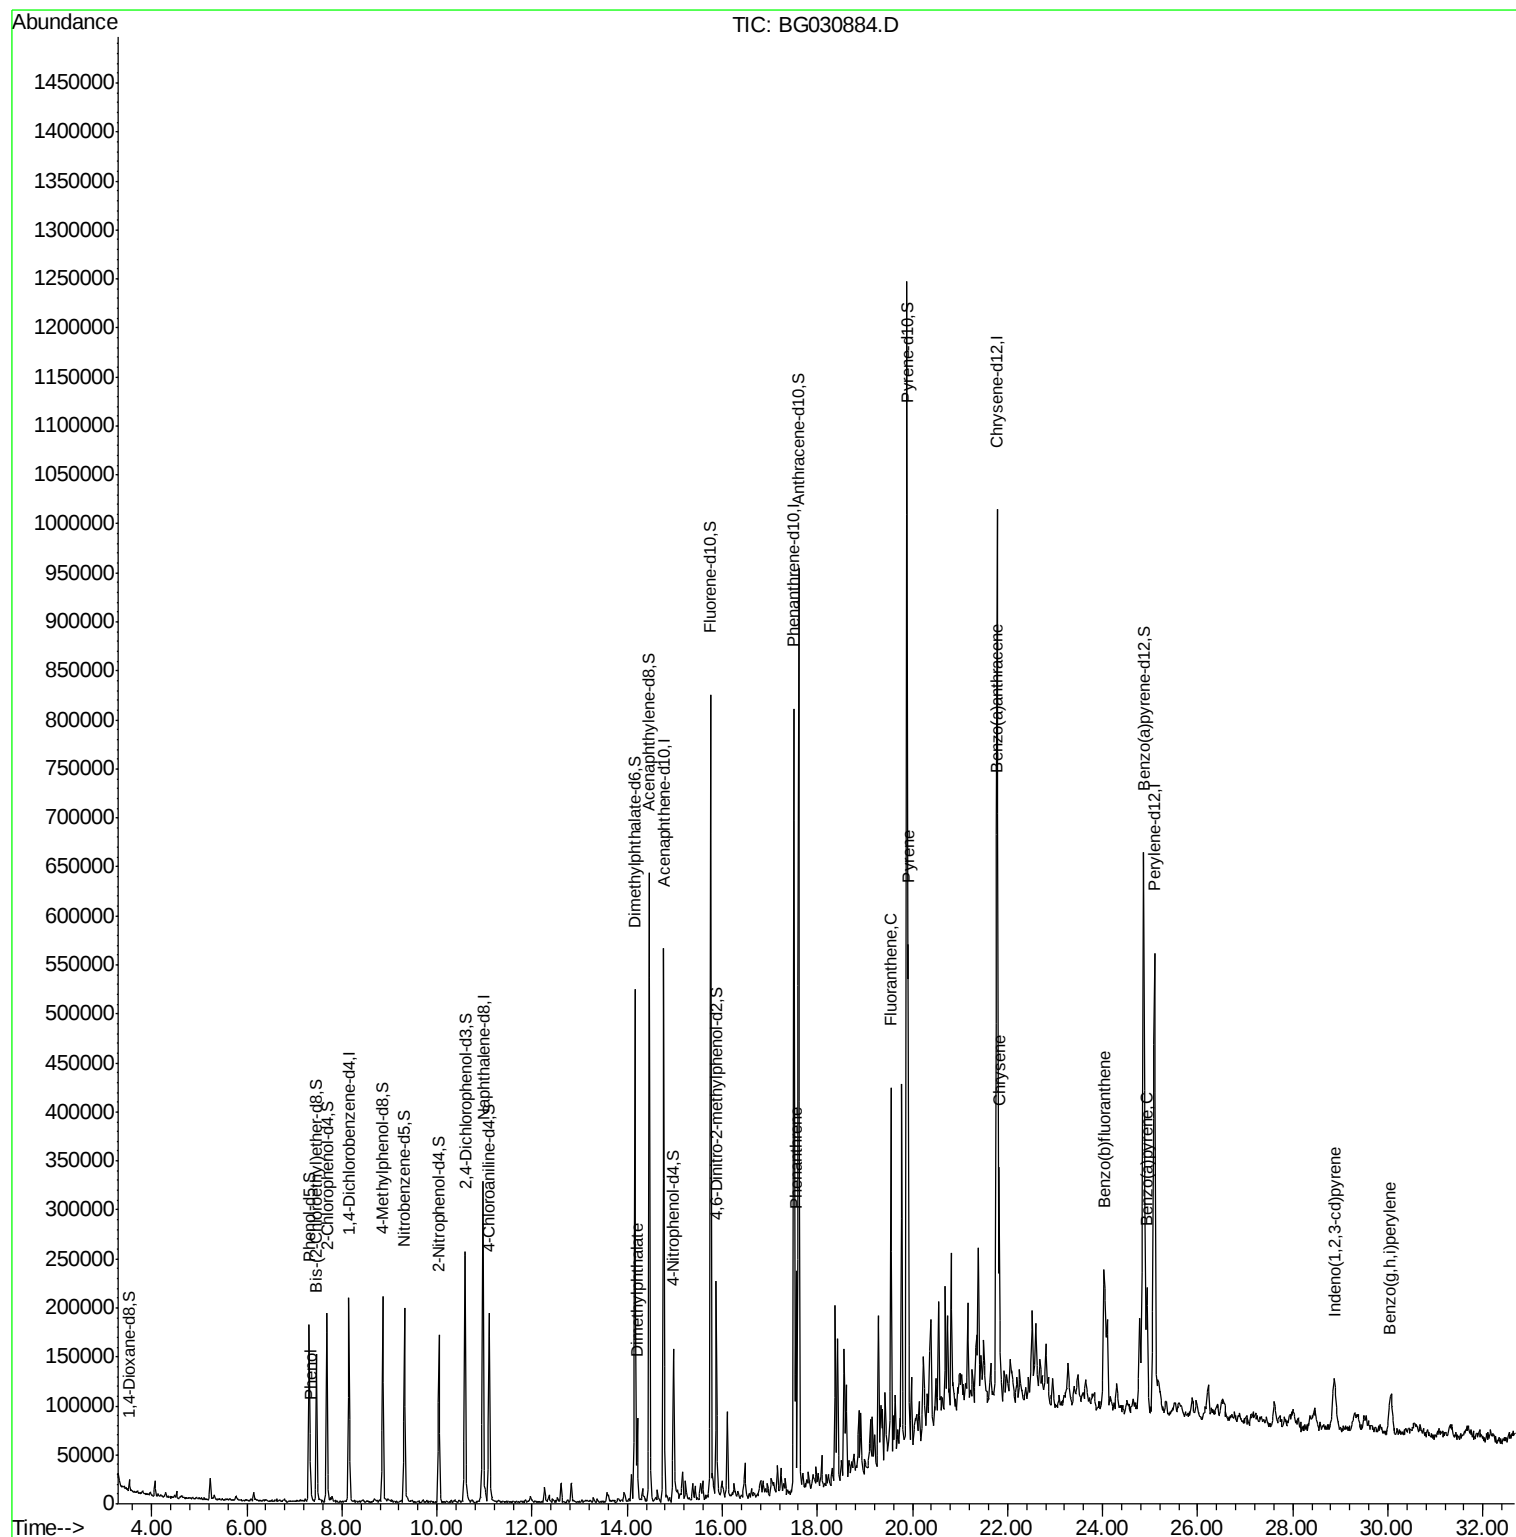

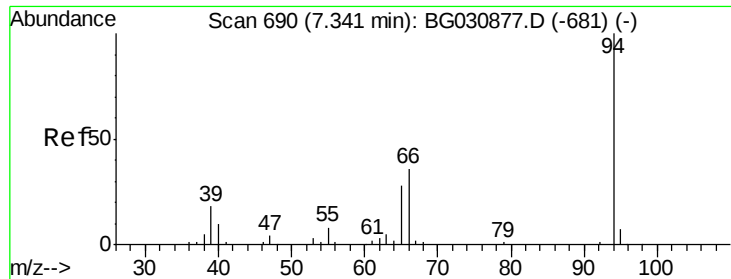

#6

Phenol

Concen: 1.38 ng/ul

RT: 7.34 min Scan# 690

Delta R.T. 0.00 min

Lab File: BG030884.D

Acq: 9 Nov 2017 17:41

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 94 Resp: 8703

Ion Ratio Lower Upper




94 100

65 25.1 27.1 40.7#

66 49.4 34.6 52.0

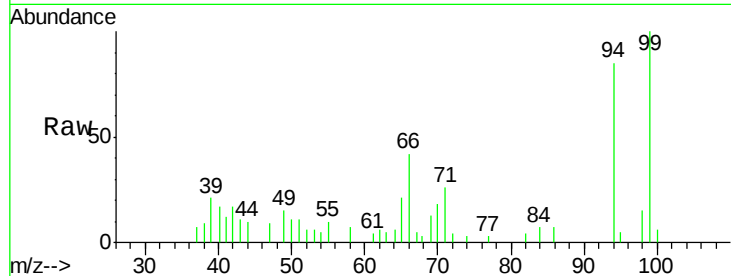

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

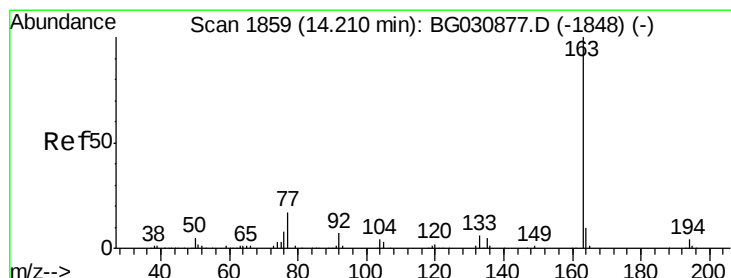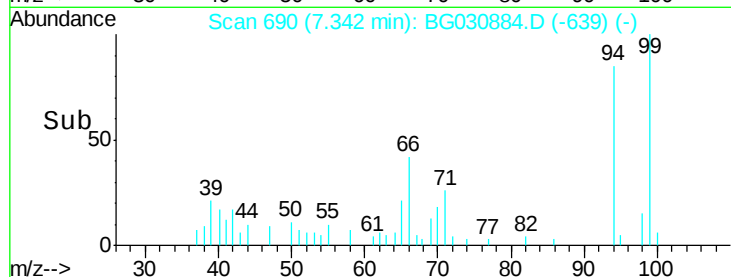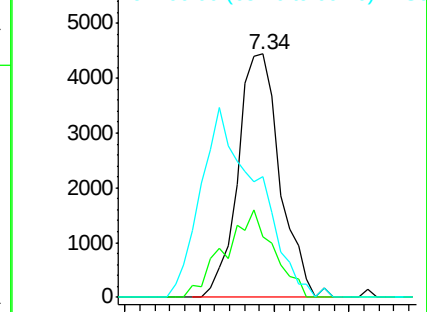

#44

Dimethylphthalate

Concen: 3.57 ng/ul

RT: 14.21 min Scan# 1859

Delta R.T. 0.00 min

Lab File: BG030884.D

Acq: 9 Nov 2017 17:41


Tgt Ion:163 Resp: 58611

Ion Ratio Lower Upper



163 100


194 5.1 3.5 5.3

164 10.0 7.6 11.4

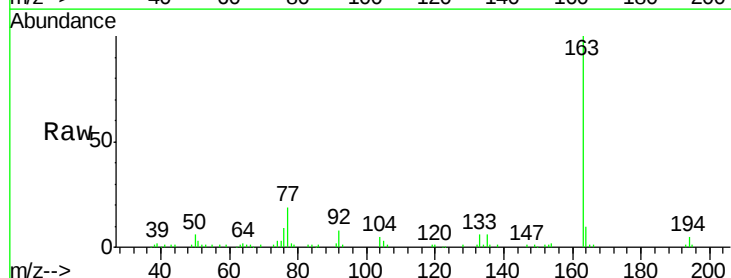

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

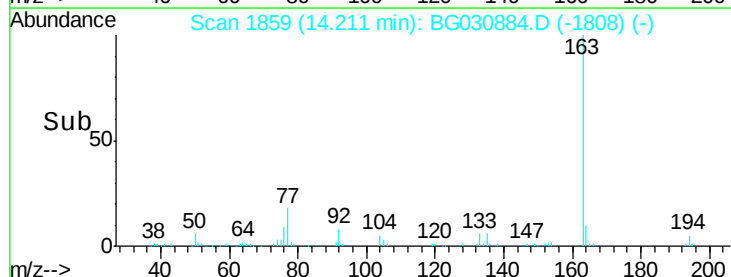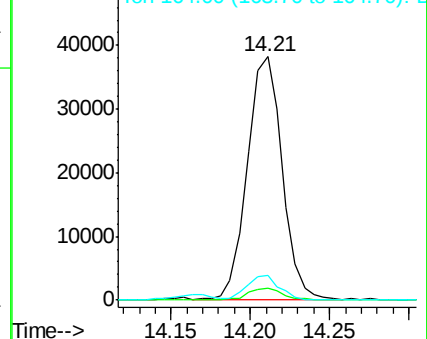

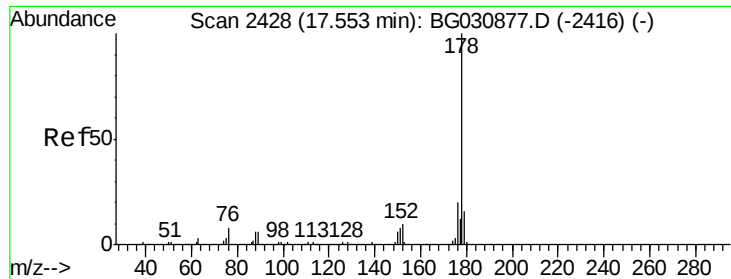

#69

Phenanthrene

Concen: 5.63 ng/ul

RT: 17.55 min Scan# 2427

Delta R.T. -0.00 min

Lab File: BG030884.D

Acq: 9 Nov 2017 17:41

Instrument :

BNA_G

ClientSampleId :


Tot Ion:178 Resp: 146113

Ion Ratio Lower Upper

178 100

179 15.6 13.0 19.6




176 19.5 15.3 22.9

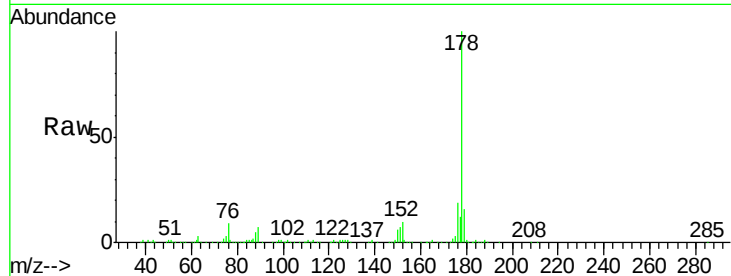

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

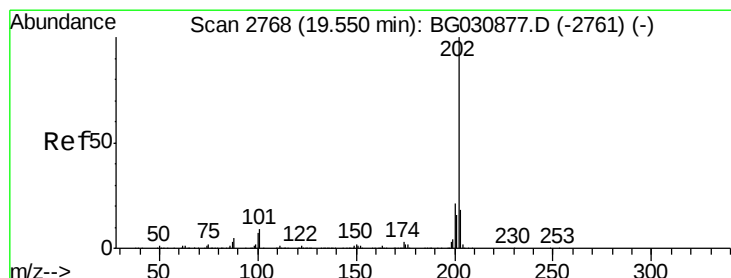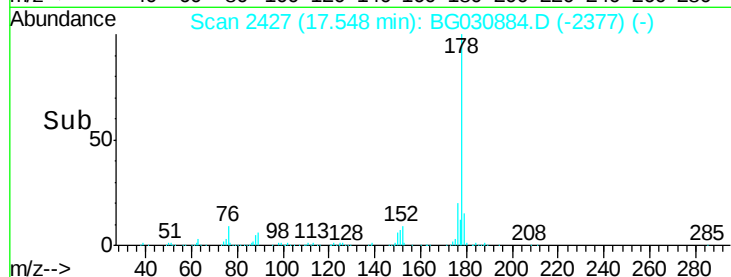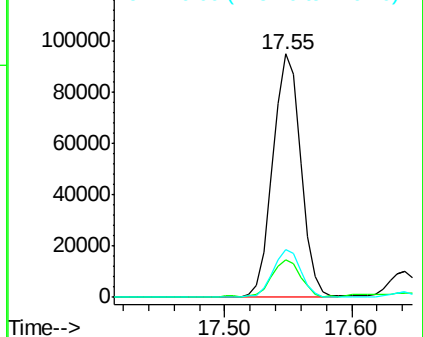

#74

Fluoranthene

Concen: 7.85 ng/ul

RT: 19.55 min Scan# 2767

Delta R.T. -0.00 min

Lab File: BG030884.D

Acq: 9 Nov 2017 17:41


Tgt Ion:202 Resp: 227647

Ion Ratio Lower Upper

202 100

101 8.8 7.4 11.2



100 6.9 5.6 8.4

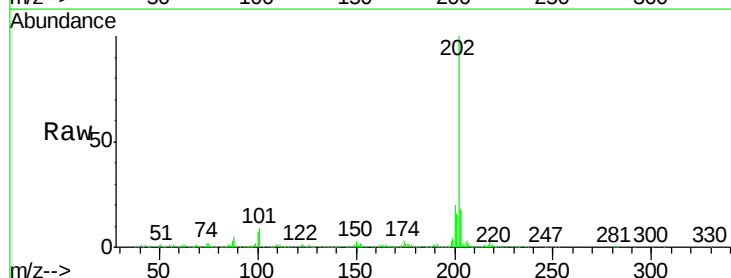


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

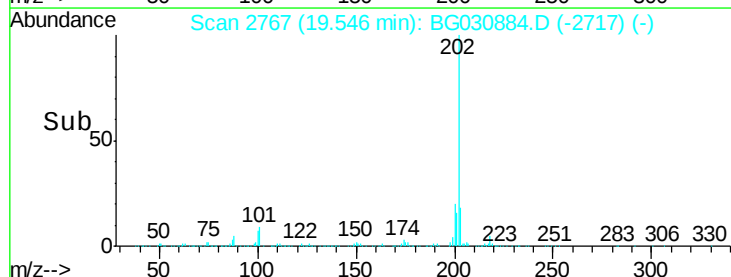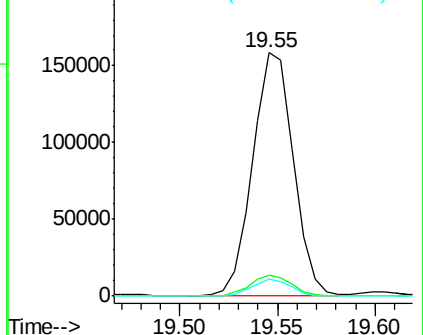

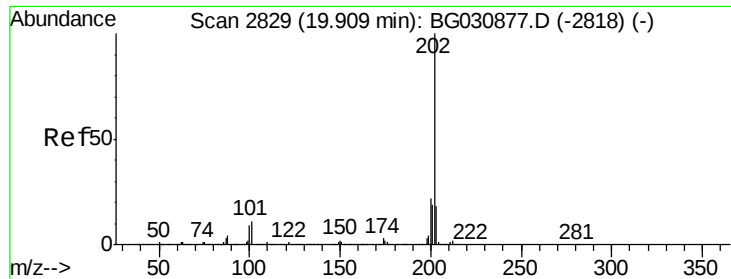

#77

Pvrene

Concen: 8.53 ng/ul

RT: 19.91 min Scan# 2829

Delta R.T. 0.00 min

Lab File: BG030884.D

Acq: 9 Nov 2017 17:41

Instrument :

BNA_G

ClientSampleId :


Tot Ion:202 Resp: 300127

Ion Ratio Lower Upper

202 100

101 9.9 8.4 12.6

100 8.0 7.0 10.6



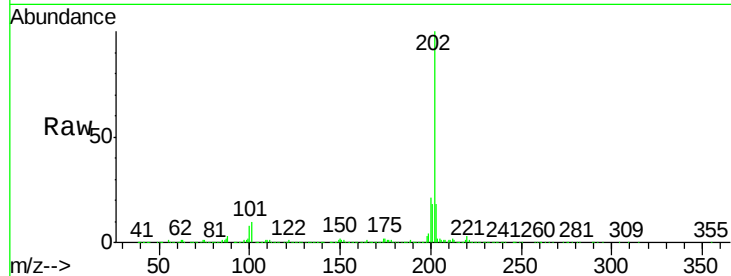


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

Time--> 19.80 19.85 19.90 19.95

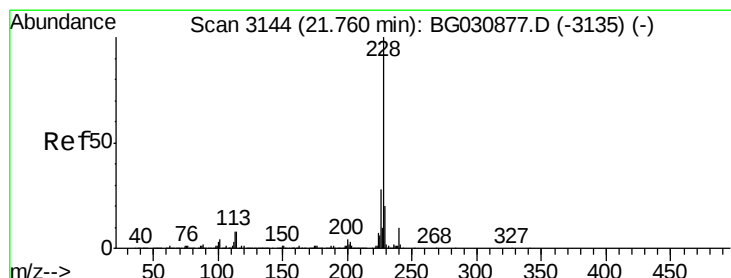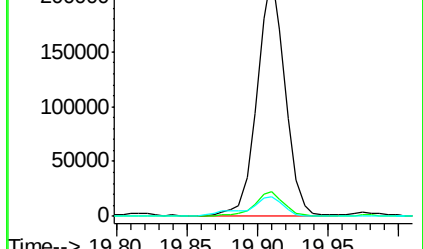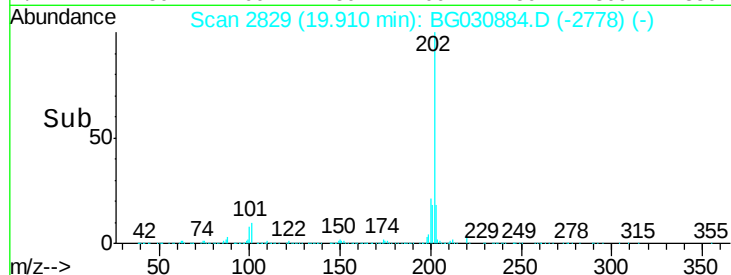

#80

Benzo(a)anthracene

Concen: 4.12 ng/ul

RT: 21.76 min Scan# 3144

Delta R.T. 0.00 min

Lab File: BG030884.D

Acq: 9 Nov 2017 17:41


Tgt Ion:228 Resp: 135586

Ion Ratio Lower Upper

228 100

229 22.9 16.2 24.4

226 29.0 22.2 33.2


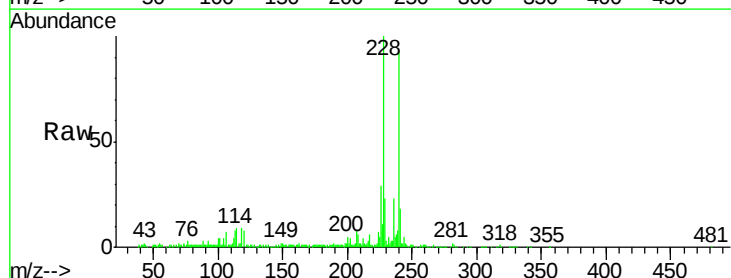



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

Time--> 21.70 21.75 21.80

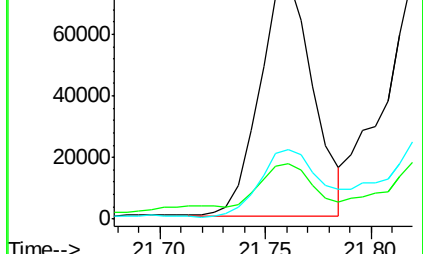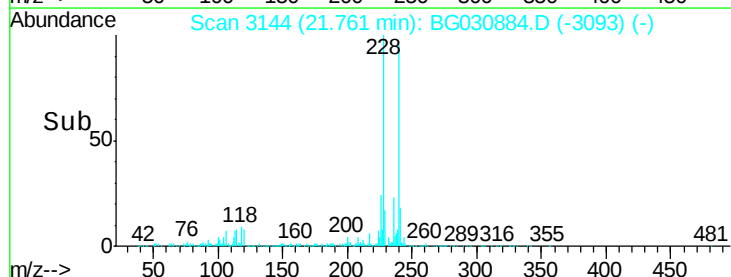

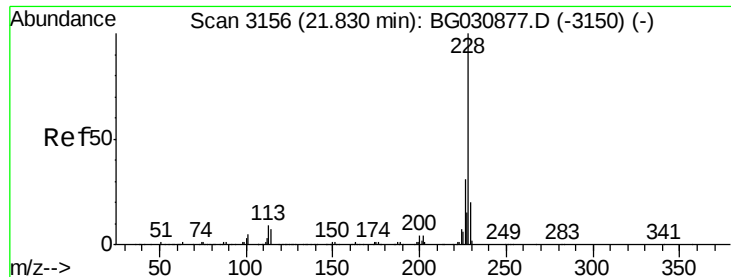

#82

Chrysene

Concen: 6.13 ng/ul

RT: 21.83 min Scan# 3155

Delta R.T. -0.00 min

Lab File: BG030884.D

Acq: 9 Nov 2017 17:41

Instrument :

BNA_G

ClientSampleId :


Tot Ion:228 Resp: 183427

Ion Ratio Lower Upper

228 100

226 29.5 24.2 36.2




229 21.3 15.2 22.8

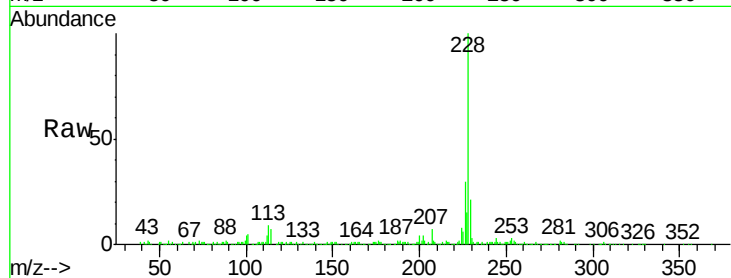

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

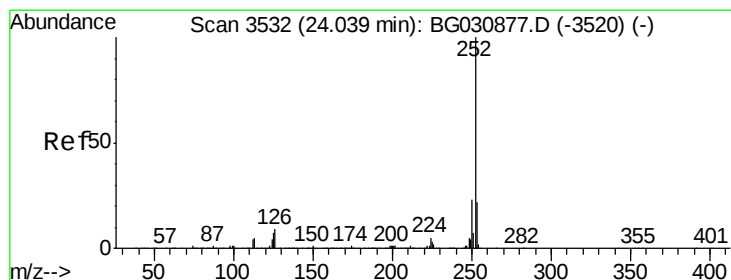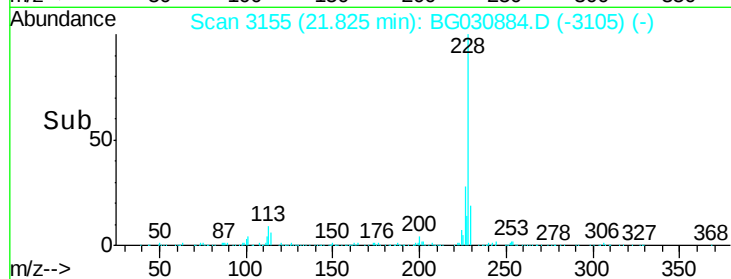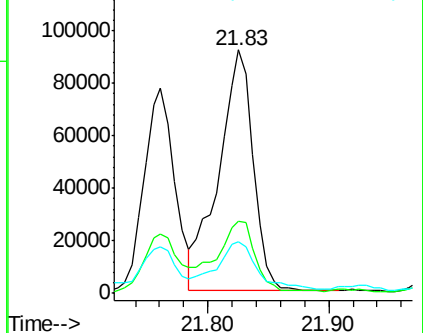

#85

Benzo(b)fluoranthene

Concen: 6.18 ng/ul

RT: 24.03 min Scan# 3531

Delta R.T. -0.00 min

Lab File: BG030884.D

Acq: 9 Nov 2017 17:41


Tgt Ion:252 Resp: 193698

Ion Ratio Lower Upper

252 100

253 23.8 17.0 25.4



125 7.4 7.5 11.3#

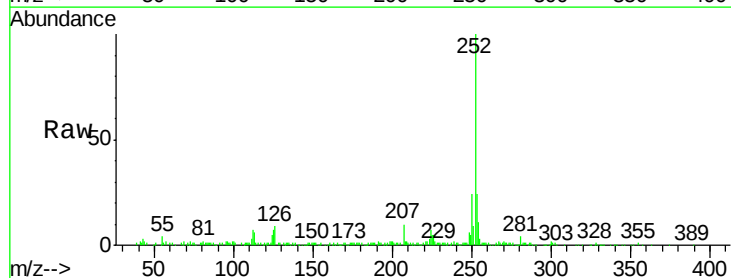


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



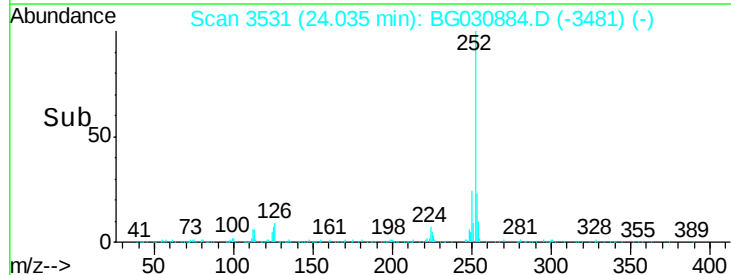
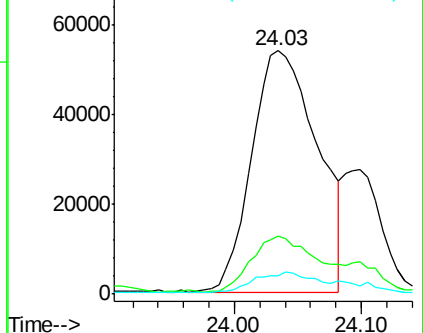


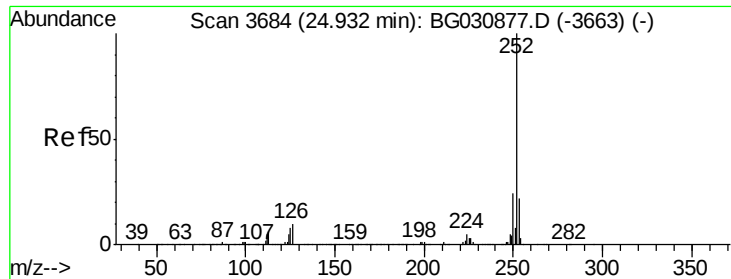

#88
Benzo(a)pyrene
Concen: 4.43 ng/ul
RT: 24.93 min Scan# 3683
Delta R.T. -0.00 min
Lab File: BG030884.D
Acq: 9 Nov 2017 17:41




Instrument :
BNA_G
ClientSampleId :


Tot Ion:252 Resp: 134995
Ion Ratio Lower Upper
252 100
253 23.1 17.1 25.7
125 8.9 7.8 11.8

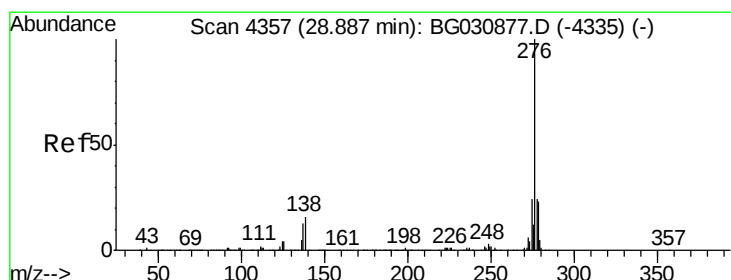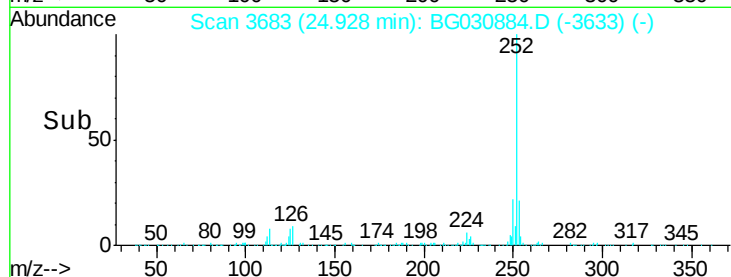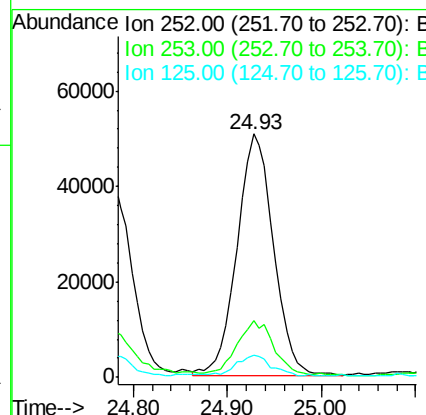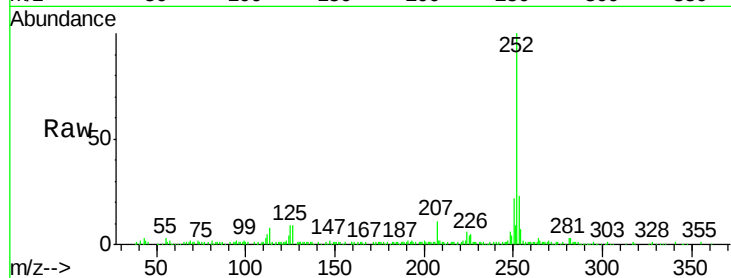

#89
Indeno(1,2,3-cd)pyrene
Concen: 2.61 ng/ul
RT: 28.87 min Scan# 4354
Delta R.T. -0.02 min
Lab File: BG030884.D
Acq: 9 Nov 2017 17:41

Tgt Ion:276 Resp: 90009
Ion Ratio Lower Upper
276 100
138 16.2 13.4 20.0
277 23.9 18.6 28.0

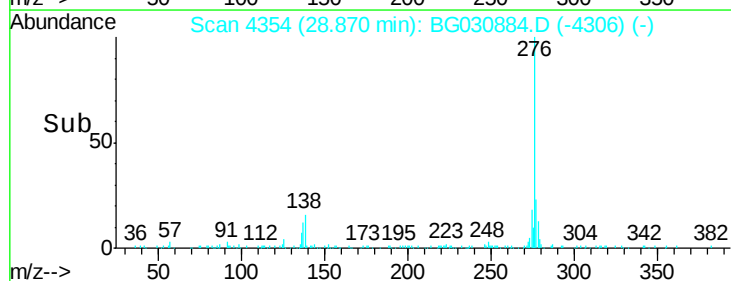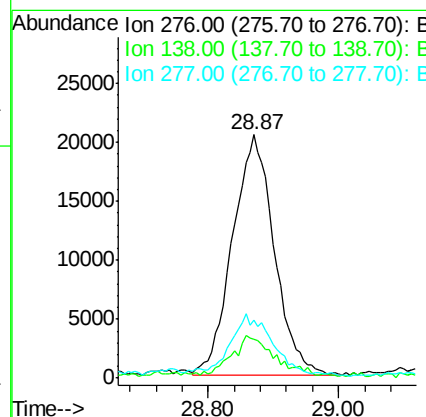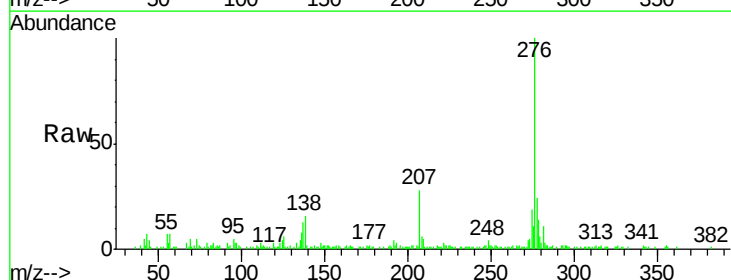

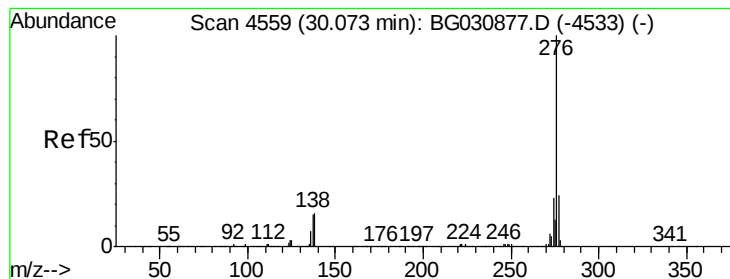

#91

Benzo(a,h,i)perylene

Concen: 2.83 ng/ul

RT: 30.06 min Scan# 4556

Delta R.T. -0.02 min

Lab File: BG030884.D

Acq: 9 Nov 2017 17:41

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 276 Resp: 80967

Ion Ratio Lower Upper

276 100

138 18.4 12.1 18.1#

277 25.4 17.7 26.5

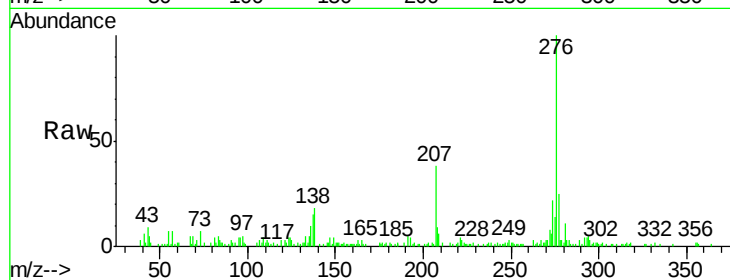

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

