

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110917\
 Data File : BG030897.D
 Acq On : 10 Nov 2017 1:50
 Operator : SJ/JU
 Sample : I6286-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 10 03:50:57 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 03:42:09 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	80497	20.00	ng/ul	0.00
18) Naphthalene-d8	10.96	136	379729	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.77	164	249959	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	606294	20.00	ng/ul	0.00
75) Chrysene-d12	21.78	240	638562	20.00	ng/ul	0.00
83) Perylene-d12	25.10	264	649749	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	5029	2.54	ng/uL	0.00
5) Phenol-d5	7.32	99	116014	15.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	69718	14.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	98158	18.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	71558	11.47	ng/ul	0.00
19) Nitrobenzene-d5	9.31	128	51427	18.87	ng/ul	0.00
22) 2-Nitrophenol-d4	10.04	143	61979	22.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	109389	17.19	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	100685	13.62	ng/ul	0.00
43) Dimethylphthalate-d6	14.17	166	368020	17.22	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	465505	17.91	ng/ul	0.00
51) 4-Nitrophenol-d4	14.98	143	52177	13.23	ng/ul	0.00
57) Fluorene-d10	15.76	176	344458	19.68	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.88	200	56920	19.23	ng/ul	0.00
70) Anthracene-d10	17.61	188	540062	18.83	ng/ul	0.00
76) Pyrene-d10	19.88	212	622398	18.83	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.87	264	587026	19.08	ng/ul	0.00

Target Compounds


					Ovalue	
6) Phenol	7.34	94	9737	1.22	ng/ul	98
44) Dimethylphthalate	14.21	163	29432	1.41	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110917\
Data File : BG030897.D
Acq On : 10 Nov 2017 1:50
Operator : SJ/JU
Sample : I6286-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 10 03:50:57 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 03:42:09 2017
Response via : Initial Calibration

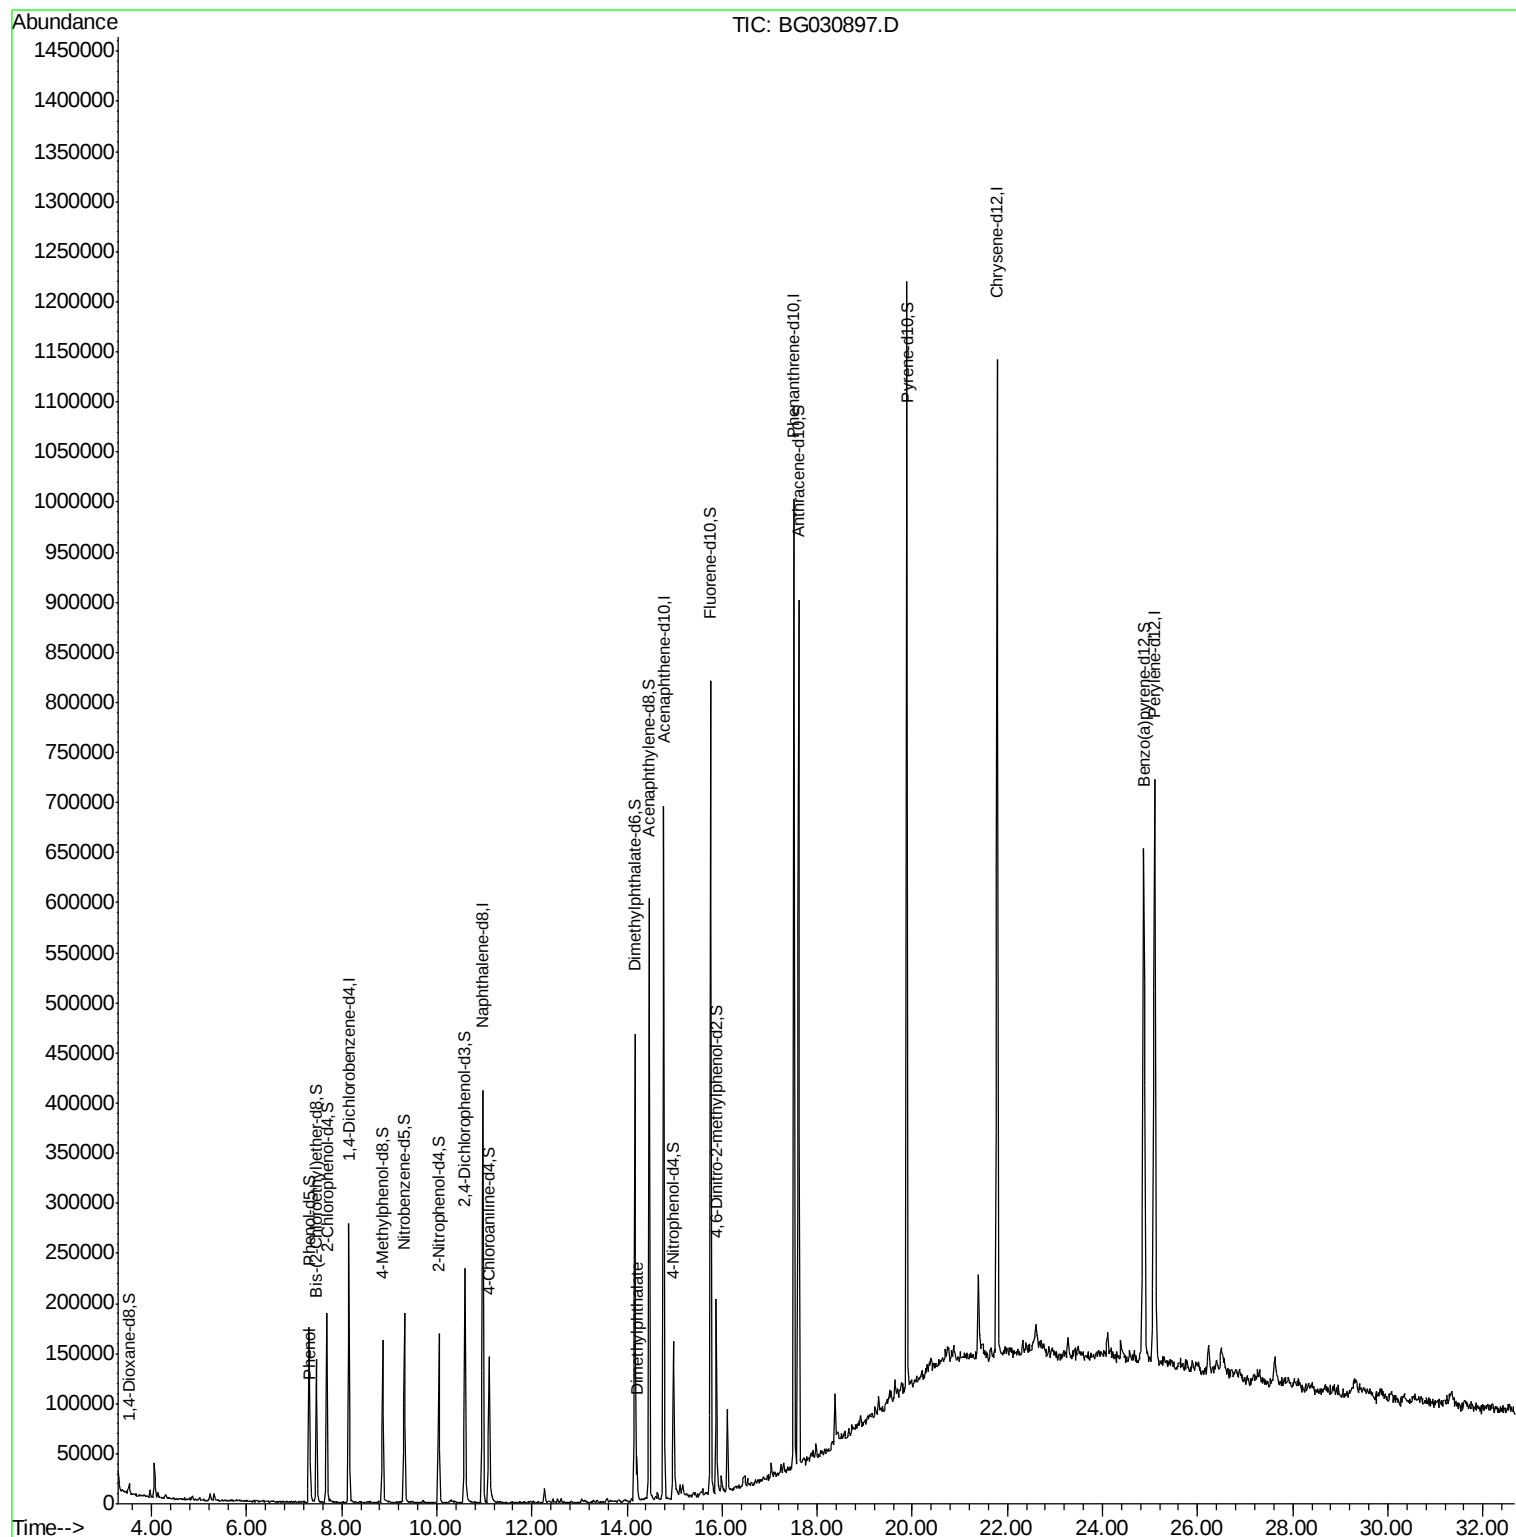

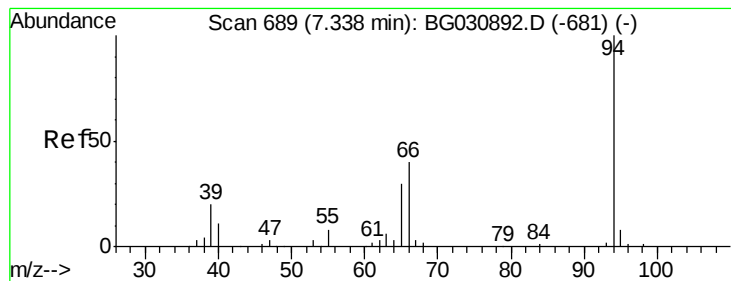

#6

Phenol

Concen: 1.22 ng/ul

RT: 7.34 min Scan# 689

Delta R.T. 0.00 min

Lab File: BG030897.D

Acq: 10 Nov 2017 1:50

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 94 Resp: 9737

Ion Ratio Lower Upper




94 100

65 31.5 27.1 40.7

66 44.0 34.6 52.0

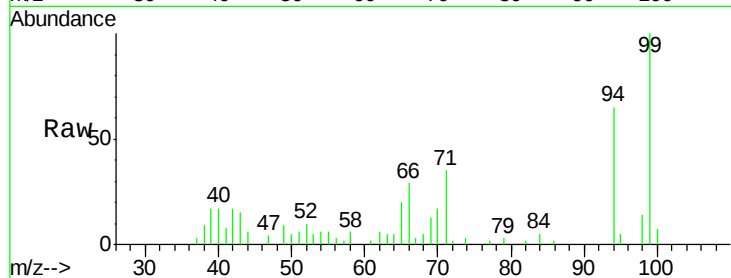

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

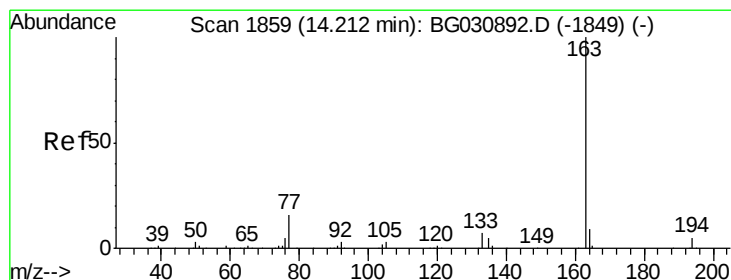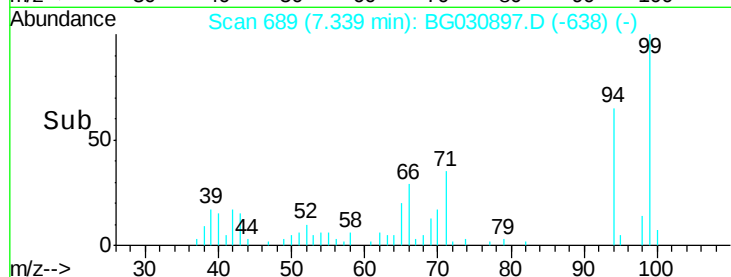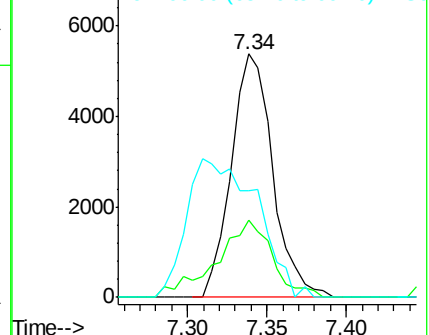

#44

Dimethylphthalate

Concen: 1.41 ng/ul

RT: 14.21 min Scan# 1858

Delta R.T. -0.01 min

Lab File: BG030897.D

Acq: 10 Nov 2017 1:50


Tgt Ion:163 Resp: 29432

Ion Ratio Lower Upper

163 100

194 5.4 3.5 5.3#

164 11.6 7.6 11.4#

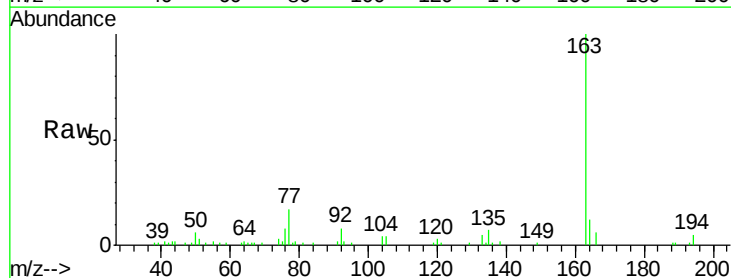

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

