

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110920\
 Data File : BG047253.D
 Acq On : 9 Nov 2020 13:24
 Operator : CG/JU
 Sample : PB132773BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.574	37	40	41	rBV	1392	1156	0.12%	0.027%
2	3.615	45	47	50	rVV	1515	1824	0.19%	0.043%
3	3.668	52	56	61	rVB3	7288	9563	1.00%	0.225%
4	3.914	97	98	101	rBV2	1115	1284	0.13%	0.030%
5	3.973	105	108	112	rVB3	1553	2349	0.25%	0.055%
6	4.144	132	137	141	rBV2	4211	5882	0.62%	0.138%
7	4.326	166	168	171	rBV2	1726	1631	0.17%	0.038%
8	4.408	179	182	183	rVB	1501	1279	0.13%	0.030%
9	4.432	183	186	188	rBV2	1496	1473	0.15%	0.035%
10	4.461	188	191	194	rVV3	858	1256	0.13%	0.030%
11	4.514	197	200	202	rVB	1476	1345	0.14%	0.032%
12	4.667	225	226	229	rBV	1255	1121	0.12%	0.026%
13	4.743	232	239	244	rVB3	1174	1895	0.20%	0.045%
14	5.019	283	286	290	rBV2	2063	3185	0.33%	0.075%
15	5.078	293	296	301	rVB3	2559	3480	0.36%	0.082%
16	5.125	303	304	308	rVB2	1359	1263	0.13%	0.030%
17	5.154	308	309	311	rBV	1520	1270	0.13%	0.030%
18	5.307	333	335	336	rBV	1276	1247	0.13%	0.029%
19	5.407	349	352	355	rBV2	982	1263	0.13%	0.030%
20	5.900	433	436	438	rBV	1402	1606	0.17%	0.038%
21	6.088	464	468	470	rVB	1112	1426	0.15%	0.034%
22	6.182	483	484	486	rBV	1633	1118	0.12%	0.026%
23	6.229	489	492	495	rBV2	1007	1138	0.12%	0.027%
24	6.423	523	525	528	rVB	1606	1267	0.13%	0.030%
25	6.776	584	585	588	rBV	1270	1322	0.14%	0.031%
26	6.905	603	607	608	rVB2	1178	1304	0.14%	0.031%
27	7.146	646	648	651	rBV	792	1219	0.13%	0.029%
28	7.175	651	653	656	rVB	1444	1358	0.14%	0.032%
29	7.293	670	673	674	rBV	1417	1156	0.12%	0.027%
30	7.528	710	713	716	rVB	1256	1119	0.12%	0.026%
31	8.004	785	794	802	rBV	220925	370307	38.83%	8.715%
32	8.104	810	811	814	rVB	1495	1158	0.12%	0.027%
33	9.144	986	988	992	rBV	1389	2240	0.23%	0.053%
34	9.279	1006	1011	1014	rBV2	1090	1369	0.14%	0.032%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110920\
 Data File : BG047253.D
 Acq On : 9 Nov 2020 13:24
 Operator : CG/JU
 Sample : PB132773BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
 Title : SVOA CALIBRATION

35	9.467	1040	1043	1047	rVB2	1195	1773	0.19%	0.042%
36	9.508	1047	1050	1051	rVB2	1381	1179	0.12%	0.028%
37	9.708	1081	1084	1087	rBV2	986	1192	0.13%	0.028%
38	10.231	1169	1173	1174	rBV	893	1165	0.12%	0.027%
39	10.319	1184	1188	1192	rBV	1080	1242	0.13%	0.029%
40	10.595	1230	1235	1236	rBV	827	1118	0.12%	0.026%
41	10.812	1262	1272	1282	rBV	259243	462231	48.47%	10.879%
42	11.282	1349	1352	1355	rBV2	1397	2078	0.22%	0.049%
43	11.382	1367	1369	1374	rBV2	915	1275	0.13%	0.030%
44	12.704	1593	1594	1597	rBV2	1159	1151	0.12%	0.027%
45	12.763	1602	1604	1607	rVV2	1200	1212	0.13%	0.029%
46	12.898	1621	1627	1628	rVB	870	1371	0.14%	0.032%
47	13.609	1745	1748	1752	rBV2	1045	1504	0.16%	0.035%
48	13.768	1772	1775	1776	rBV2	1177	1114	0.12%	0.026%
49	13.850	1787	1789	1791	rVB	1706	1217	0.13%	0.029%
50	13.903	1791	1798	1802	rBV2	932	1896	0.20%	0.045%
51	14.185	1842	1846	1847	rBV	1306	1118	0.12%	0.026%
52	14.643	1916	1924	1934	rBV2	389858	626391	65.69%	14.742%
53	15.219	2016	2022	2027	rVB2	1482	2635	0.28%	0.062%
54	15.272	2027	2031	2032	rBV	1167	1501	0.16%	0.035%
55	15.818	2123	2124	2129	rBV2	2005	1279	0.13%	0.030%
56	15.947	2142	2146	2148	rBV	800	1139	0.12%	0.027%
57	16.036	2157	2161	2162	rVB	1338	1146	0.12%	0.027%
58	16.118	2173	2175	2180	rVB	1202	1609	0.17%	0.038%
59	16.341	2210	2213	2217	rBV2	1607	2041	0.21%	0.048%
60	16.629	2259	2262	2265	rBV2	1621	1331	0.14%	0.031%
61	16.723	2277	2278	2281	rBV2	1718	1293	0.14%	0.030%
62	16.811	2291	2293	2295	rBV3	1566	1397	0.15%	0.033%
63	17.140	2347	2349	2351	rVB2	1813	1453	0.15%	0.034%
64	17.258	2364	2369	2370	rBV	1079	1305	0.14%	0.031%
65	17.387	2384	2391	2401	rBV	487470	764970	80.22%	18.004%
66	17.616	2427	2430	2433	rBV2	1445	1493	0.16%	0.035%
67	17.869	2471	2473	2475	rVB	1259	1148	0.12%	0.027%
68	17.898	2475	2478	2480	rBV2	1416	1495	0.16%	0.035%
69	18.051	2501	2504	2507	rBV3	2040	2016	0.21%	0.047%
70	18.086	2508	2510	2515	rVV	1240	1531	0.16%	0.036%
71	18.145	2518	2520	2525	rBV2	1406	2476	0.26%	0.058%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110920\
 Data File : BG047253.D
 Acq On : 9 Nov 2020 13:24
 Operator : CG/JU
 Sample : PB132773BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
 Title : SVOA CALIBRATION

72	18.215	2529	2532	2534	rBV3	1742	1460	0.15%	0.034%
73	18.327	2549	2551	2555	rVB	1312	1547	0.16%	0.036%
74	18.644	2603	2605	2607	rVB4	1794	1502	0.16%	0.035%
75	18.727	2616	2619	2621	rBV	1373	1698	0.18%	0.040%
76	18.756	2623	2624	2627	rBV	2129	2117	0.22%	0.050%
77	18.850	2638	2640	2642	rBV2	1241	1161	0.12%	0.027%
78	18.985	2661	2663	2664	rVB2	2055	1350	0.14%	0.032%
79	19.009	2664	2667	2669	rBV3	2042	2197	0.23%	0.052%
80	19.214	2700	2702	2703	rVB2	2919	1381	0.14%	0.033%
81	19.273	2710	2712	2715	rBV2	2804	1813	0.19%	0.043%
82	19.338	2719	2723	2725	rBV	1273	1570	0.16%	0.037%
83	19.467	2744	2745	2748	rBV3	1941	1893	0.20%	0.045%
84	19.608	2768	2769	2771	rBV2	2646	1997	0.21%	0.047%
85	19.814	2802	2804	2807	rBV2	4025	3908	0.41%	0.092%
86	19.855	2809	2811	2814	rVV2	2363	1901	0.20%	0.045%
87	19.902	2817	2819	2821	rBV2	3022	2655	0.28%	0.062%
88	20.242	2875	2877	2878	rBV2	2786	1819	0.19%	0.043%
89	20.607	2937	2939	2941	rBV3	3899	2015	0.21%	0.047%
90	21.647	3109	3116	3127	rBV	564365	953587	100.00%	22.443%
91	24.837	3649	3659	3673	rVB	320576	925072	97.01%	21.772%


Sum of corrected areas: 4249001

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG110920\
Data File : BG047253.D
Acq On : 9 Nov 2020 13:24
Operator : CG/JU
Sample : PB132773BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK73

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

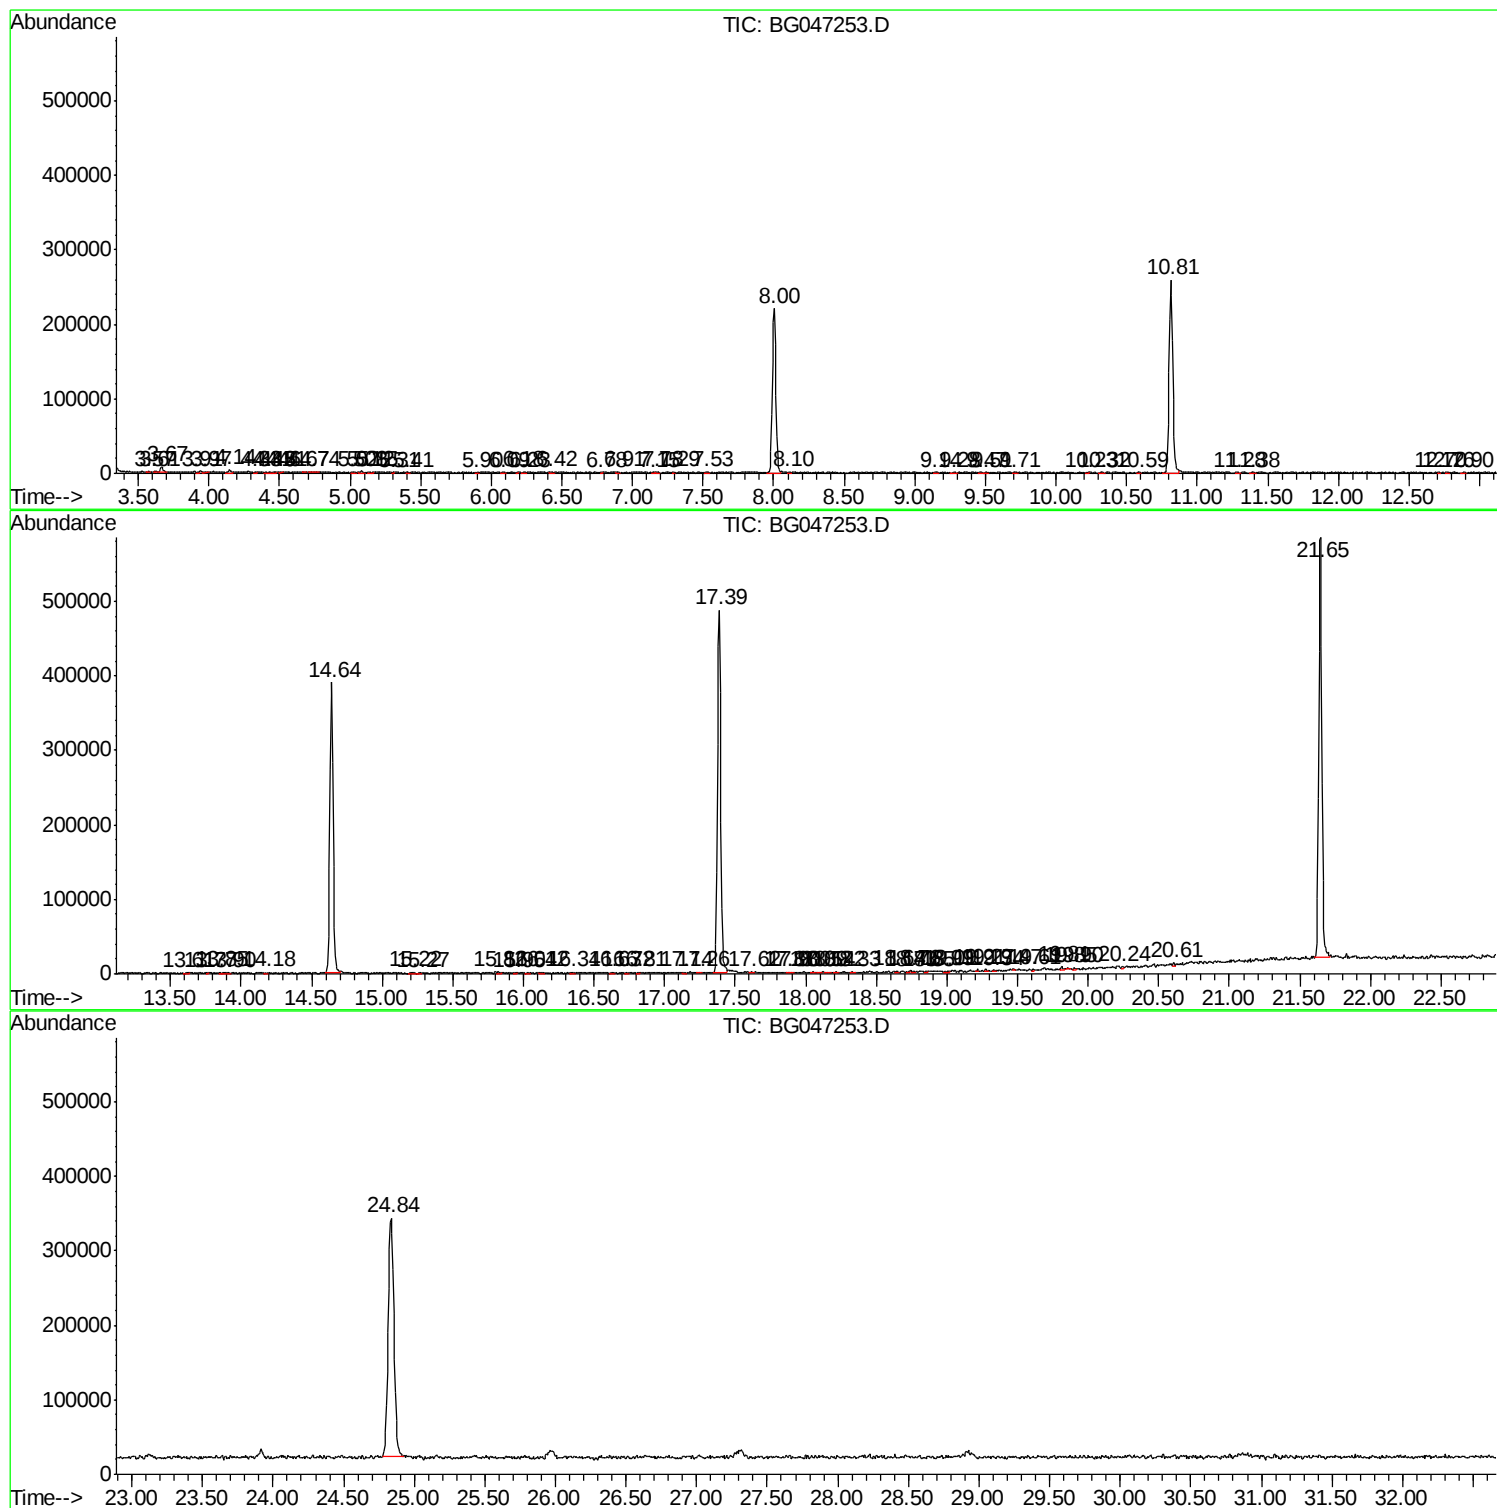

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG110920\
Data_File : BG047253.D
Acq_On : 9 Nov 2020 13:244
Operator : CG/JUU
Sample : PB132773BLL
Misc :
ALS_Vial : 5 Sample Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
SBLK73

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG102220MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
