
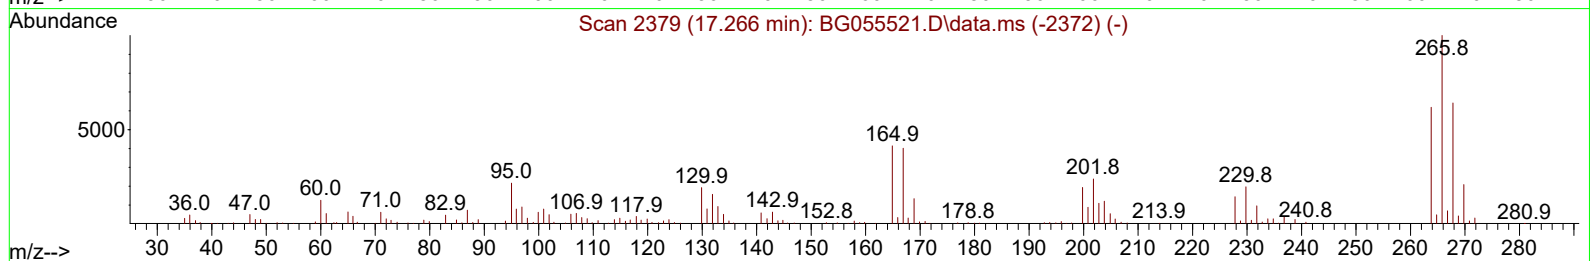
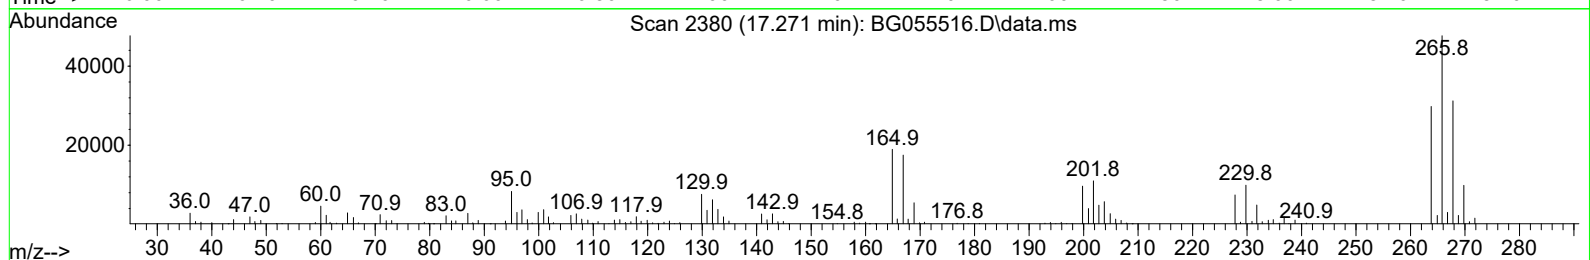


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110922\
Data File : BG055516.D
Acq On : 9 Nov 2022 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 16:21:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 16:20:23 2022
Response via : Initial Calibration

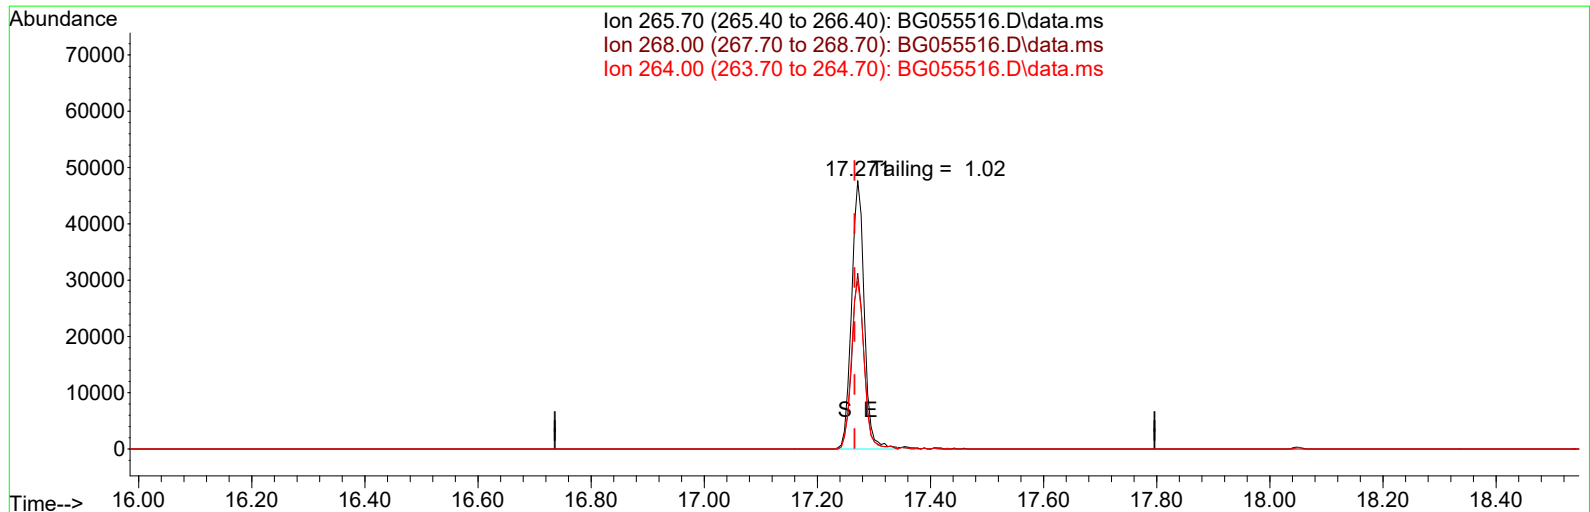

TIC: BG055516.D\data.ms

(70) Pentachlorophenol (C)




17.271min (+ 0.005) 17349.30 ng

response 74816

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	65.44
264.00	61.90	62.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110922\
Data File : BG055516.D
Acq On : 9 Nov 2022 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 16:21:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 09 16:20:23 2022
Response via : Initial Calibration

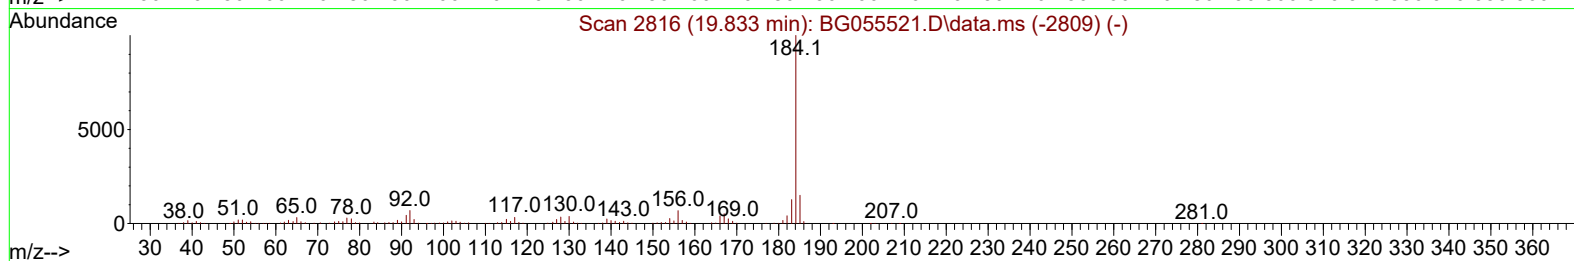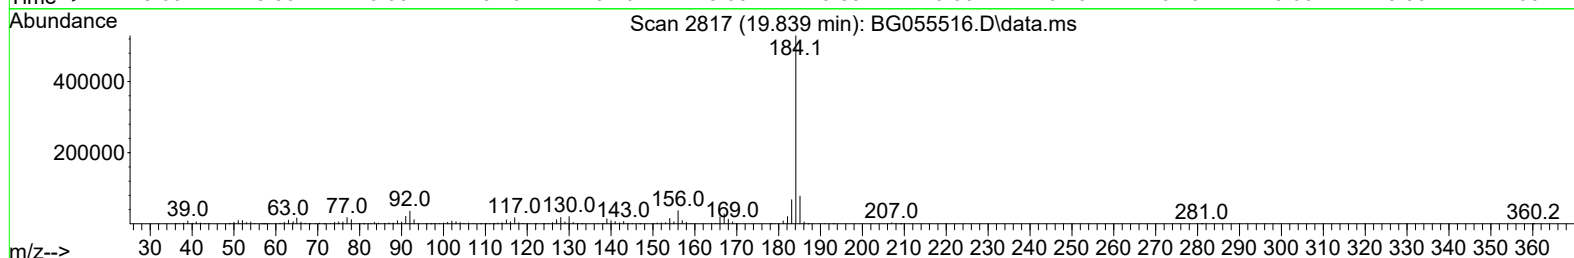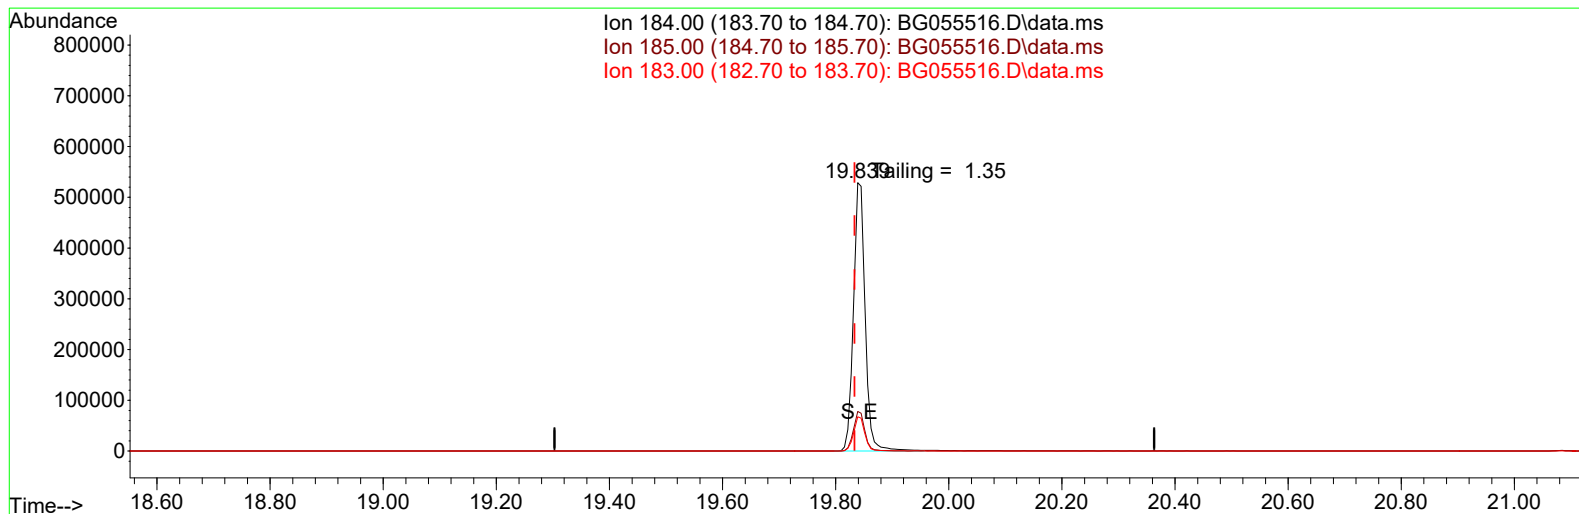

TIC: BG055516.D\data.ms

(77) Benzidine**19.839min (+ 0.006) 85400.85 ng****response 762445**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.75
183.00	12.70	12.78
0.00	0.00	0.00